

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS042123\
 Data File : PS022794.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Apr 2023 10:48
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 21 21:29:19 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS041223.M
 Quant Title : 8080.M
 QLast Update : Wed Apr 12 14:05:56 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.486	0.000	1615327	0	<MDL	N.D. #
Target Compounds							
1) T	Dalapon	2.582	0.000	852323	0	<MDL	N.D. #
2) T	3,5-DICHL...	5.853	0.000	335501	0	<MDL	N.D. #
3) T	4-Nitroph...	6.315	0.000	15843084	0	8.538	N.D. #
5) T	DICAMBA	6.580f	0.000	465032	0	<MDL	N.D. #
6) T	MCP	6.816	7.175f	18338061	1734975	2.179	<MDL #
7) T	MCPA	6.948	0.000	241181	0	<MDL	N.D. #
8) T	DICHLORPROP	7.243	7.665	5012190	5020527	1.648	4.508 #
9) T	2,4-D	7.448	7.935	5047245	2439097	1.363	1.904 #
10) T	Pentachlo...	7.694	8.361	12077795	1274649	<MDL	<MDL #
11) T	2,4,5-TP ...	8.218	8.685f	20907424	640730	1.141	<MDL #
12) T	2,4,5-T	8.482	9.105	8107837	1808575	<MDL	<MDL #
13) T	2,4-DB	8.980	9.626	40333409	4267471	9.439	5.696 #
15) T	Picloram	9.893	10.911	203.1E6	35644094	6.819	4.382 #
16) T	DCPA	10.342	10.911	5845806	35644094	<MDL	5.133 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS042123\
Data File : PS022794.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Apr 2023 10:48
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 21 21:29:19 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS041223.M
Quant Title : 8080.M
QLast Update : Wed Apr 12 14:05:56 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

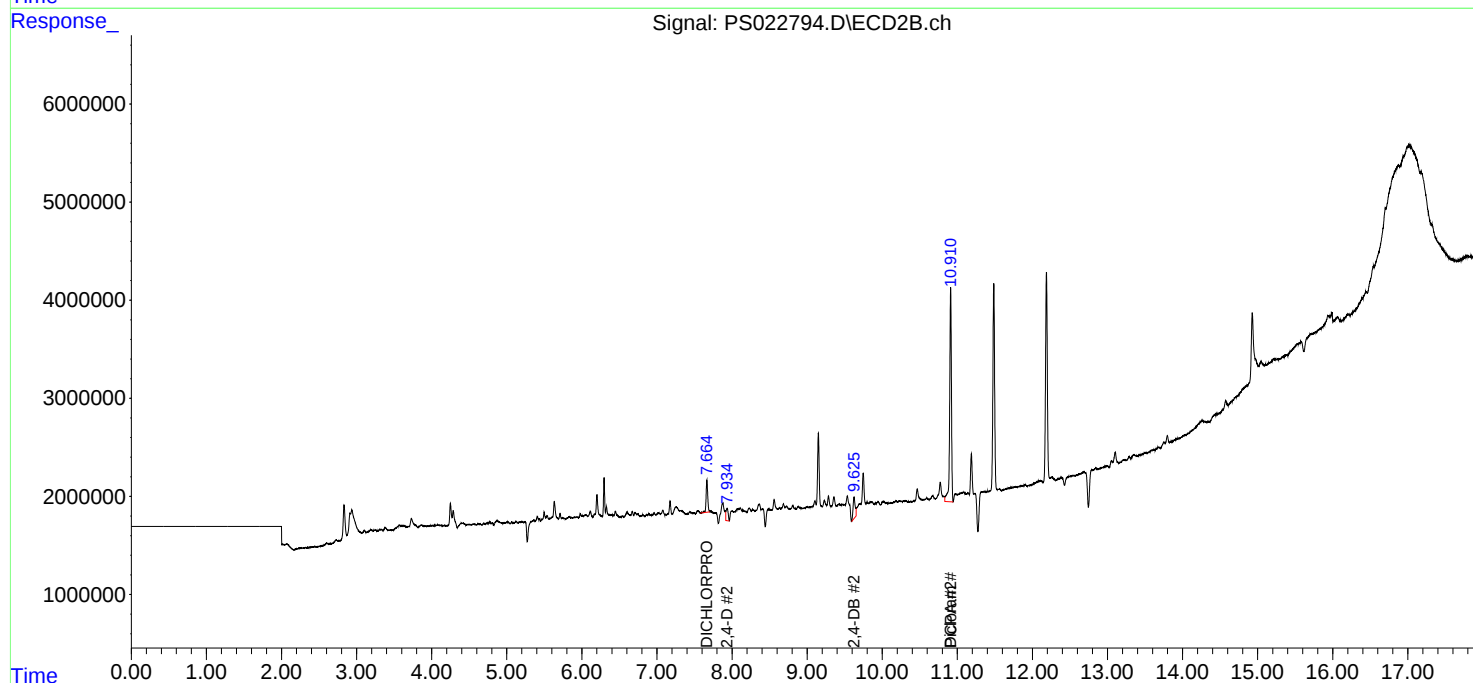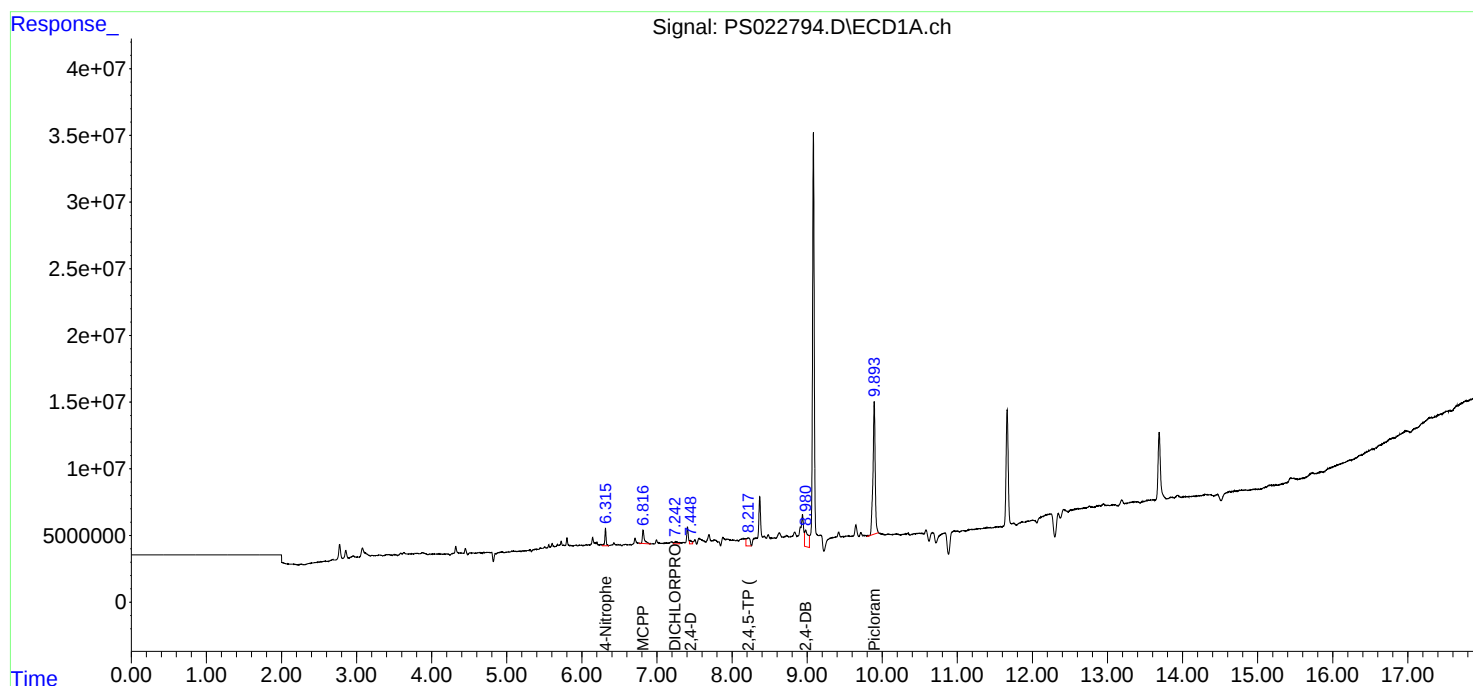


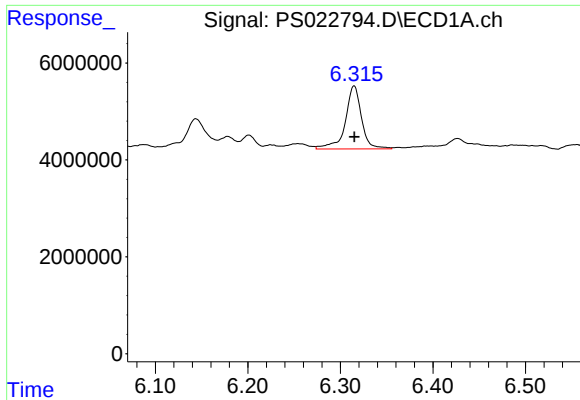

#3 4-Nitrophenol


R.T.: 6.315 min
Delta R.T.: 0.000 min
Response: 15843084
Conc: 8.54 ng/ml

Instrument :
ECD_S
ClientSampleId :

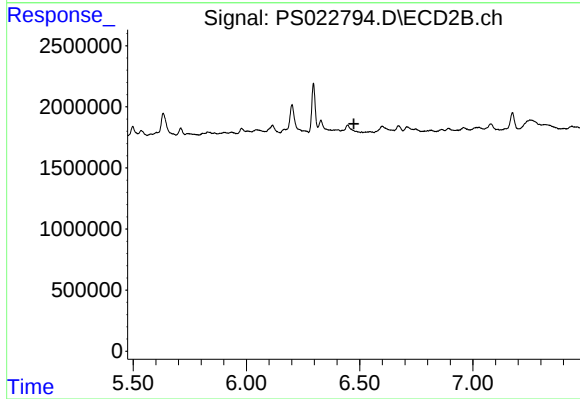


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 6.474 min
Response: 0
Conc: N.D.

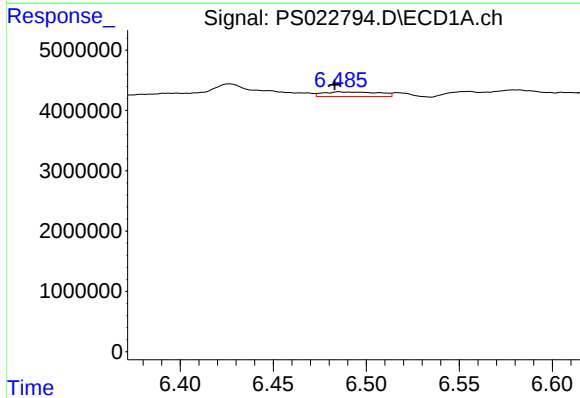


#4 2,4-DCAA

R.T.: 6.486 min
Delta R.T.: 0.003 min
Response: 1615327
Conc: N.D.

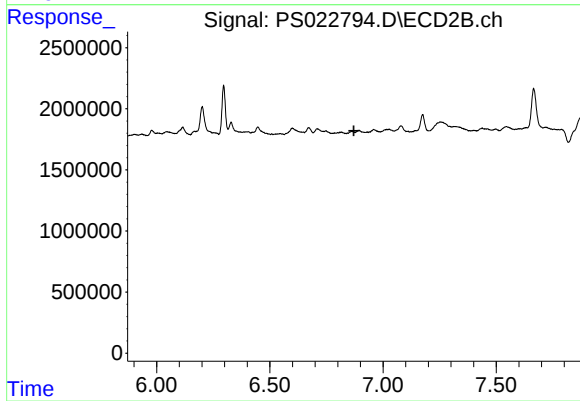

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T. : 6.871 min
Response: 0
Conc: N.D.

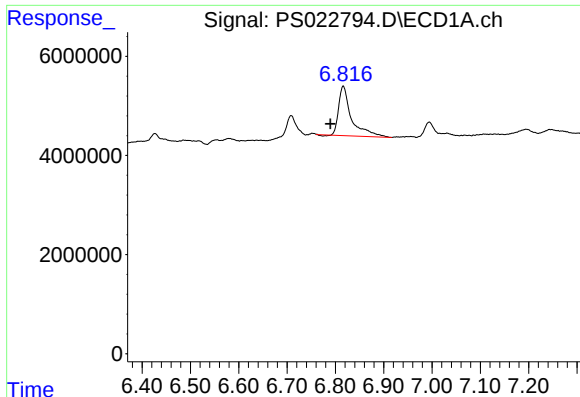

#6 MCPP


R.T.: 6.816 min
Delta R.T.: 0.027 min
Response: 18338061
Conc: 2.18 ug/ml

Instrument :
ECD_S
ClientSampleId :

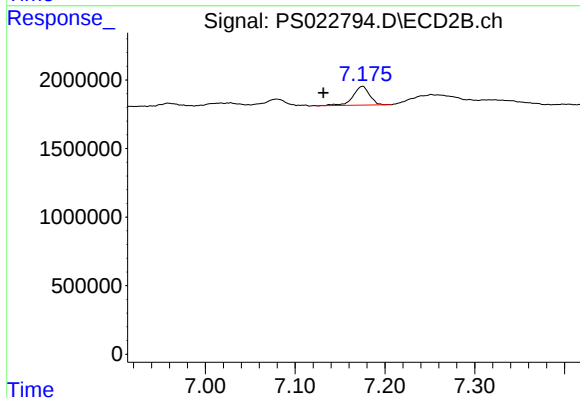


#6 MCPP

R.T.: 7.175 min
Delta R.T.: 0.043 min
Response: 1734975
Conc: N.D.

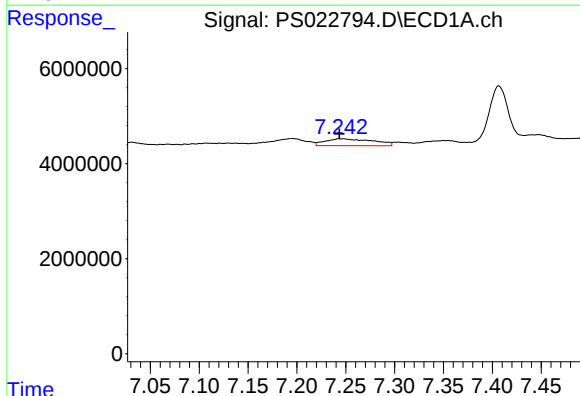


#8 DICHLORPROP

R.T.: 7.243 min
Delta R.T.: 0.000 min
Response: 5012190
Conc: 1.65 ng/ml

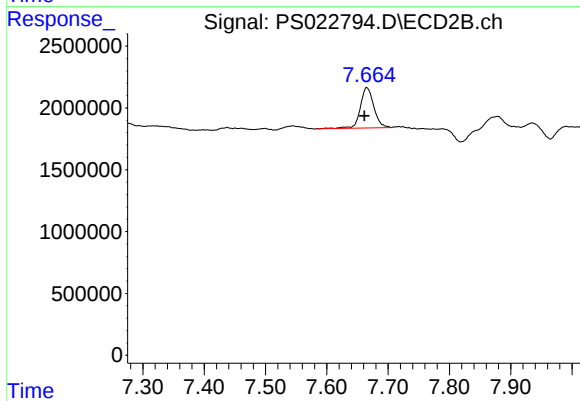

#8 DICHLORPROP


R.T.: 7.665 min
Delta R.T.: 0.004 min
Response: 5020527
Conc: 4.51 ng/ml

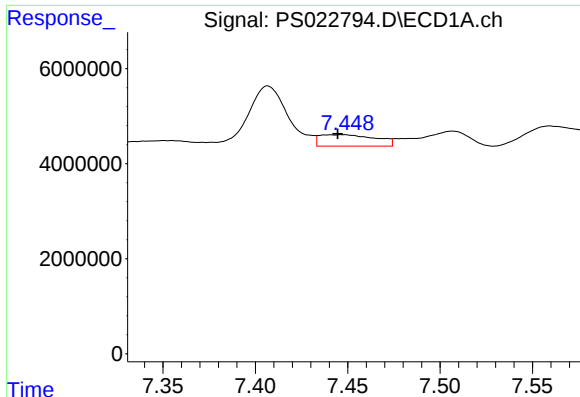

#9 2,4-D


R.T.: 7.448 min
Delta R.T.: 0.003 min
Response: 5047245
Conc: 1.36 ng/ml

Instrument :
ECD_S
ClientSampleId :

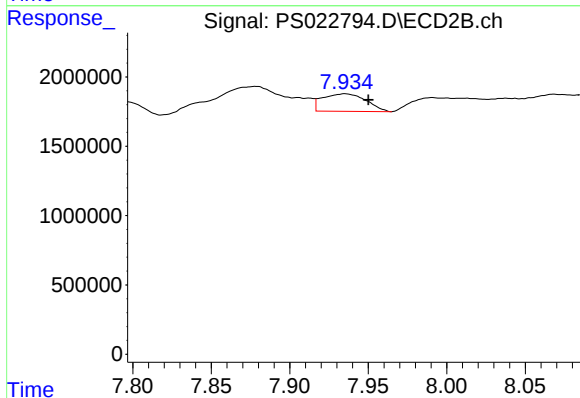


#9 2,4-D

R.T.: 7.935 min
Delta R.T.: -0.015 min
Response: 2439097
Conc: 1.90 ng/ml

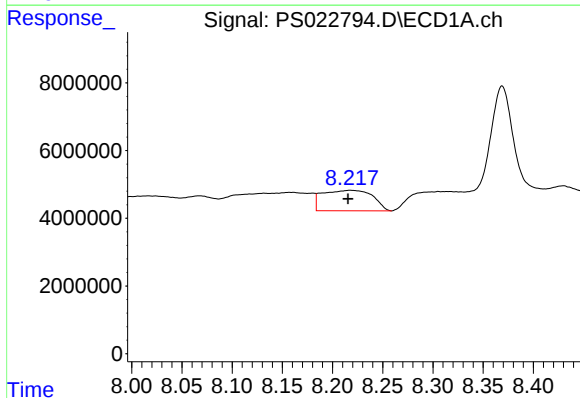


#11 2,4,5-TP (SILVEX)

R.T.: 8.218 min
Delta R.T.: 0.002 min
Response: 20907424
Conc: 1.14 ng/ml

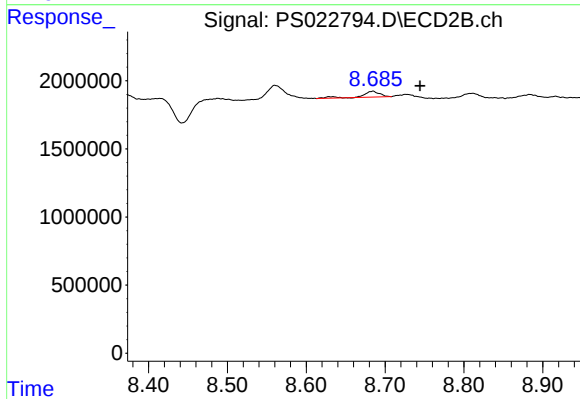

#11 2,4,5-TP (SILVEX)


R.T.: 8.685 min
Delta R.T.: -0.060 min
Response: 640730
Conc: N.D.

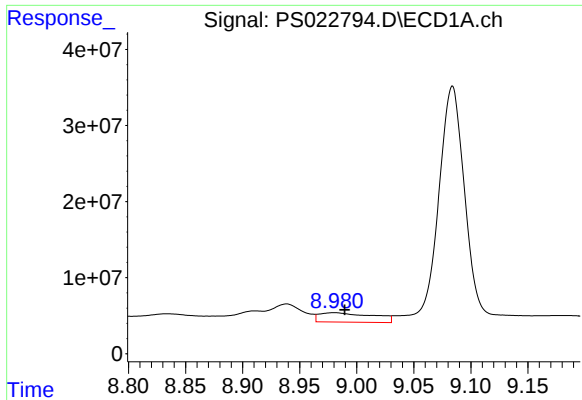

#13 2,4-DB


R.T.: 8.980 min
Delta R.T.: -0.009 min
Response: 40333409
Conc: 9.44 ng/ml

Instrument :
ECD_S
ClientSampleId :

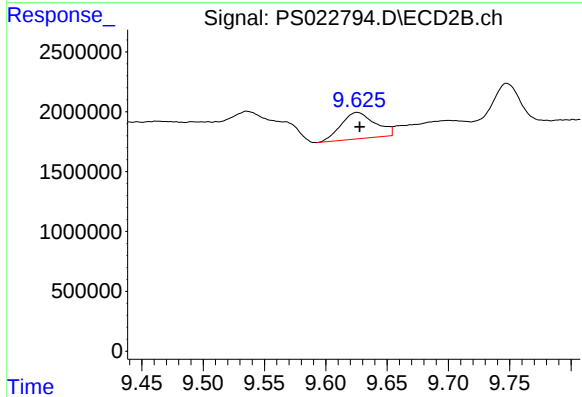


#13 2,4-DB

R.T.: 9.626 min
Delta R.T.: -0.002 min
Response: 4267471
Conc: 5.70 ng/ml

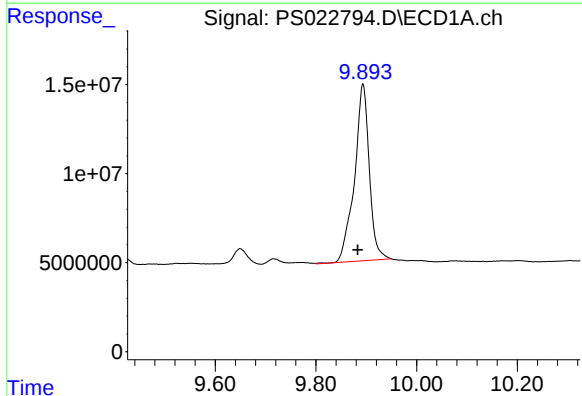


#15 Picloram

R.T.: 9.893 min
Delta R.T.: 0.010 min
Response: 203119023
Conc: 6.82 ng/ml

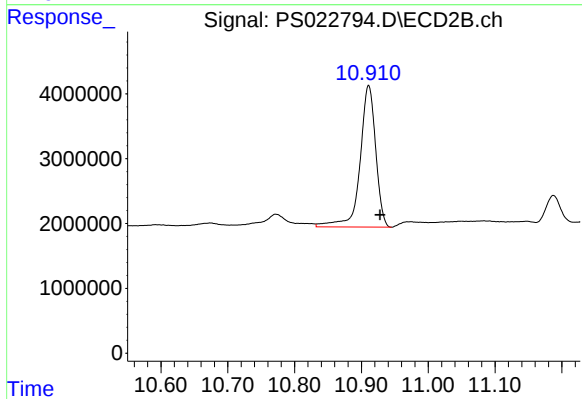

#15 Picloram


R.T.: 10.911 min
Delta R.T.: -0.017 min
Response: 35644094
Conc: 4.38 ng/ml

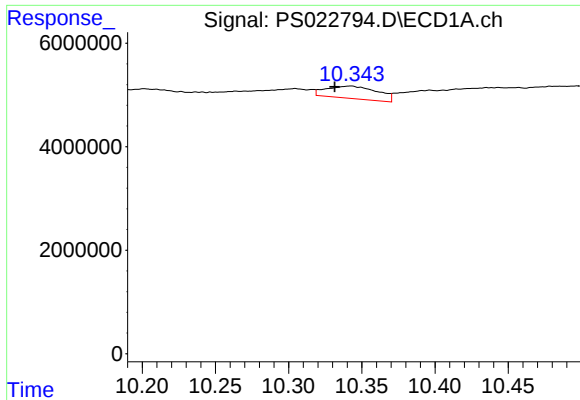

#16 DCPA

R.T.: 10.342 min
Delta R.T.: 0.010 min
Response: 5845806
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

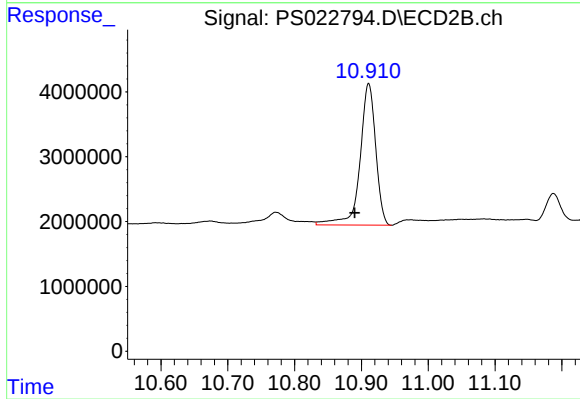

#16 DCPA

R.T.: 10.911 min
Delta R.T.: 0.021 min
Response: 35644094
Conc: 5.13 ng/ml