

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS042123\
 Data File : PS022795.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Apr 2023 11:12
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 21 21:29:57 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS041223.M
 Quant Title : 8080.M
 QLast Update : Wed Apr 12 14:05:56 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.484	6.858	1345.8E6	540.0E6	540.529	529.919
Target Compounds							
1) T	Dalapon	2.575	0.000	5060799	0	1.714	N.D. #
2) T	3,5-DICHL...	5.833	6.102f	494302	105218	<MDL	<MDL #
3) T	4-Nitroph...	6.319	0.000	6732686	0	3.628	N.D. #
5) T	DICAMBA	6.631	0.000	336976	0	<MDL	N.D. #
6) T	MCP	6.818	0.000	10969626	0	1.304	N.D. #
7) T	MCPA	6.931	0.000	113261	0	<MDL	N.D. #
8) T	DICHLORPROP	7.243	7.668	885949	3372378	<MDL	3.028 #
9) T	2,4-D	7.406	7.883f	7437147	726117	2.008	<MDL #
10) T	Pentachlo...	7.681	8.368	2495650	1127731	<MDL	<MDL #
11) T	2,4,5-TP ...	8.216	0.000	3308370	0	<MDL	N.D. #
12) T	2,4,5-T	8.479	9.104	4098612	831986	<MDL	<MDL #
13) T	2,4-DB	8.977	9.692f	10743745	1275201	2.514	1.702 #
14) T	DINOSEB	10.074	0.000	1109318	0	<MDL	N.D. #
15) T	Picloram	9.891	10.911	107.5E6	22506245	3.611	2.767
16) T	DCPA	10.339	10.911	3161682	22506245	<MDL	3.241 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS042123\
Data File : PS022795.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Apr 2023 11:12
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 21 21:29:57 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS041223.M
Quant Title : 8080.M
QLast Update : Wed Apr 12 14:05:56 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

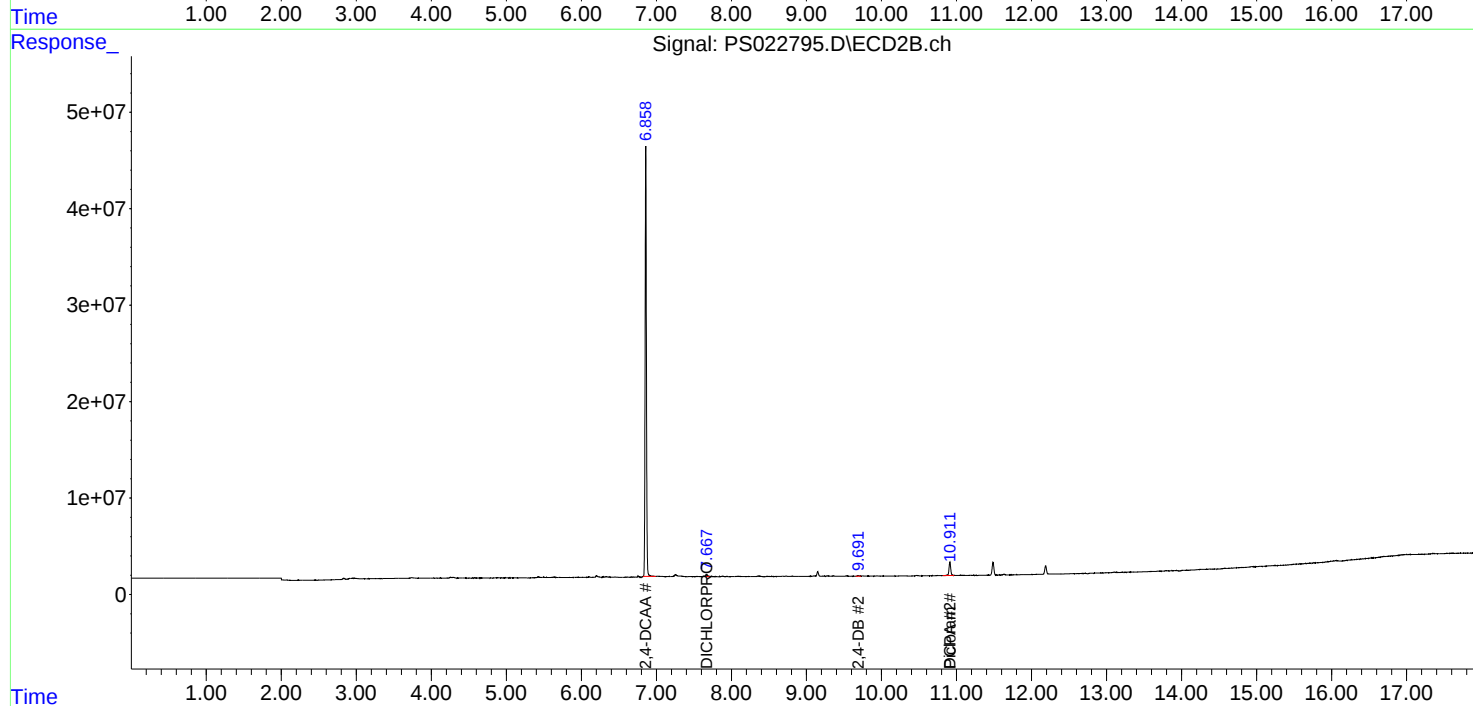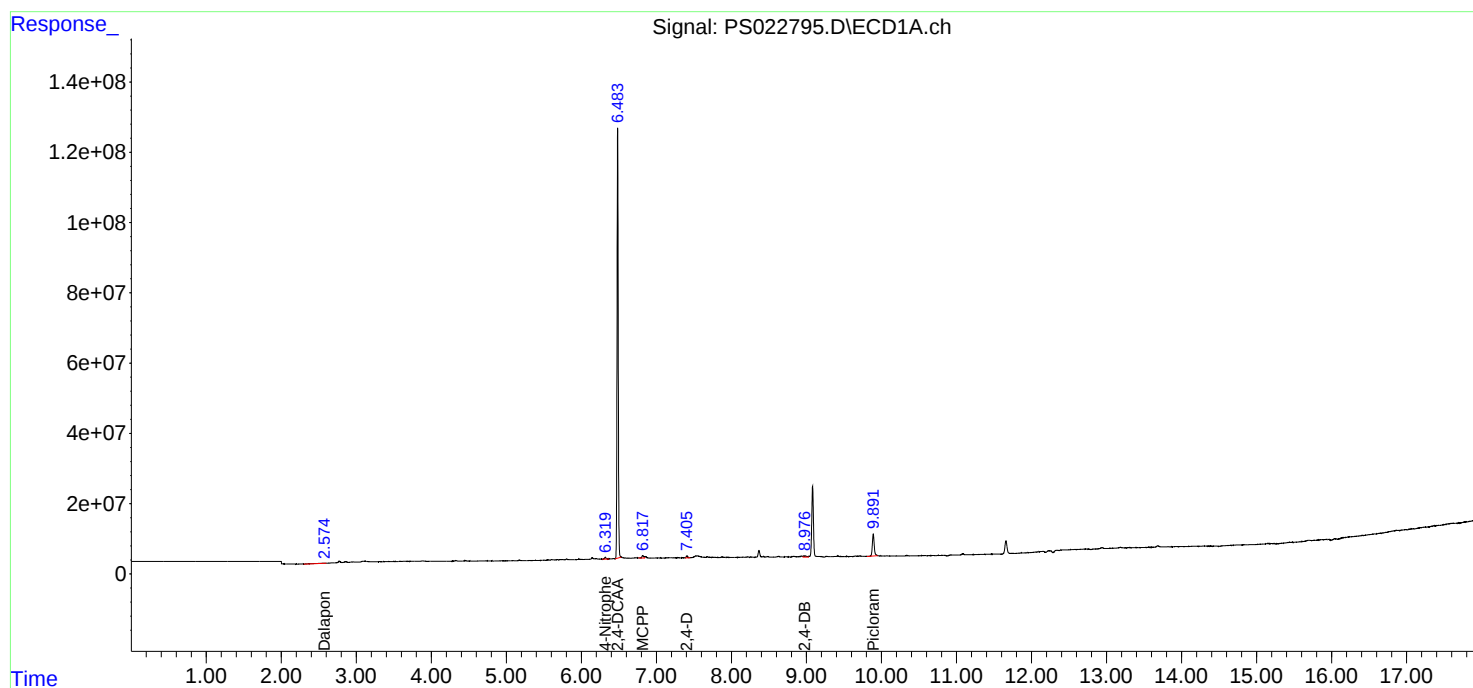


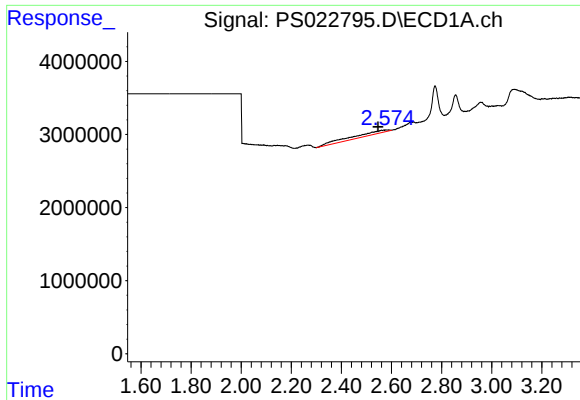

#1 Dalapon


R.T.: 2.575 min
Delta R.T.: 0.028 min
Response: 5060799
Conc: 1.71 ng/ml

Instrument :
ECD_S
ClientSampleId :

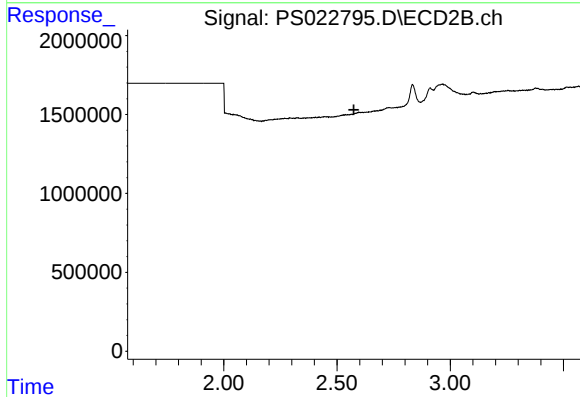


#1 Dalapon

R.T.: 0.000 min
Exp R.T. : 2.574 min
Response: 0
Conc: N.D.

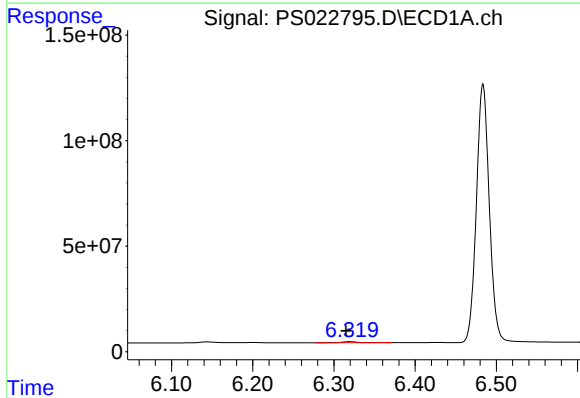


#3 4-Nitrophenol

R.T.: 6.319 min
Delta R.T.: 0.004 min
Response: 6732686
Conc: 3.63 ng/ml

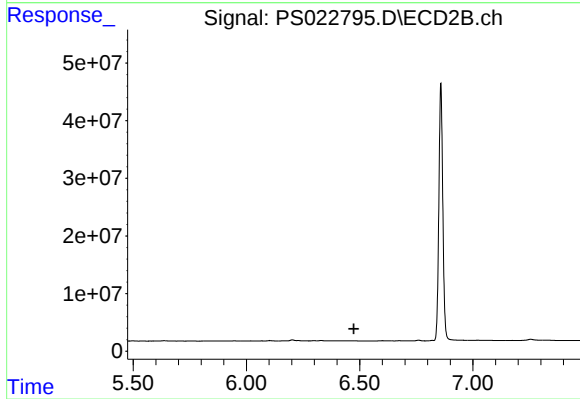

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T. : 6.474 min
Response: 0
Conc: N.D.

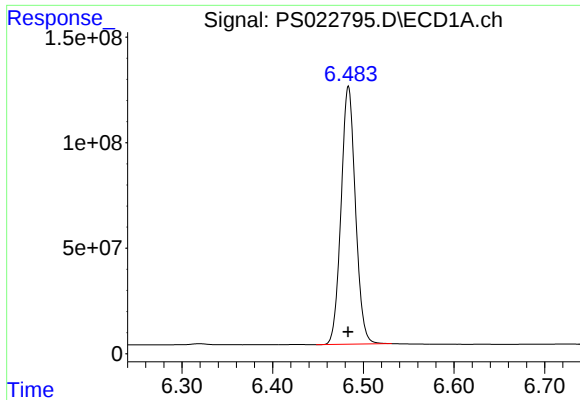

#4 2,4-DCAA


R.T.: 6.484 min
Delta R.T.: 0.000 min
Response: 1345757340
Conc: 540.53 ng/ml

Instrument :
ECD_S
ClientSampleId :

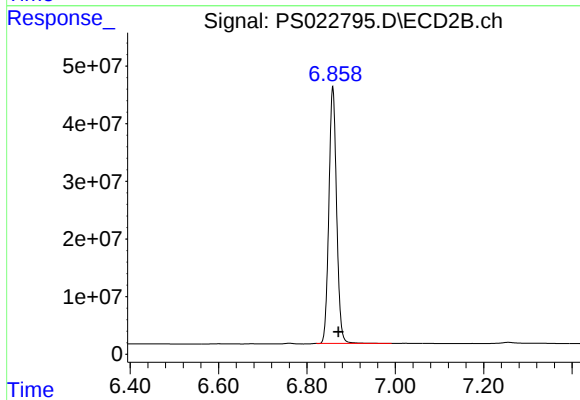


#4 2,4-DCAA

R.T.: 6.858 min
Delta R.T.: -0.013 min
Response: 539958054
Conc: 529.92 ng/ml

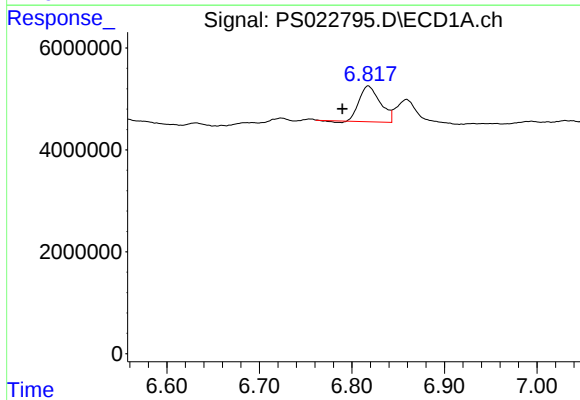


#6 MCP

R.T.: 6.818 min
Delta R.T.: 0.028 min
Response: 10969626
Conc: 1.30 ug/ml

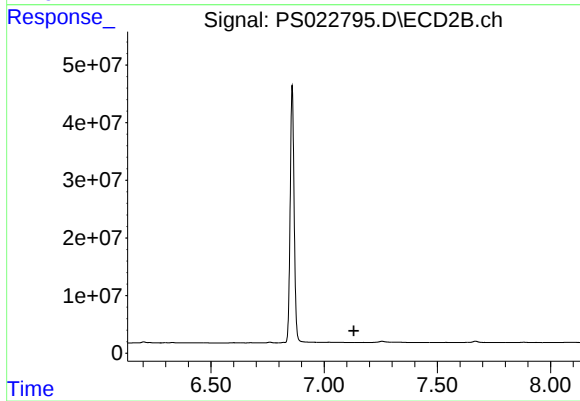

#6 MCP


R.T.: 0.000 min
Exp R.T. : 7.132 min
Response: 0
Conc: N.D.

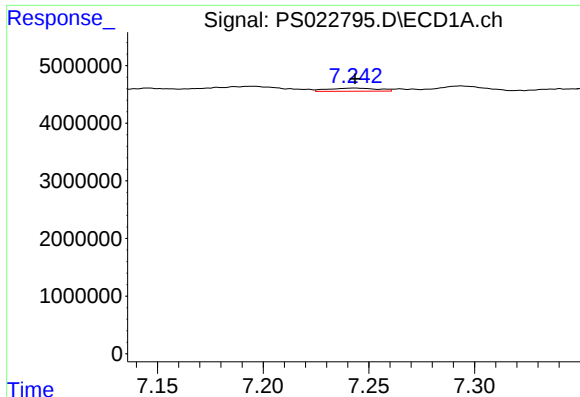

#8 DICHLORPROP


R.T.: 7.243 min
Delta R.T.: 0.000 min
Response: 885949
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

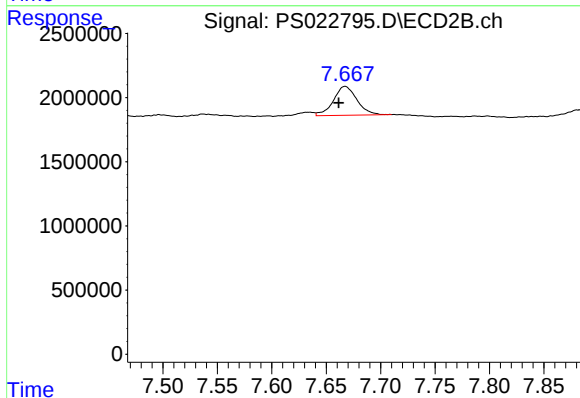


#8 DICHLORPROP

R.T.: 7.668 min
Delta R.T.: 0.006 min
Response: 3372378
Conc: 3.03 ng/ml

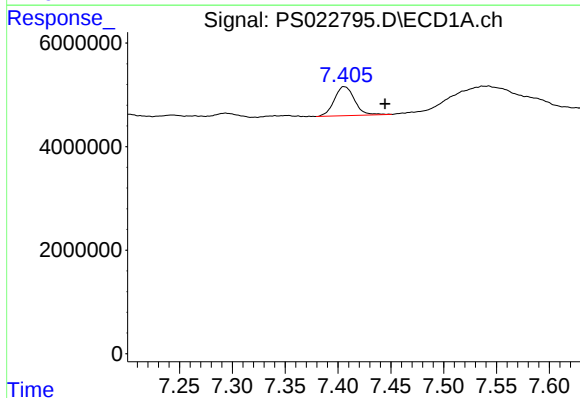


#9 2,4-D

R.T.: 7.406 min
Delta R.T.: -0.039 min
Response: 7437147
Conc: 2.01 ng/ml

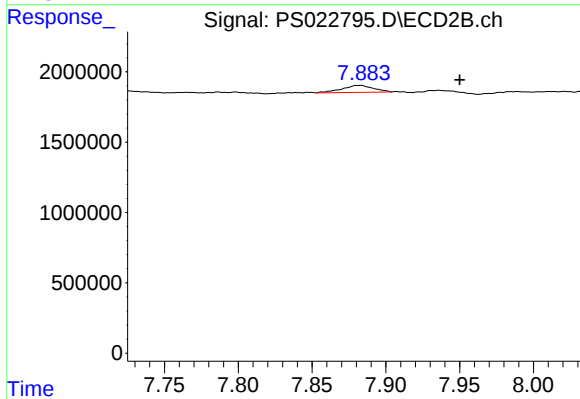

#9 2,4-D


R.T.: 7.883 min
Delta R.T.: -0.067 min
Response: 726117
Conc: N.D.

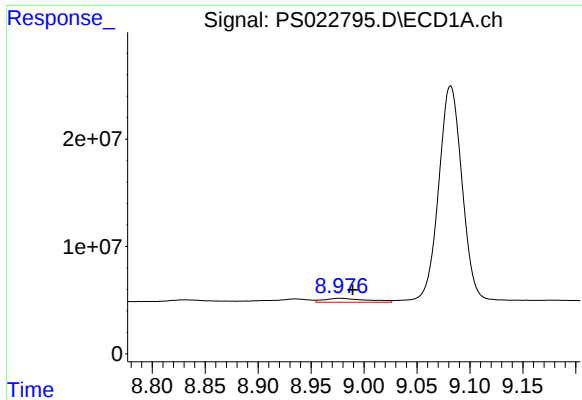

#13 2,4-DB


R.T.: 8.977 min
Delta R.T.: -0.012 min
Response: 10743745
Conc: 2.51 ng/ml

Instrument :
ECD_S
ClientSampleId :

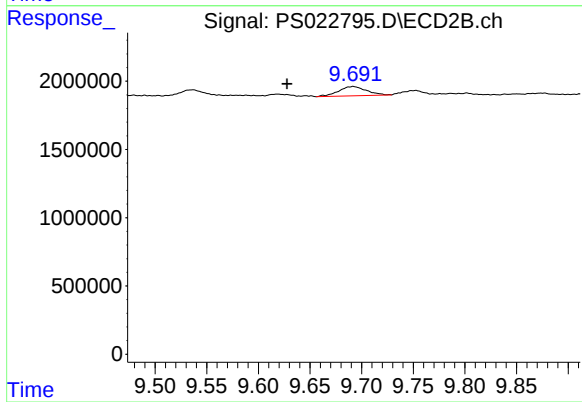


#13 2,4-DB

R.T.: 9.692 min
Delta R.T.: 0.064 min
Response: 1275201
Conc: 1.70 ng/ml

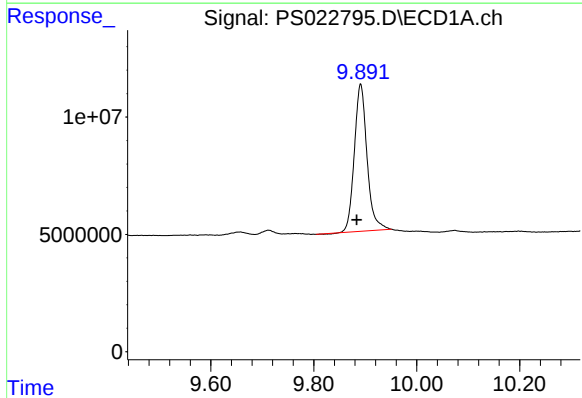


#15 Picloram

R.T.: 9.891 min
Delta R.T.: 0.008 min
Response: 107544298
Conc: 3.61 ng/ml

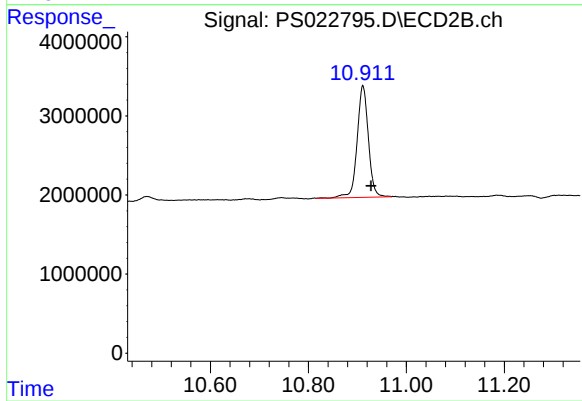

#15 Picloram


R.T.: 10.911 min
Delta R.T.: -0.017 min
Response: 22506245
Conc: 2.77 ng/ml

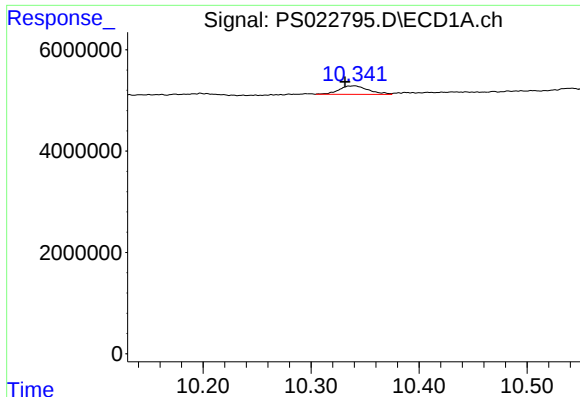

#16 DCPA

R.T.: 10.339 min
Delta R.T.: 0.007 min
Response: 3161682
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

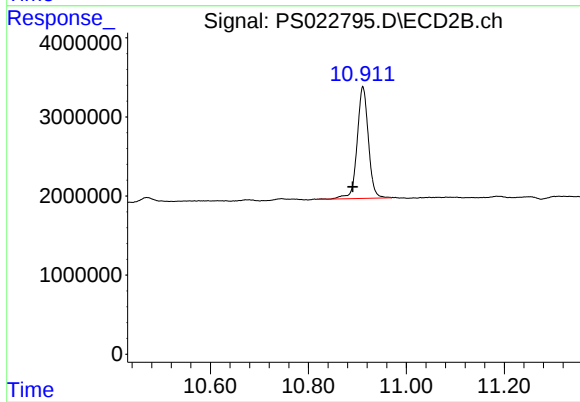

#16 DCPA

R.T.: 10.911 min
Delta R.T.: 0.021 min
Response: 22506245
Conc: 3.24 ng/ml