

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS042221\
 Data File : PS014752.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Apr 2021 08:57
 Operator : DD\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 22 10:40:33 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS040821.M
 Quant Title : 8080.M
 QLast Update : Thu Apr 08 14:34:06 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds							
2) T	3,5-DICHL...	6.428f	0.000	3521942	0	1.700	N.D. #
5) T	DICAMBA	0.000	7.118f	0	1928629	N.D.	<MDL
6) T	MCP	0.000	7.118	0	1928629	N.D.	1.145
8) T	DICHLORPROP	0.000	7.707	0	3341193	N.D.	6.619
13) T	2,4-DB	0.000	9.584f	0	4324678	N.D.	12.468
15) T	Picloram	10.937	10.970	60960474	24052656	5.449	6.414



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS042221\
Data File : PS014752.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Apr 2021 08:57
Operator : DD\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 22 10:40:33 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS040821.M
Quant Title : 8080.M
QLast Update : Thu Apr 08 14:34:06 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

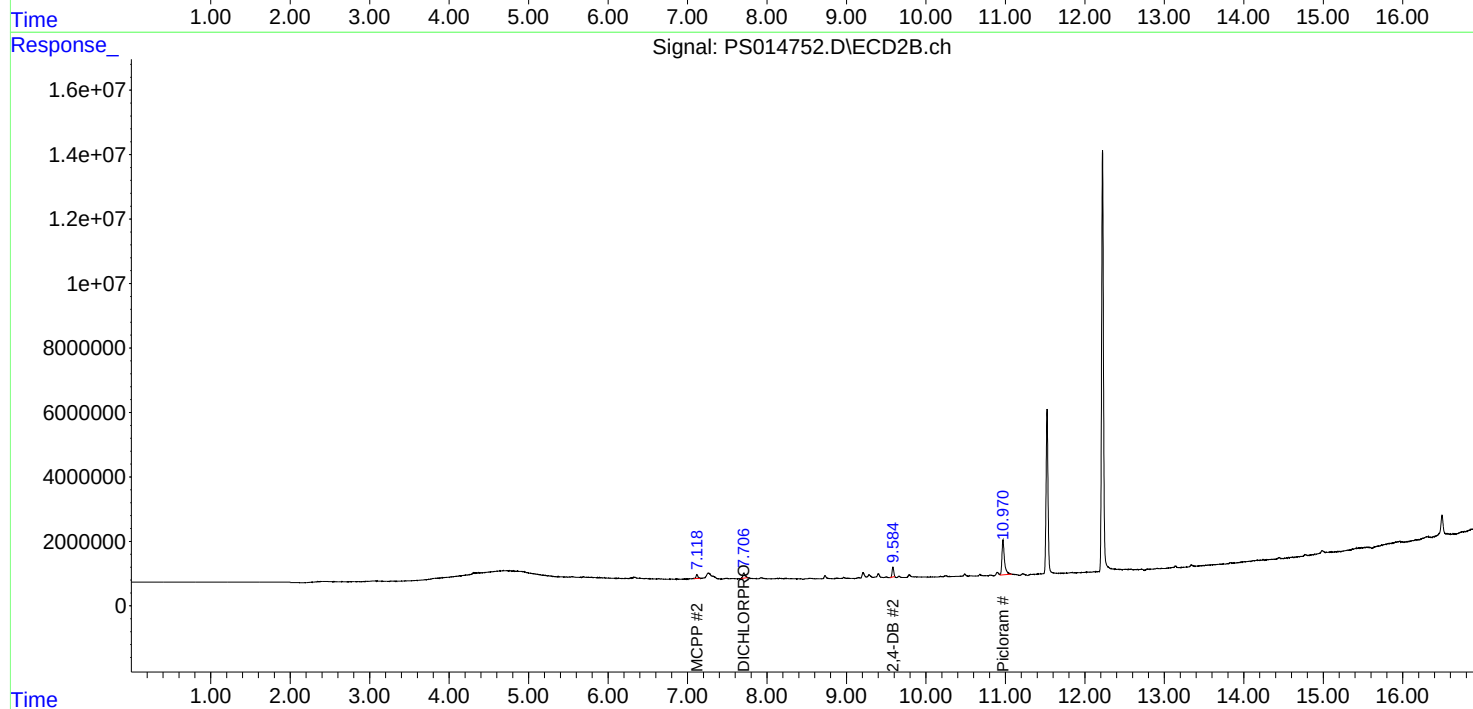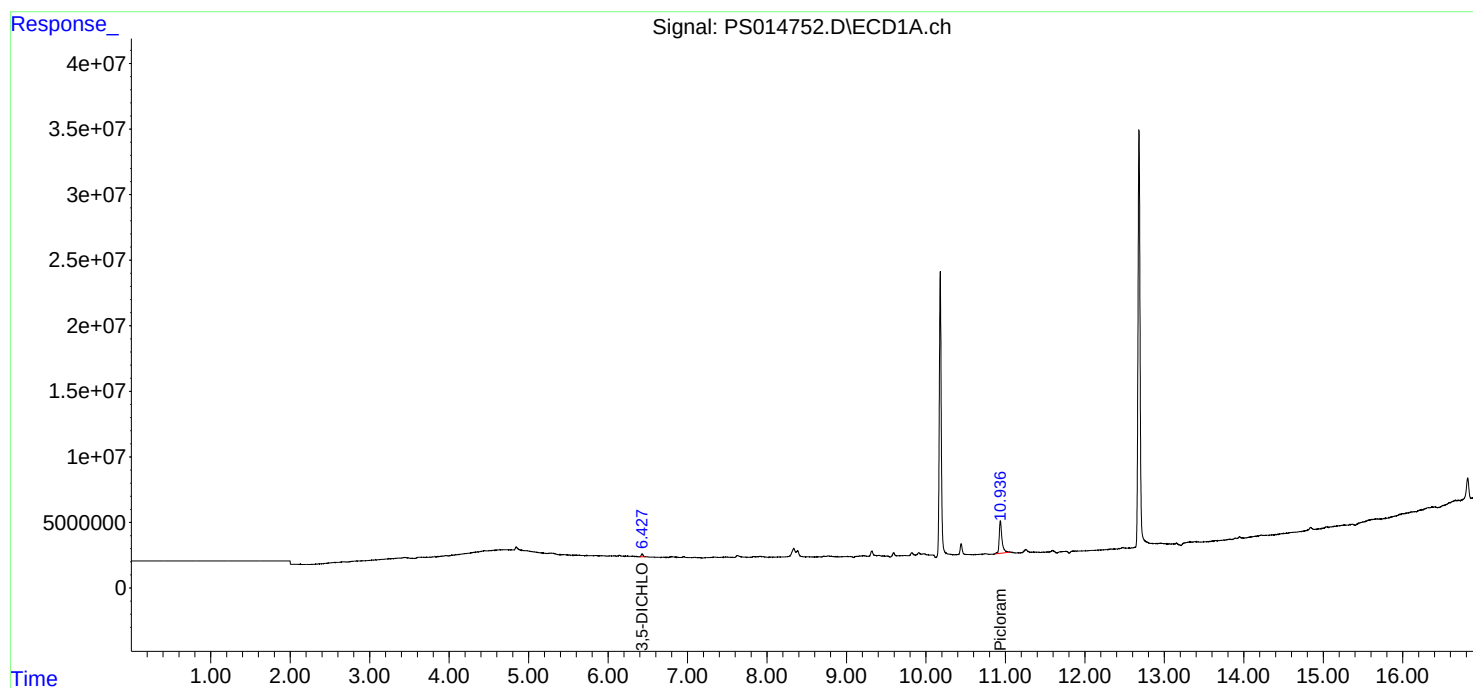


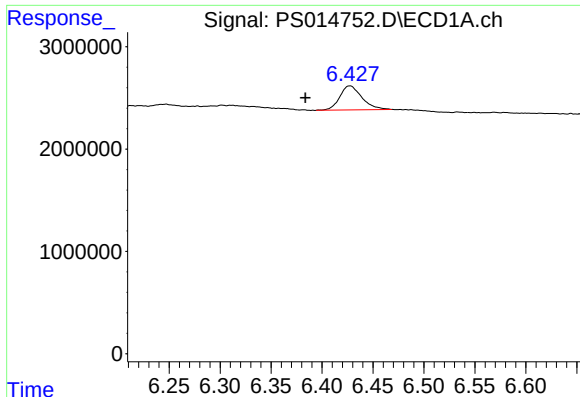

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.428 min
Delta R.T.: 0.044 min
Response: 3521942
Conc: 1.70 ng/ml

Instrument :
ECD_S
ClientSampleId :

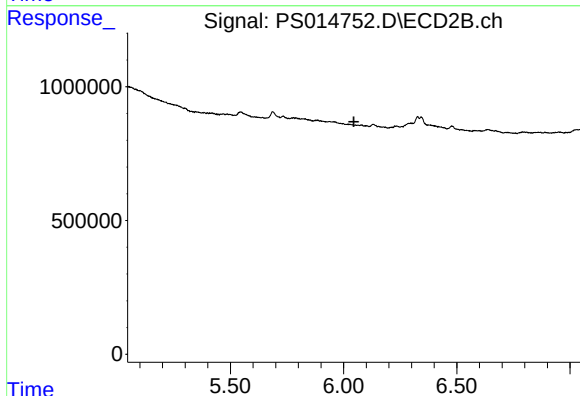


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.045 min
Response: 0
Conc: N.D.

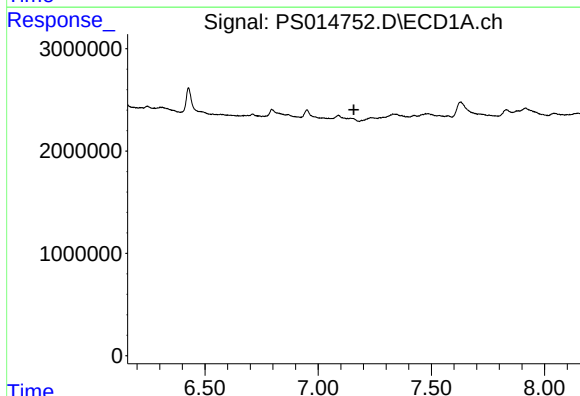


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T. : 7.158 min
Response: 0
Conc: N.D.

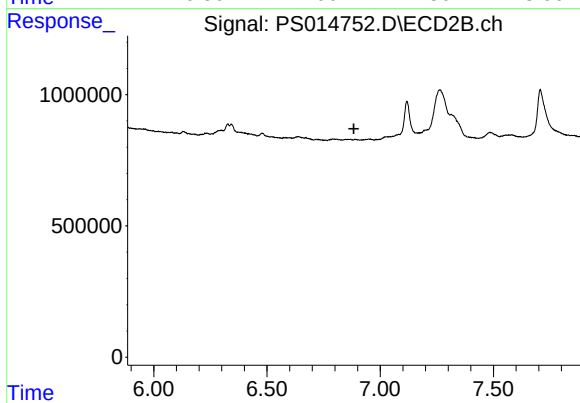

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T. : 6.884 min
Response: 0
Conc: N.D.

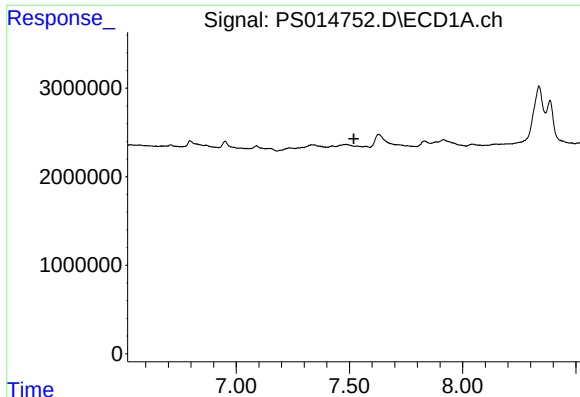

#6 MCP


R.T.: 0.000 min
Exp R.T.: 7.520 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

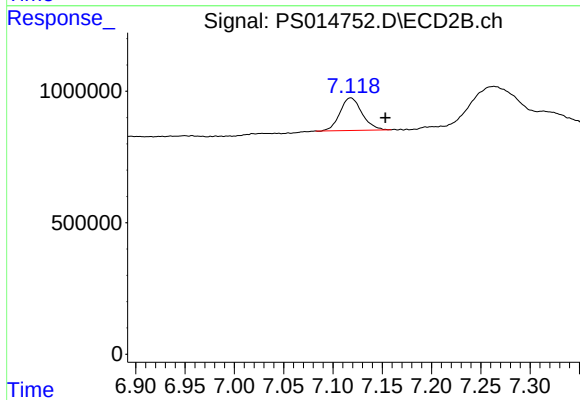


#6 MCP

R.T.: 7.118 min
Delta R.T.: -0.035 min
Response: 1928629
Conc: 1.15 ug/ml

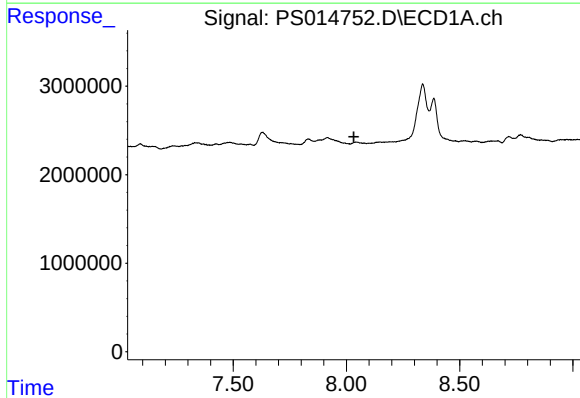


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T.: 8.033 min
Response: 0
Conc: N.D.

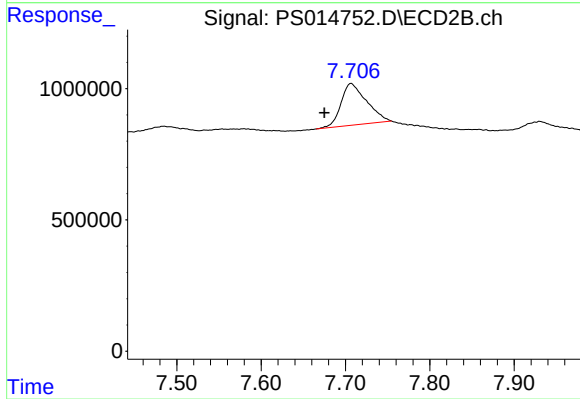

#8 DICHLORPROP


R.T.: 7.707 min
Delta R.T.: 0.032 min
Response: 3341193
Conc: 6.62 ng/ml

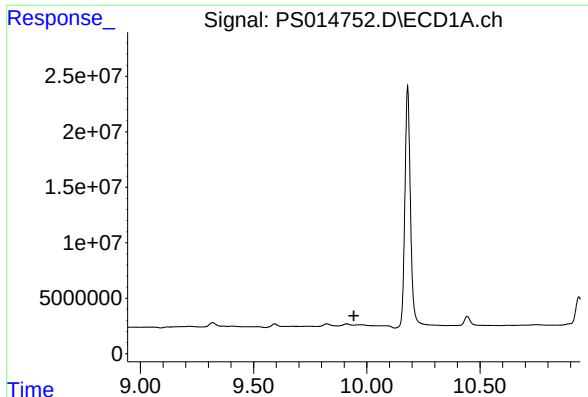

#13 2,4-DB


R.T.: 0.000 min
Exp R.T.: 9.943 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

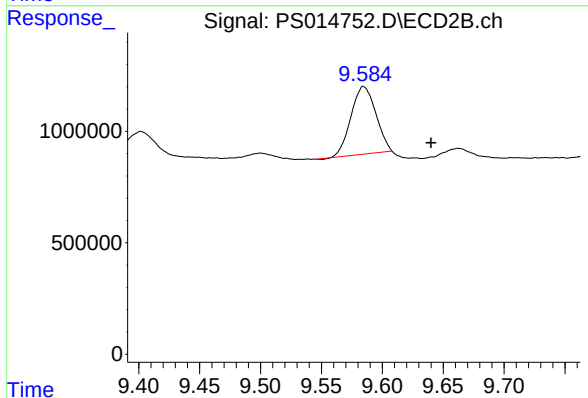


#13 2,4-DB

R.T.: 9.584 min
Delta R.T.: -0.056 min
Response: 4324678
Conc: 12.47 ng/ml

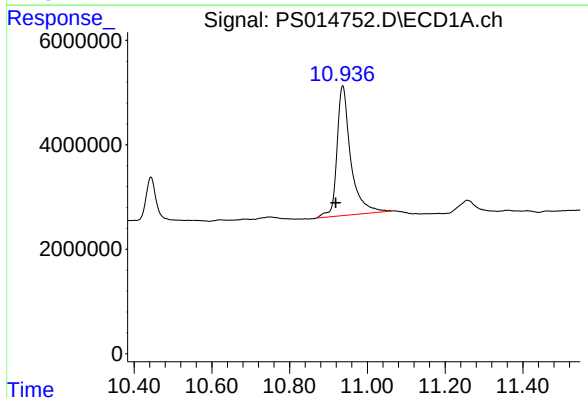

#15 Picloram

R.T.: 10.937 min
Delta R.T.: 0.018 min
Response: 60960474
Conc: 5.45 ng/ml

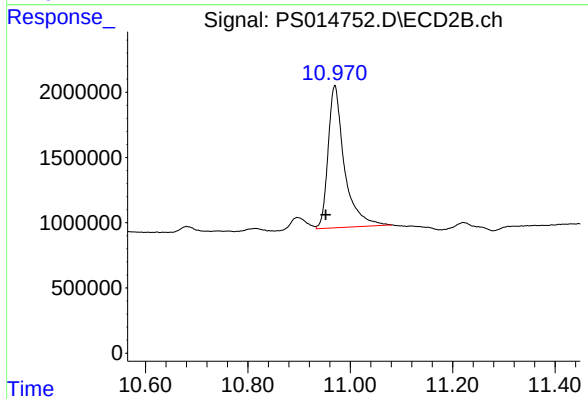

#15 Picloram

R.T.: 10.970 min
Delta R.T.: 0.018 min
Response: 24052656
Conc: 6.41 ng/ml