

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS042221\
 Data File : PS014753.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Apr 2021 09:20
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 22 10:40:55 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS040821.M
 Quant Title : 8080.M
 QLast Update : Thu Apr 08 14:34:06 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.157	6.884	702.4E6	256.4E6	461.741	550.943
Target Compounds							
2) T	3,5-DICHL...	6.428f	0.000	3380092	0	1.631	N.D. #
5) T	DICAMBA	0.000	7.117f	0	1811450	N.D.	<MDL
6) T	MCP	0.000	7.117	0	1811450	N.D.	1.076
8) T	DICHLORPROP	0.000	7.705	0	3581911	N.D.	7.095
11) T	2,4,5-TP ...	0.000	8.731	0	1925974	N.D.	<MDL
13) T	2,4-DB	0.000	9.586f	0	4827846	N.D.	13.918
15) T	Picloram	10.938	10.970	68402270	25854781	6.114	6.895
16) T	DCPA	0.000	10.900	0	2043739	N.D.	<MDL



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS042221\
Data File : PS014753.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Apr 2021 09:20
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 22 10:40:55 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS040821.M
Quant Title : 8080.M
QLast Update : Thu Apr 08 14:34:06 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

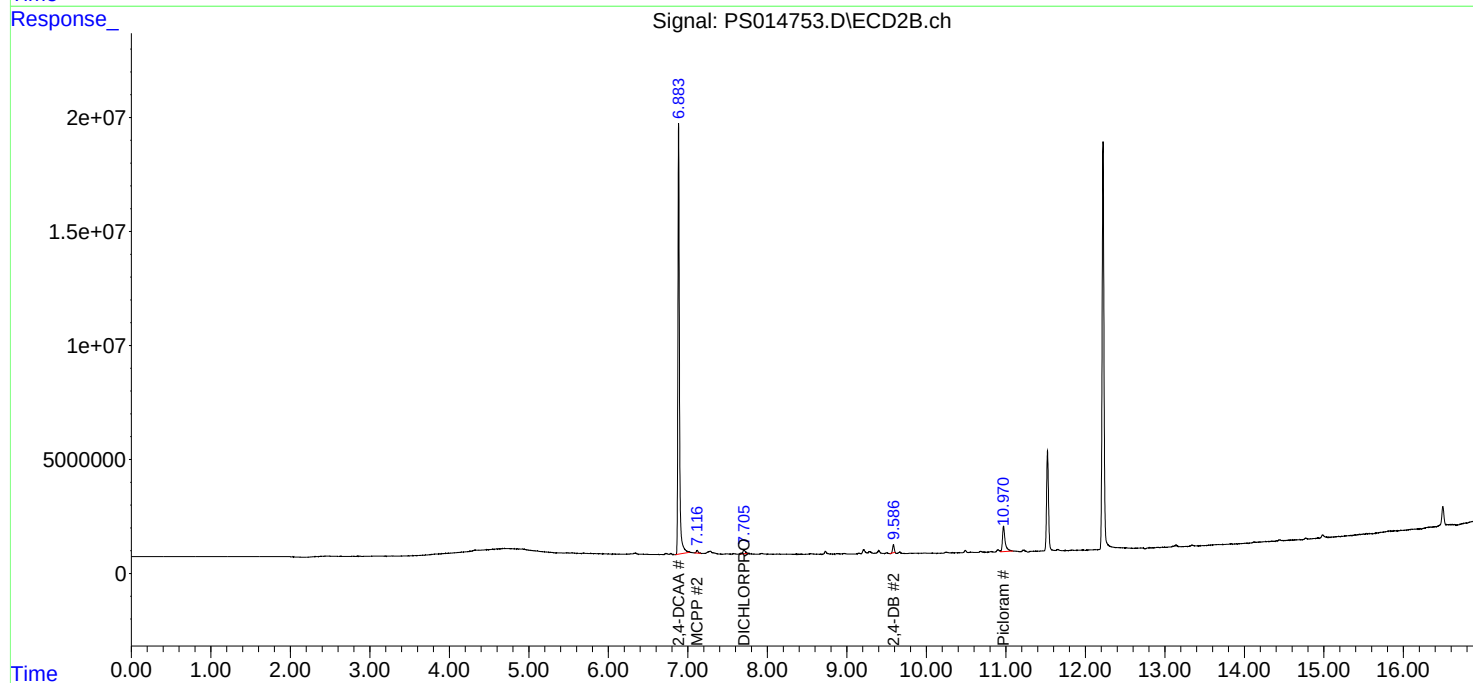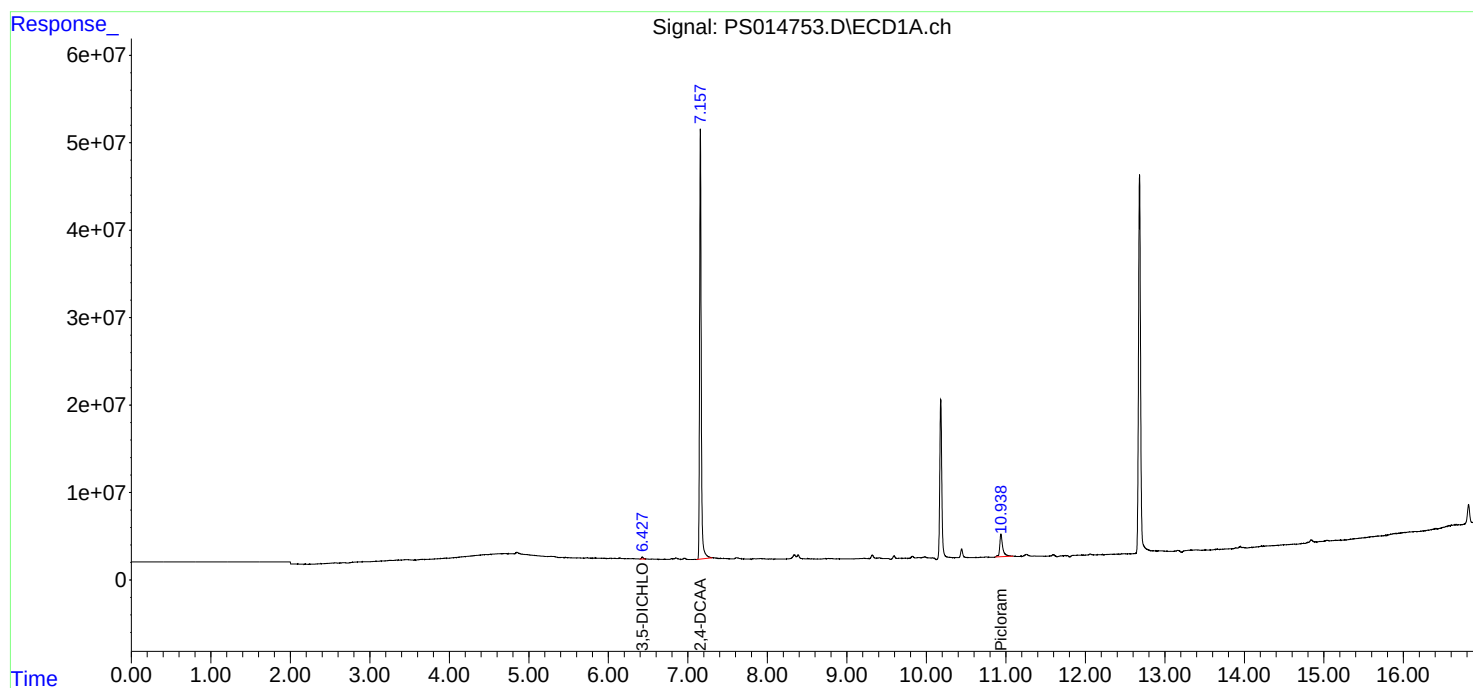


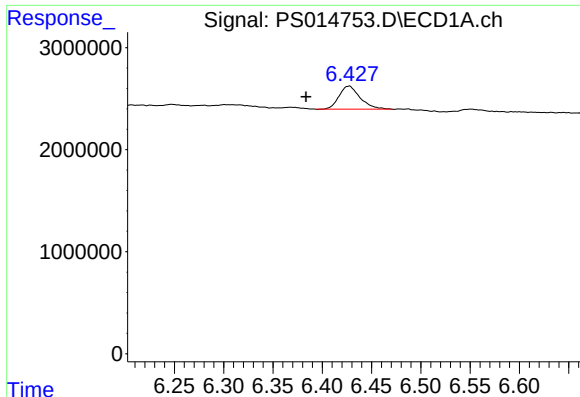

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.428 min
Delta R.T.: 0.044 min
Response: 3380092
Conc: 1.63 ng/ml

Instrument :
ECD_S
ClientSampleId :

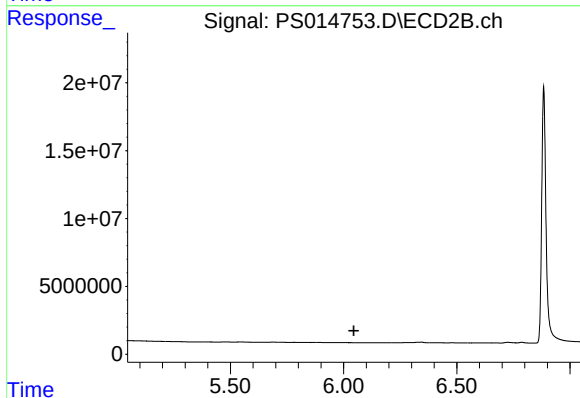


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.045 min
Response: 0
Conc: N.D.

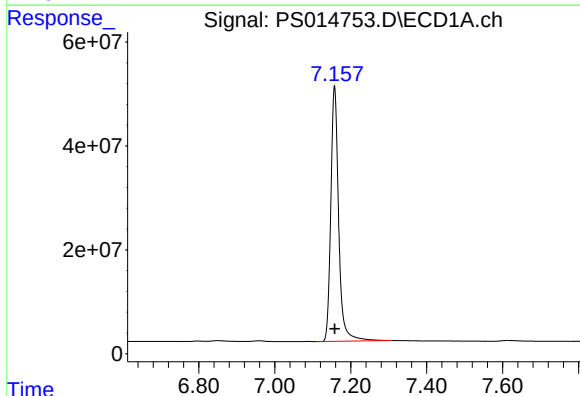


#4 2,4-DCAA

R.T.: 7.157 min
Delta R.T.: 0.000 min
Response: 702398222
Conc: 461.74 ng/ml

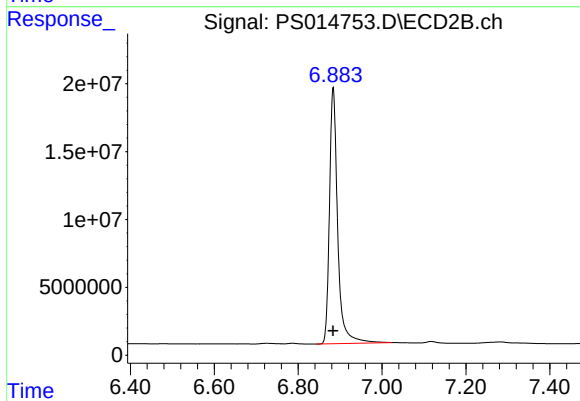

#4 2,4-DCAA


R.T.: 6.884 min
Delta R.T.: 0.000 min
Response: 256438889
Conc: 550.94 ng/ml

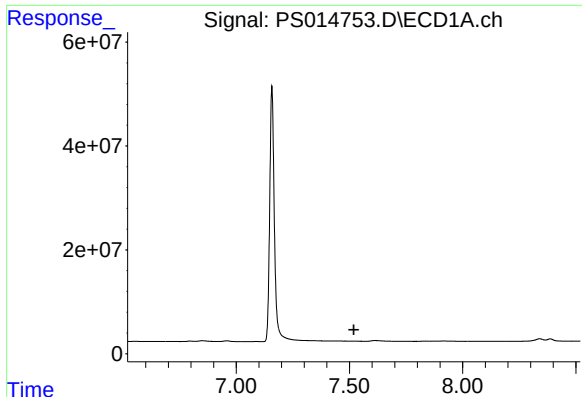

#6 MCP


R.T.: 0.000 min
Exp R.T.: 7.520 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

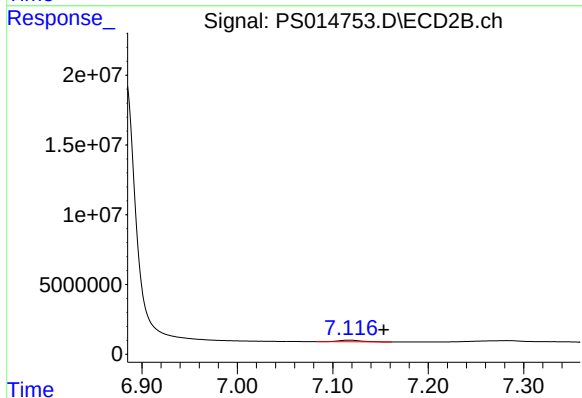


#6 MCP

R.T.: 7.117 min
Delta R.T.: -0.037 min
Response: 1811450
Conc: 1.08 ug/ml

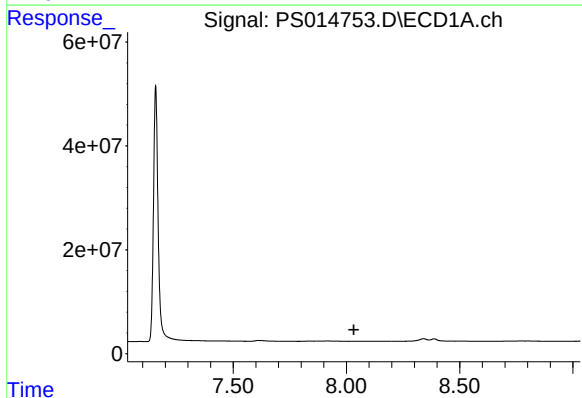


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T.: 8.033 min
Response: 0
Conc: N.D.

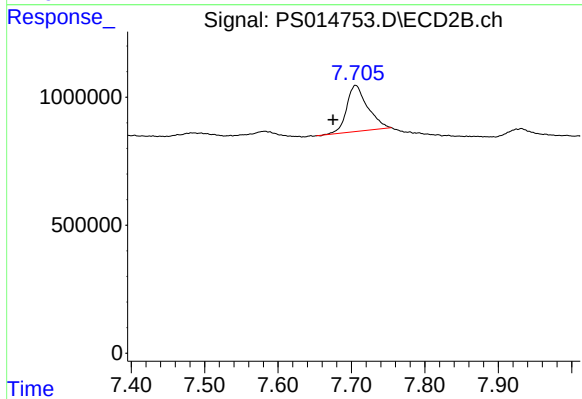

#8 DICHLORPROP


R.T.: 7.705 min
Delta R.T.: 0.031 min
Response: 3581911
Conc: 7.10 ng/ml

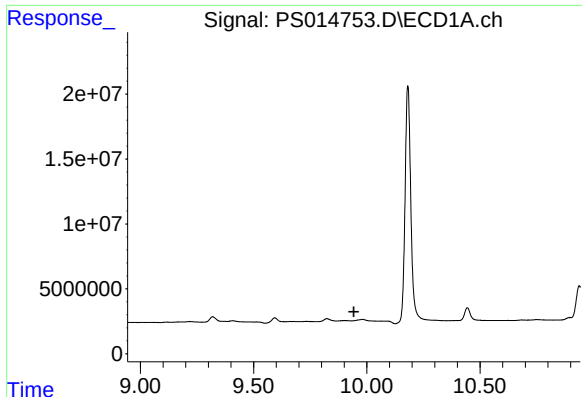

#13 2,4-DB


R.T.: 0.000 min
Exp R.T.: 9.943 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

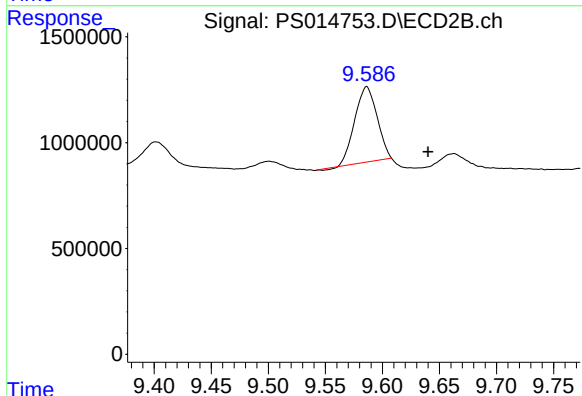


#13 2,4-DB

R.T.: 9.586 min
Delta R.T.: -0.054 min
Response: 4827846
Conc: 13.92 ng/ml

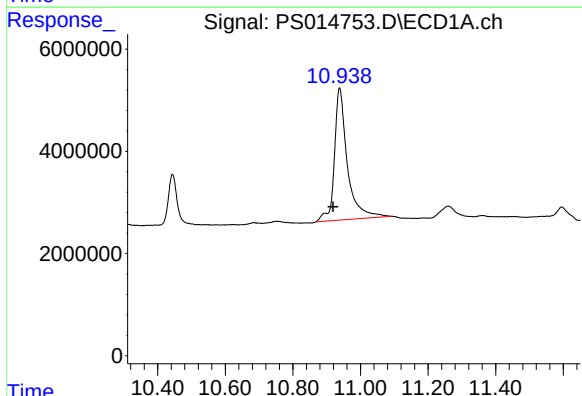

#15 Picloram

R.T.: 10.938 min
Delta R.T.: 0.019 min
Response: 68402270
Conc: 6.11 ng/ml

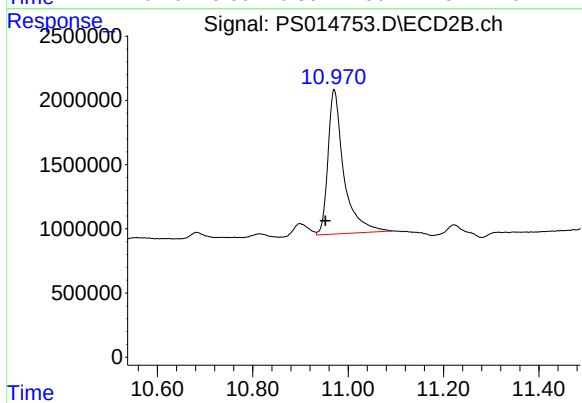

#15 Picloram

R.T.: 10.970 min
Delta R.T.: 0.018 min
Response: 25854781
Conc: 6.89 ng/ml