

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS042221\
 Data File : PS014762.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Apr 2021 16:07
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 22 17:35:58 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS040821.M
 Quant Title : 8080.M
 QLast Update : Thu Apr 08 14:34:06 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.156	6.880	697.2E6	242.2E6	458.354	520.414
Target Compounds							
5) T	DICAMBA	0.000	7.112f	0	3569959	N.D.	1.765
6) T	MCPD	0.000	7.112f	0	3569959	N.D.	2.120
7) T	MCPA	7.607f	0.000	10214237	0	1.641	N.D. #
8) T	DICHLORPROP	0.000	7.702	0	5023104	N.D.	9.950
9) T	2,4-D	8.265	0.000	26316491	0	16.551	N.D. #
11) T	2,4,5-TP ...	0.000	8.726	0	4289101	N.D.	1.570
12) T	2,4,5-T	9.401	9.143	5381525	1419646	<MDL	<MDL #
13) T	2,4-DB	9.953	9.657	12336599	3197498	8.107	9.218
15) T	Picloram	10.931	10.964	61264851	20802835	5.476	5.548
16) T	DCPA	0.000	10.964f	0	20802835	N.D.	5.123



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS042221\
Data File : PS014762.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Apr 2021 16:07
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 22 17:35:58 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS040821.M
Quant Title : 8080.M
QLast Update : Thu Apr 08 14:34:06 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

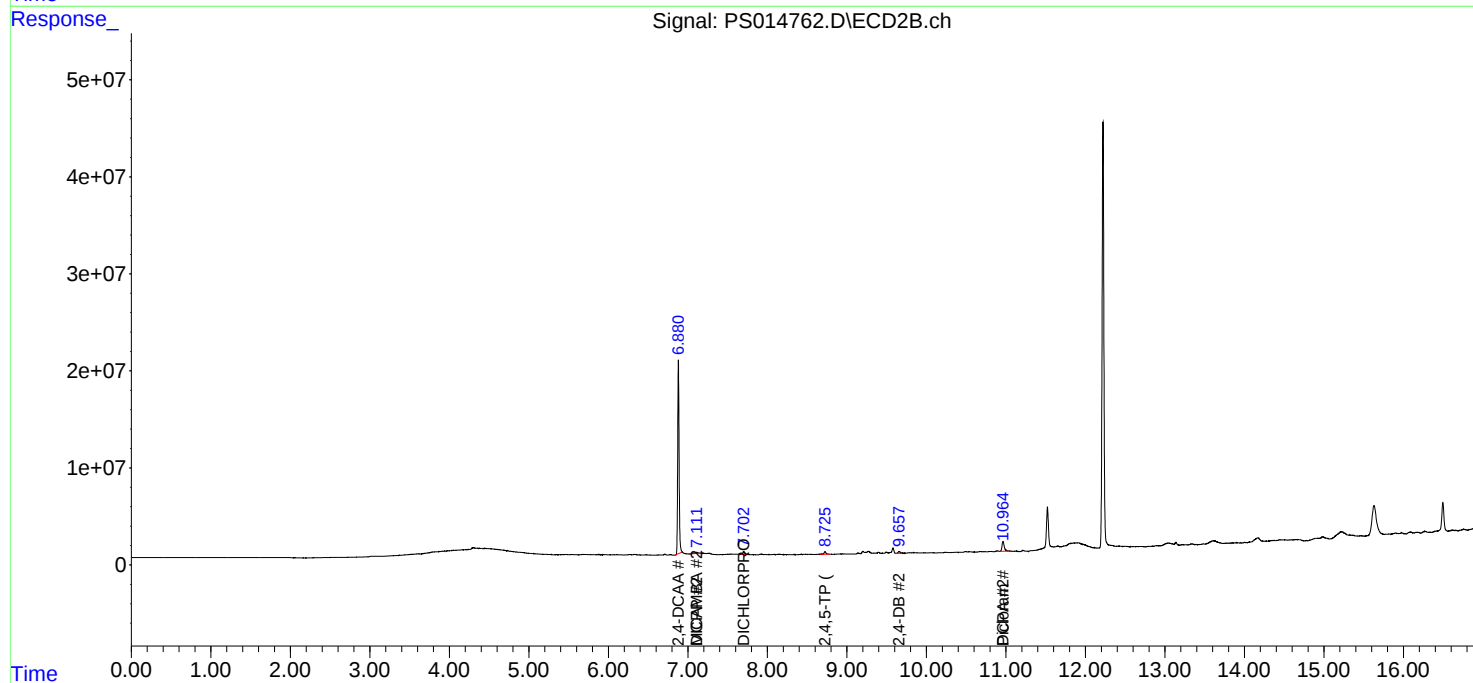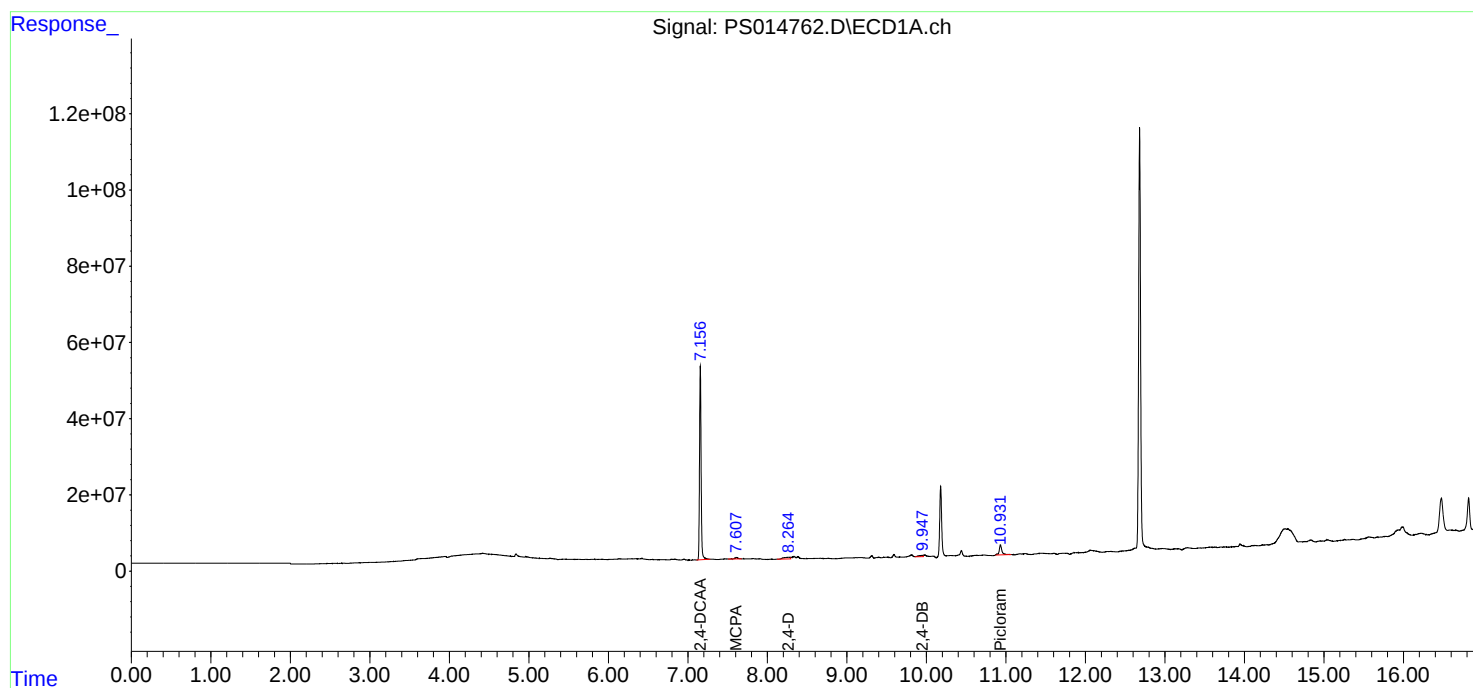


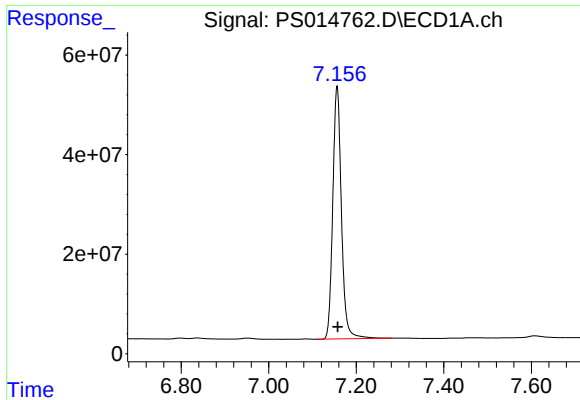

#4 2,4-DCAA


R.T.: 7.156 min
Delta R.T.: -0.002 min
Response: 697245856
Conc: 458.35 ng/ml

Instrument :
ECD_S
ClientSampleId :

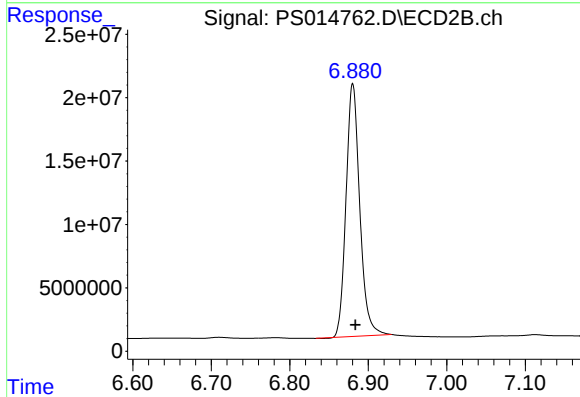


#4 2,4-DCAA

R.T.: 6.880 min
Delta R.T.: -0.003 min
Response: 242229235
Conc: 520.41 ng/ml

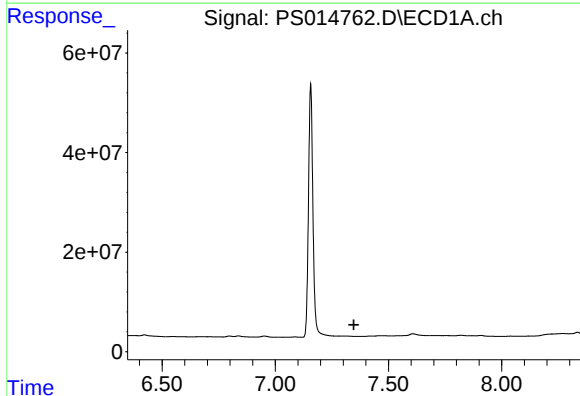


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 7.347 min
Response: 0
Conc: N.D.

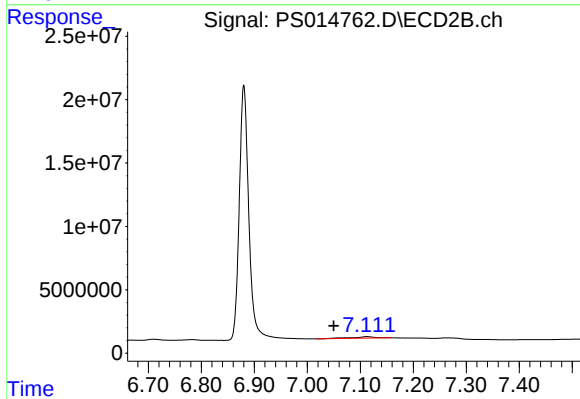

#5 DICAMBA


R.T.: 7.112 min
Delta R.T.: 0.061 min
Response: 3569959
Conc: 1.77 ng/ml

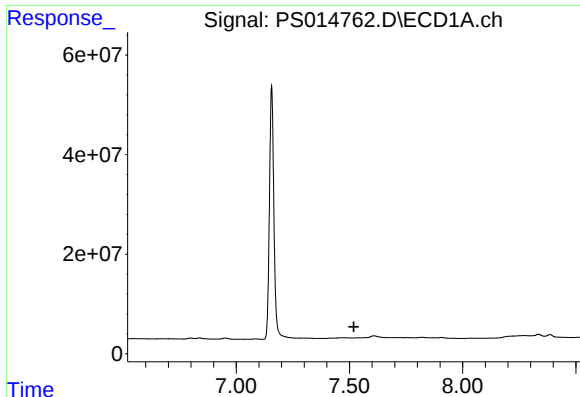

#6 MCP


R.T.: 0.000 min
Exp R.T.: 7.520 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

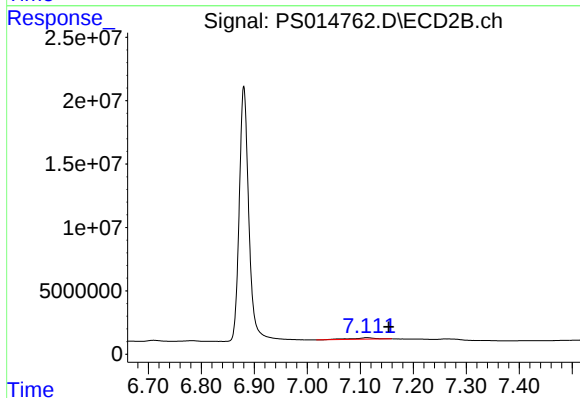


#6 MCP

R.T.: 7.112 min
Delta R.T.: -0.042 min
Response: 3569959
Conc: 2.12 ug/ml

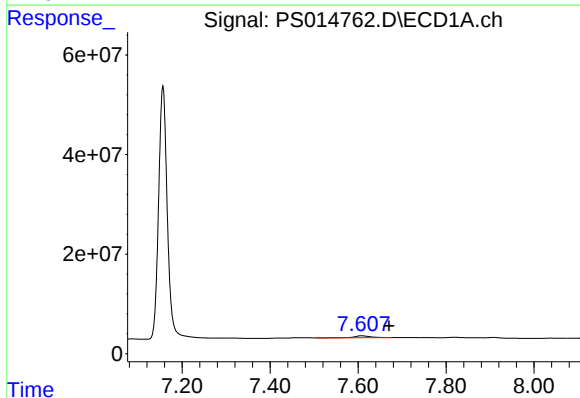


#7 MCPA

R.T.: 7.607 min
Delta R.T.: -0.063 min
Response: 10214237
Conc: 1.64 ug/ml

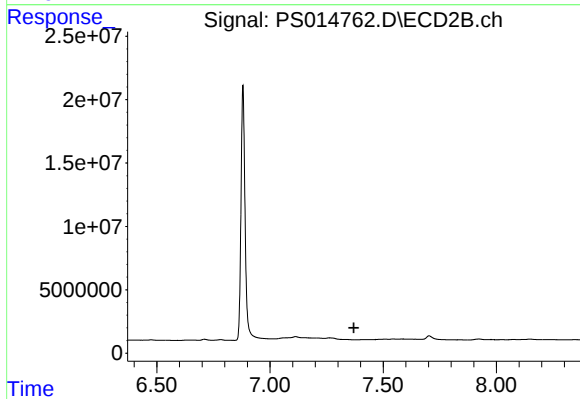

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 7.370 min
Response: 0
Conc: N.D.

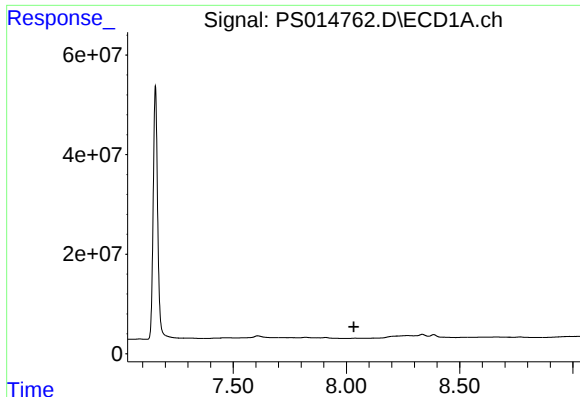

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 8.033 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

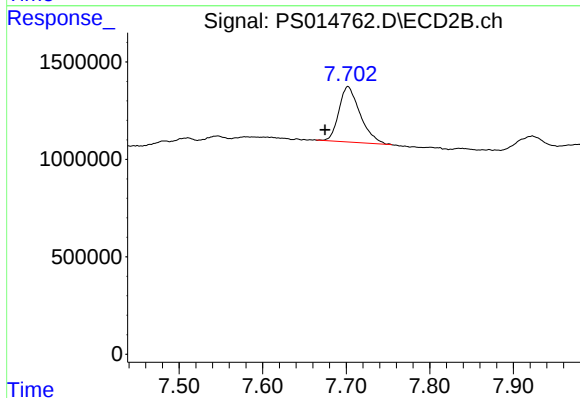


#8 DICHLORPROP

R.T.: 7.702 min
Delta R.T.: 0.027 min
Response: 5023104
Conc: 9.95 ng/ml

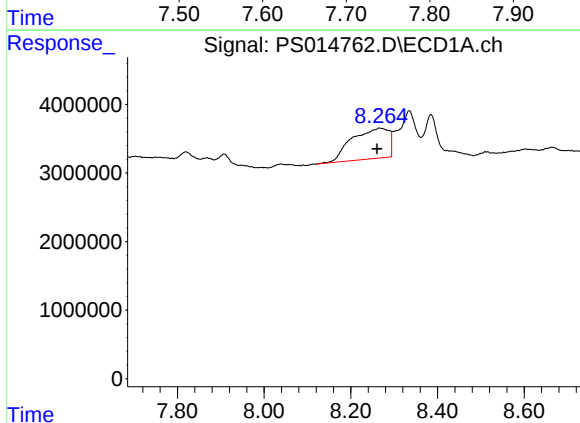


#9 2,4-D

R.T.: 8.265 min
Delta R.T.: 0.004 min
Response: 26316491
Conc: 16.55 ng/ml

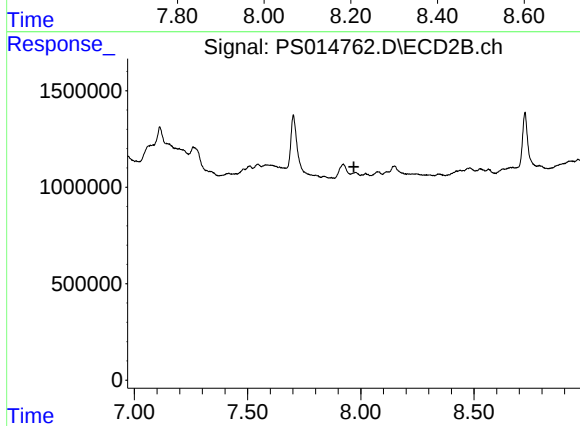

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 7.970 min
Response: 0
Conc: N.D.

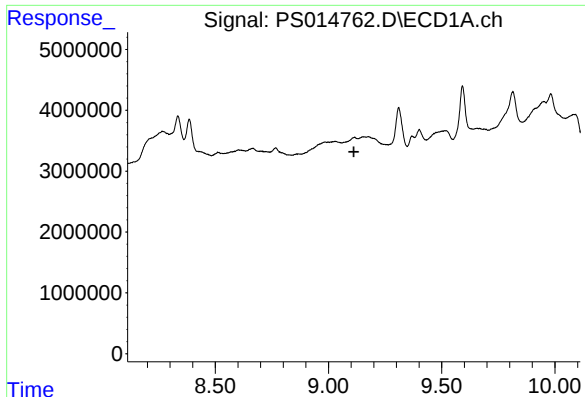

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 9.112 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

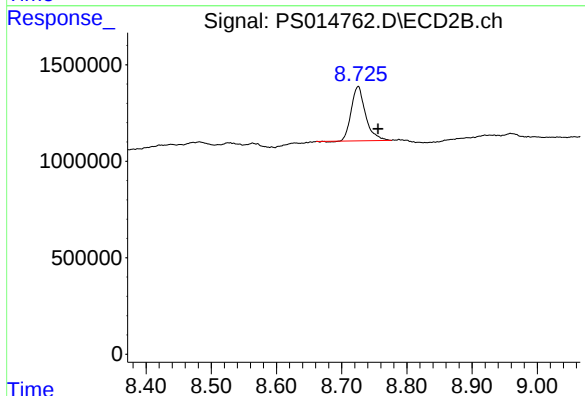


#11 2,4,5-TP (SILVEX)

R.T.: 8.726 min
Delta R.T.: -0.030 min
Response: 4289101
Conc: 1.57 ng/ml

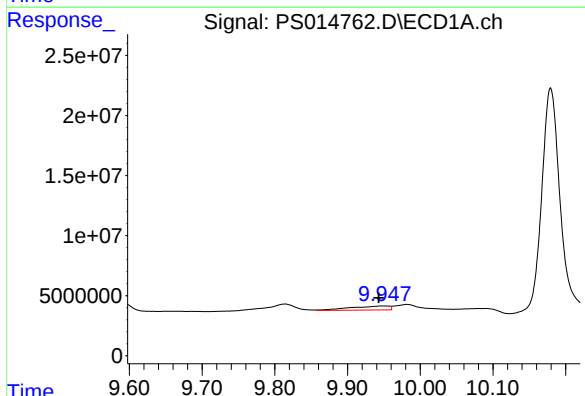


#13 2,4-DB

R.T.: 9.953 min
Delta R.T.: 0.010 min
Response: 12336599
Conc: 8.11 ng/ml

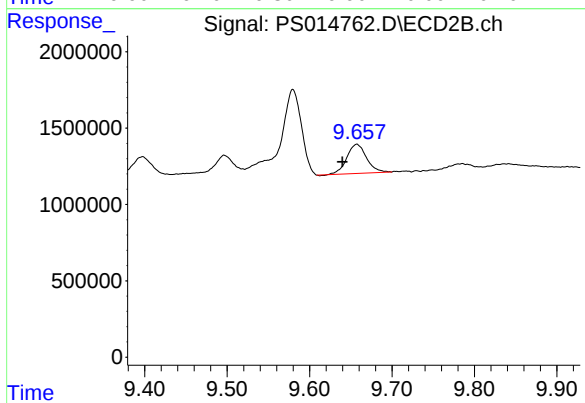

#13 2,4-DB


R.T.: 9.657 min
Delta R.T.: 0.017 min
Response: 3197498
Conc: 9.22 ng/ml

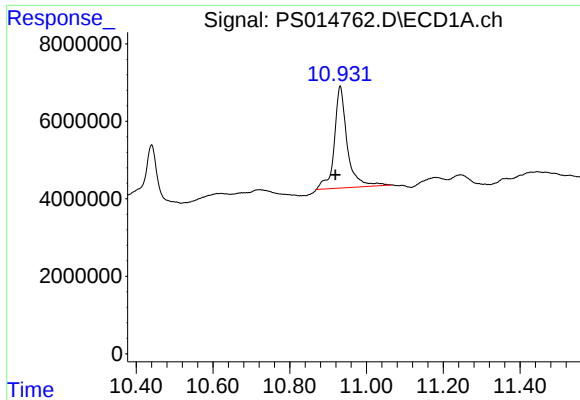

#15 Picloram


R.T.: 10.931 min
Delta R.T.: 0.012 min
Response: 61264851
Conc: 5.48 ng/ml

Instrument :
ECD_S
ClientSampleId :

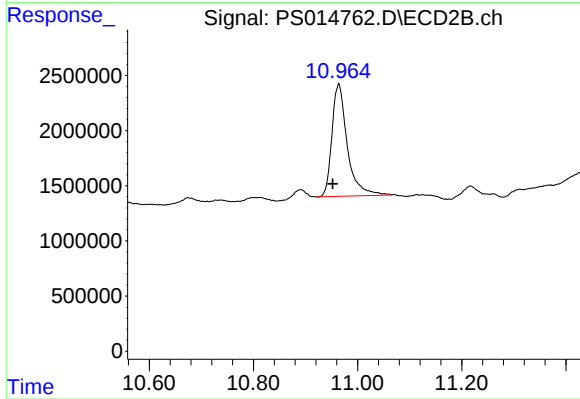


#15 Picloram

R.T.: 10.964 min
Delta R.T.: 0.011 min
Response: 20802835
Conc: 5.55 ng/ml

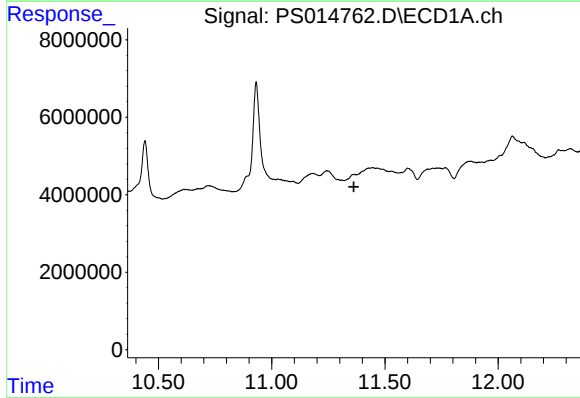

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 11.363 min
Response: 0
Conc: N.D.

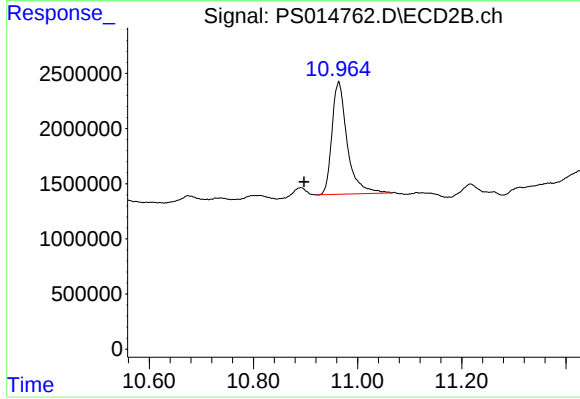

#16 DCPA

R.T.: 10.964 min
Delta R.T.: 0.067 min
Response: 20802835
Conc: 5.12 ng/ml