

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS042222\
 Data File : PS019117.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Apr 2022 09:18
 Operator : AJ\MA
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 22 22:47:50 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS041822.M
 Quant Title : 8080.M
 QLast Update : Mon Apr 18 17:28:16 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds							
2) T	3,5-DICHL...	6.471f	0.000	12355282	0	2.485	N.D. #
5) T	DICAMBA	0.000	7.021f	0	2078357	N.D.	<MDL
6) T	MCP	0.000	7.021f	0	2078357	N.D.	<MDL
8) T	DICHLORPROP	0.000	7.607	0	2420022	N.D.	2.896
9) T	2,4-D	8.340	0.000	17269875	0	4.208	N.D. #
10) T	Pentachlo...	8.649	0.000	9538950	0	<MDL	N.D. #
11) T	2,4,5-TP ...	9.202	8.626f	7604774	1295082	<MDL	<MDL #
12) T	2,4,5-T	9.487	9.102f	6753156	5585514	<MDL	1.293 #
13) T	2,4-DB	10.037	0.000	10402774	0	2.954	N.D. #
15) T	Picloram	11.028	10.865	119.4E6	26201842	4.456	4.425
16) T	DCPA	11.464	10.865f	5943568	26201842	<MDL	4.578 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS042222\
Data File : PS019117.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Apr 2022 09:18
Operator : AJ\MA
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 22 22:47:50 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS041822.M
Quant Title : 8080.M
QLast Update : Mon Apr 18 17:28:16 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

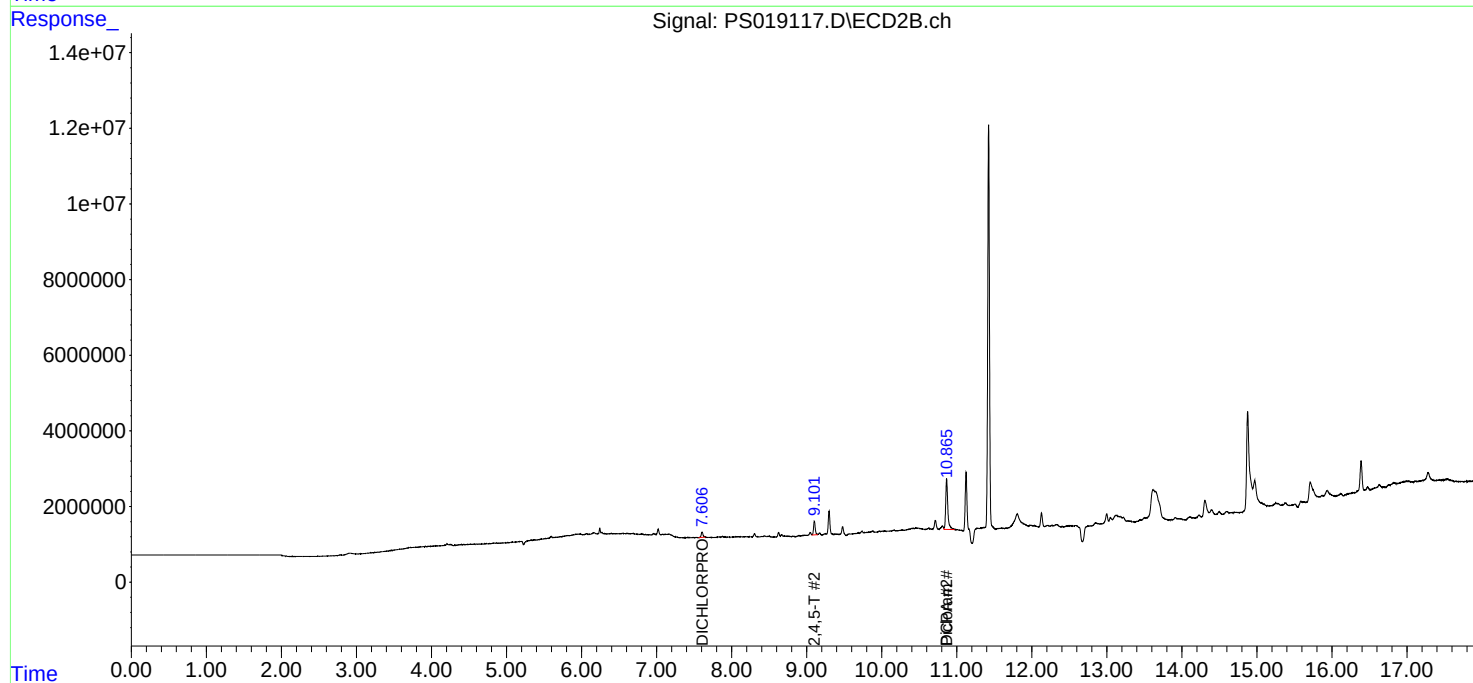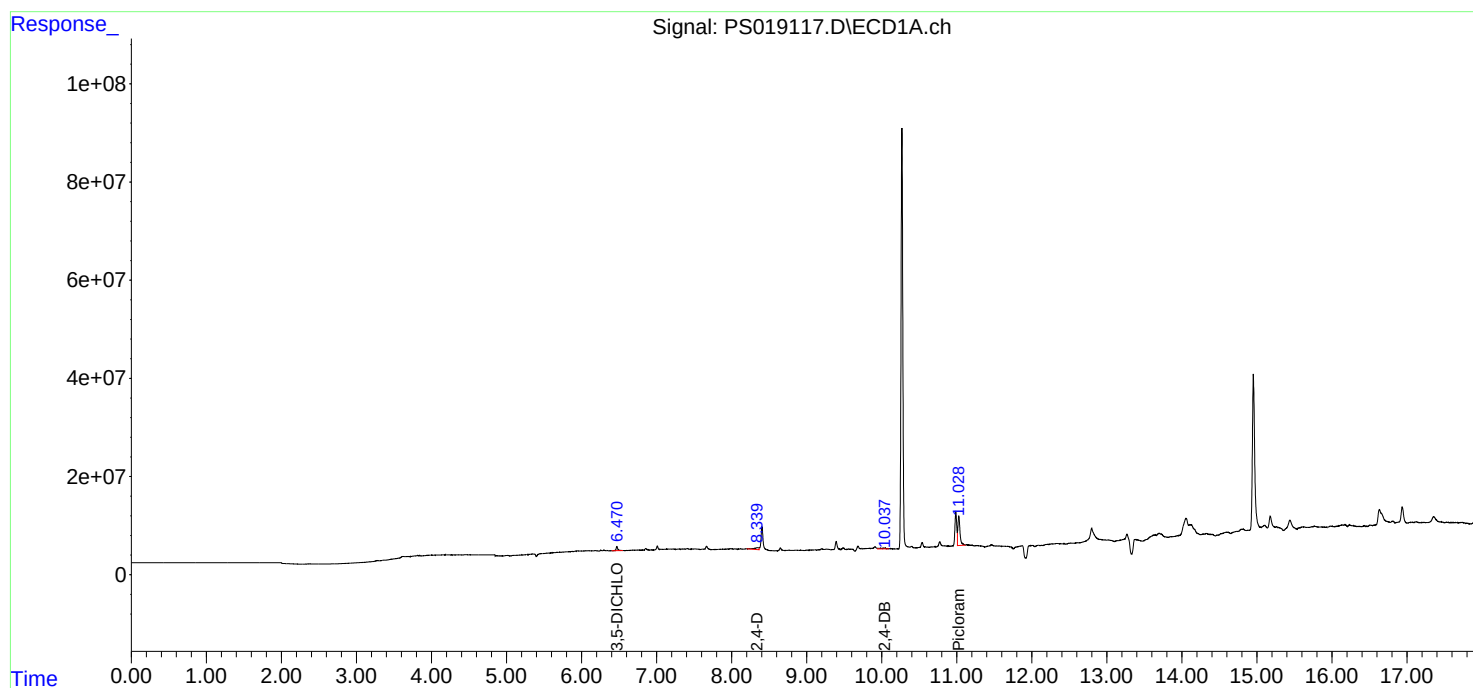


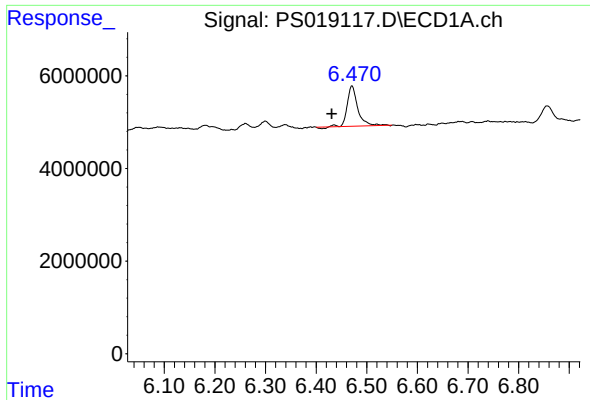

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.471 min
Delta R.T.: 0.040 min
Response: 12355282
Conc: 2.48 ng/ml

Instrument :
ECD_S
ClientSampleId :

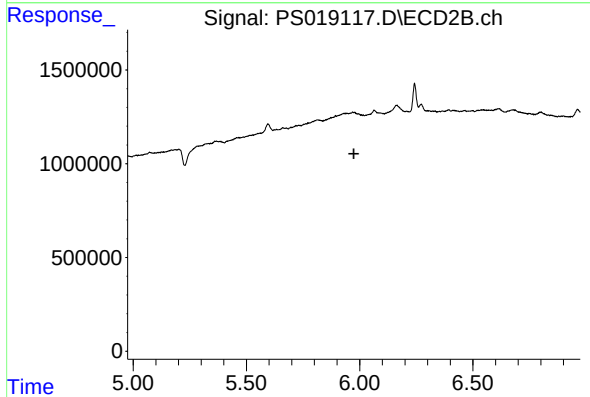


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 5.975 min
Response: 0
Conc: N.D.

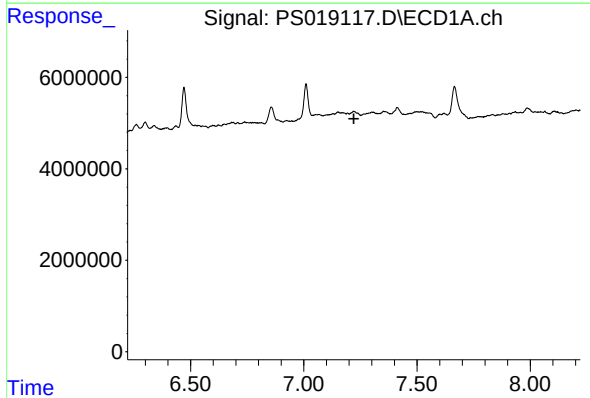


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T. : 7.221 min
Response: 0
Conc: N.D.

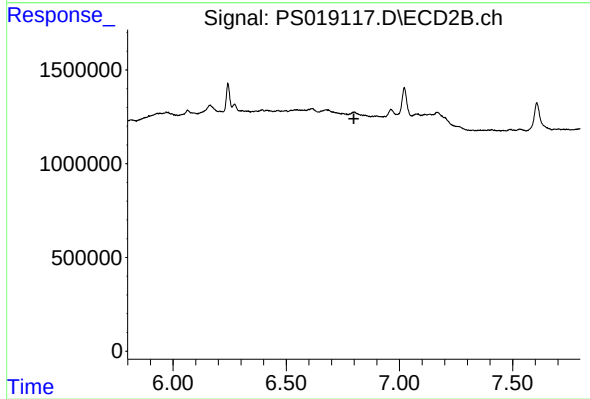

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T. : 6.799 min
Response: 0
Conc: N.D.

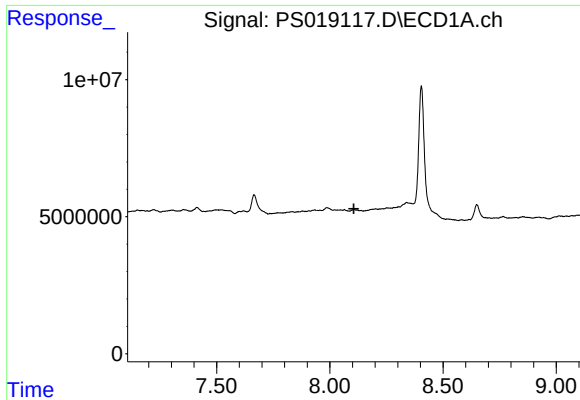

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 8.106 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

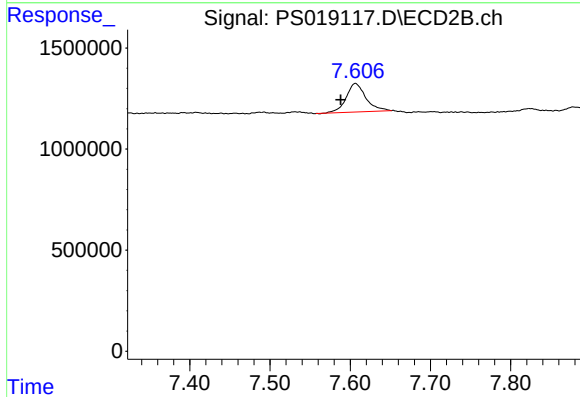


#8 DICHLORPROP

R.T.: 7.607 min
Delta R.T.: 0.018 min
Response: 2420022
Conc: 2.90 ng/ml

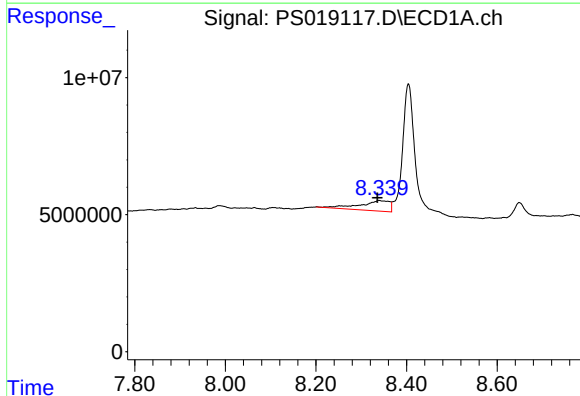


#9 2,4-D

R.T.: 8.340 min
Delta R.T.: 0.004 min
Response: 17269875
Conc: 4.21 ng/ml

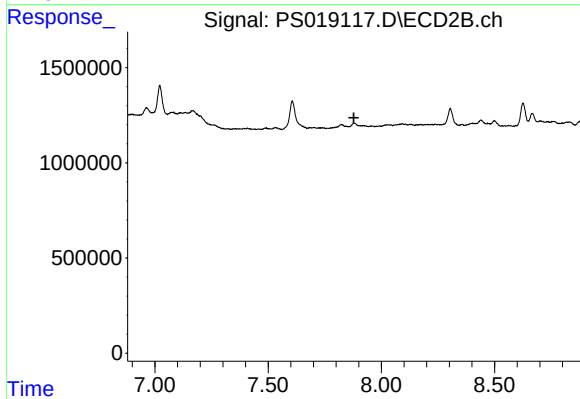

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 7.879 min
Response: 0
Conc: N.D.

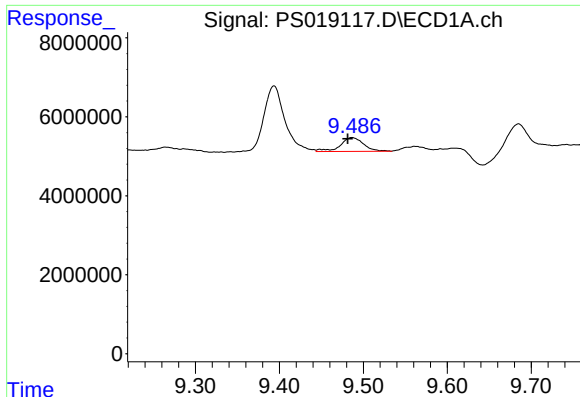

#12 2,4,5-T


R.T.: 9.487 min
Delta R.T.: 0.005 min
Response: 6753156
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

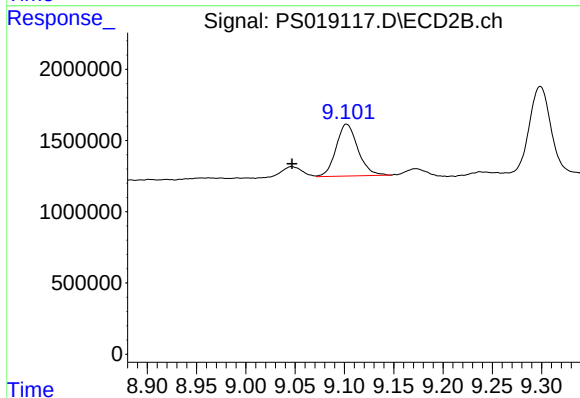


#12 2,4,5-T

R.T.: 9.102 min
Delta R.T.: 0.055 min
Response: 5585514
Conc: 1.29 ng/ml

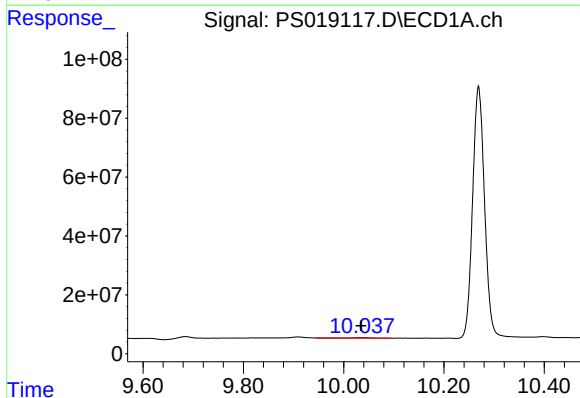


#13 2,4-DB

R.T.: 10.037 min
Delta R.T.: 0.003 min
Response: 10402774
Conc: 2.95 ng/ml

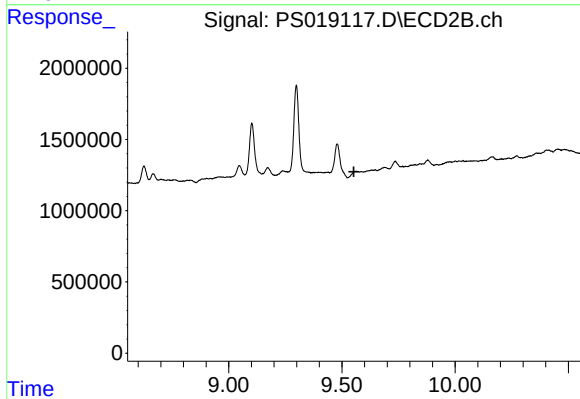

#13 2,4-DB


R.T.: 0.000 min
Exp R.T. : 9.553 min
Response: 0
Conc: N.D.

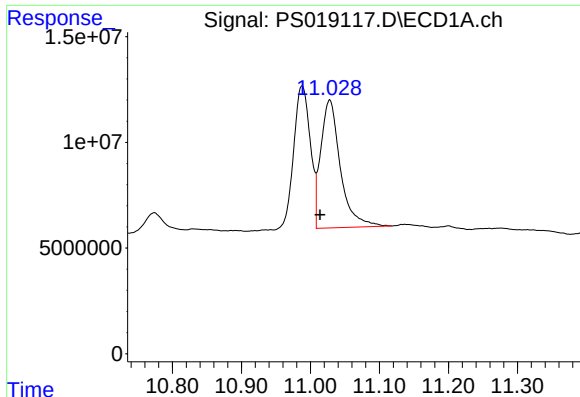

#15 Picloram


R.T.: 11.028 min
Delta R.T.: 0.014 min
Response: 119407929
Conc: 4.46 ng/ml

Instrument :
ECD_S
ClientSampleId :

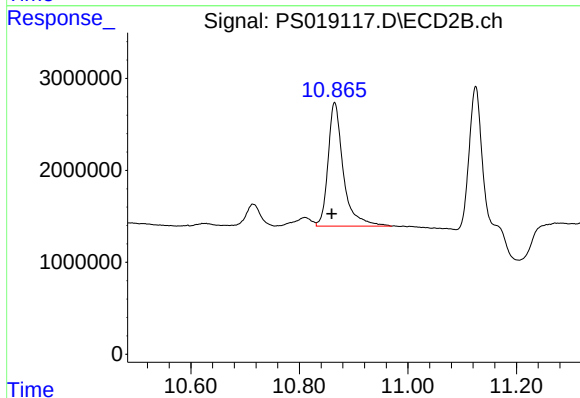


#15 Picloram

R.T.: 10.865 min
Delta R.T.: 0.005 min
Response: 26201842
Conc: 4.43 ng/ml

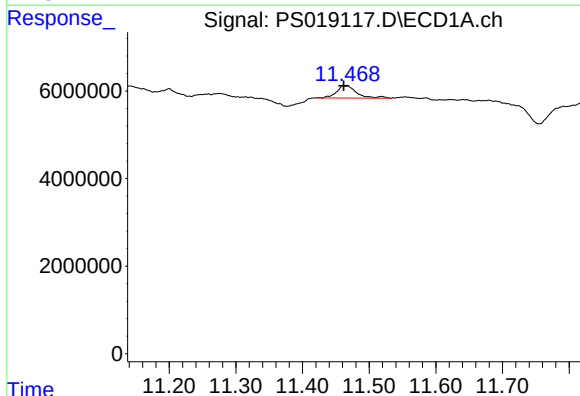

#16 DCPA

R.T.: 11.464 min
Delta R.T.: 0.002 min
Response: 5943568
Conc: N.D.

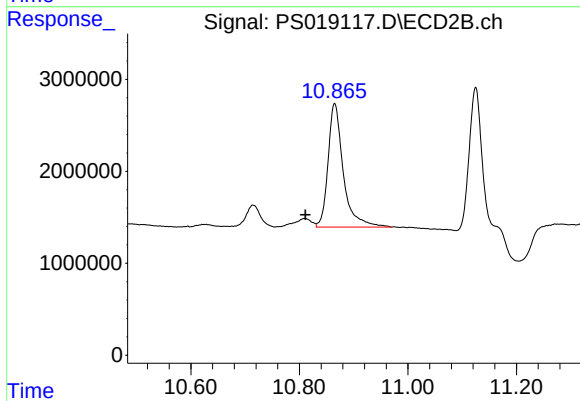

#16 DCPA

R.T.: 10.865 min
Delta R.T.: 0.054 min
Response: 26201842
Conc: 4.58 ng/ml