

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS042222\
 Data File : PS019118.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Apr 2022 09:42
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 22 22:48:13 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS041822.M
 Quant Title : 8080.M
 QLast Update : Mon Apr 18 17:28:16 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.220	6.798	1533.1E6	366.6E6	409.902	505.017
Target Compounds							
2) T	3,5-DICHL...	6.471f	0.000	3733268	0	<MDL	N.D. #
7) T	MCPA	7.678f	0.000	7991793	0	<MDL	N.D. #
11) T	2,4,5-TP ...	9.207	8.632	1452138	2116471	<MDL	<MDL #
12) T	2,4,5-T	9.493	0.000	5780735	0	<MDL	N.D. #
13) T	2,4-DB	0.000	9.484f	0	5745640	N.D.	10.365
15) T	Picloram	10.991	10.892	16678539	14240006	<MDL	2.405 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS042222\
Data File : PS019118.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Apr 2022 09:42
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 22 22:48:13 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS041822.M
Quant Title : 8080.M
QLast Update : Mon Apr 18 17:28:16 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

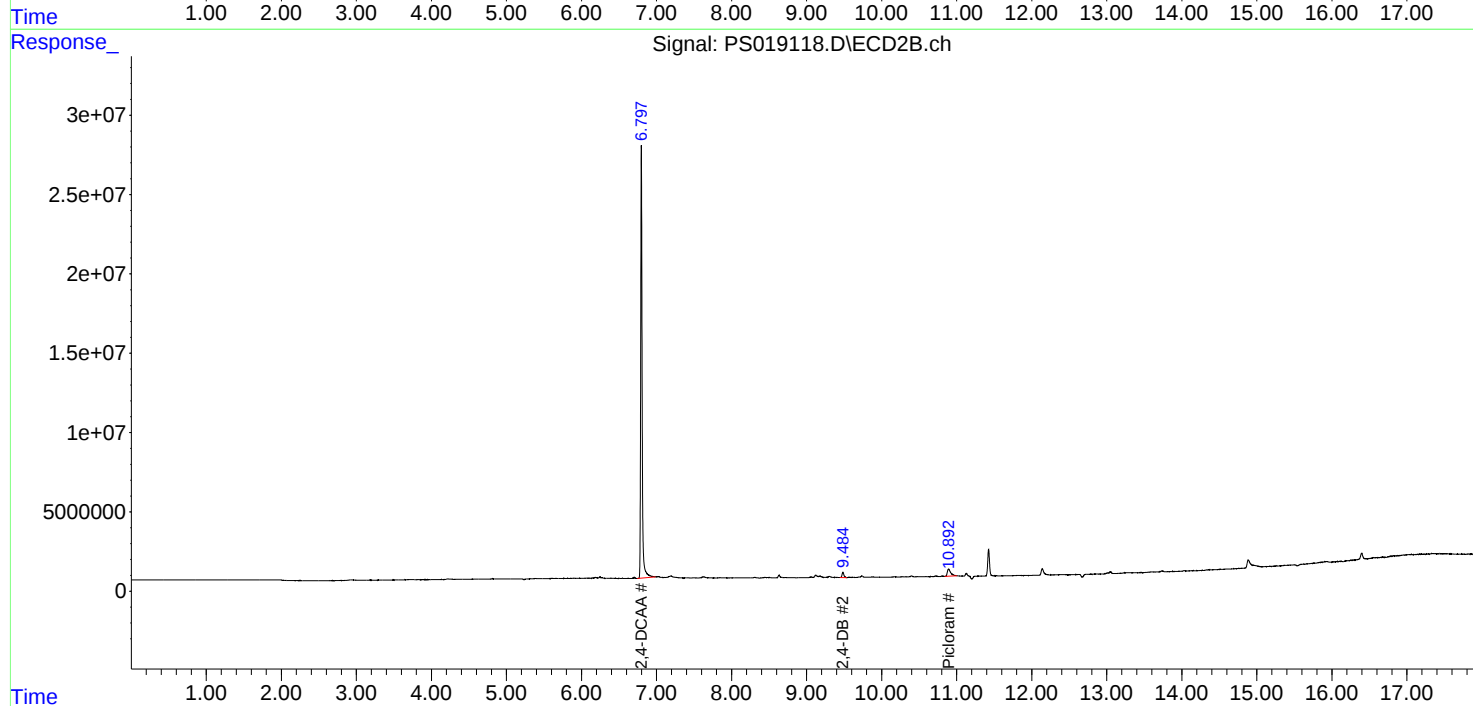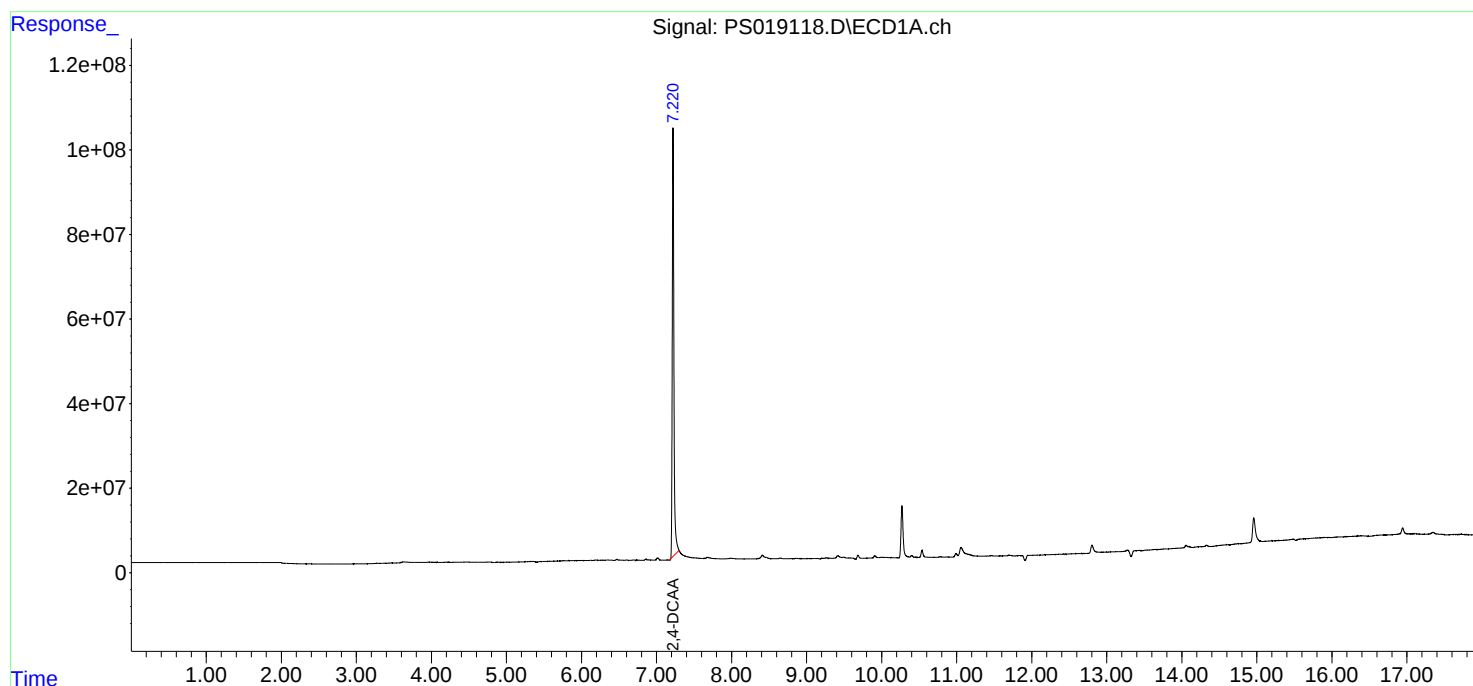


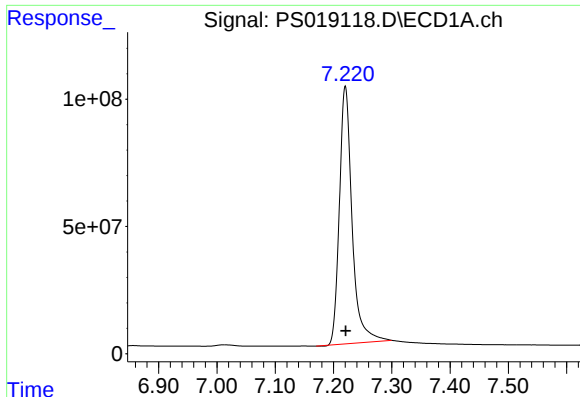

#4 2,4-DCAA


R.T.: 7.220 min
Delta R.T.: 0.000 min
Response: 1533053498
Conc: 409.90 ng/ml

Instrument :
ECD_S
ClientSampleId :

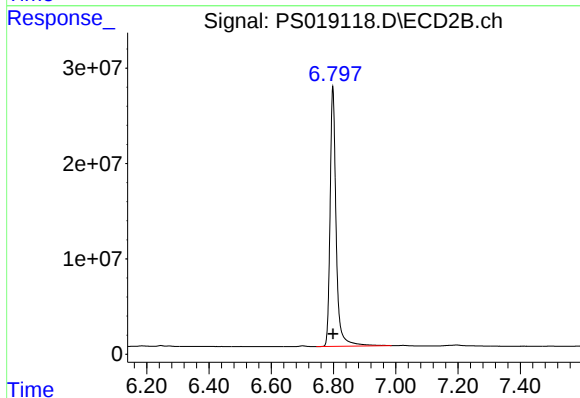


#4 2,4-DCAA

R.T.: 6.798 min
Delta R.T.: -0.001 min
Response: 366580431
Conc: 505.02 ng/ml

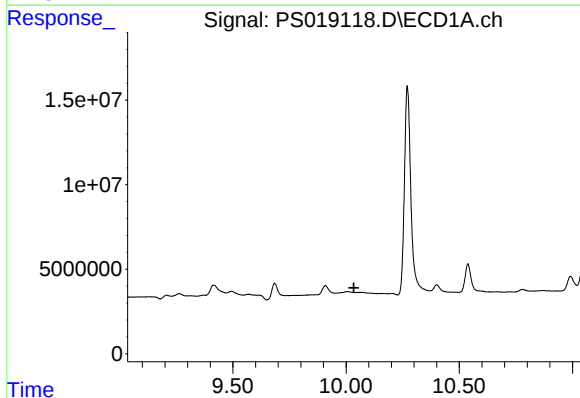


#13 2,4-DB

R.T.: 0.000 min
Exp R.T. : 10.034 min
Response: 0
Conc: N.D.

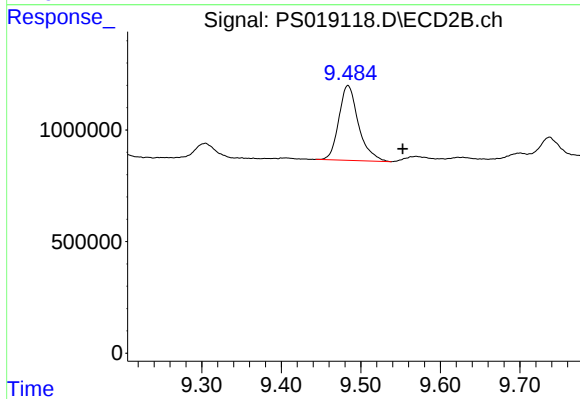

#13 2,4-DB


R.T.: 9.484 min
Delta R.T.: -0.069 min
Response: 5745640
Conc: 10.37 ng/ml

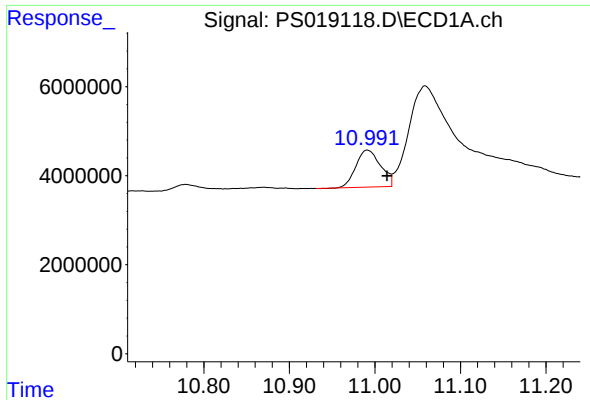

#15 Picloram

R.T.: 10.991 min
Delta R.T.: -0.023 min
Response: 16678539
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

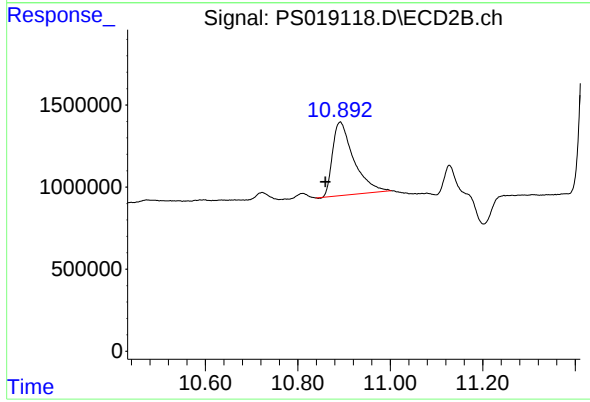

#15 Picloram

R.T.: 10.892 min
Delta R.T.: 0.032 min
Response: 14240006
Conc: 2.40 ng/ml