

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS042224\
 Data File : PS026513.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Apr 2024 20:35
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 23 04:30:48 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS041924.M
 Quant Title : 8080.M
 QLast Update : Fri Apr 19 12:45:38 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.313	7.800	1245.0E6	867.8E6	506.031	489.467
Target Compounds							
1) T	Dalapon	0.000	2.749f	0	37211849	N.D.	13.140
2) T	3,5-DICHL...	6.457	6.733	1729543	1556657	<MDL	<MDL #
3) T	4-Nitroph...	7.104	7.298f	8676520	1379636	5.348	1.148 #
5) T	DICAMBA	7.512	7.992	-72743	713047	N.D.	<MDL
6) T	MCPD	0.000	8.100	0	561923	N.D.	<MDL
7) T	MCPA	7.865	8.333f	404234	223036	<MDL	<MDL #
8) T	DICHLORPROP	8.182f	0.000	5168138	0	1.760	N.D. #
10) T	Pentachlo...	8.753	0.000	727618	0	<MDL	N.D. #
11) T	2,4,5-TP ...	9.329	9.930f	1546153	16365287	<MDL	1.353 #
12) T	2,4,5-T	0.000	10.386	0	1161339	N.D.	<MDL
13) T	2,4-DB	0.000	10.981f	0	1934580	N.D.	1.211
14) T	DINOSEB	11.436	11.299f	-155700	1357640	N.D.	<MDL
15) T	Picloram	11.241	12.396f	1941910	752.0E6	<MDL	41.020 #
16) T	DCPA	11.693f	12.396f	5826186	752.0E6	<MDL	50.555 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS042224\
Data File : PS026513.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Apr 2024 20:35
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 23 04:30:48 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS041924.M
Quant Title : 8080.M
QLast Update : Fri Apr 19 12:45:38 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

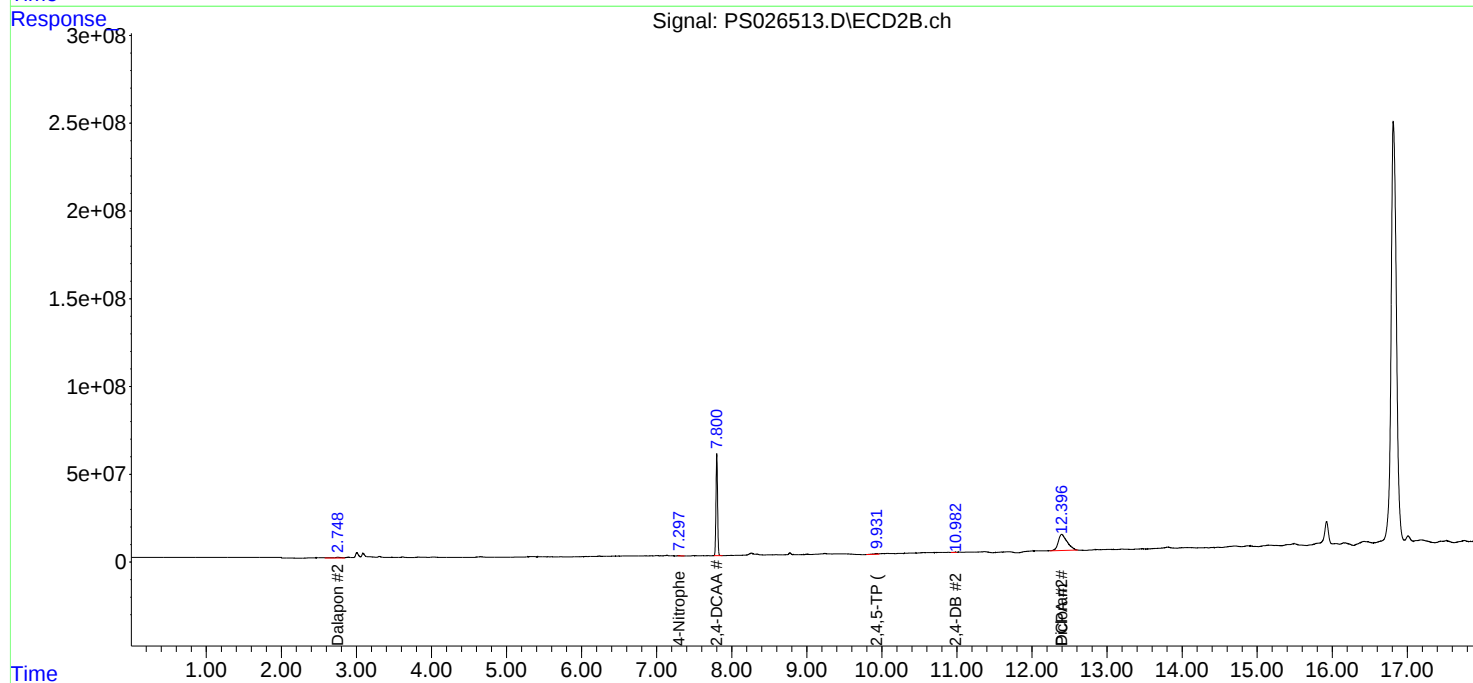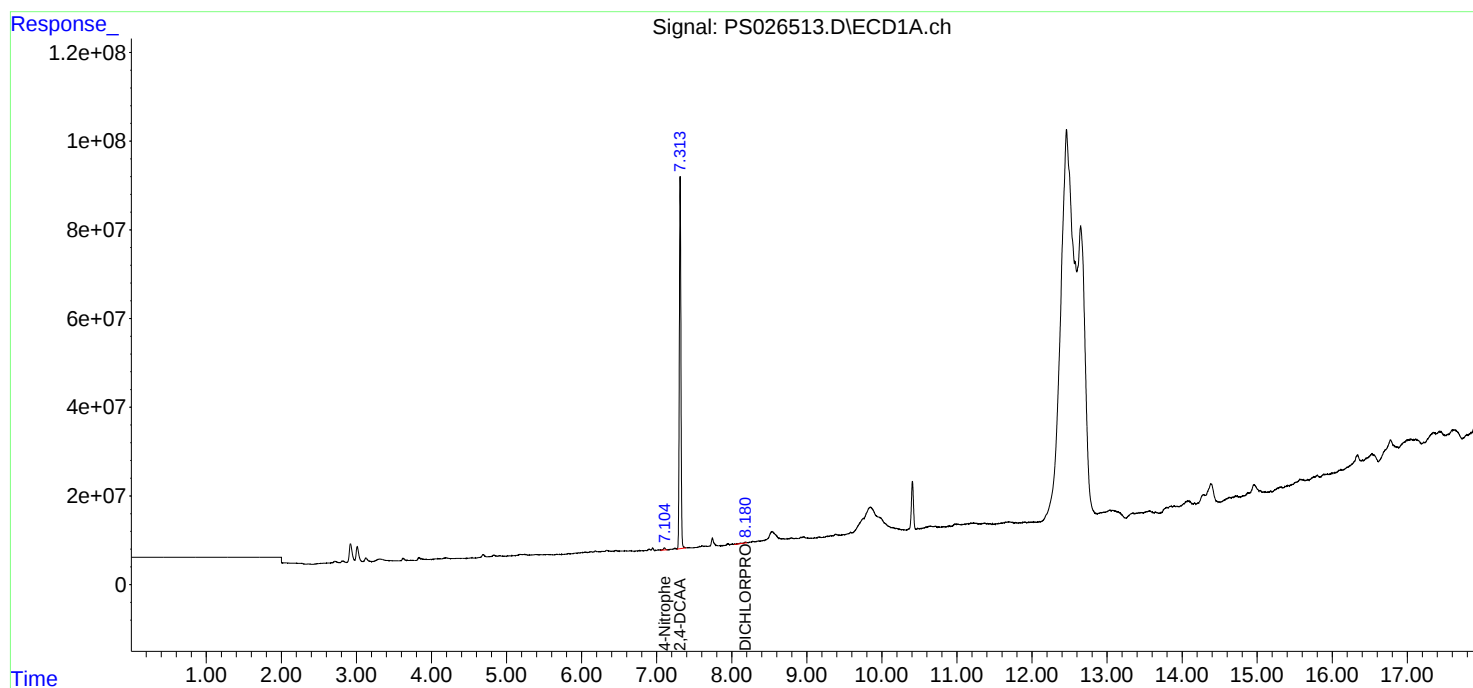


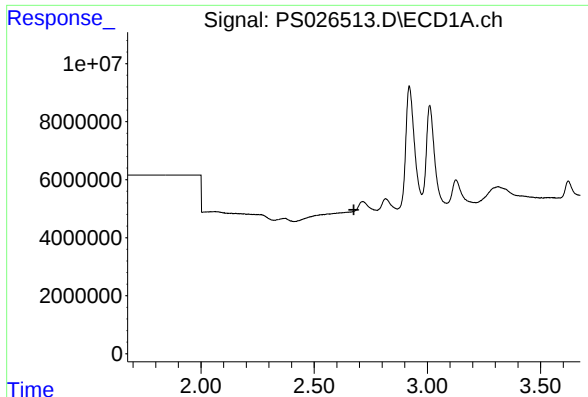

#1 Dalapon


R.T.: 0.000 min
Exp R.T.: 2.675 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

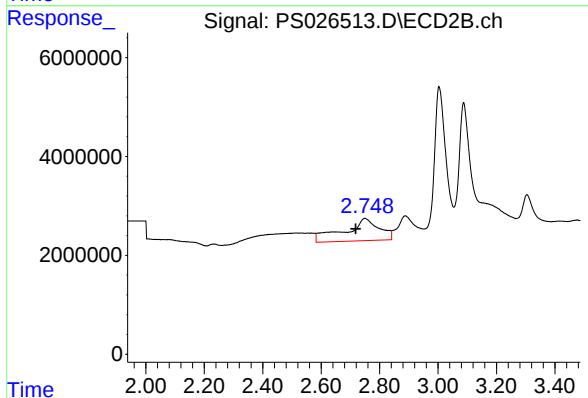


#1 Dalapon

R.T.: 2.749 min
Delta R.T.: 0.031 min
Response: 37211849
Conc: 13.14 ng/ml

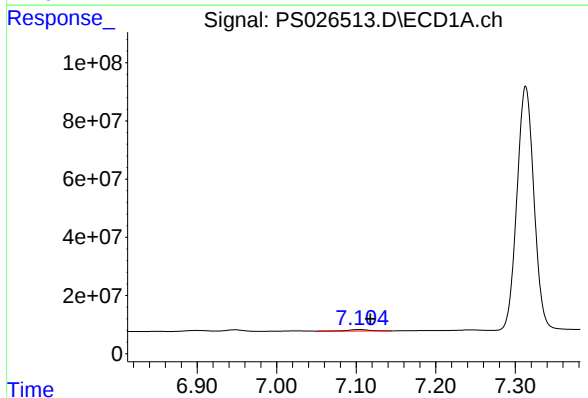


#3 4-Nitrophenol

R.T.: 7.104 min
Delta R.T.: -0.014 min
Response: 8676520
Conc: 5.35 ng/ml

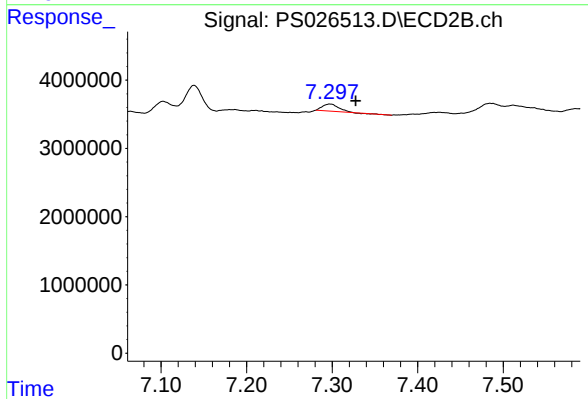

#3 4-Nitrophenol


R.T.: 7.298 min
Delta R.T.: -0.030 min
Response: 1379636
Conc: 1.15 ng/ml

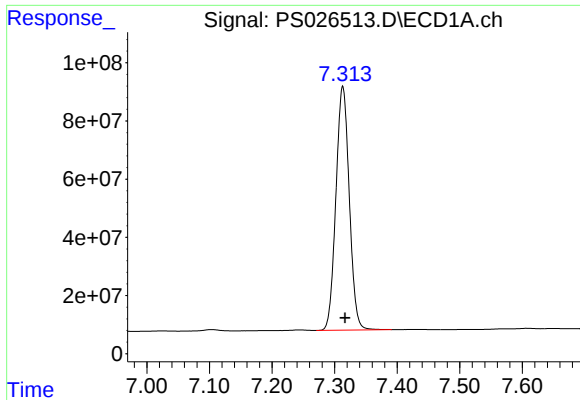

#4 2,4-DCAA


R.T.: 7.313 min
Delta R.T.: -0.004 min
Response: 1245037312
Conc: 506.03 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

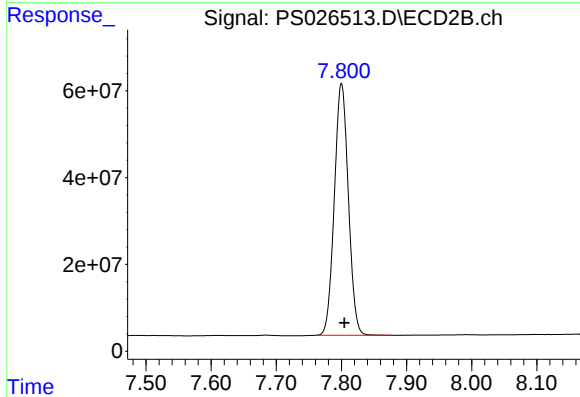


#4 2,4-DCAA

R.T.: 7.800 min
Delta R.T.: -0.004 min
Response: 867809964
Conc: 489.47 ng/ml

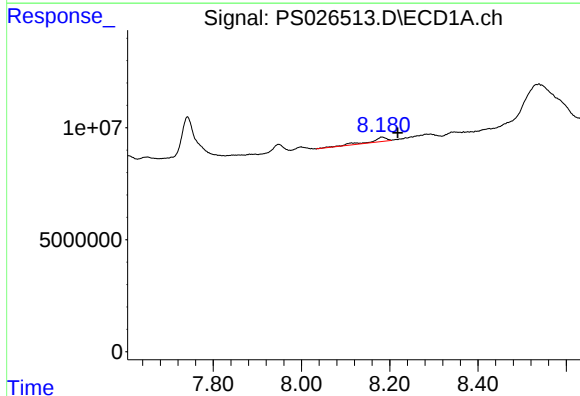


#8 DICHLORPROP

R.T.: 8.182 min
Delta R.T.: -0.037 min
Response: 5168138
Conc: 1.76 ng/ml

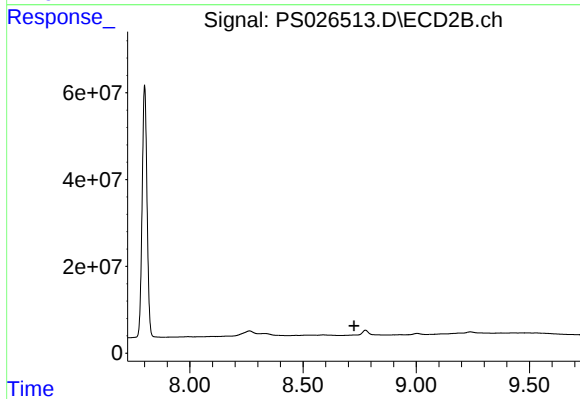

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 8.725 min
Response: 0
Conc: N.D.

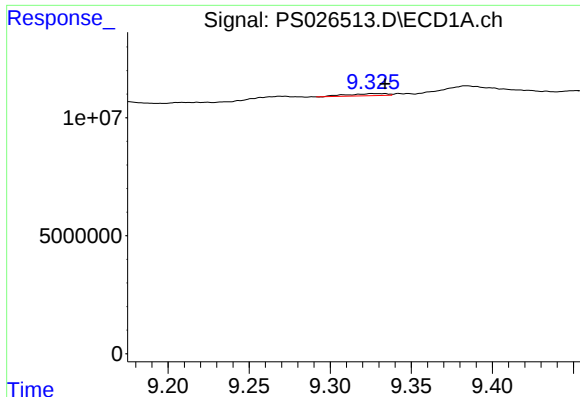

#11 2,4,5-TP (SILVEX)


R.T.: 9.329 min
Delta R.T.: -0.005 min
Response: 1546153
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

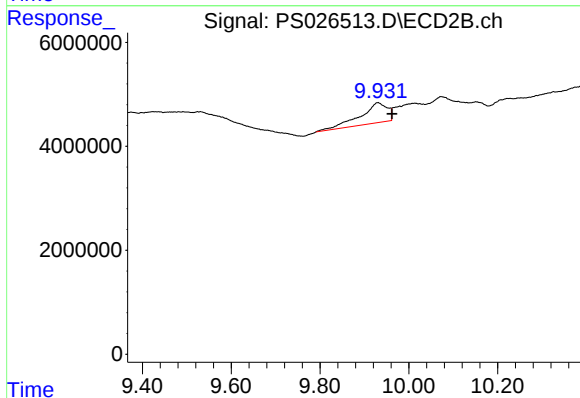


#11 2,4,5-TP (SILVEX)

R.T.: 9.930 min
Delta R.T.: -0.032 min
Response: 16365287
Conc: 1.35 ng/ml

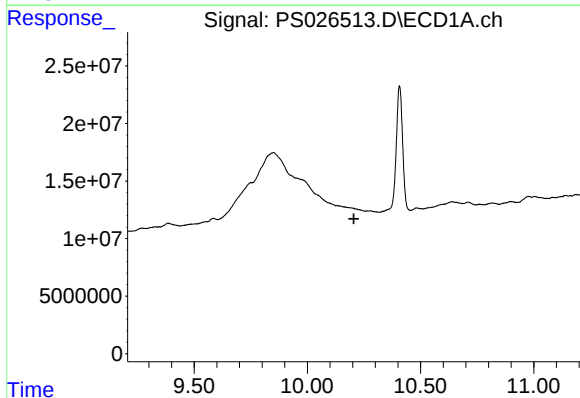


#13 2,4-DB

R.T.: 0.000 min
Exp R.T. : 10.205 min
Response: 0
Conc: N.D.

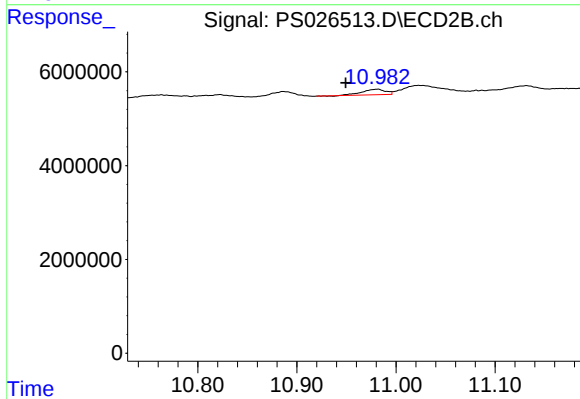

#13 2,4-DB


R.T.: 10.981 min
Delta R.T.: 0.032 min
Response: 1934580
Conc: 1.21 ng/ml

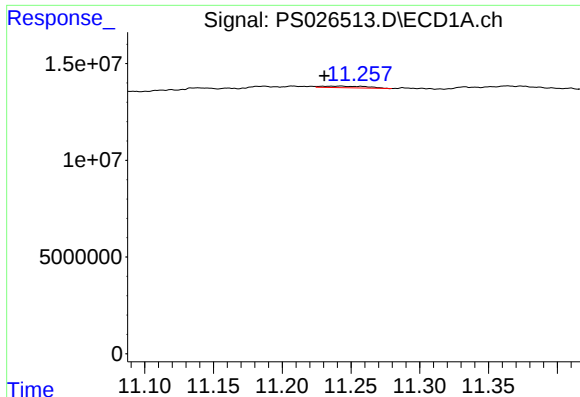

#15 Picloram


R.T.: 11.241 min
Delta R.T.: 0.011 min
Response: 1941910
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

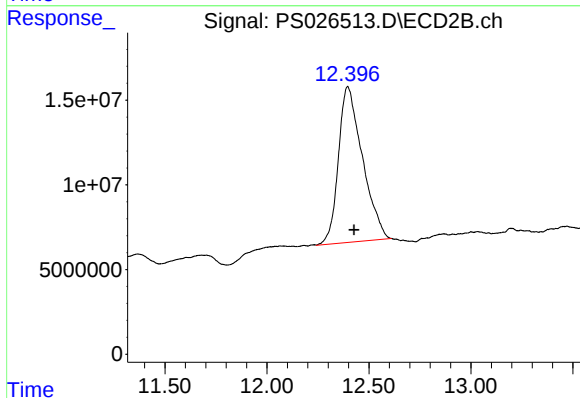


#15 Picloram

R.T.: 12.396 min
Delta R.T.: -0.032 min
Response: 751966086
Conc: 41.02 ng/ml

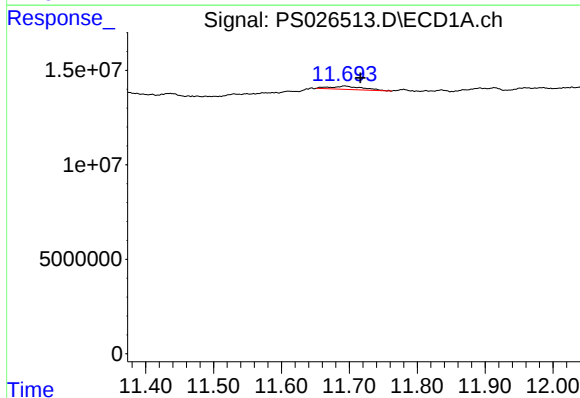

#16 DCPA

R.T.: 11.693 min
Delta R.T.: -0.023 min
Response: 5826186
Conc: N.D.

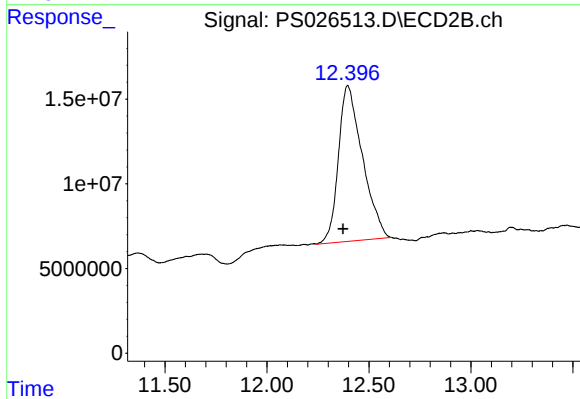

#16 DCPA

R.T.: 12.396 min
Delta R.T.: 0.022 min
Response: 751966086
Conc: 50.55 ng/ml