

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS042224\
 Data File : PS026509.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Apr 2024 18:58
 Operator : AR\AJ
 Sample : P2177-05 (Sig #1); P1277-05 (Sig #2)
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 LKWD-BACKFILL-21

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 04/23/2024
 Supervised By :Ankita Jodhani 04/23/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 23 04:29:30 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS041924.M
 Quant Title : 8080.M
 QLast Update : Fri Apr 19 12:45:38 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
4) S 2,4-DCAA	7.313	7.801	807.1E6	483.0E6	328.039m	272.430m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS042224\
Data File : PS026509.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Apr 2024 18:58
Operator : AR\AJ
Sample : P2177-05 (Sig #1); P1277-05 (Sig #2)
Misc :
ALS Vial : 8 Sample Multiplier: 1



Instrument :
ECD_S
ClientSampleId :
LKWD-BACKFILL-21


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 04/23/2024
Supervised By : Ankita Jodhani 04/23/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 23 04:29:30 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS041924.M
Quant Title : 8080.M
QLast Update : Fri Apr 19 12:45:38 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

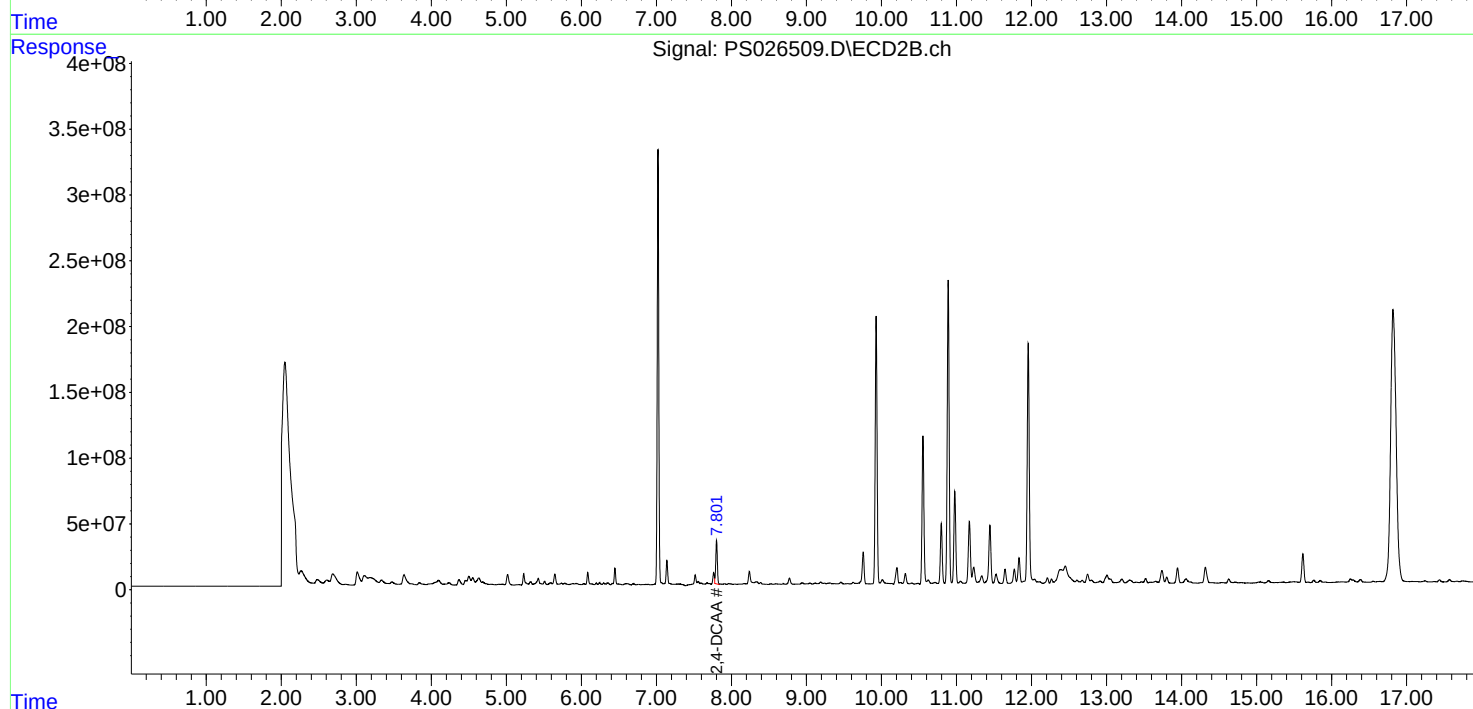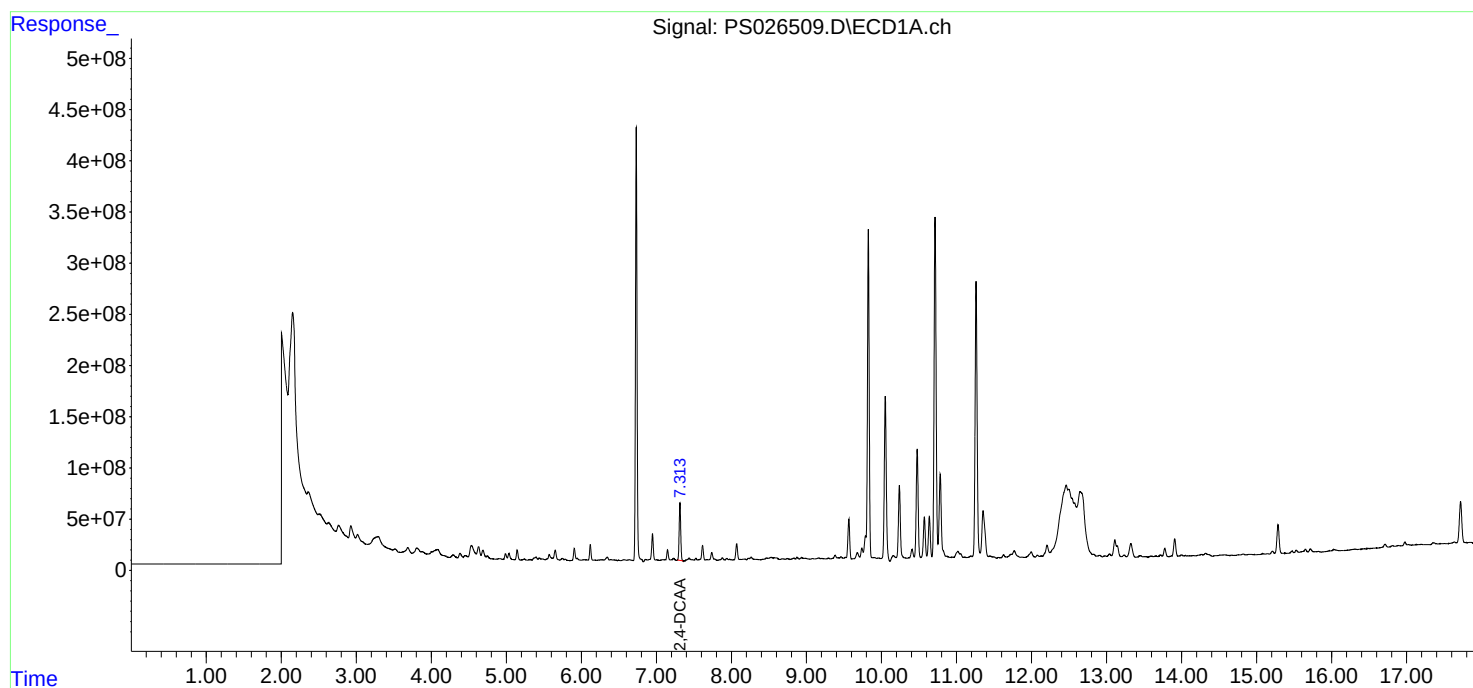

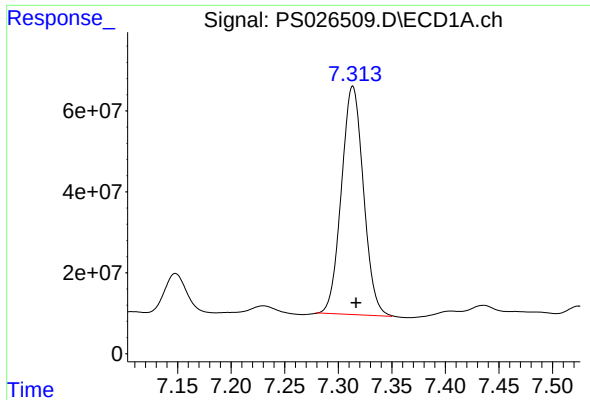


#4 2,4-DCAA

R.T.: 7.313 min
Delta R.T.: -0.004 min
Response: 807105174
Conc: 328.04 ng/ml

Instrument :
ECD_S
ClientSampleId :
LKWD-BACKFILL-21

Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 04/23/2024
Supervised By :Ankita Jodhani 04/23/2024

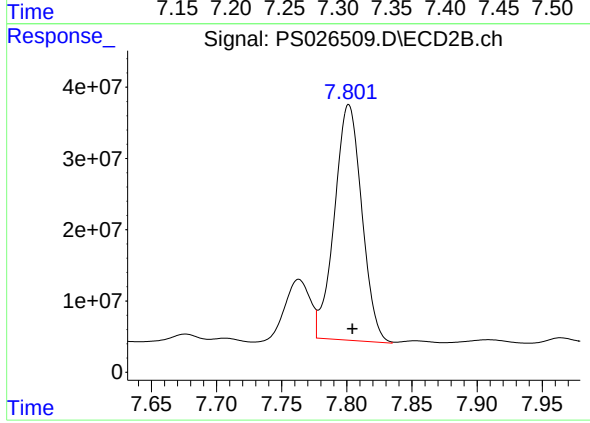

#4 2,4-DCAA

R.T.: 7.801 min
Delta R.T.: -0.003 min
Response: 483010840
Conc: 272.43 ng/ml m