

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS042319\
 Data File : PS004216.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Apr 2019 08:13
 Operator : EI\SJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 24 01:30:43 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS041119.M
 Quant Title : 8080.M
 QLast Update : Thu Apr 11 14:18:42 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds						
5) T	DICAMBA	11.545	11.014	1180029	1817274	<MDL 1.104 #
9) T	2,4-D	13.071	0.000	6300848	0	13.838 N.D. #
10) T	Pentachlo...	13.450	13.135	3456292	2647597	<MDL <MDL #
11) T	2,4,5-TP ...	14.368	13.786	1881361	1643615	<MDL <MDL #
14) T	DINOSEB	16.926	15.403	26212723	1437439	10.463 <MDL #
15) T	Picloram	16.691	16.701	743552	23423705	<MDL 6.842 #
16) T	DCPA	17.270	16.571	3589427	2310988	<MDL <MDL #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS042319\
Data File : PS004216.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Apr 2019 08:13
Operator : EI\SJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 24 01:30:43 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS041119.M
Quant Title : 8080.M
QLast Update : Thu Apr 11 14:18:42 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

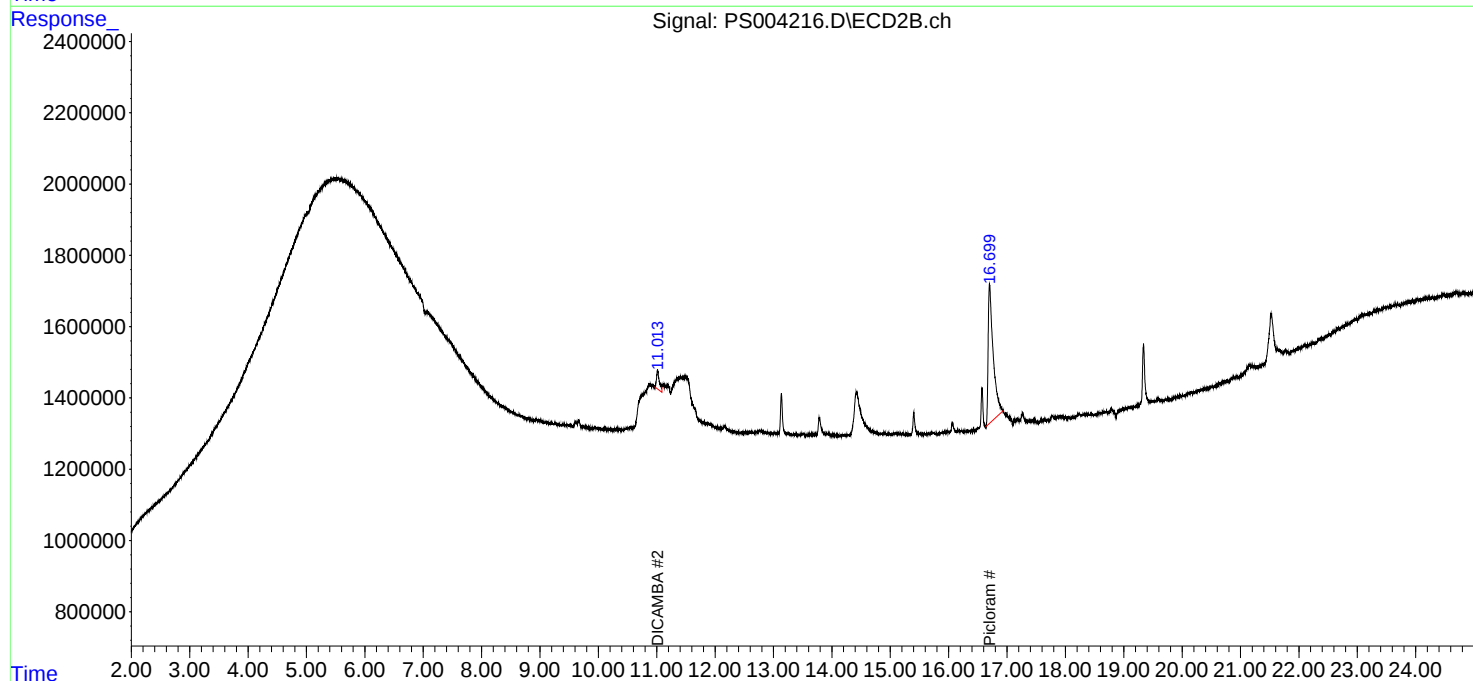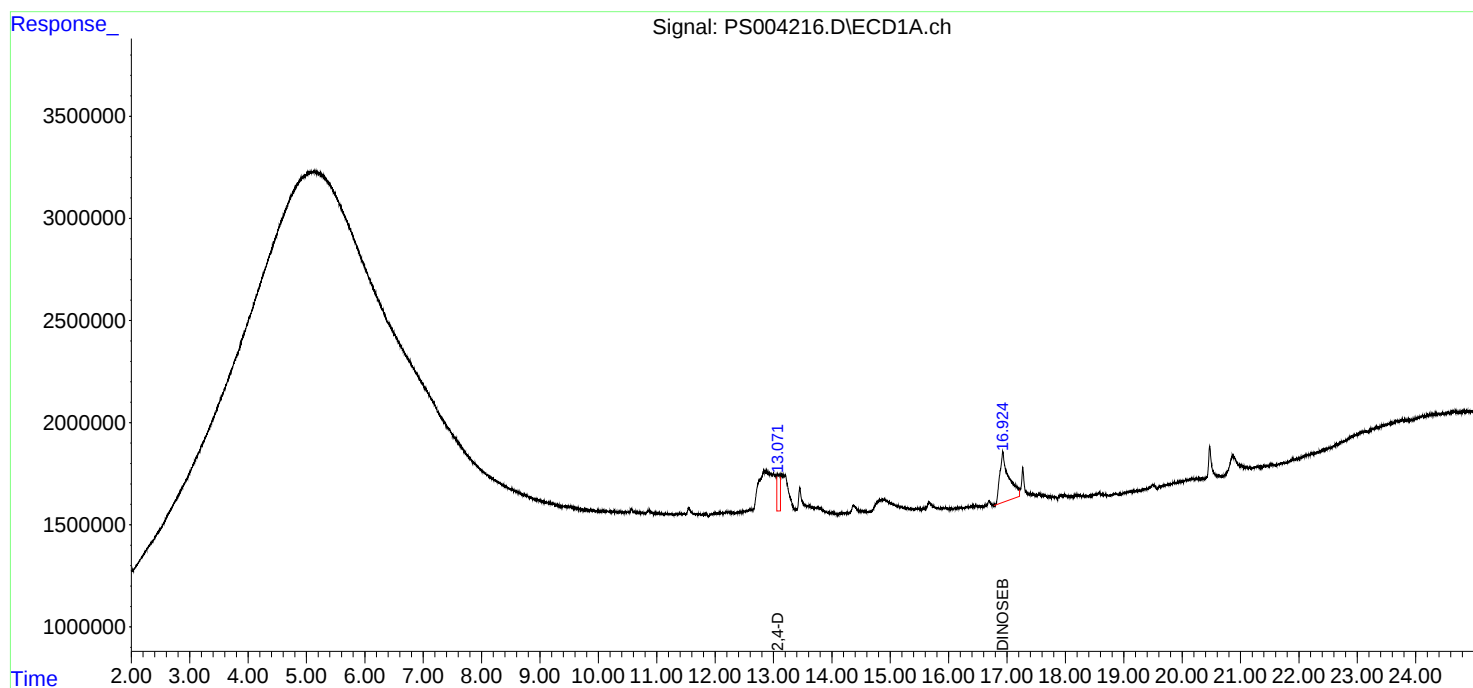


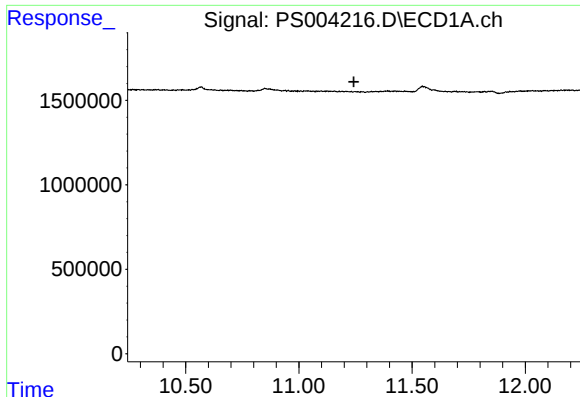

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T.: 11.243 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HEXANE

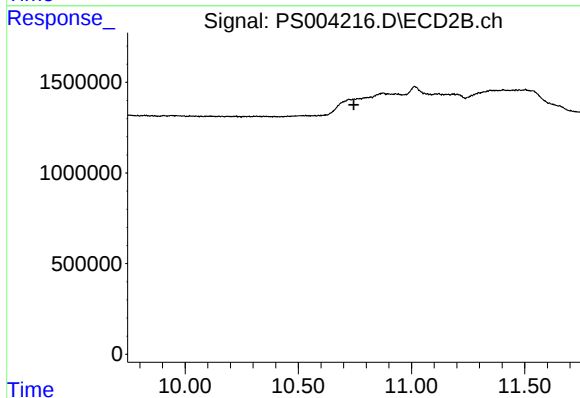


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T.: 10.746 min
Response: 0
Conc: N.D.

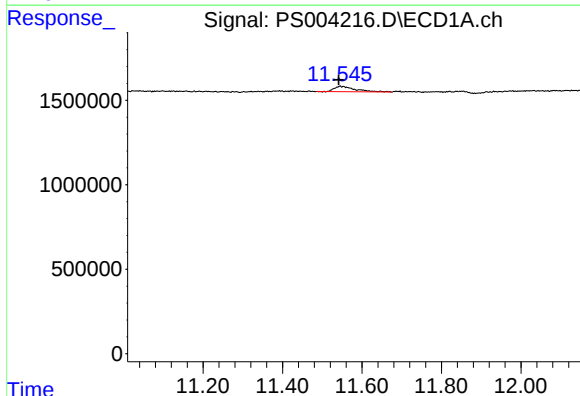


#5 DICAMBA

R.T.: 11.545 min
Delta R.T.: 0.003 min
Response: 1180029
Conc: N.D.

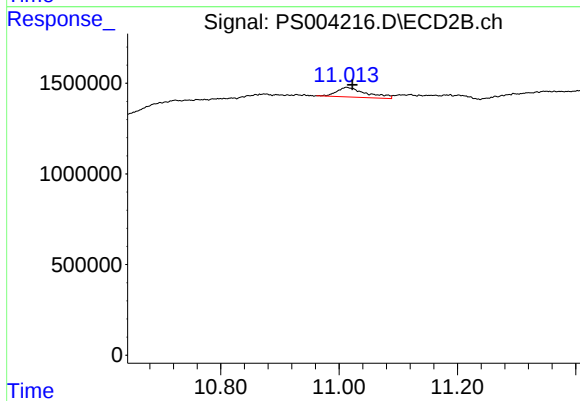

#5 DICAMBA


R.T.: 11.014 min
Delta R.T.: -0.008 min
Response: 1817274
Conc: 1.10 ng/ml

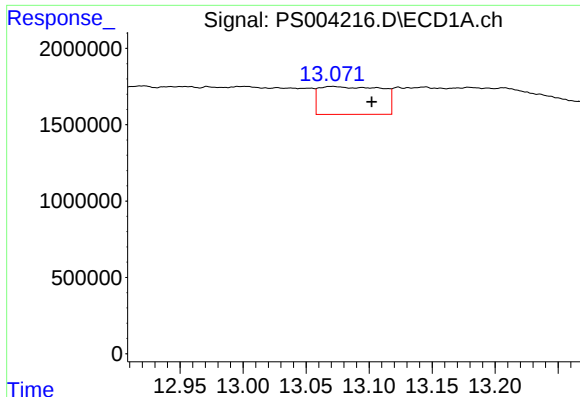

#9 2,4-D


R.T.: 13.071 min
Delta R.T.: -0.031 min
Response: 6300848
Conc: 13.84 ng/ml

Instrument :
ECD_S
ClientSampleId :
HEXANE

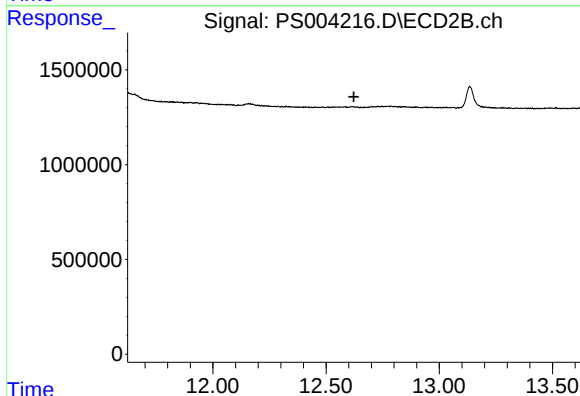


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 12.623 min
Response: 0
Conc: N.D.

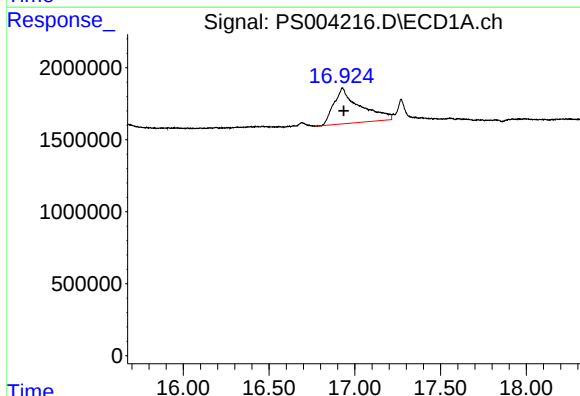


#14 DINOSEB

R.T.: 16.926 min
Delta R.T.: -0.010 min
Response: 26212723
Conc: 10.46 ng/ml

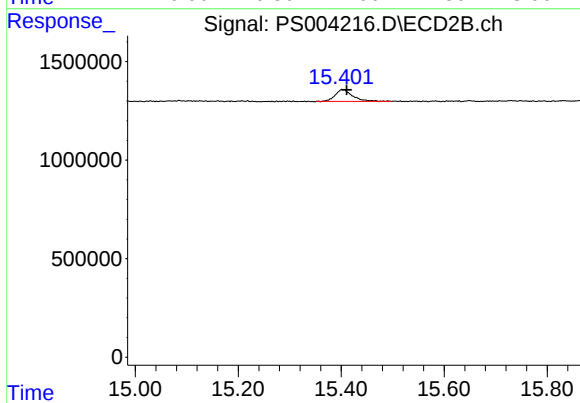

#14 DINOSEB


R.T.: 15.403 min
Delta R.T.: -0.008 min
Response: 1437439
Conc: N.D.

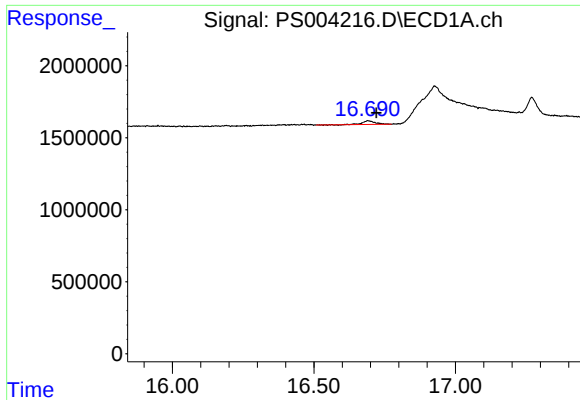

#15 Picloram

R.T.: 16.691 min
Delta R.T.: -0.030 min
Response: 743552
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HEXANE

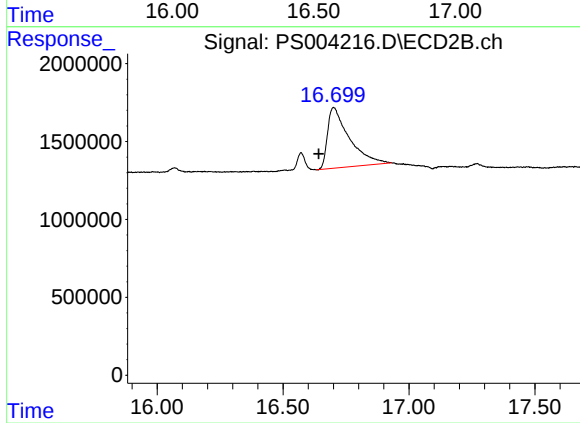

#15 Picloram

R.T.: 16.701 min
Delta R.T.: 0.059 min
Response: 23423705
Conc: 6.84 ng/ml