

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS042319\
 Data File : PS004243.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Apr 2019 06:56
 Operator : EI\SJ
 Sample : K2515-04
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 TP-15

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 24 08:23:00 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS041119.M
 Quant Title : 8080.M
 QLast Update : Thu Apr 11 14:18:42 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.211	10.712	194.4E6	174.4E6	400.641	379.806
Target Compounds							
2) T	3,5-DICHL...	0.000	8.961	0	127.1E6	N.D.	222.317
3) T	4-Nitroph...	10.840	9.925	13748370	11329432	54.428	47.244
6) T	MCP	11.883	0.000	13038058	0	9.987	N.D. #
7) T	MCPA	12.073	0.000	14303572	0	6.933	N.D. #
10) T	Pentachlo...	13.442	13.198	2762699	1994318	<MDL	<MDL #
11) T	2,4,5-TP ...	14.384	0.000	5066415	0	1.871	N.D. #
12) T	2,4,5-T	0.000	14.317	0	2389819	N.D.	1.036
13) T	2,4-DB	15.465	0.000	2507030	0	8.050	N.D. #
14) T	DINOSEB	16.867	15.371	531682	531115	<MDL	<MDL #
15) T	Picloram	16.695	16.688	1121002	5783583	<MDL	1.689 #
16) T	DCPA	17.234	16.568	4745238	1334600	1.318	<MDL #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS042319\
Data File : PS004243.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Apr 2019 06:56
Operator : EI\SJ
Sample : K2515-04
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampled :
TP-15

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 24 08:23:00 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS041119.M
Quant Title : 8080.M
QLast Update : Thu Apr 11 14:18:42 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

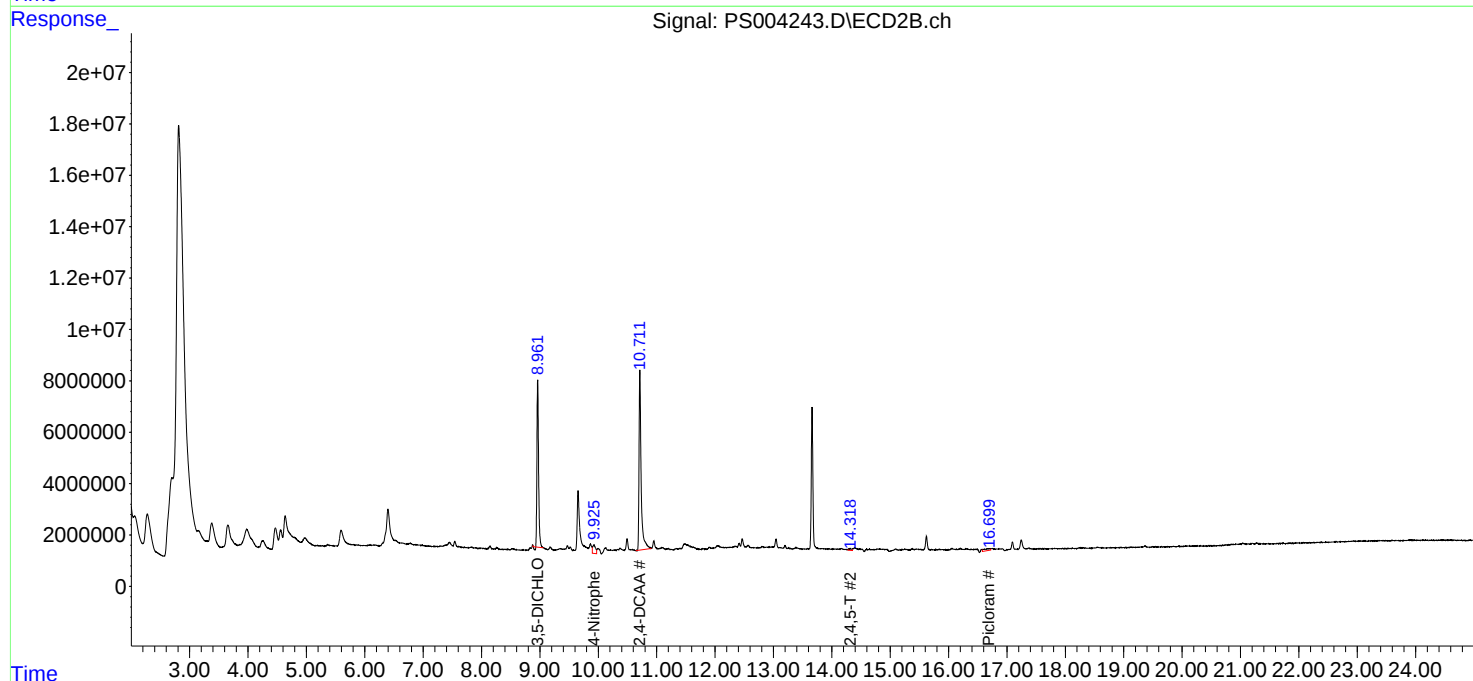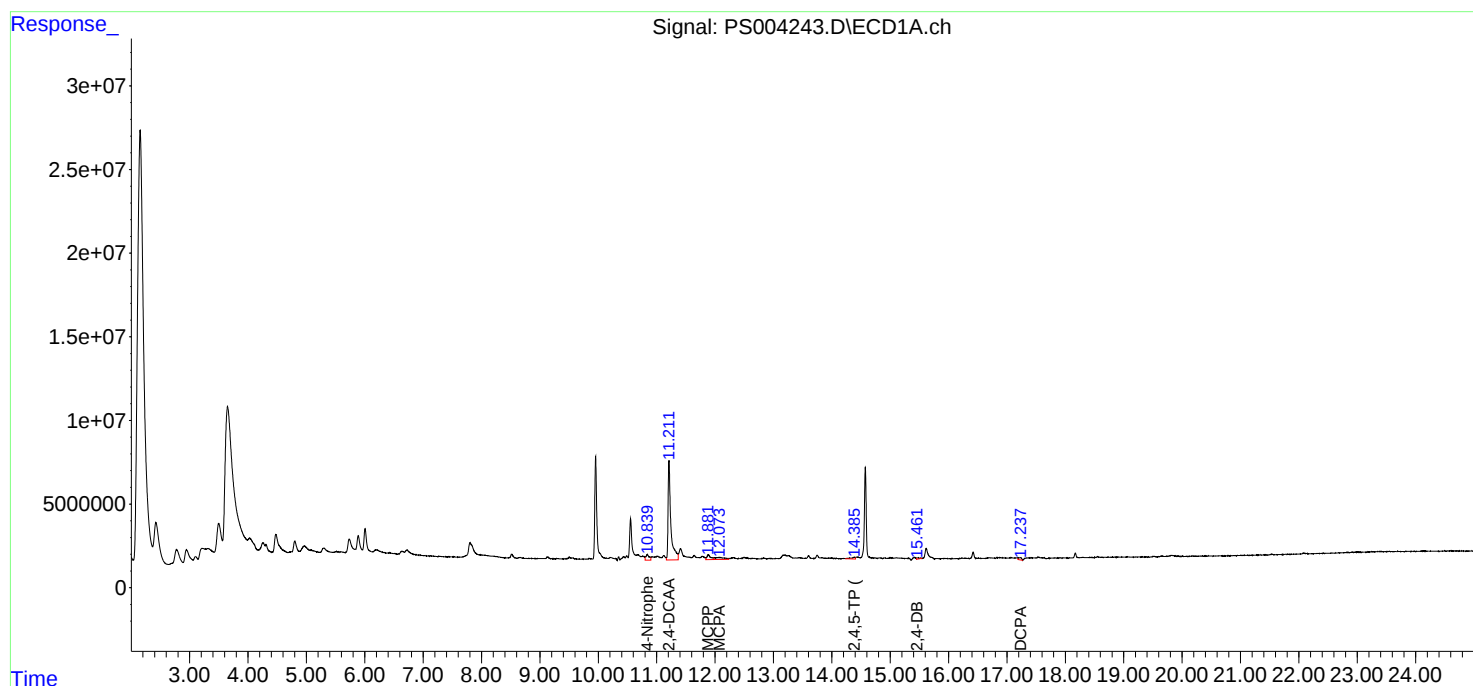


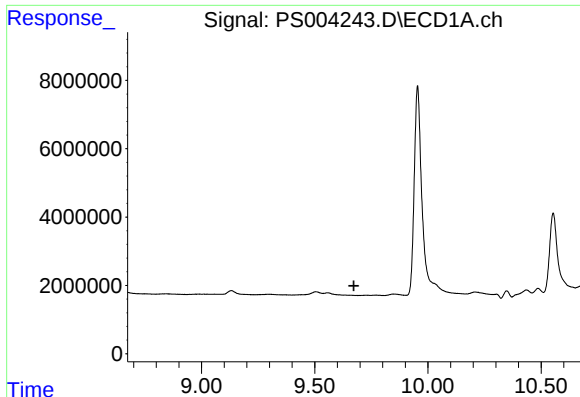

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 9.673 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
TP-15

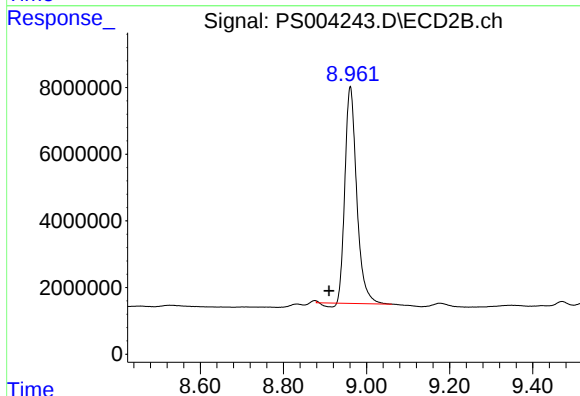


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 8.961 min
Delta R.T.: 0.052 min
Response: 127082007
Conc: 222.32 ng/ml

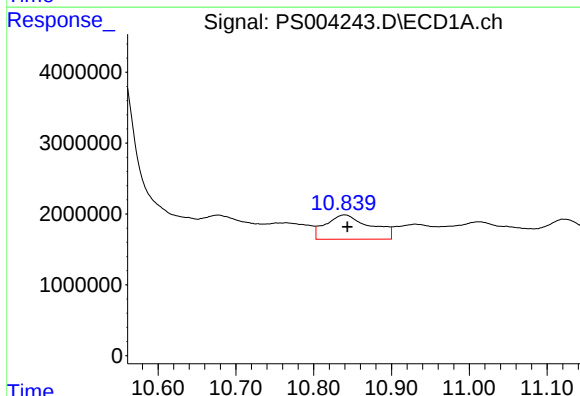


#3 4-Nitrophenol

R.T.: 10.840 min
Delta R.T.: -0.004 min
Response: 13748370
Conc: 54.43 ng/ml

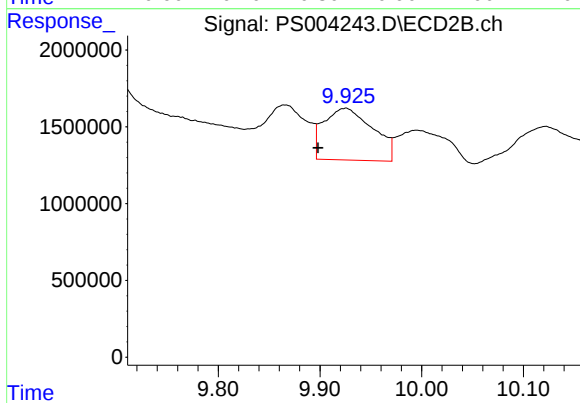

#3 4-Nitrophenol


R.T.: 9.925 min
Delta R.T.: 0.027 min
Response: 11329432
Conc: 47.24 ng/ml

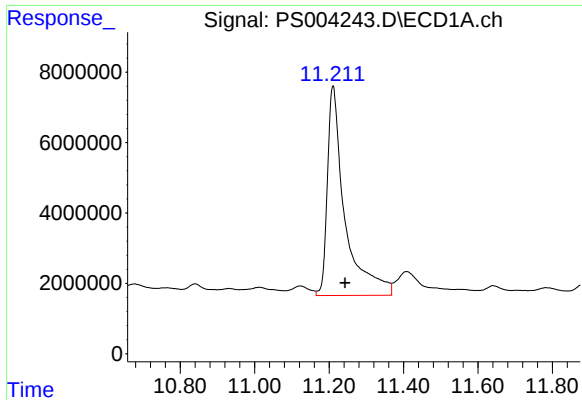

#4 2,4-DCAA


R.T.: 11.211 min
Delta R.T.: -0.033 min
Response: 194397060
Conc: 400.64 ng/ml

Instrument :
ECD_S
ClientSampleId :
TP-15

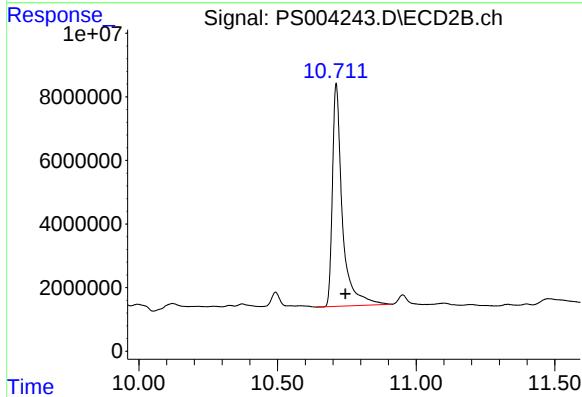


#4 2,4-DCAA

R.T.: 10.712 min
Delta R.T.: -0.034 min
Response: 174422962
Conc: 379.81 ng/ml

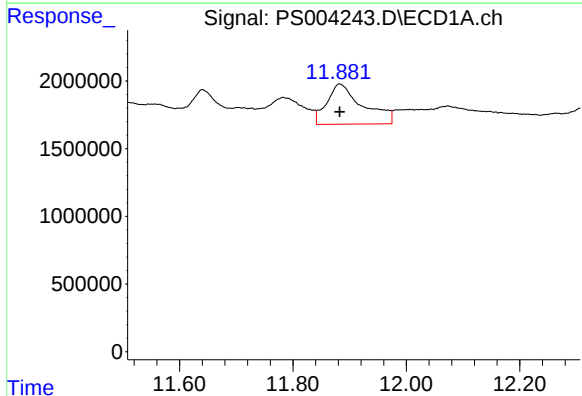


#6 MCP

R.T.: 11.883 min
Delta R.T.: 0.000 min
Response: 13038058
Conc: 9.99 ug/ml

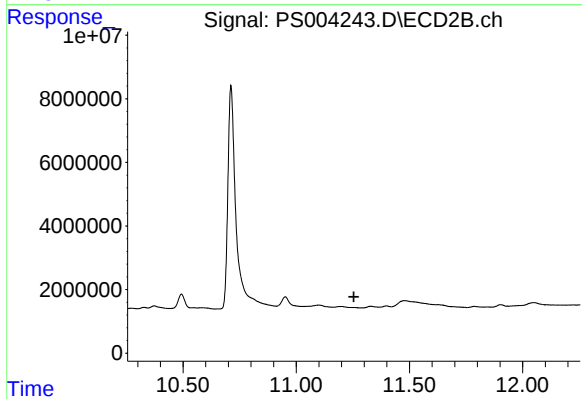

#6 MCP


R.T.: 0.000 min
Exp R.T.: 11.255 min
Response: 0
Conc: N.D.

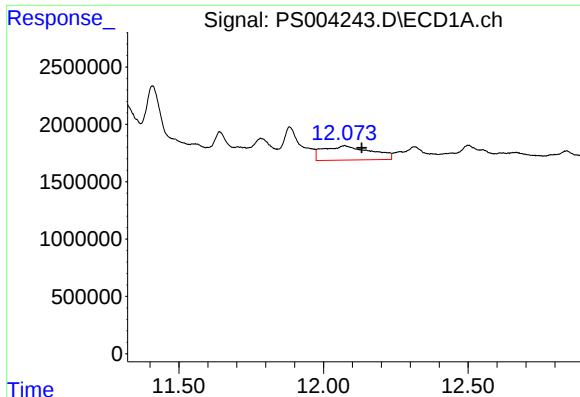

#7 MCPA


R.T.: 12.073 min
Delta R.T.: -0.059 min
Response: 14303572
Conc: 6.93 ug/ml

Instrument :
ECD_S
ClientSampleId :
TP-15

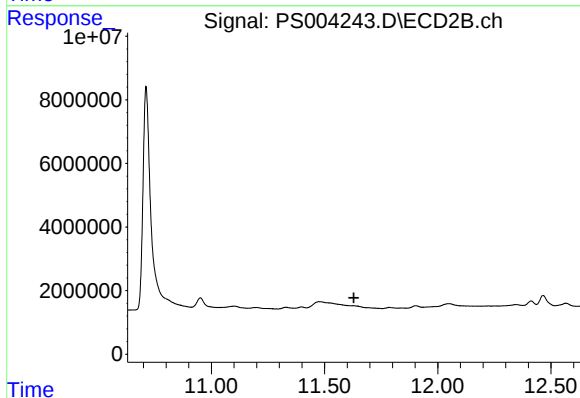


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 11.630 min
Response: 0
Conc: N.D.

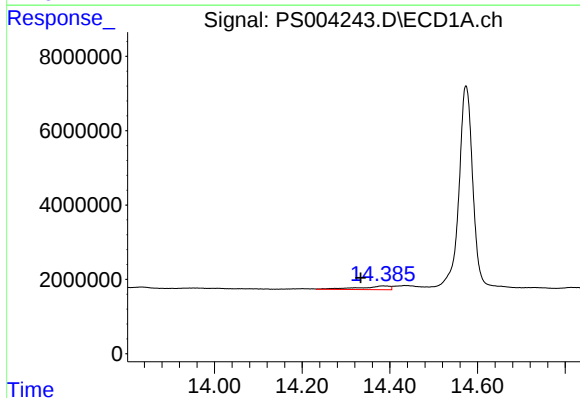


#11 2,4,5-TP (SILVEX)

R.T.: 14.384 min
Delta R.T.: 0.050 min
Response: 5066415
Conc: 1.87 ng/ml

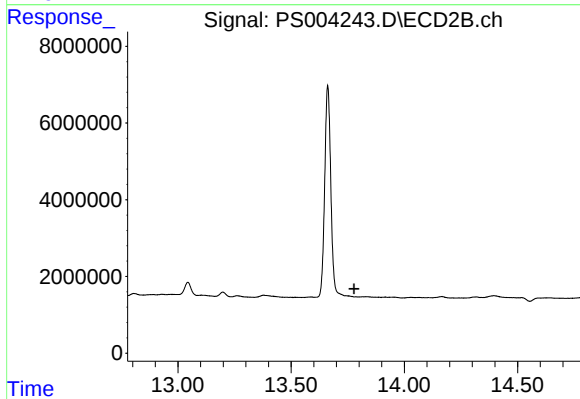

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T. : 13.777 min
Response: 0
Conc: N.D.

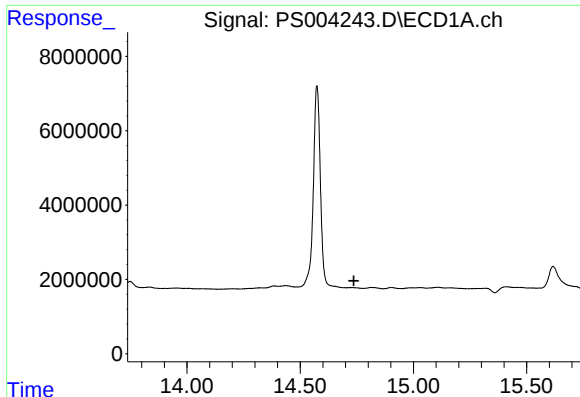

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 14.737 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
TP-15

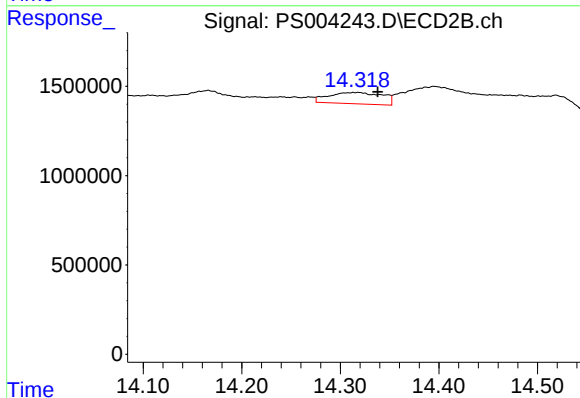


#12 2,4,5-T

R.T.: 14.317 min
Delta R.T.: -0.021 min
Response: 2389819
Conc: 1.04 ng/ml

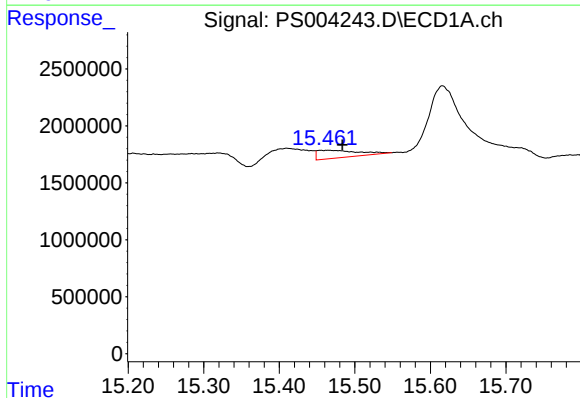


#13 2,4-DB

R.T.: 15.465 min
Delta R.T.: -0.019 min
Response: 2507030
Conc: 8.05 ng/ml

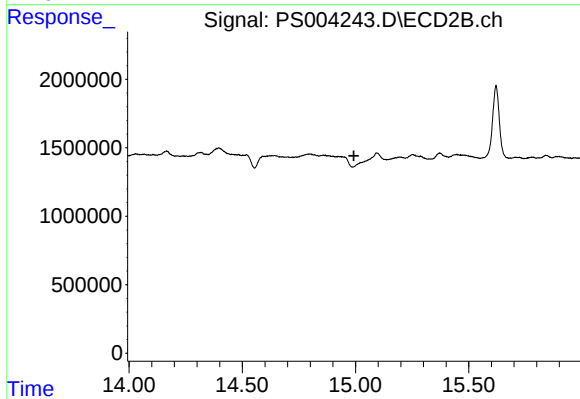

#13 2,4-DB


R.T.: 0.000 min
Exp R.T.: 14.993 min
Response: 0
Conc: N.D.

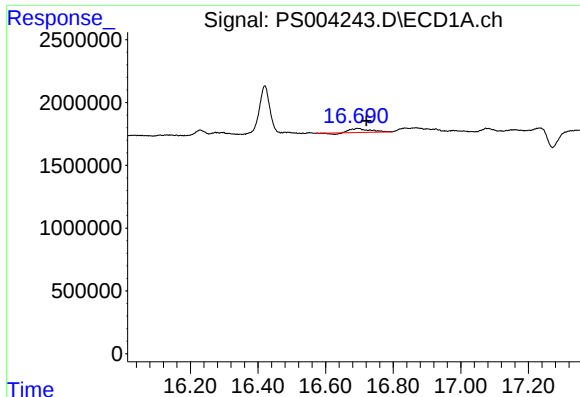

#15 Picloram


R.T.: 16.695 min
Delta R.T.: -0.026 min
Response: 1121002
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
TP-15

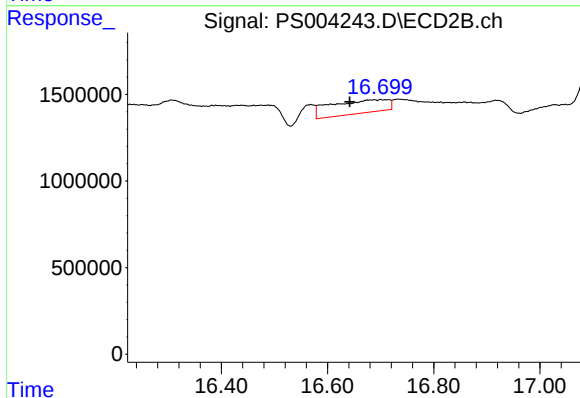


#15 Picloram

R.T.: 16.688 min
Delta R.T.: 0.046 min
Response: 5783583
Conc: 1.69 ng/ml

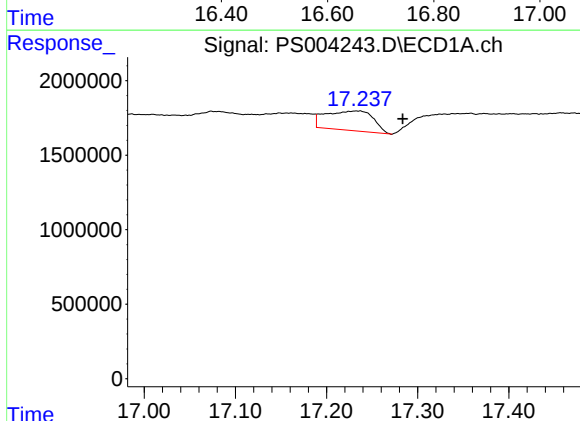

#16 DCPA

R.T.: 17.234 min
Delta R.T.: -0.050 min
Response: 4745238
Conc: 1.32 ng/ml

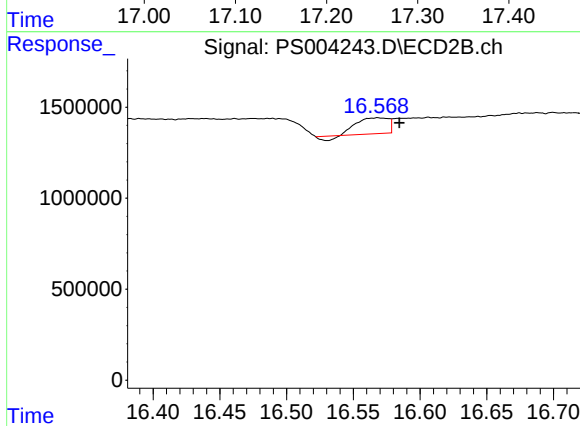

#16 DCPA

R.T.: 16.568 min
Delta R.T.: -0.016 min
Response: 1334600
Conc: N.D.