

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS042319\
 Data File : PS004247.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Apr 2019 09:06
 Operator : EI\SJ
 Sample : K2515-16
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 TP-12

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 24 10:50:00 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS041119.M
 Quant Title : 8080.M
 QLast Update : Thu Apr 11 14:18:42 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.208	10.710	160.1E6	141.1E6	330.018	307.327
Target Compounds							
2) T	3,5-DICHL...	0.000	8.958	0	125.4E6	N.D.	219.425
3) T	4-Nitroph...	10.838	9.921	14309231	11465050	56.649	47.809
6) T	MCP	11.879	0.000	12430357	0	9.522	N.D. #
8) T	DICHLORPROP	0.000	12.216	0	110195	N.D.	<MDL
9) T	2,4-D	13.185	0.000	14059753	0	30.878	N.D. #
10) T	Pentachlo...	0.000	13.197	0	1629755	N.D.	<MDL
11) T	2,4,5-TP ...	14.316	0.000	1303191	0	<MDL	N.D. #
12) T	2,4,5-T	0.000	14.389	0	8402547	N.D.	3.643
14) T	DINOSEB	16.981	0.000	3942184	0	1.573	N.D. #
15) T	Picloram	16.687	0.000	4477101	0	1.248	N.D. #
16) T	DCPA	17.228	0.000	8666828	0	2.408	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS042319\
Data File : PS004247.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Apr 2019 09:06
Operator : EI\SJ
Sample : K2515-16
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
TP-12

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 24 10:50:00 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS041119.M
Quant Title : 8080.M
QLast Update : Thu Apr 11 14:18:42 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

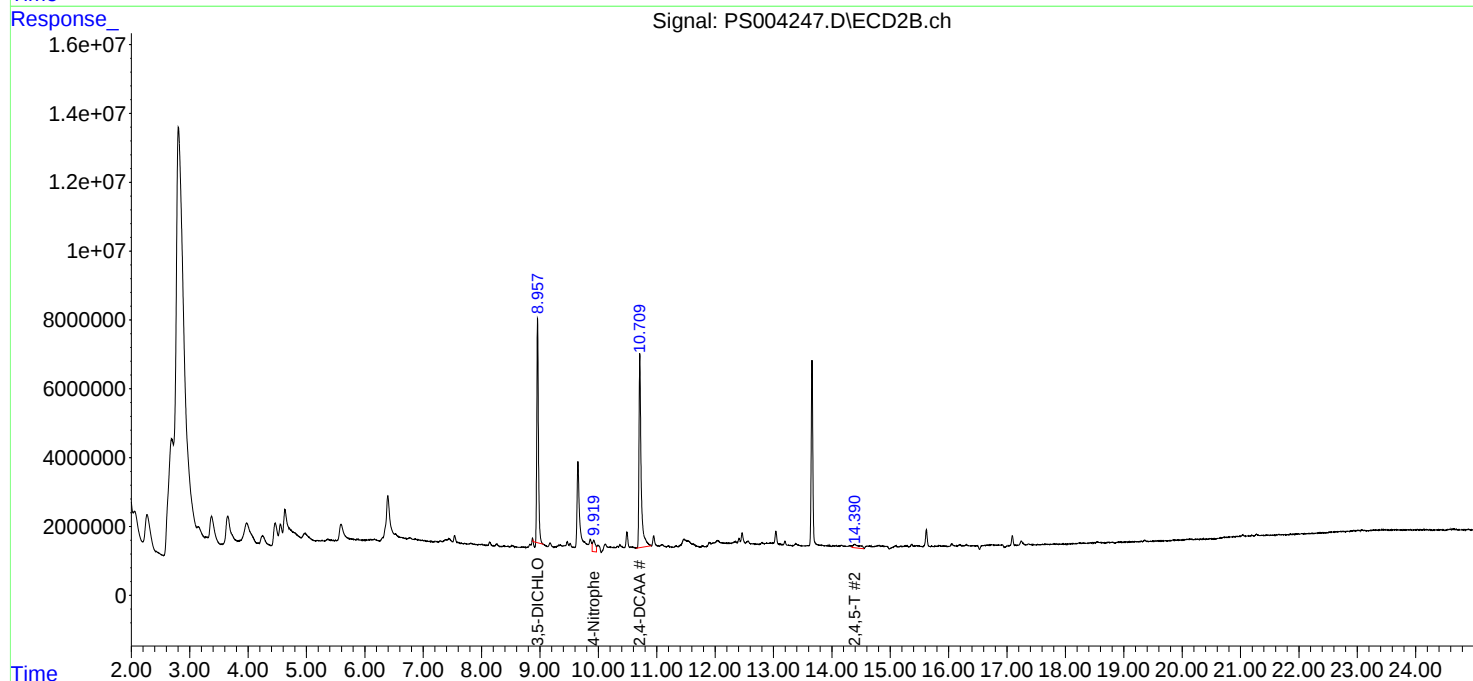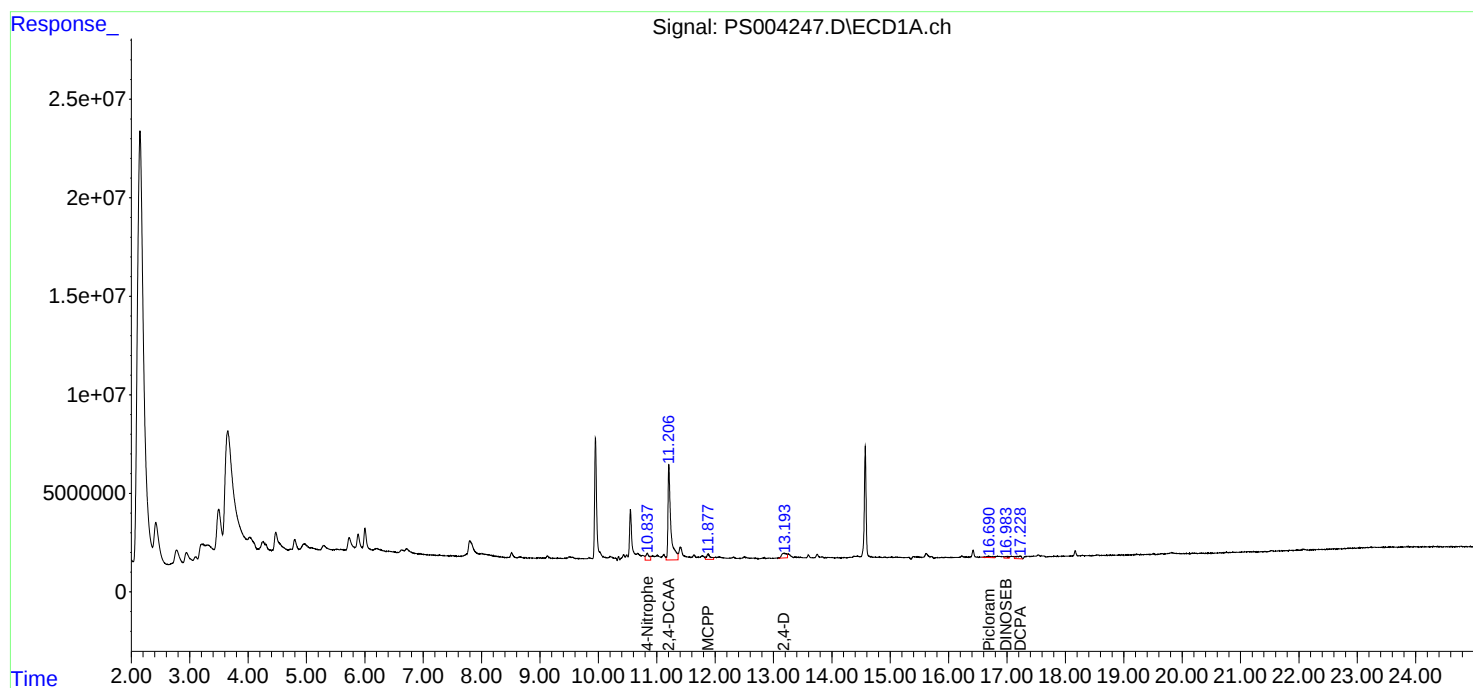


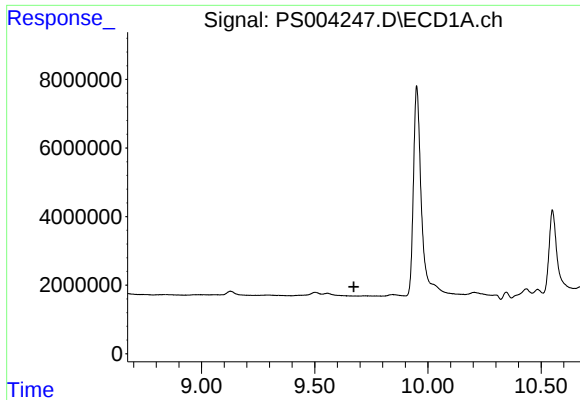

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 9.673 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
TP-12

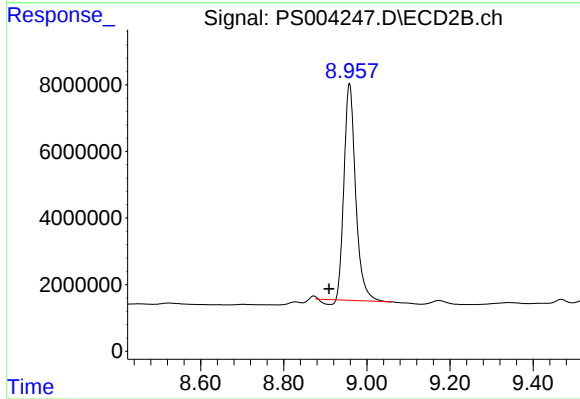


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 8.958 min
Delta R.T.: 0.049 min
Response: 125428724
Conc: 219.42 ng/ml

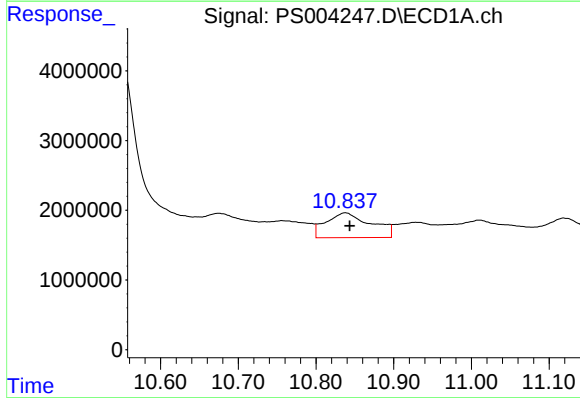


#3 4-Nitrophenol

R.T.: 10.838 min
Delta R.T.: -0.006 min
Response: 14309231
Conc: 56.65 ng/ml

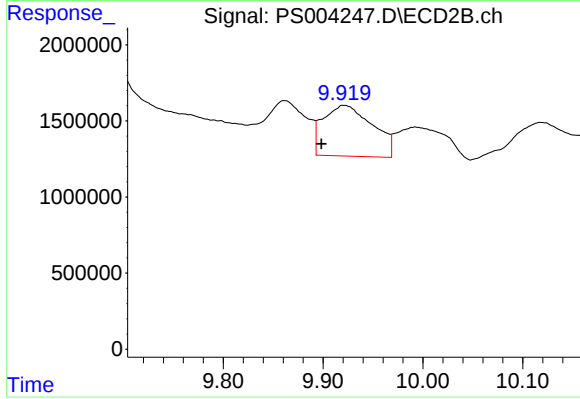

#3 4-Nitrophenol


R.T.: 9.921 min
Delta R.T.: 0.023 min
Response: 11465050
Conc: 47.81 ng/ml

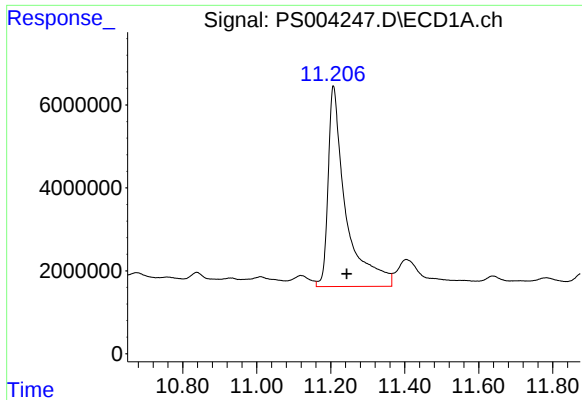

#4 2,4-DCAA


R.T.: 11.208 min
Delta R.T.: -0.035 min
Response: 160129636
Conc: 330.02 ng/ml

Instrument :
ECD_S
ClientSampleId :
TP-12

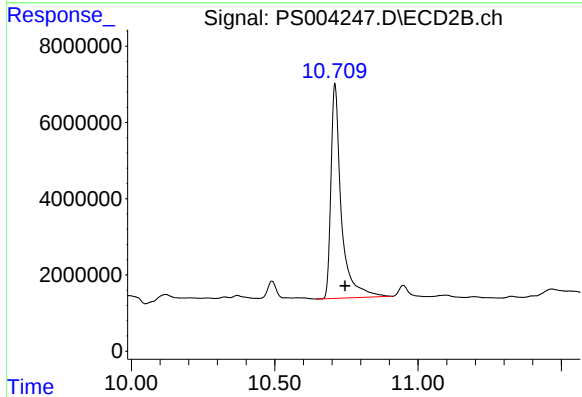


#4 2,4-DCAA

R.T.: 10.710 min
Delta R.T.: -0.036 min
Response: 141137560
Conc: 307.33 ng/ml

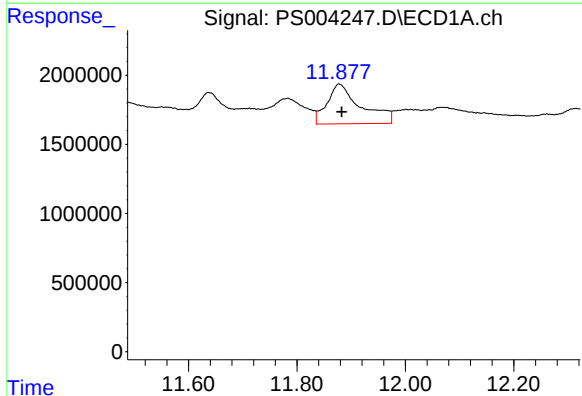


#6 MCP

R.T.: 11.879 min
Delta R.T.: -0.004 min
Response: 12430357
Conc: 9.52 ug/ml

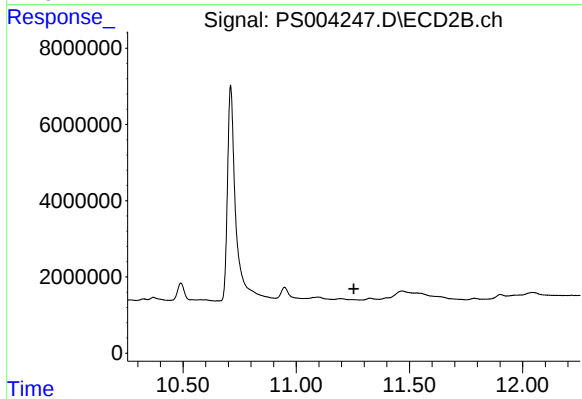

#6 MCP


R.T.: 0.000 min
Exp R.T.: 11.255 min
Response: 0
Conc: N.D.

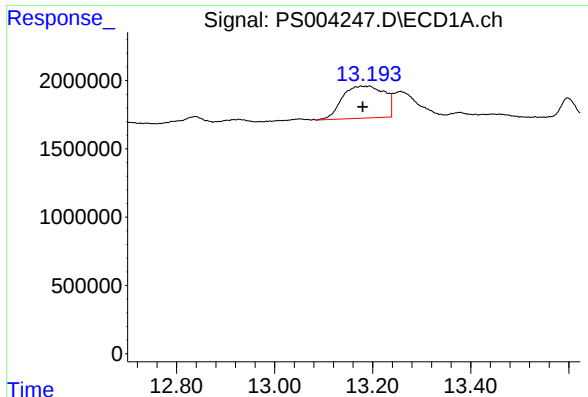

#9 2,4-D


R.T.: 13.185 min
Delta R.T.: 0.005 min
Response: 14059753
Conc: 30.88 ng/ml

Instrument :
ECD_S
ClientSampleId :
TP-12

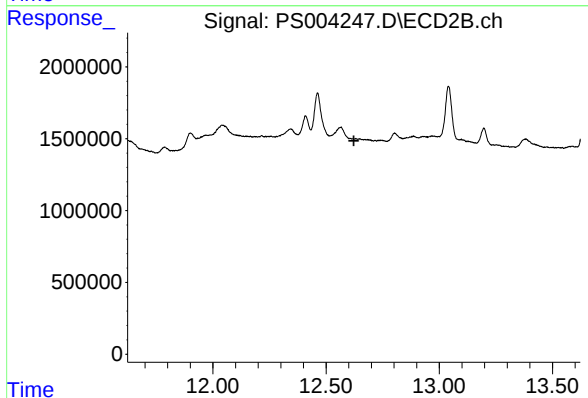


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 12.623 min
Response: 0
Conc: N.D.

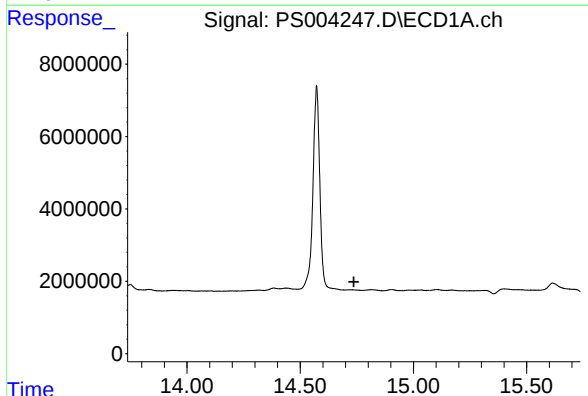


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 14.737 min
Response: 0
Conc: N.D.

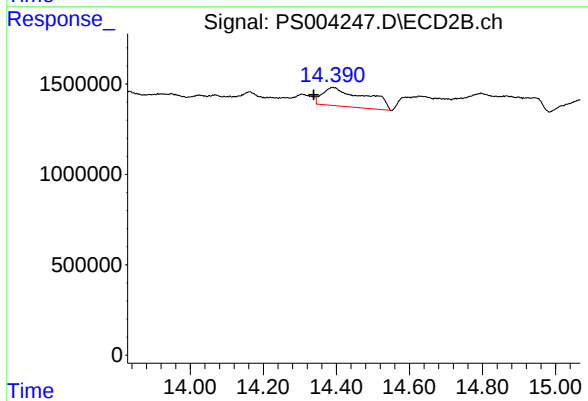

#12 2,4,5-T


R.T.: 14.389 min
Delta R.T.: 0.051 min
Response: 8402547
Conc: 3.64 ng/ml

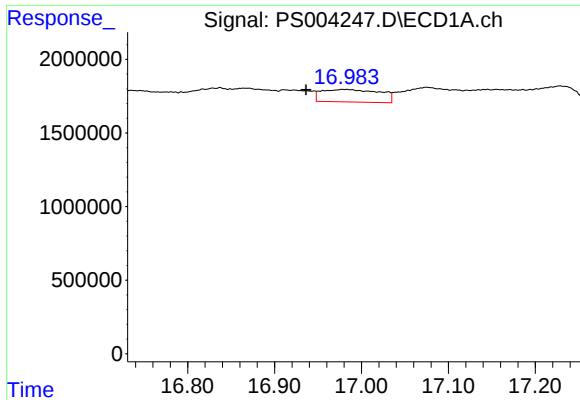

#14 DINOSEB


R.T.: 16.981 min
Delta R.T.: 0.045 min
Response: 3942184
Conc: 1.57 ng/ml

Instrument :
ECD_S
ClientSampleId :
TP-12

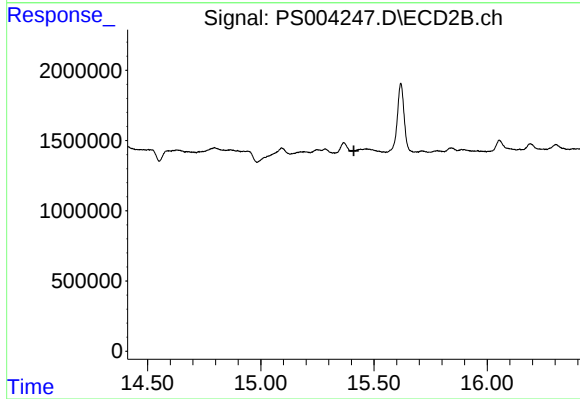


#14 DINOSEB

R.T.: 0.000 min
Exp R.T. : 15.411 min
Response: 0
Conc: N.D.

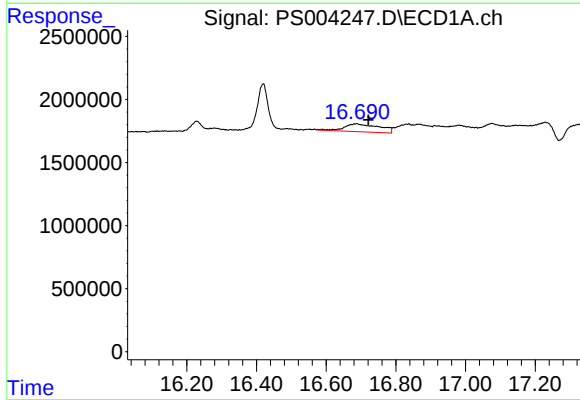


#15 Picloram

R.T.: 16.687 min
Delta R.T.: -0.034 min
Response: 4477101
Conc: 1.25 ng/ml

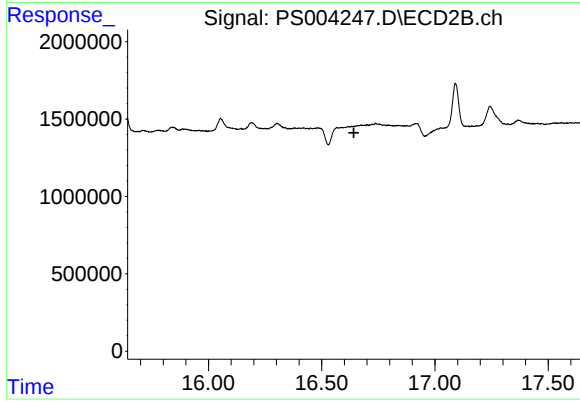

#15 Picloram


R.T.: 0.000 min
Exp R.T. : 16.642 min
Response: 0
Conc: N.D.

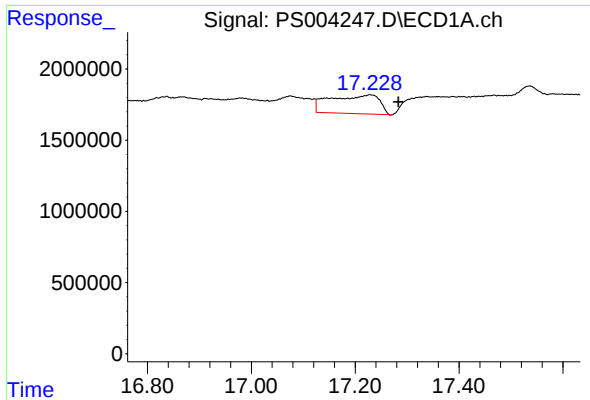

#16 DCPA

R.T.: 17.228 min
Delta R.T.: -0.055 min
Response: 8666828
Conc: 2.41 ng/ml

Instrument :
ECD_S
ClientSampleId :
TP-12

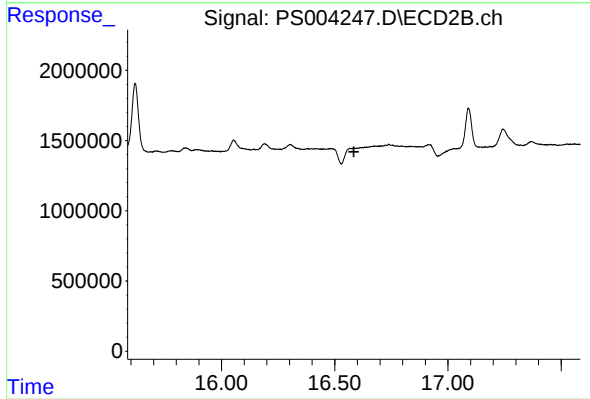

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 16.584 min
Response: 0
Conc: N.D.