

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS042319\
 Data File : PS004223.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Apr 2019 19:04
 Operator : EI\SJ
 Sample : MDL-BL-WATER-06
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 MDL-BL-WATER-06

Manual Integrations
 APPROVED

Sohil
 4/26/2019 5:48:02 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 24 01:32:50 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS041119.M
 Quant Title : 8080.M
 QLast Update : Thu Apr 11 14:18:42 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

4) S	2,4-DCAA	11.245	10.719	180.1E6	160.4E6	371.207m 349.166m
------	----------	--------	--------	---------	---------	-------------------

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS042319\
Data File : PS004223.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Apr 2019 19:04
Operator : EI\SJ
Sample : MDL-BL-WATER-06
Misc :
ALS Vial : 8 Sample Multiplier: 1



Instrument :
ECD_S
ClientSampleId :
MDL-BL-WATER-06


Manual Integrations
APPROVED

Sohil
4/26/2019 5:48:02 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 24 01:32:50 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS041119.M
Quant Title : 8080.M
QLast Update : Thu Apr 11 14:18:42 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

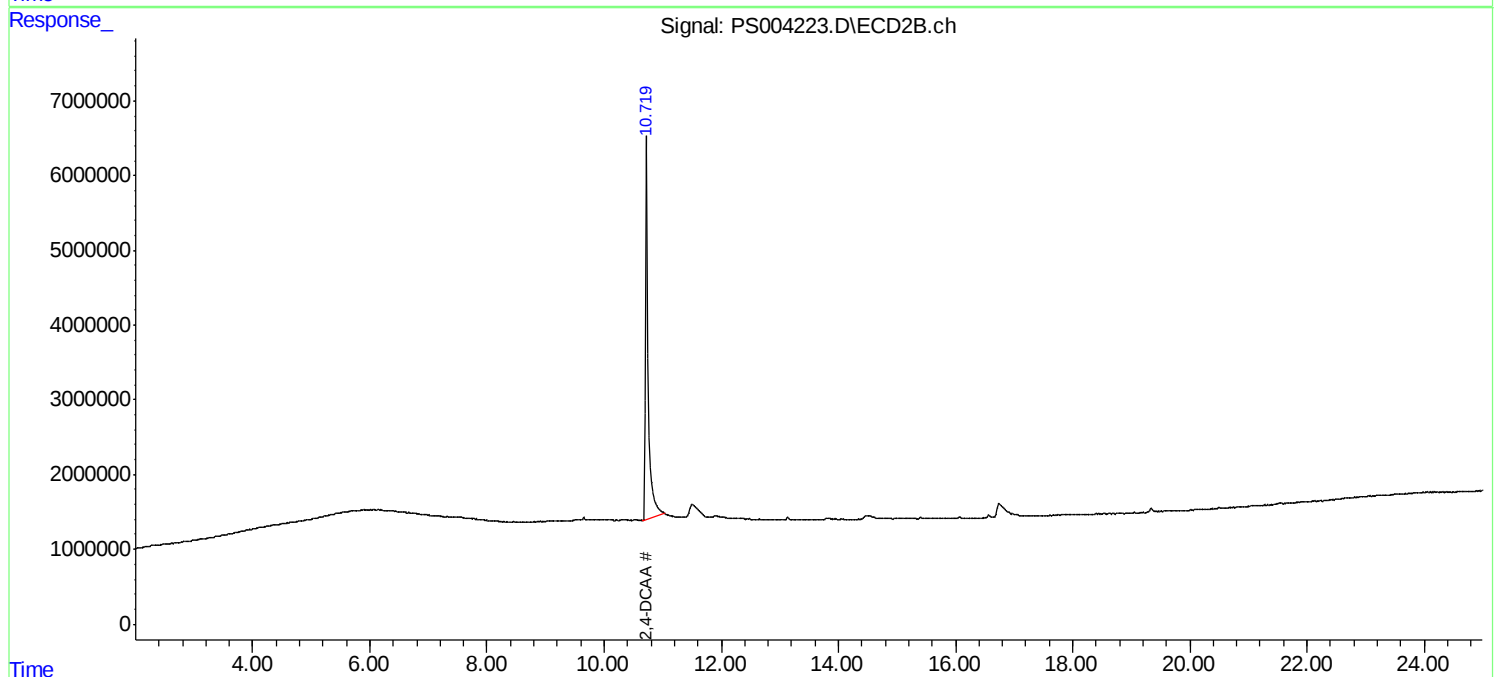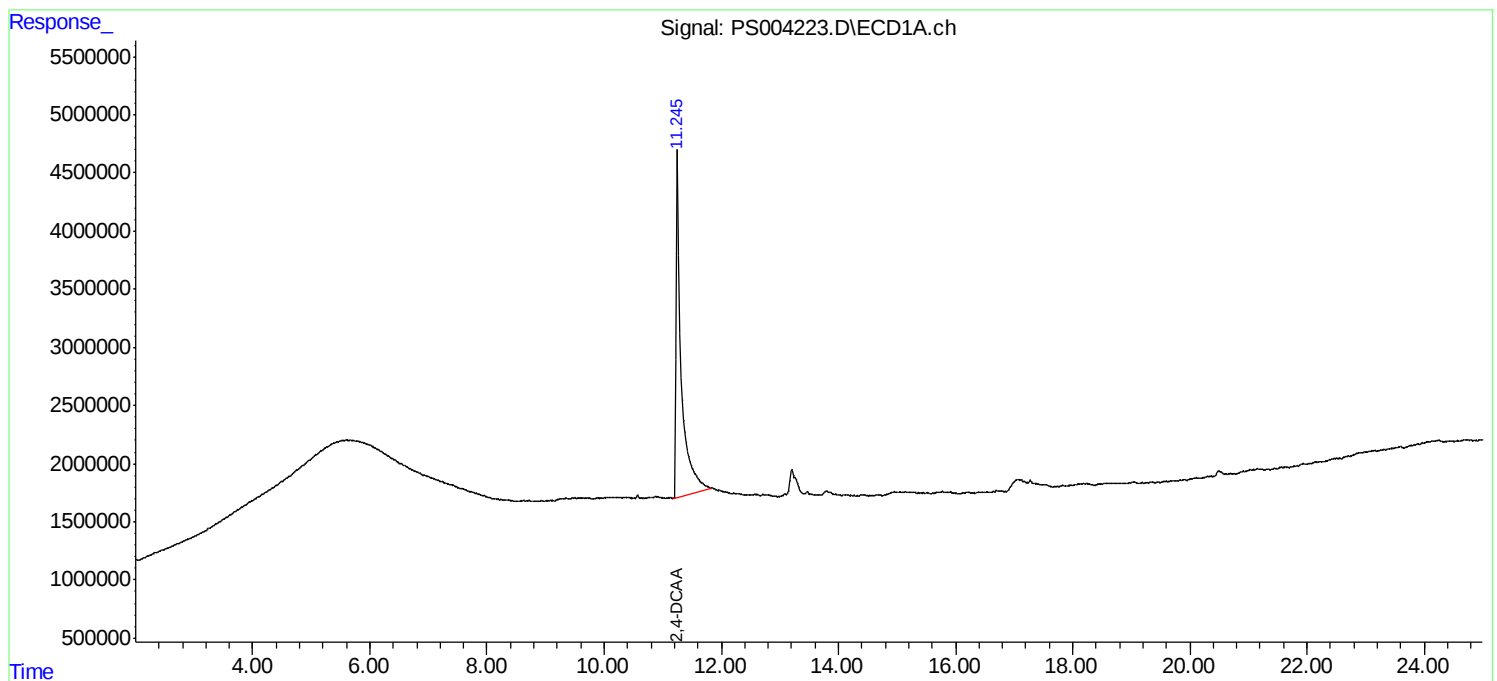

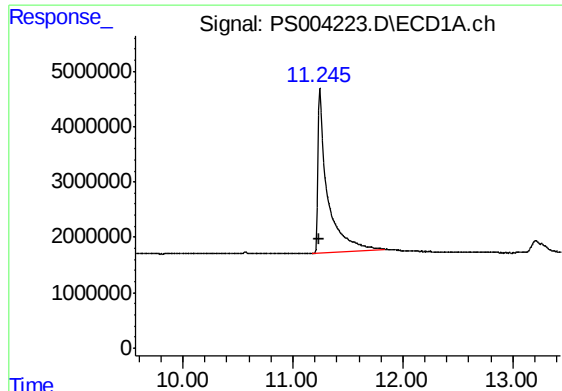


#4 2,4-DCAA

R.T.: 11.245 min
Delta R.T.: 0.002 min
Response: 180114971
Conc: 371.21 ng/ml m

Instrument :
ECD_S
ClientSampleId :
MDL-BL-WATER-06

Manual Integrations
APPROVED

Sohil
4/26/2019 5:48:02 PM

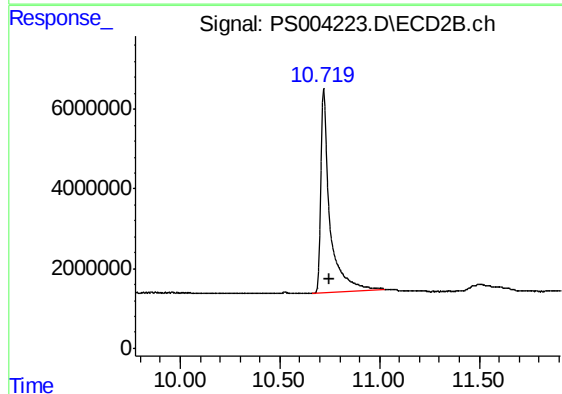

#4 2,4-DCAA

R.T.: 10.719 min
Delta R.T.: -0.027 min
Response: 160351721
Conc: 349.17 ng/ml m