

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS042321\
 Data File : PS014773.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Apr 2021 07:59
 Operator : DD\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 23 10:27:02 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS040821.M
 Quant Title : 8080.M
 QLast Update : Thu Apr 08 14:34:06 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds							
2) T	3,5-DICHL...	6.427f	0.000	9549852	0	4.609	N.D. #
5) T	DICAMBA	0.000	7.117f	0	5182317	N.D.	2.562
6) T	MCP	0.000	7.117	0	5182317	N.D.	3.077
8) T	DICHLORPROP	0.000	7.705	0	2592443	N.D.	5.135
13) T	2,4-DB	0.000	9.585f	0	3209139	N.D.	9.252
15) T	Picloram	10.938	10.969	42973250	17012266	3.841	4.537



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS042321\
Data File : PS014773.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Apr 2021 07:59
Operator : DD\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 23 10:27:02 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS040821.M
Quant Title : 8080.M
QLast Update : Thu Apr 08 14:34:06 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

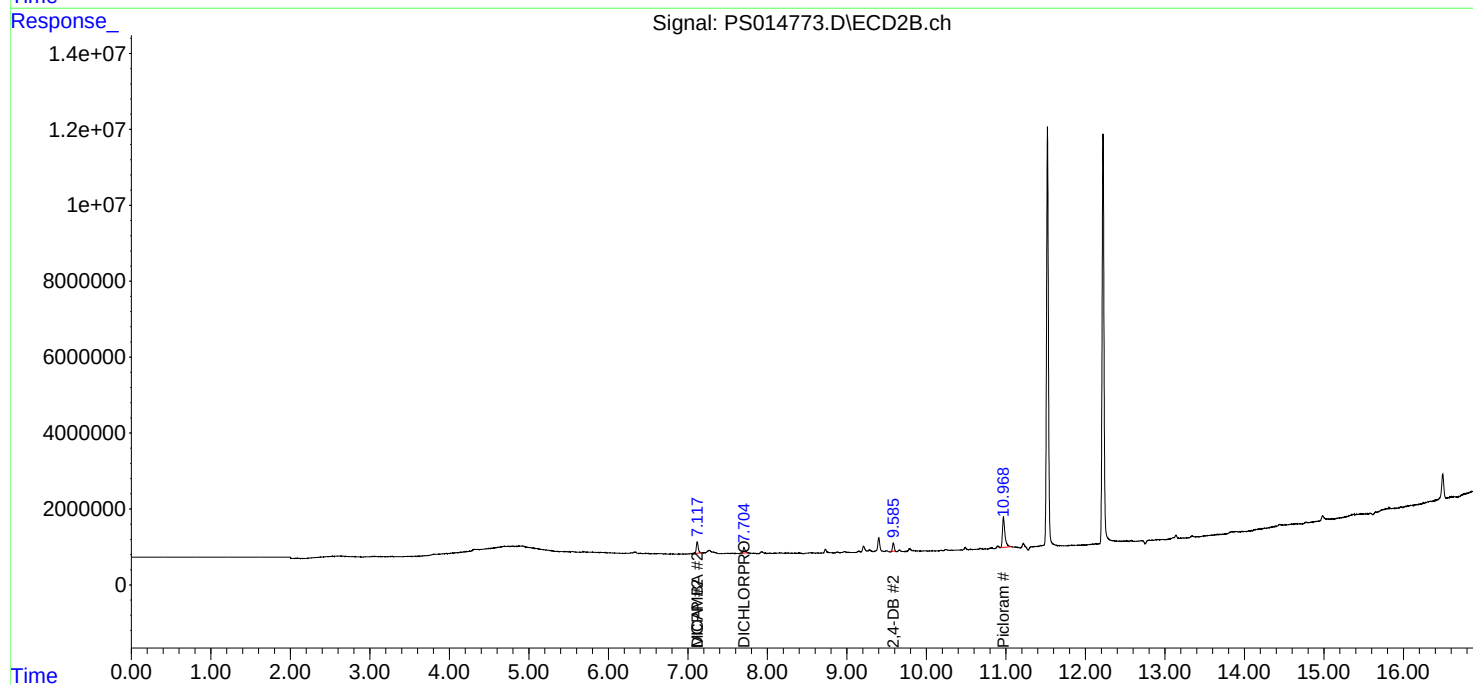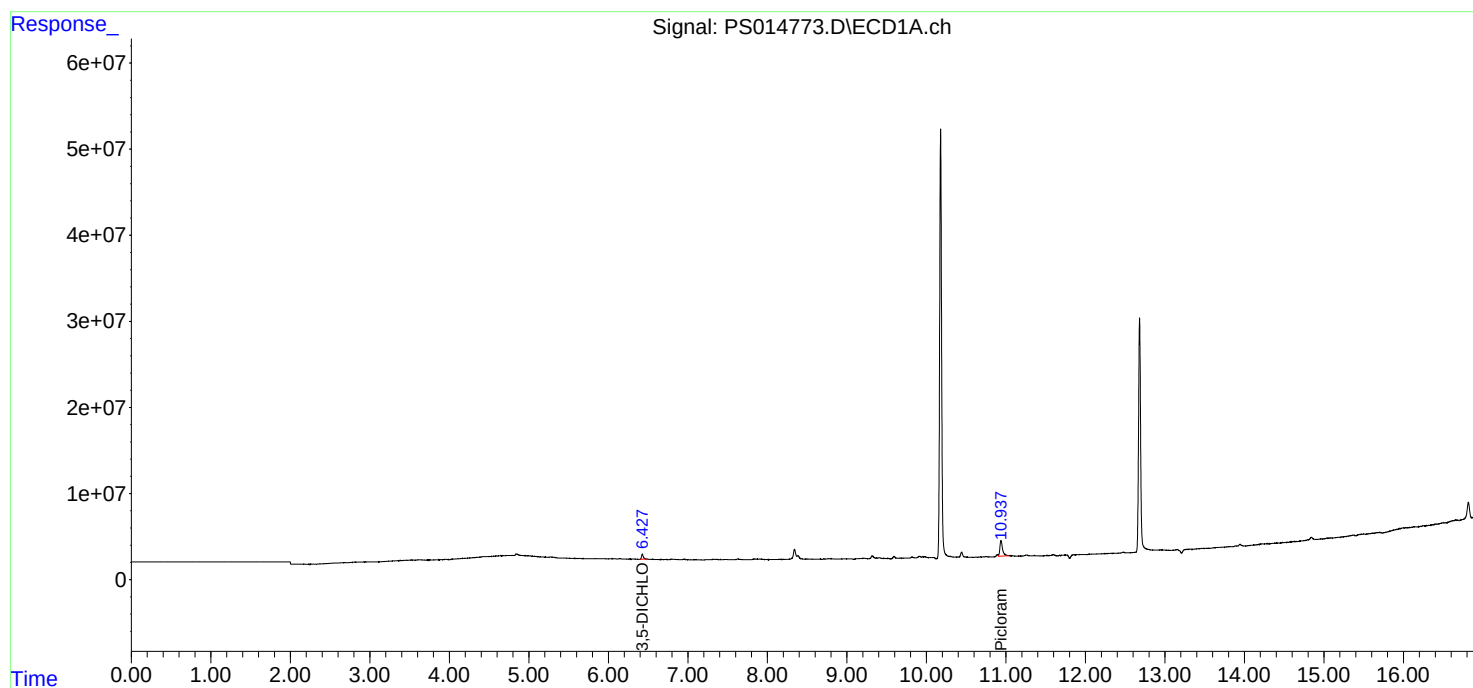


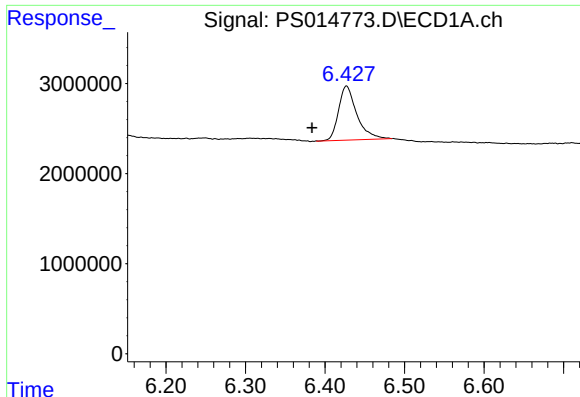

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.427 min
Delta R.T.: 0.043 min
Response: 9549852
Conc: 4.61 ng/ml

Instrument :
ECD_S
ClientSampleId :

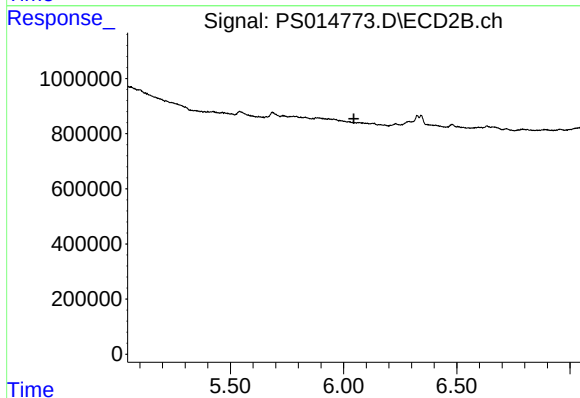


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.045 min
Response: 0
Conc: N.D.

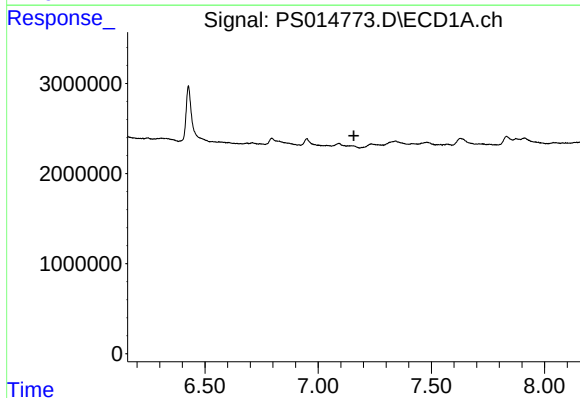


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T. : 7.158 min
Response: 0
Conc: N.D.

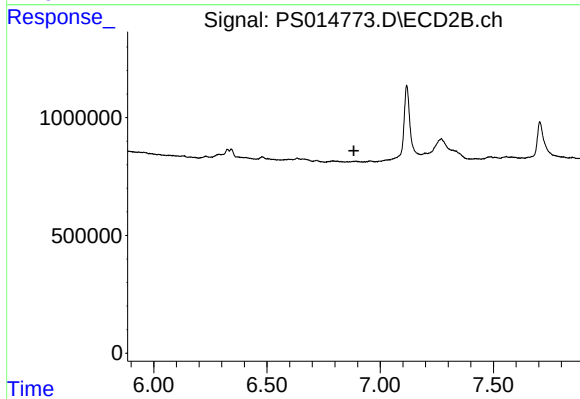

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T. : 6.884 min
Response: 0
Conc: N.D.

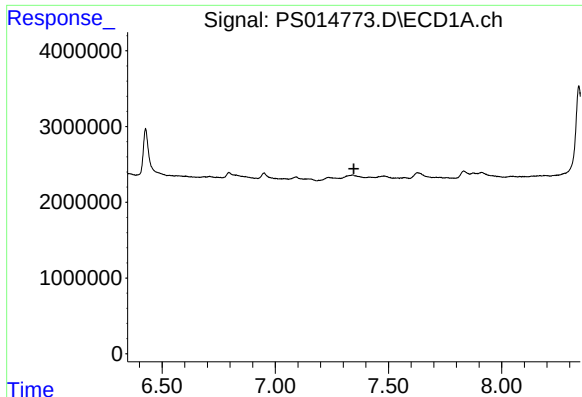

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 7.347 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

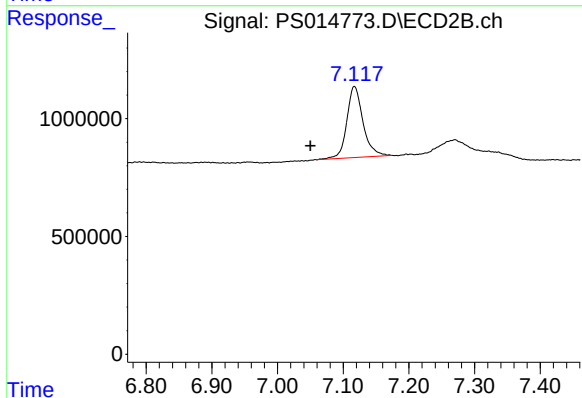


#5 DICAMBA

R.T.: 7.117 min
Delta R.T.: 0.067 min
Response: 5182317
Conc: 2.56 ng/ml

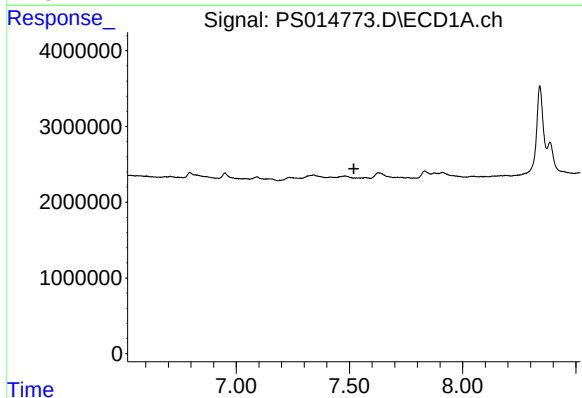


#6 MCP

R.T.: 0.000 min
Exp R.T.: 7.520 min
Response: 0
Conc: N.D.

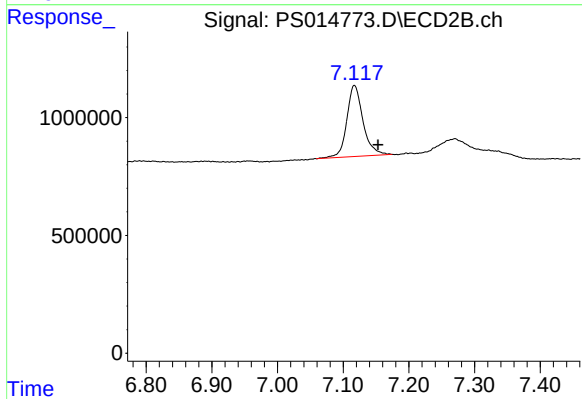

#6 MCP


R.T.: 7.117 min
Delta R.T.: -0.036 min
Response: 5182317
Conc: 3.08 ug/ml

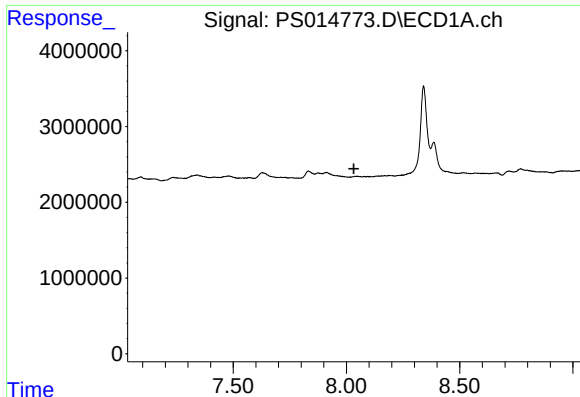

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 8.033 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

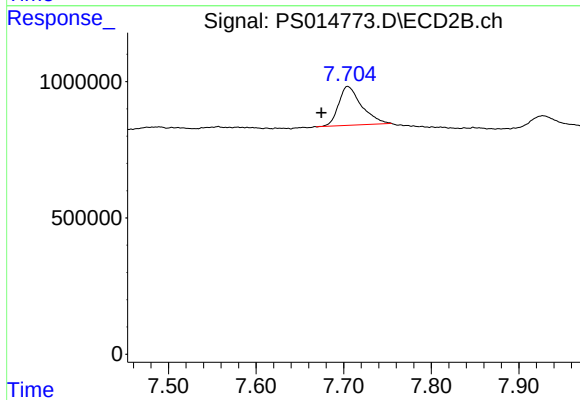


#8 DICHLORPROP

R.T.: 7.705 min
Delta R.T.: 0.030 min
Response: 2592443
Conc: 5.14 ng/ml

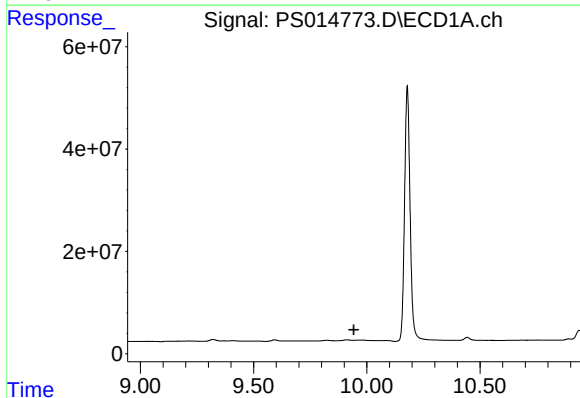


#13 2,4-DB

R.T.: 0.000 min
Exp R.T.: 9.943 min
Response: 0
Conc: N.D.

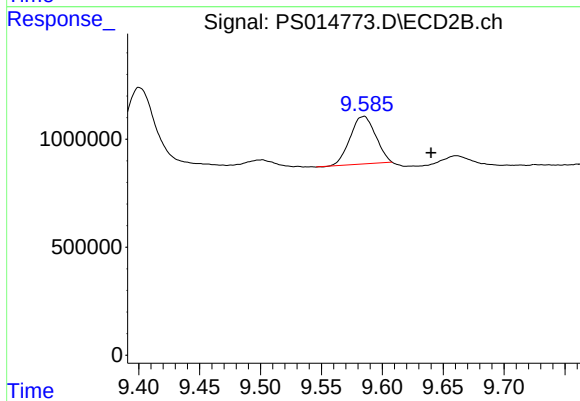

#13 2,4-DB


R.T.: 9.585 min
Delta R.T.: -0.055 min
Response: 3209139
Conc: 9.25 ng/ml

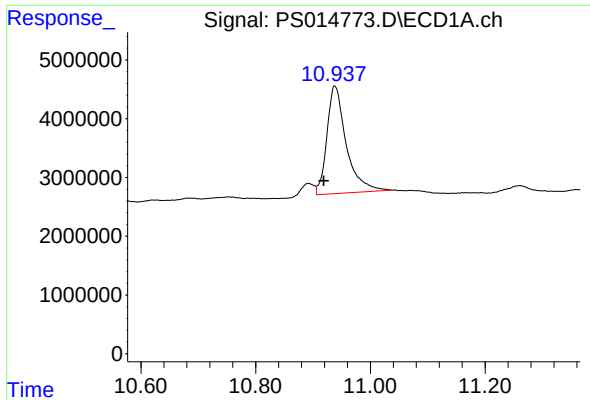

#15 Picloram

R.T.: 10.938 min
Delta R.T.: 0.019 min
Response: 42973250
Conc: 3.84 ng/ml

Instrument :
ECD_S
ClientSampleId :

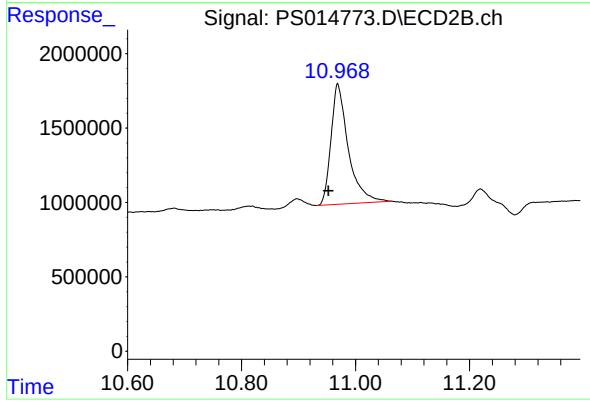

#15 Picloram

R.T.: 10.969 min
Delta R.T.: 0.016 min
Response: 17012266
Conc: 4.54 ng/ml