

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS042321\
 Data File : PS014778.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Apr 2021 13:36
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 23 16:45:26 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS040821.M
 Quant Title : 8080.M
 QLast Update : Thu Apr 08 14:34:06 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.157	6.882	718.9E6	248.3E6	472.590	533.444
Target Compounds							
2) T	3,5-DICHL...	6.424	0.000	7867686	0	3.797	N.D. #
5) T	DICAMBA	0.000	7.114f	0	4091386	N.D.	2.023
6) T	MCP	0.000	7.114	0	4091386	N.D.	2.429
7) T	MCPA	7.607f	0.000	6252927	0	1.005	N.D. #
8) T	DICHLORPROP	0.000	7.703	0	4468052	N.D.	8.851
9) T	2,4-D	8.237	0.000	5860082	0	3.686	N.D. #
11) T	2,4,5-TP ...	0.000	8.726	0	3327825	N.D.	1.218
12) T	2,4,5-T	0.000	9.204f	0	3160776	N.D.	1.208
13) T	2,4-DB	9.982	9.659	27856675	1991968	18.306	5.743 #
14) T	DINOSEB	11.030f	0.000	10794530	0	1.675	N.D. #
15) T	Picloram	10.935	10.967	63885252	17470309	5.710	4.659
16) T	DCPA	11.430f	10.967f	5259048	17470309	<MDL	4.302 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS042321\
Data File : PS014778.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Apr 2021 13:36
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 23 16:45:26 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS040821.M
Quant Title : 8080.M
QLast Update : Thu Apr 08 14:34:06 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

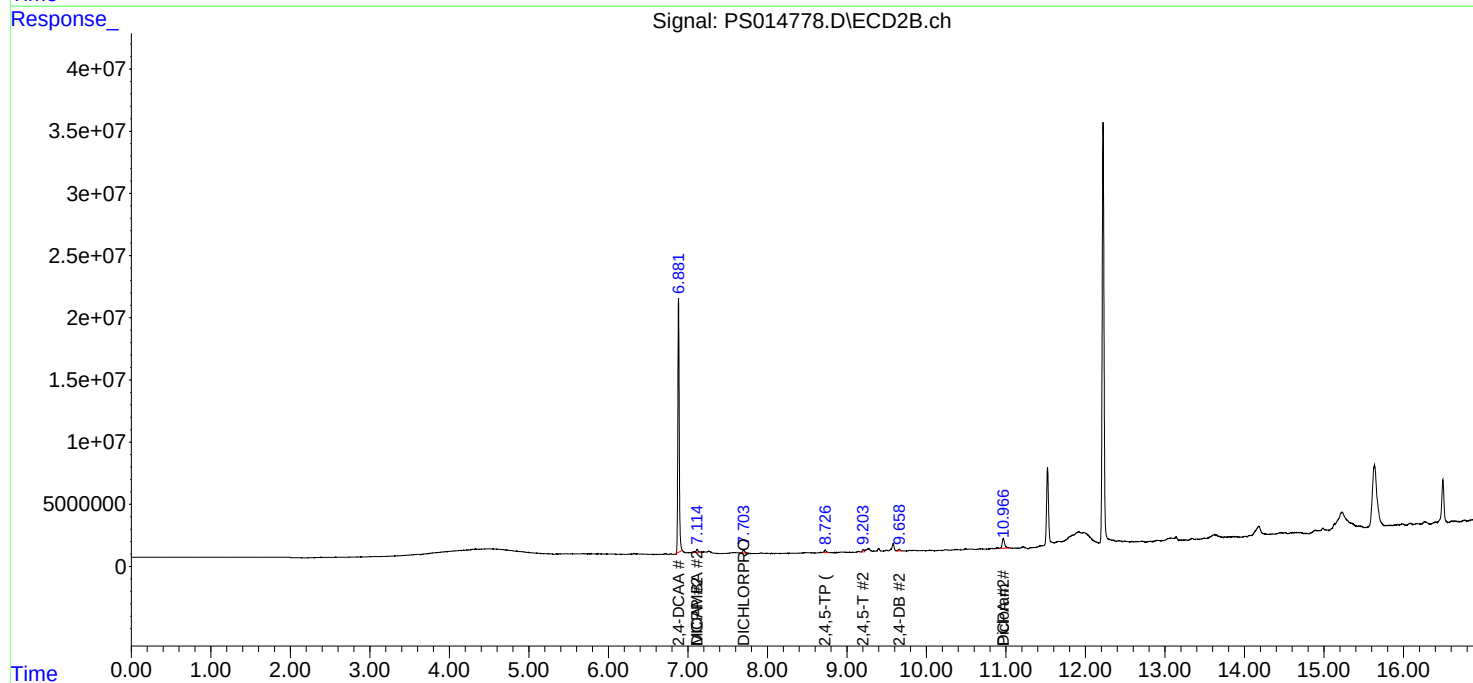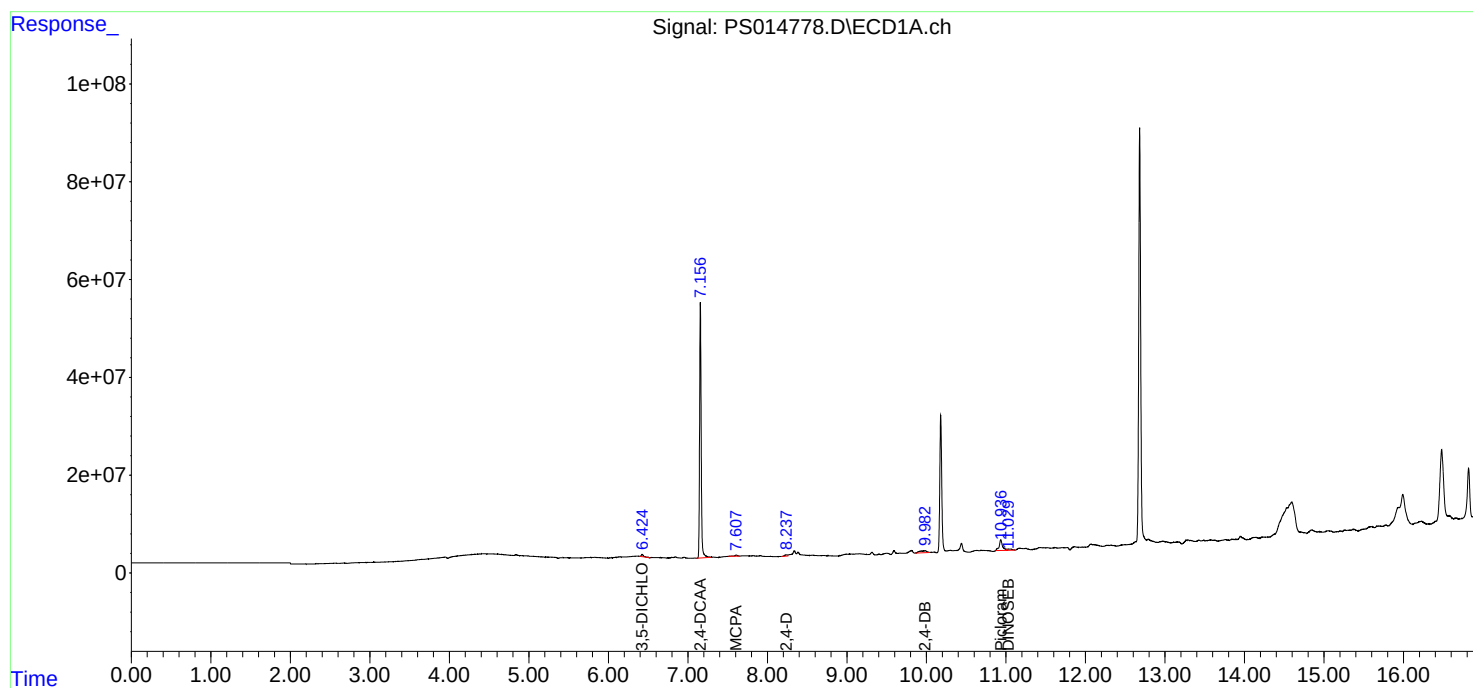


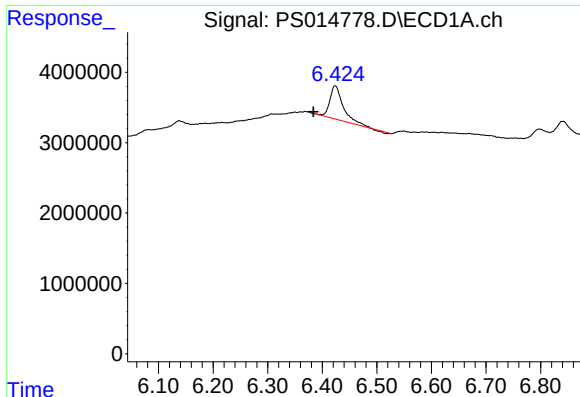

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.424 min
Delta R.T.: 0.040 min
Response: 7867686
Conc: 3.80 ng/ml

Instrument :
ECD_S
ClientSampleId :

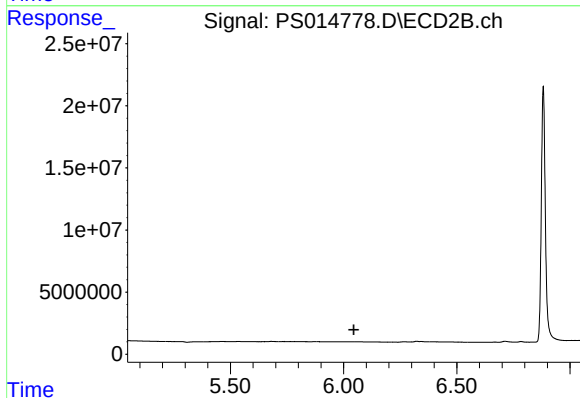


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.045 min
Response: 0
Conc: N.D.

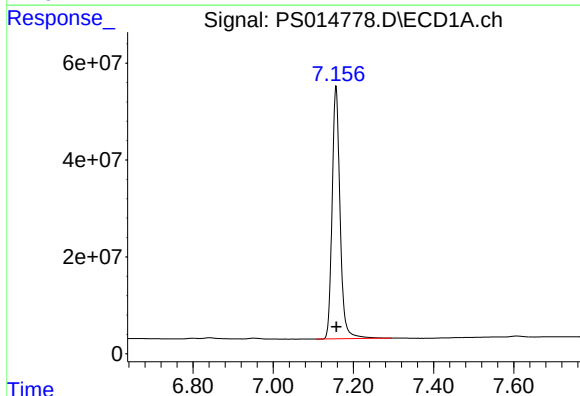


#4 2,4-DCAA

R.T.: 7.157 min
Delta R.T.: -0.001 min
Response: 718902179
Conc: 472.59 ng/ml

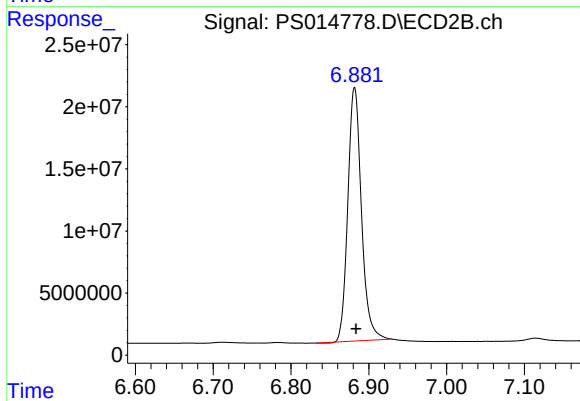

#4 2,4-DCAA


R.T.: 6.882 min
Delta R.T.: -0.002 min
Response: 248293887
Conc: 533.44 ng/ml

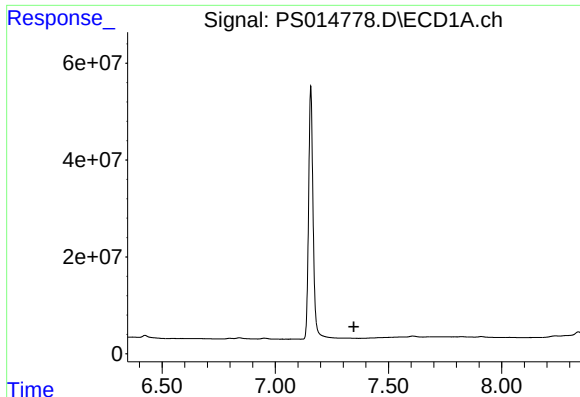

#5 DICAMBA


R.T.: 0.000 min
Exp R.T. : 7.347 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

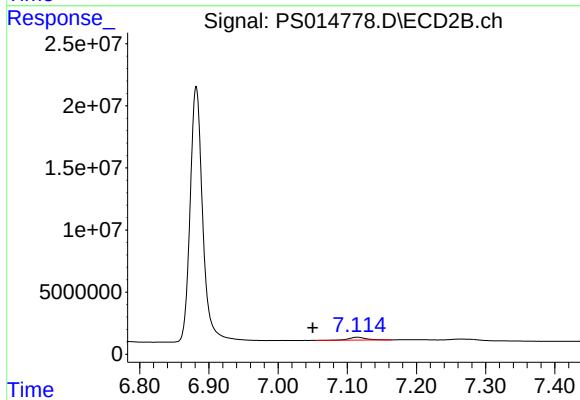


#5 DICAMBA

R.T.: 7.114 min
Delta R.T.: 0.064 min
Response: 4091386
Conc: 2.02 ng/ml

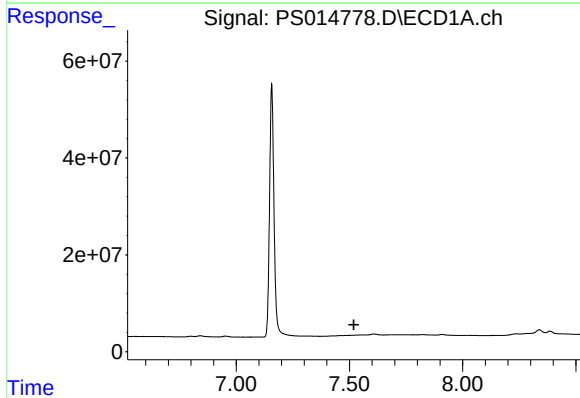


#6 MCP

R.T.: 0.000 min
Exp R.T. : 7.520 min
Response: 0
Conc: N.D.

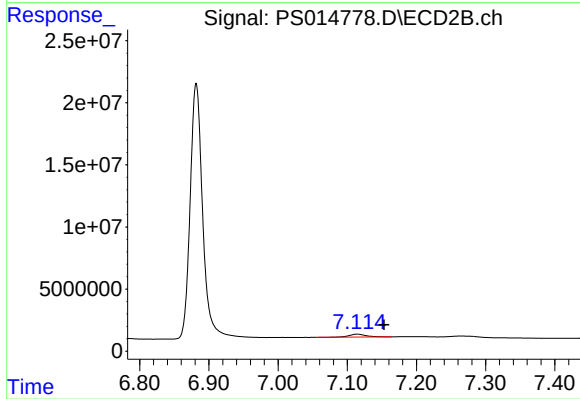

#6 MCP


R.T.: 7.114 min
Delta R.T.: -0.039 min
Response: 4091386
Conc: 2.43 ug/ml

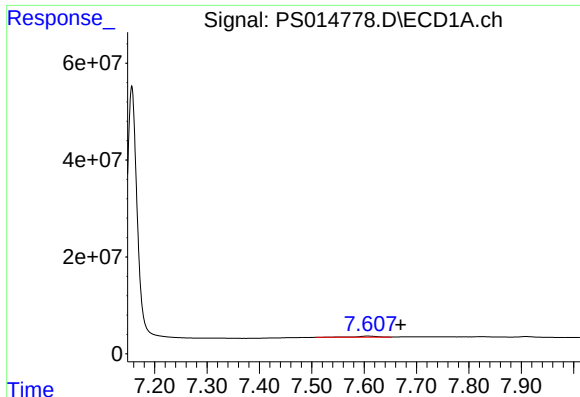

#7 MCPA


R.T.: 7.607 min
Delta R.T.: -0.063 min
Response: 6252927
Conc: 1.00 ug/ml

Instrument :
ECD_S
ClientSampleId :

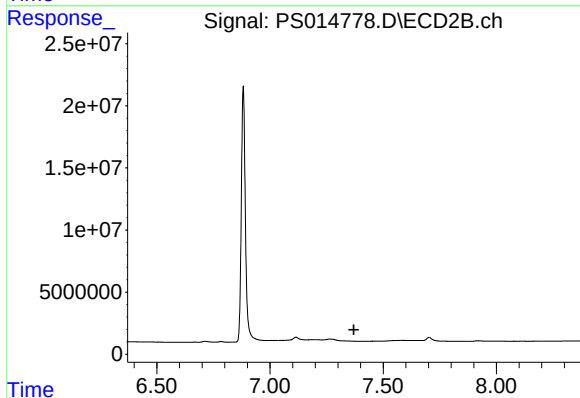


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 7.370 min
Response: 0
Conc: N.D.

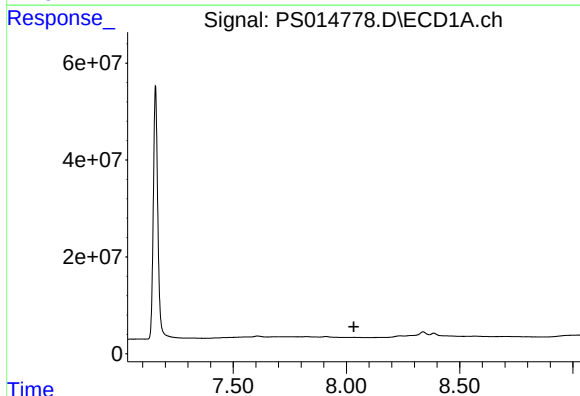


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 8.033 min
Response: 0
Conc: N.D.

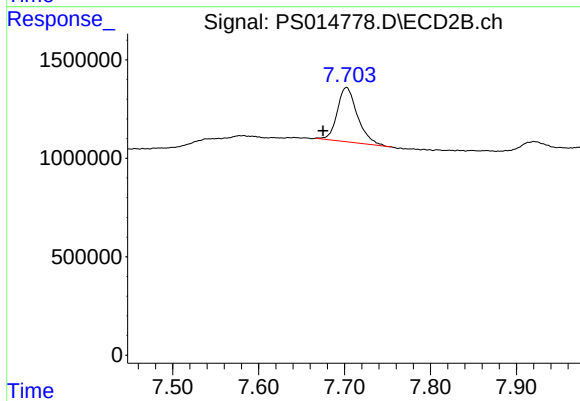

#8 DICHLORPROP


R.T.: 7.703 min
Delta R.T.: 0.028 min
Response: 4468052
Conc: 8.85 ng/ml

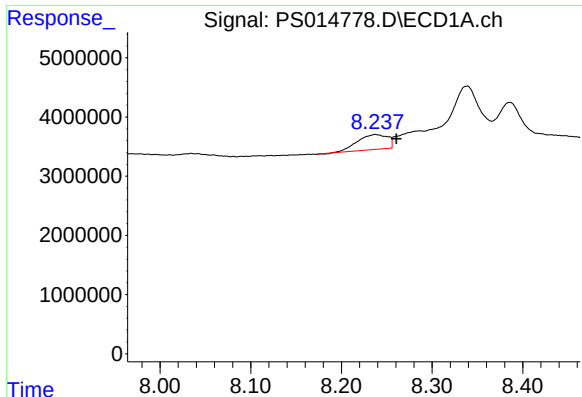

#9 2,4-D


R.T.: 8.237 min
Delta R.T.: -0.023 min
Response: 5860082
Conc: 3.69 ng/ml

Instrument :
ECD_S
ClientSampleId :

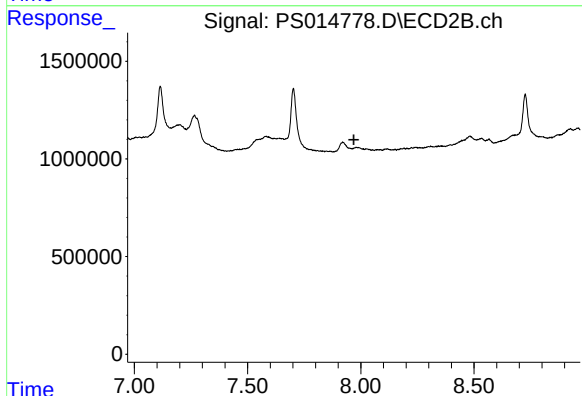


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 7.970 min
Response: 0
Conc: N.D.

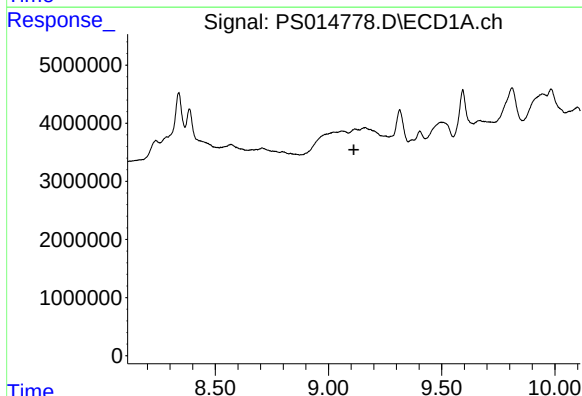


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T. : 9.112 min
Response: 0
Conc: N.D.

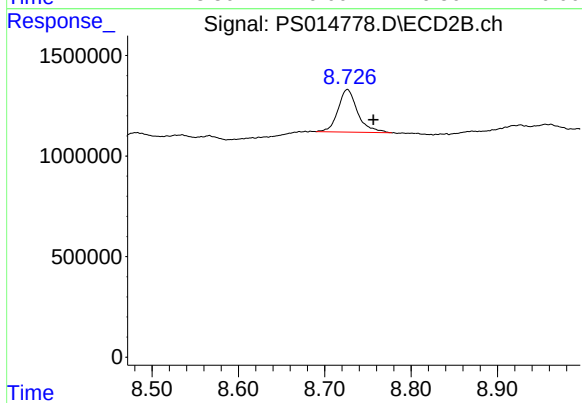

#11 2,4,5-TP (SILVEX)


R.T.: 8.726 min
Delta R.T.: -0.030 min
Response: 3327825
Conc: 1.22 ng/ml

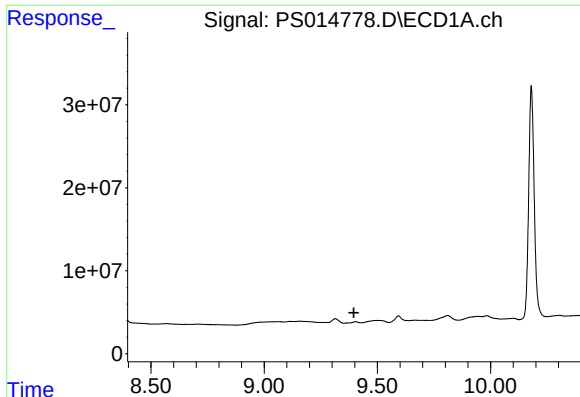

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 9.396 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

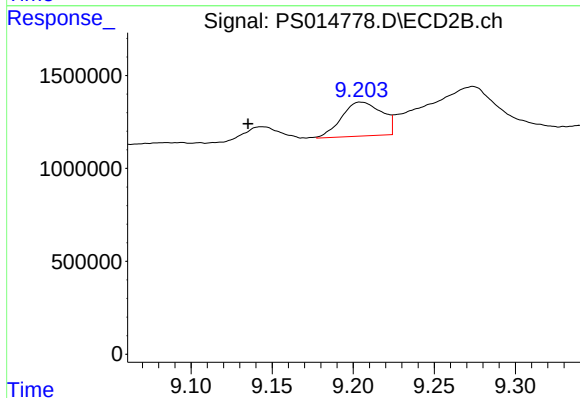


#12 2,4,5-T

R.T.: 9.204 min
Delta R.T.: 0.069 min
Response: 3160776
Conc: 1.21 ng/ml

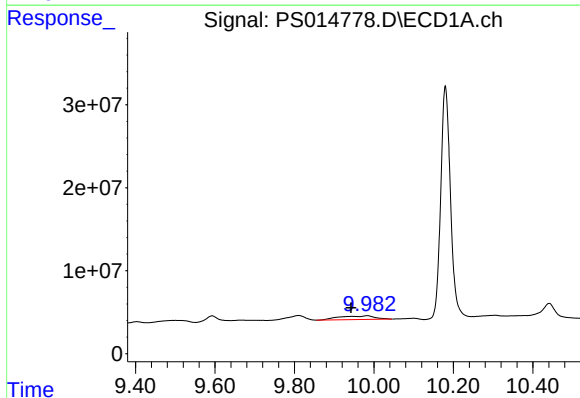


#13 2,4-DB

R.T.: 9.982 min
Delta R.T.: 0.040 min
Response: 27856675
Conc: 18.31 ng/ml

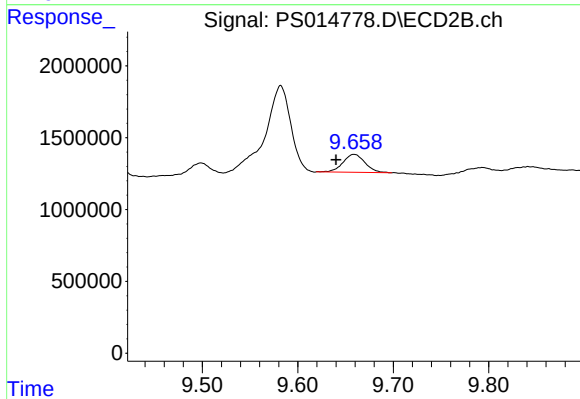

#13 2,4-DB


R.T.: 9.659 min
Delta R.T.: 0.019 min
Response: 1991968
Conc: 5.74 ng/ml

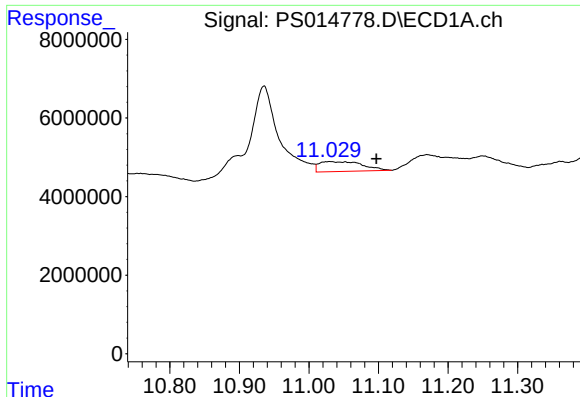

#14 DINOSEB


R.T.: 11.030 min
Delta R.T.: -0.067 min
Response: 10794530
Conc: 1.68 ng/ml

Instrument :
ECD_S
ClientSampleId :

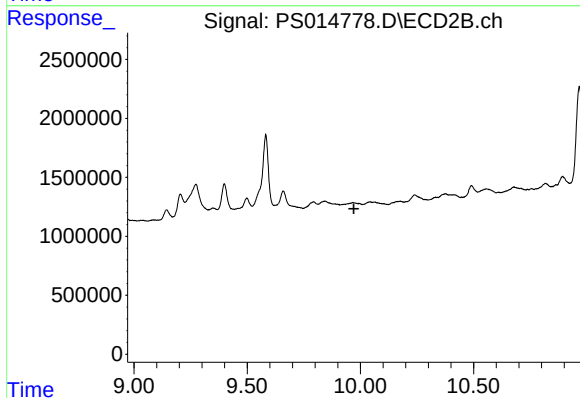


#14 DINOSEB

R.T.: 0.000 min
Exp R.T. : 9.971 min
Response: 0
Conc: N.D.

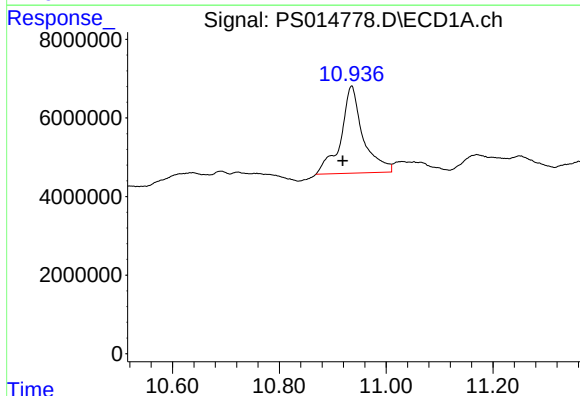


#15 Picloram

R.T.: 10.935 min
Delta R.T.: 0.016 min
Response: 63885252
Conc: 5.71 ng/ml

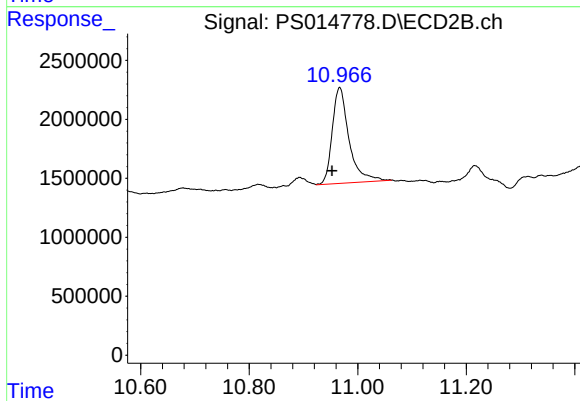

#15 Picloram


R.T.: 10.967 min
Delta R.T.: 0.014 min
Response: 17470309
Conc: 4.66 ng/ml

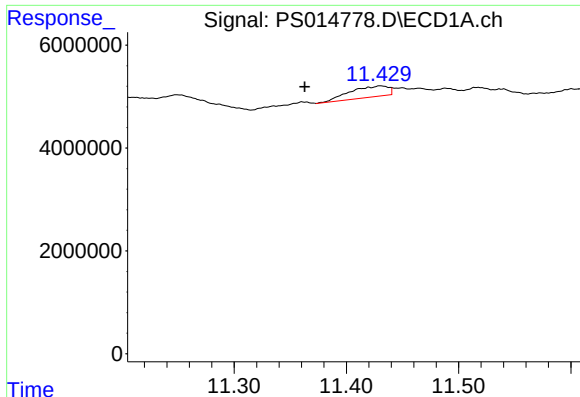

#16 DCPA

R.T.: 11.430 min
Delta R.T.: 0.067 min
Response: 5259048
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

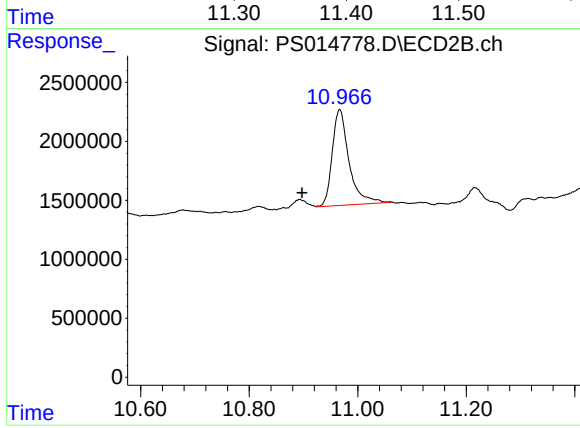

#16 DCPA

R.T.: 10.967 min
Delta R.T.: 0.069 min
Response: 17470309
Conc: 4.30 ng/ml