

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS042321\
 Data File : PS014784.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Apr 2021 18:26
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 23 18:43:01 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS040821.M
 Quant Title : 8080.M
 QLast Update : Thu Apr 08 14:34:06 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.157	6.883	741.6E6	254.6E6	487.523	547.072
Target Compounds							
2) T	3,5-DICHL...	6.426f	0.000	11128027	0	5.371	N.D. #
5) T	DICAMBA	0.000	7.117f	0	4489112	N.D.	2.220
6) T	MCP	0.000	7.117	0	4489112	N.D.	2.666
8) T	DICHLORPROP	0.000	7.703	0	6515561	N.D.	12.907
11) T	2,4,5-TP ...	0.000	8.729	0	3967806	N.D.	1.453
12) T	2,4,5-T	9.407	9.147	4234964	1908153	<MDL	<MDL #
13) T	2,4-DB	9.983f	9.660	24146807	2503763	15.868	7.218 #
15) T	Picloram	10.939	10.969	40310360	14533049	3.603	3.876
16) T	DCPA	11.430f	0.000	2578807	0	<MDL	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS042321\
Data File : PS014784.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Apr 2021 18:26
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 23 18:43:01 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS040821.M
Quant Title : 8080.M
QLast Update : Thu Apr 08 14:34:06 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

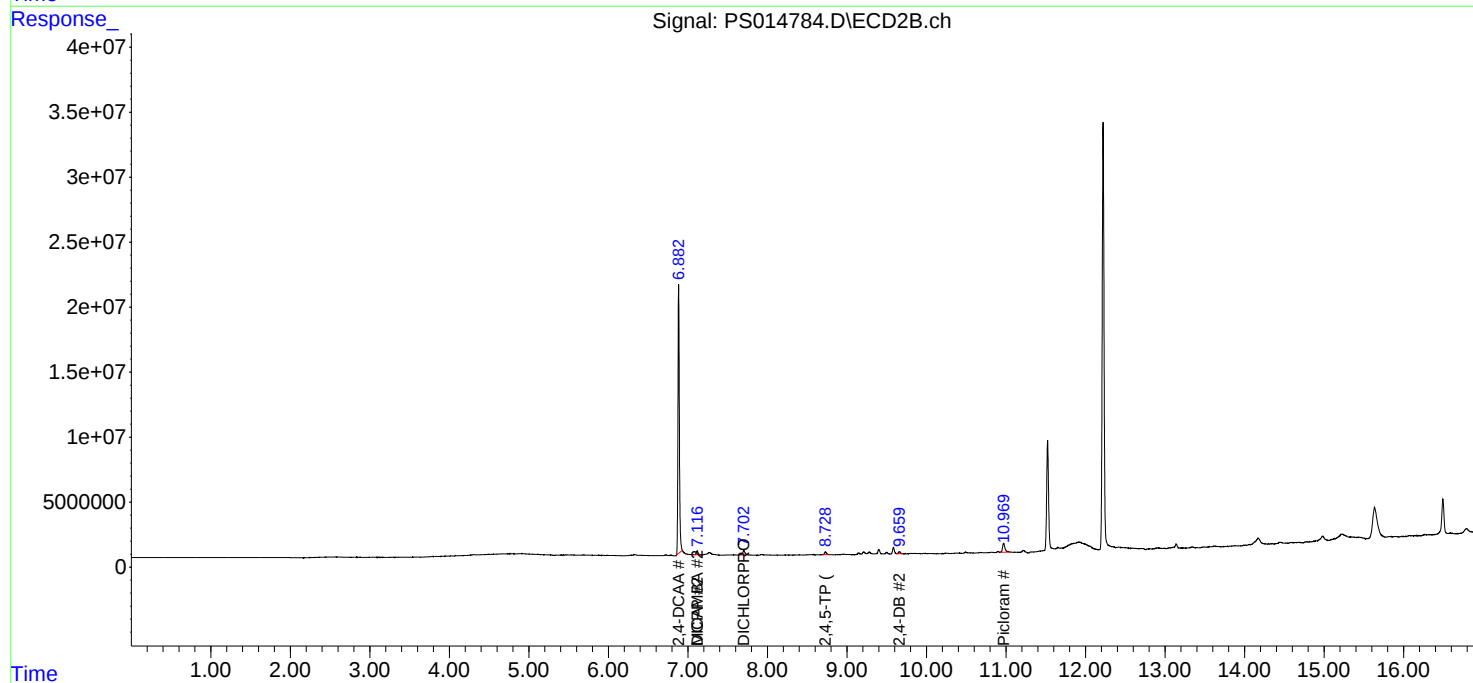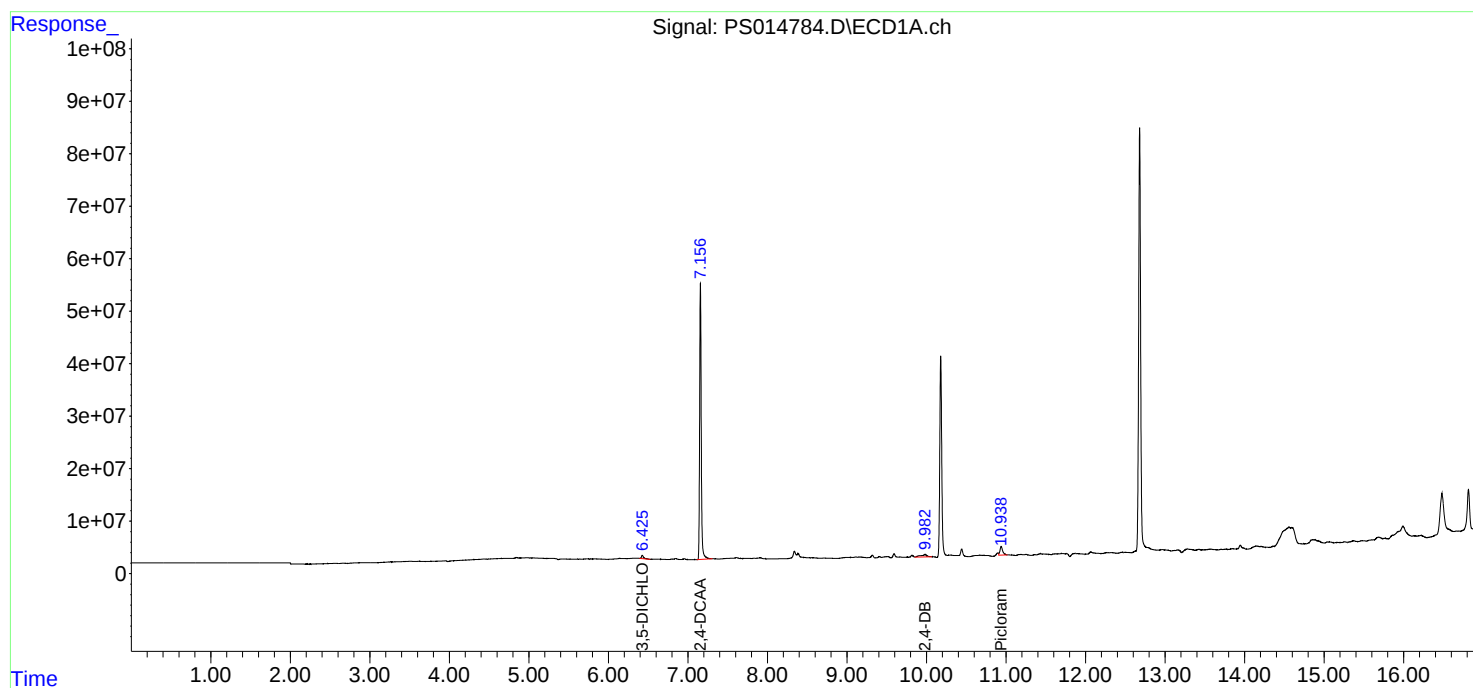


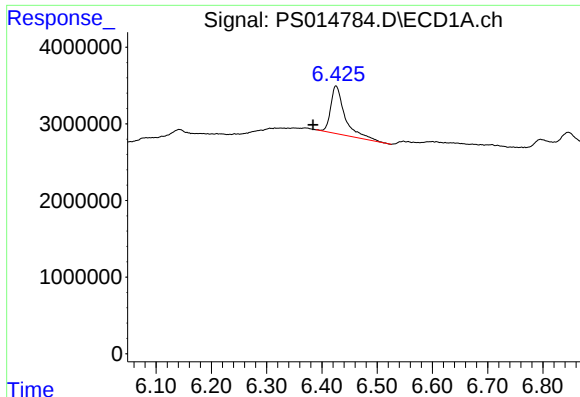

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.426 min
Delta R.T.: 0.042 min
Response: 11128027
Conc: 5.37 ng/ml

Instrument :
ECD_S
ClientSampleId :

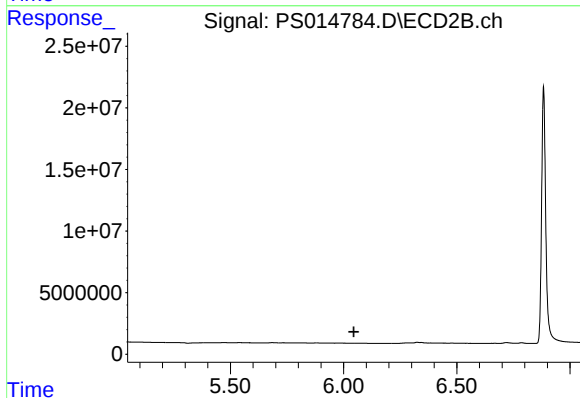


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.045 min
Response: 0
Conc: N.D.

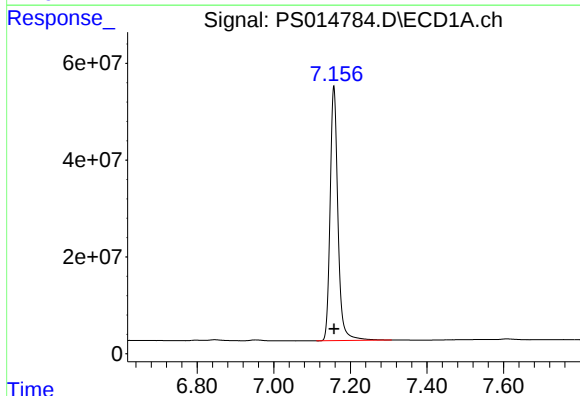


#4 2,4-DCAA

R.T.: 7.157 min
Delta R.T.: -0.001 min
Response: 741617396
Conc: 487.52 ng/ml

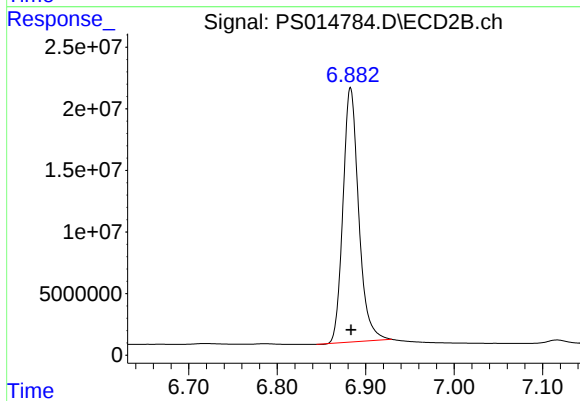

#4 2,4-DCAA


R.T.: 6.883 min
Delta R.T.: 0.000 min
Response: 254637102
Conc: 547.07 ng/ml

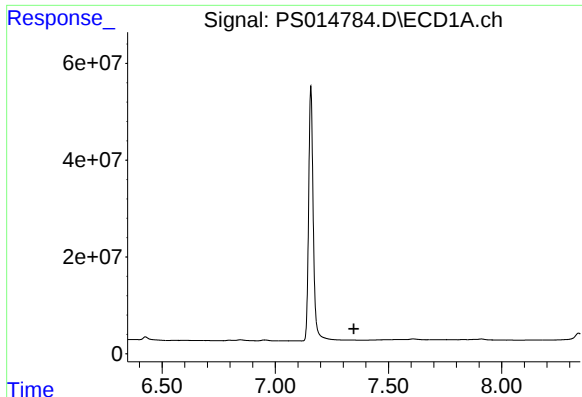

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 7.347 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

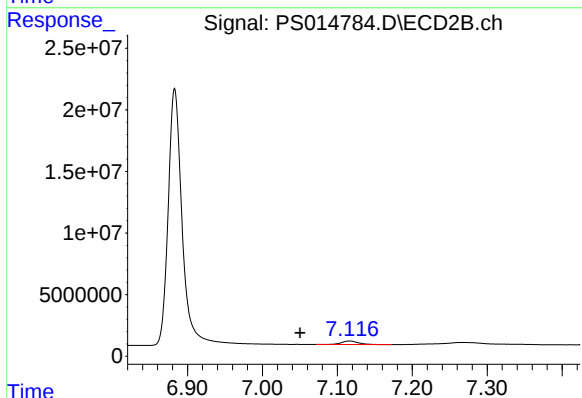


#5 DICAMBA

R.T.: 7.117 min
Delta R.T.: 0.066 min
Response: 4489112
Conc: 2.22 ng/ml

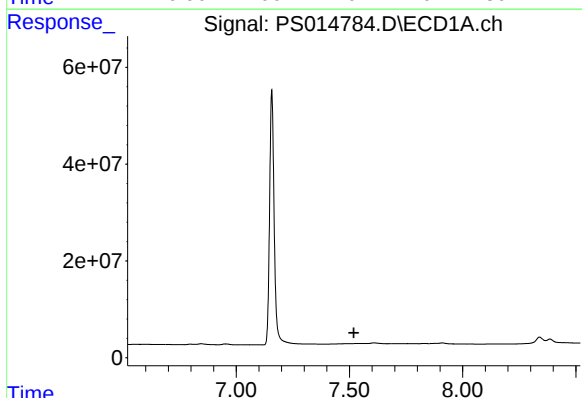


#6 MCP

R.T.: 0.000 min
Exp R.T.: 7.520 min
Response: 0
Conc: N.D.

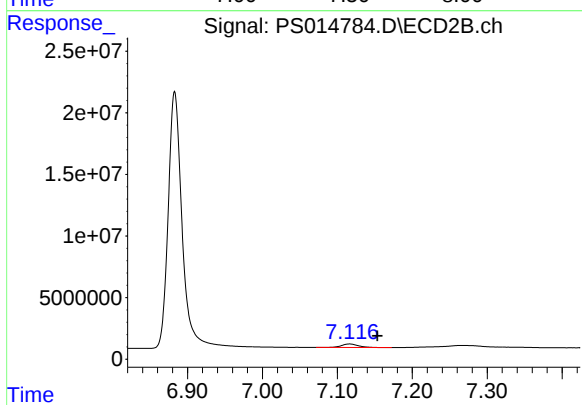

#6 MCP


R.T.: 7.117 min
Delta R.T.: -0.037 min
Response: 4489112
Conc: 2.67 ug/ml

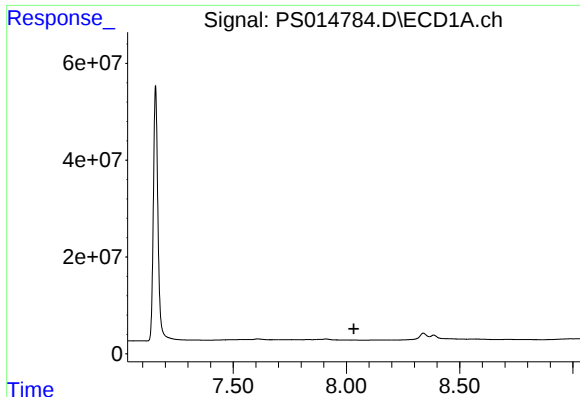

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 8.033 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

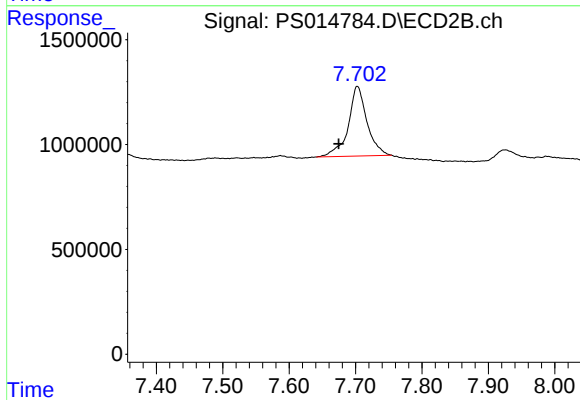


#8 DICHLORPROP

R.T.: 7.703 min
Delta R.T.: 0.028 min
Response: 6515561
Conc: 12.91 ng/ml

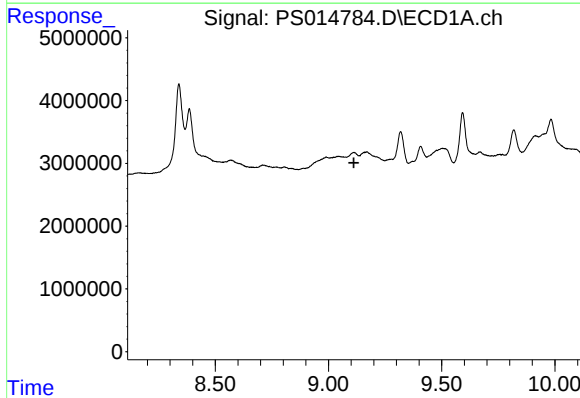


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T.: 9.112 min
Response: 0
Conc: N.D.

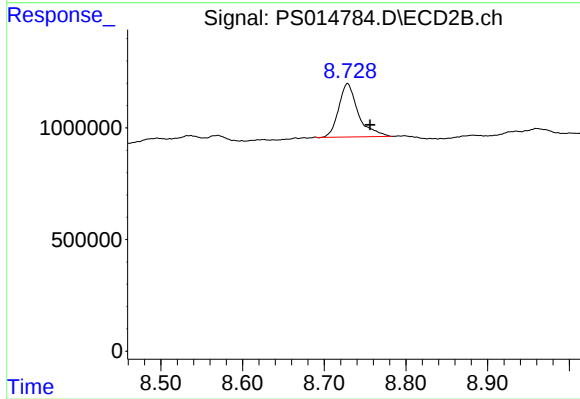

#11 2,4,5-TP (SILVEX)


R.T.: 8.729 min
Delta R.T.: -0.028 min
Response: 3967806
Conc: 1.45 ng/ml

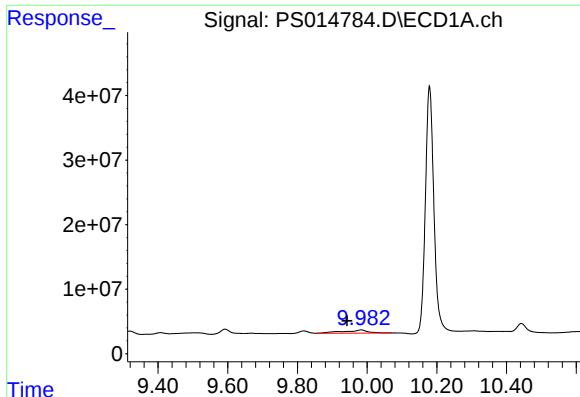

#13 2,4-DB


R.T.: 9.983 min
Delta R.T.: 0.040 min
Response: 24146807
Conc: 15.87 ng/ml

Instrument :
ECD_S
ClientSampleId :

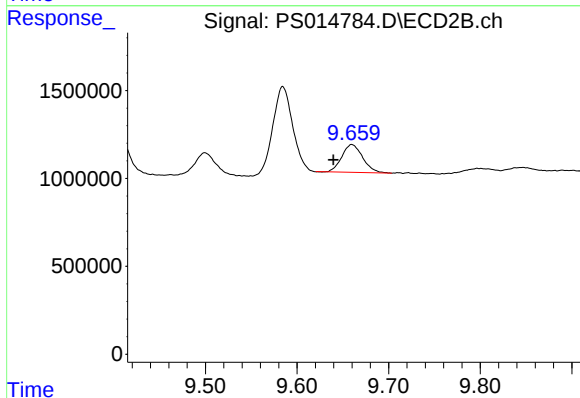


#13 2,4-DB

R.T.: 9.660 min
Delta R.T.: 0.020 min
Response: 2503763
Conc: 7.22 ng/ml

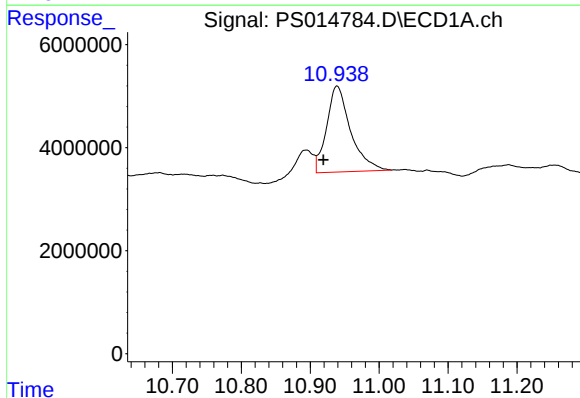

#15 Picloram

R.T.: 10.939 min
Delta R.T.: 0.020 min
Response: 40310360
Conc: 3.60 ng/ml

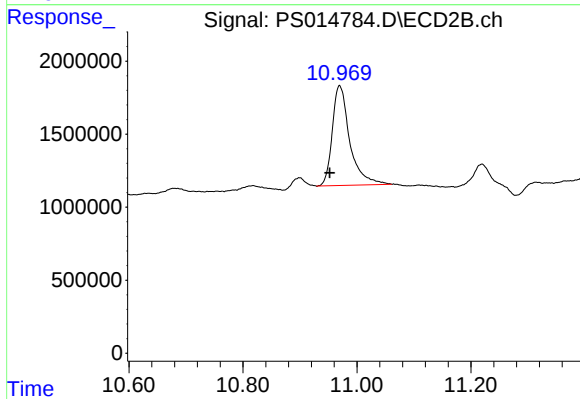

#15 Picloram

R.T.: 10.969 min
Delta R.T.: 0.017 min
Response: 14533049
Conc: 3.88 ng/ml