

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS042420\
 Data File : PS009992.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Apr 2020 06:45
 Operator : DD\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 24 15:40:44 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS040820.M
 Quant Title : 8080.M
 QLast Update : Thu Apr 09 05:27:48 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds						
5) T	DICAMBA	0.000	7.155	0	825518	N.D. <MDL
6) T	MCP	0.000	7.155	0	825518	N.D. <MDL
8) T	DICHLORPROP	0.000	7.744	0	1019519	N.D. 2.026
12) T	2,4,5-T	0.000	9.238	0	2186548	N.D. <MDL
13) T	2,4-DB	0.000	9.709	0	3039618	N.D. 8.573
15) T	Picloram	0.000	11.007	0	5027577	N.D. 1.478
16) T	DCPA	0.000	11.007	0	5027577	N.D. 1.499



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS042420\
Data File : PS009992.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Apr 2020 06:45
Operator : DD\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 24 15:40:44 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS040820.M
Quant Title : 8080.M
QLast Update : Thu Apr 09 05:27:48 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

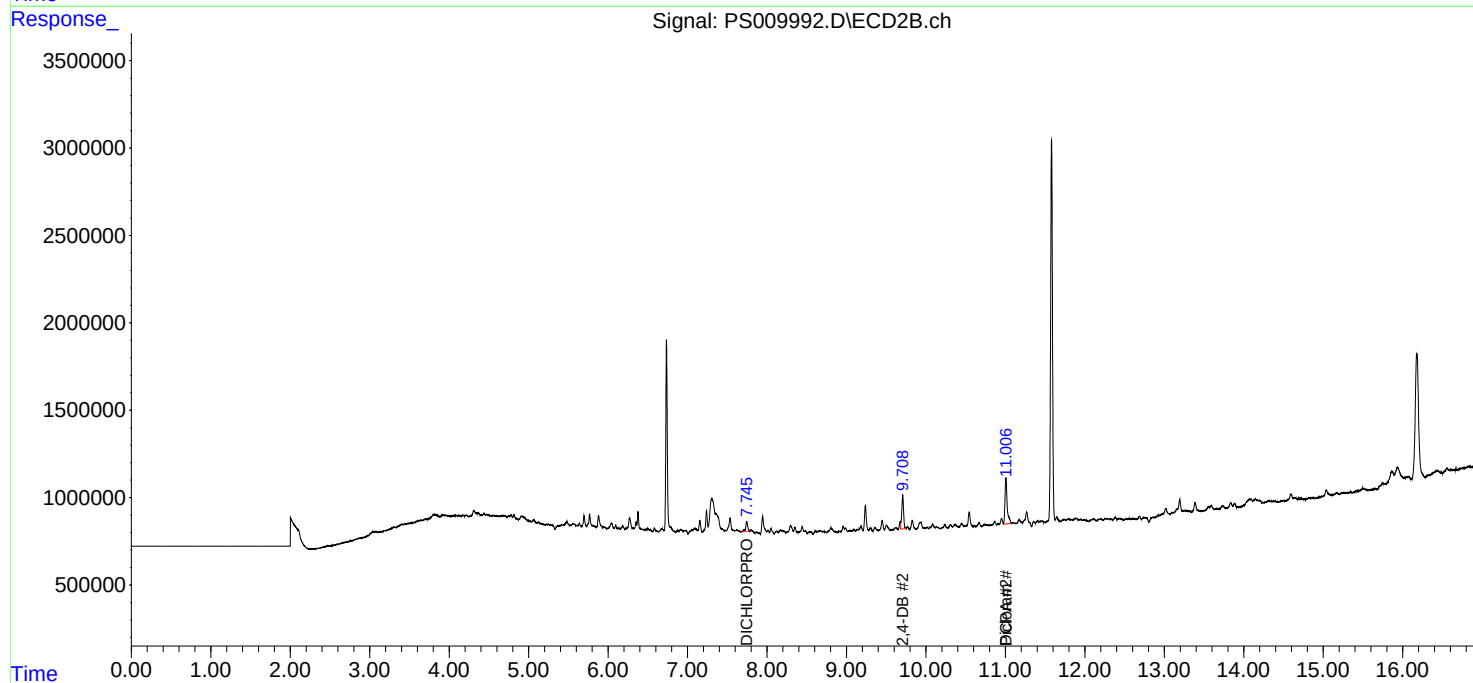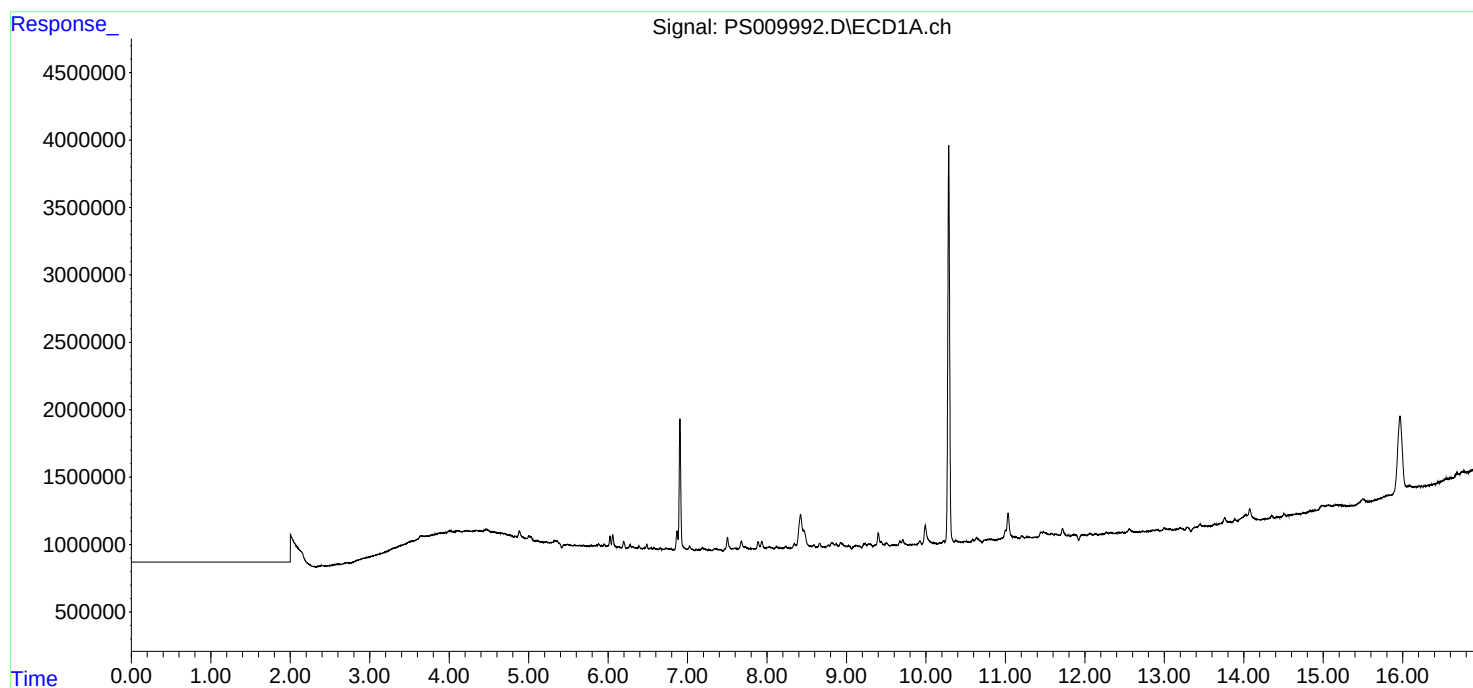


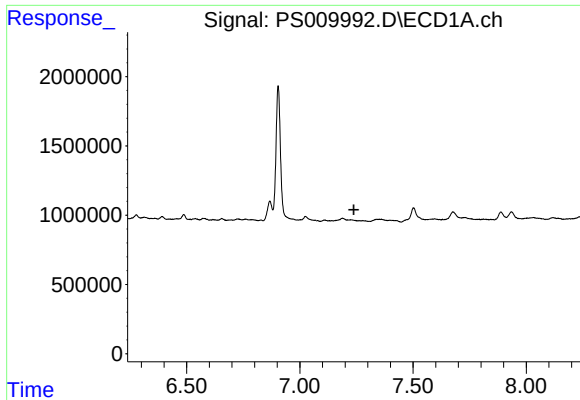

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T. : 7.239 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HEXANE

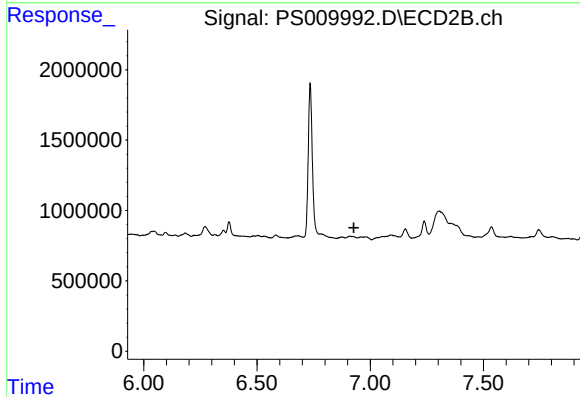


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T. : 6.928 min
Response: 0
Conc: N.D.

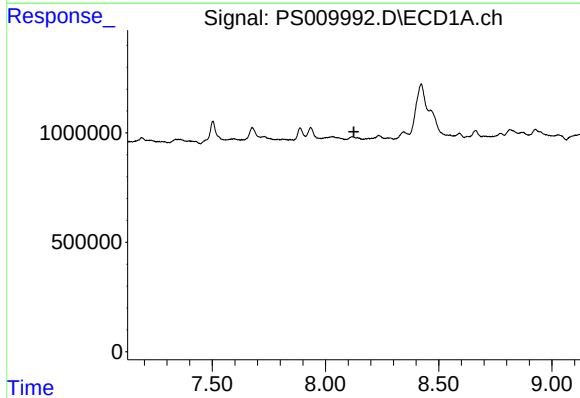


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 8.125 min
Response: 0
Conc: N.D.

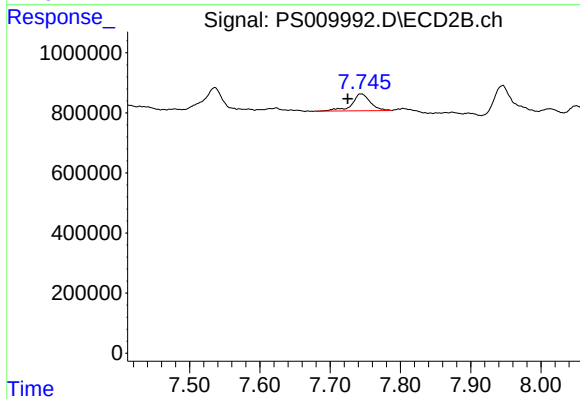

#8 DICHLORPROP


R.T.: 7.744 min
Delta R.T.: 0.019 min
Response: 1019519
Conc: 2.03 ng/ml

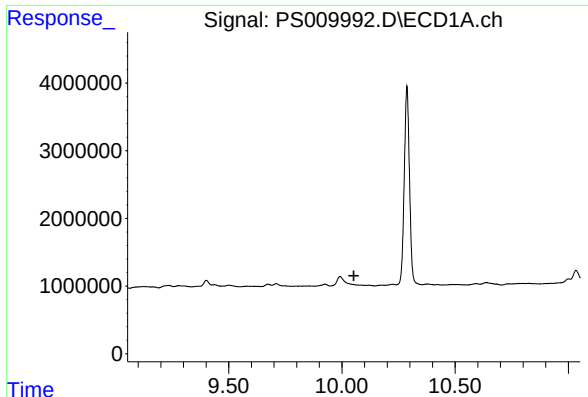

#13 2,4-DB


R.T.: 0.000 min
Exp R.T.: 10.053 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HEXANE

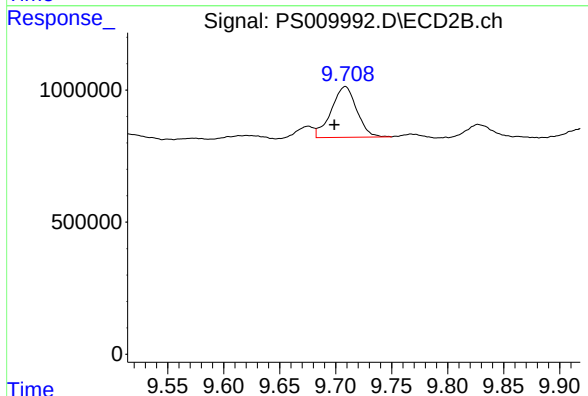


#13 2,4-DB

R.T.: 9.709 min
Delta R.T.: 0.010 min
Response: 3039618
Conc: 8.57 ng/ml

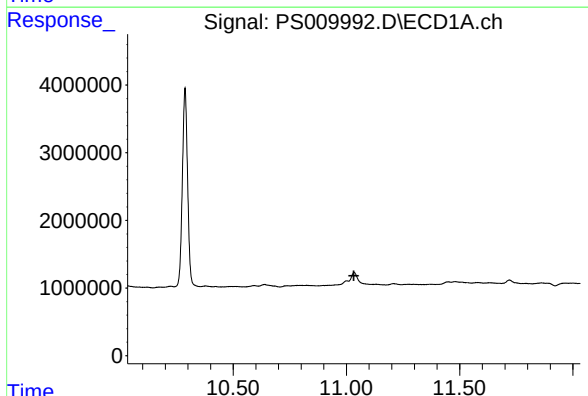


#15 Picloram

R.T.: 0.000 min
Exp R.T.: 11.033 min
Response: 0
Conc: N.D.

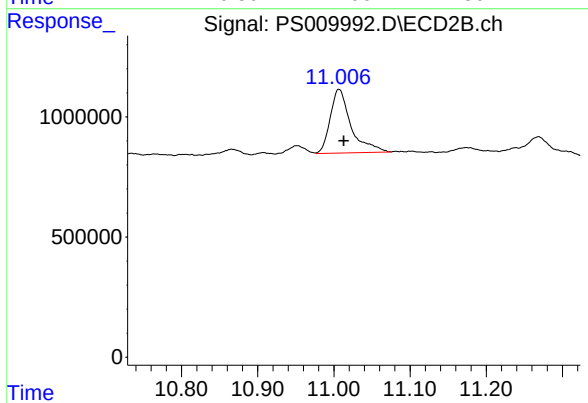

#15 Picloram


R.T.: 11.007 min
Delta R.T.: -0.006 min
Response: 5027577
Conc: 1.48 ng/ml

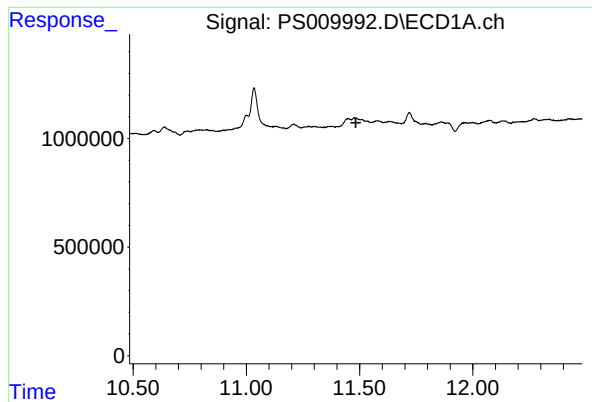

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 11.484 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HEXANE

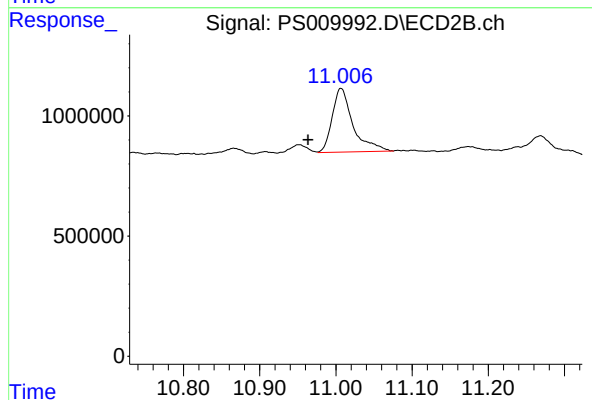

#16 DCPA

R.T.: 11.007 min
Delta R.T.: 0.043 min
Response: 5027577
Conc: 1.50 ng/ml