

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Data\PS042420\  
 Data File : PS009993.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 24 Apr 2020 07:08  
 Operator : DD\AJ  
 Sample : I.BLK  
 Misc :  
 ALS Vial : 2 Sample Multiplier: 1

Instrument :  
 ECD\_S  
 ClientSampleId :

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Apr 24 15:40:54 2020  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Method\PS040820.M  
 Quant Title : 8080.M  
 QLast Update : Thu Apr 09 05:27:48 2020  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2 µl  
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2  
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

|                             | Compound    | RT#1  | RT#2   | Resp#1  | Resp#2  | ng/ml   | ng/ml   |
|-----------------------------|-------------|-------|--------|---------|---------|---------|---------|
| -----                       |             |       |        |         |         |         |         |
| System Monitoring Compounds |             |       |        |         |         |         |         |
| 4) S                        | 2,4-DCAA    | 7.235 | 6.922  | 302.8E6 | 291.6E6 | 501.474 | 588.815 |
| Target Compounds            |             |       |        |         |         |         |         |
| 5) T                        | DICAMBA     | 0.000 | 7.156  | 0       | 1875837 | N.D.    | <MDL    |
| 6) T                        | MCPD        | 0.000 | 7.156  | 0       | 1875837 | N.D.    | 1.140   |
| 8) T                        | DICHLORPROP | 0.000 | 7.712  | 0       | 713899  | N.D.    | 1.418   |
| 12) T                       | 2,4,5-T     | 0.000 | 9.185  | 0       | 958639  | N.D.    | <MDL    |
| 15) T                       | Picloram    | 0.000 | 11.008 | 0       | 6155893 | N.D.    | 1.810   |
| 16) T                       | DCPA        | 0.000 | 10.954 | 0       | 860767  | N.D.    | <MDL    |
| -----                       |             |       |        |         |         |         |         |



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Data\PS042420\  
Data File : PS009993.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 24 Apr 2020 07:08  
Operator : DD\AJ  
Sample : I.BLK  
Misc :  
ALS Vial : 2 Sample Multiplier: 1

Instrument :  
ECD\_S  
ClientSampleId :

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Apr 24 15:40:54 2020  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Method\PS040820.M  
Quant Title : 8080.M  
QLast Update : Thu Apr 09 05:27:48 2020  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 2 µl  
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2  
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

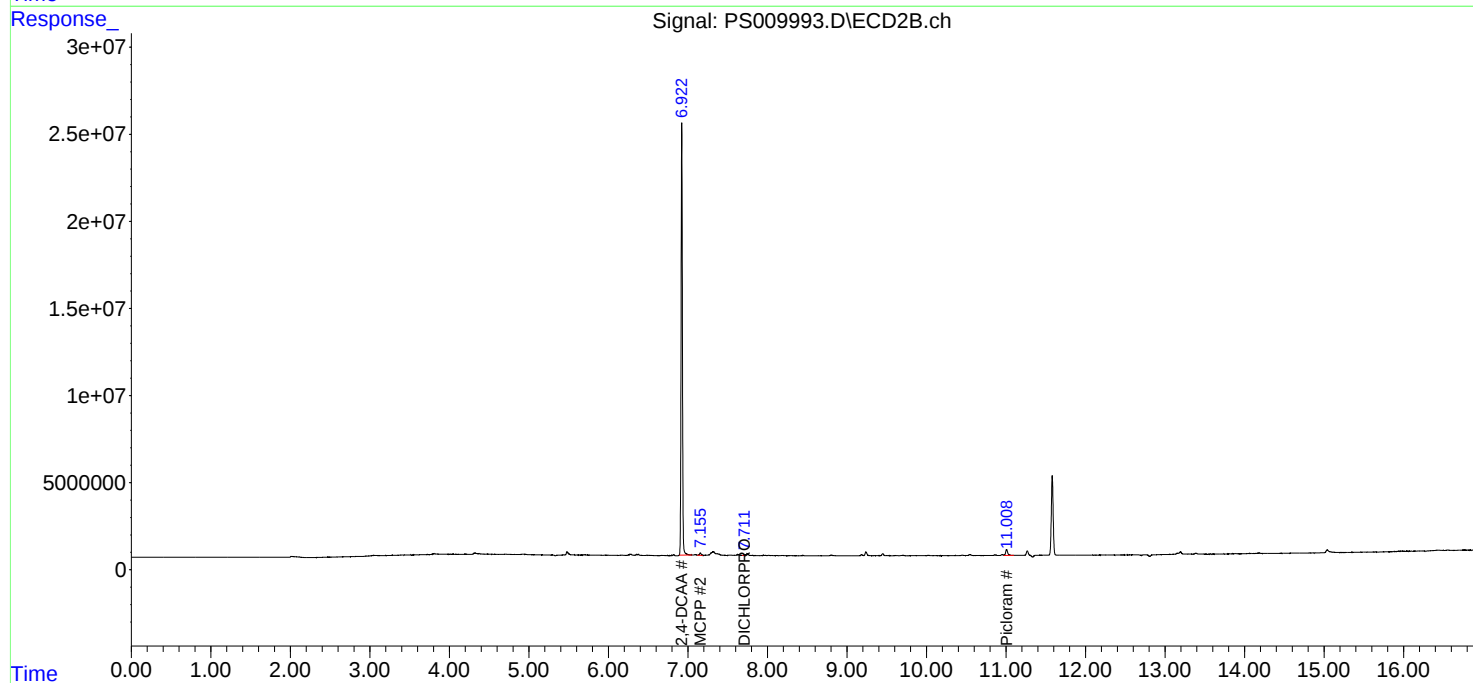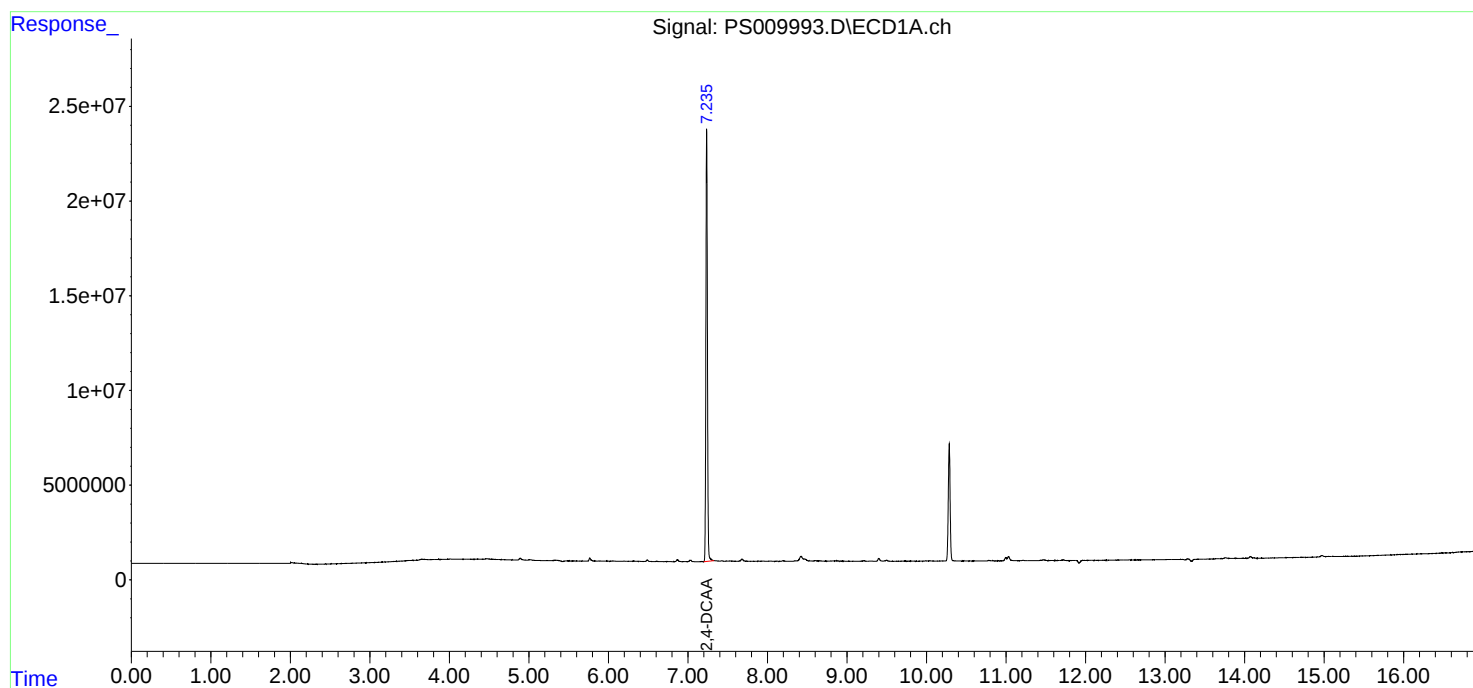


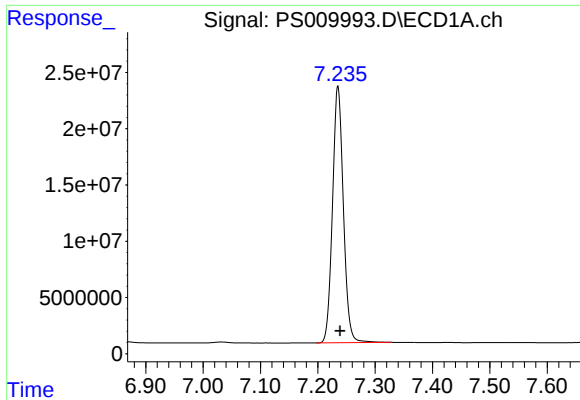

#4 2,4-DCAA


R.T.: 7.235 min  
Delta R.T.: -0.004 min  
Response: 302797952  
Conc: 501.47 ng/ml

Instrument :  
ECD\_S  
ClientSampleId :

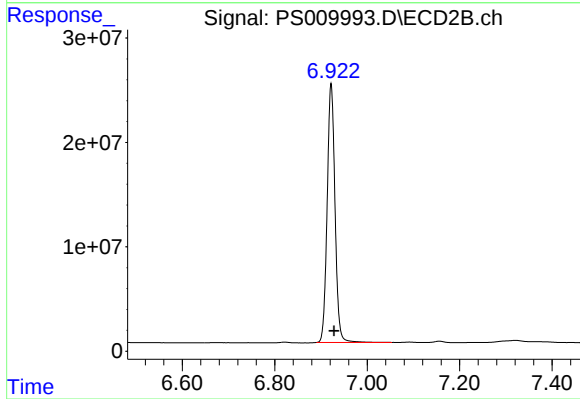


#4 2,4-DCAA

R.T.: 6.922 min  
Delta R.T.: -0.006 min  
Response: 291610401  
Conc: 588.81 ng/ml

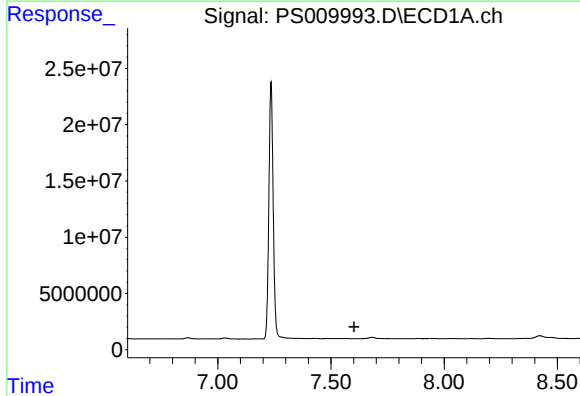


#6 MCP

R.T.: 0.000 min  
Exp R.T. : 7.602 min  
Response: 0  
Conc: N.D.

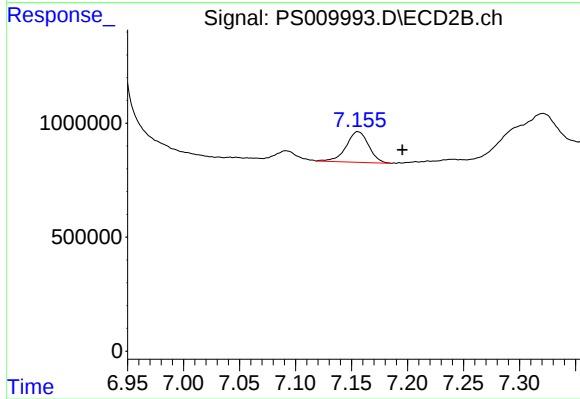

#6 MCP


R.T.: 7.156 min  
Delta R.T.: -0.040 min  
Response: 1875837  
Conc: 1.14 ug/ml

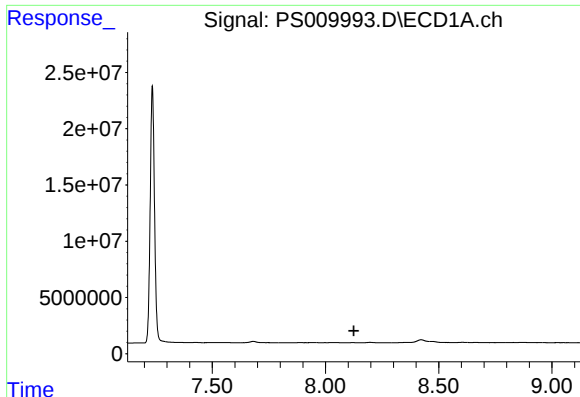

#8 DICHLORPROP


R.T.: 0.000 min  
Exp R.T. : 8.125 min  
Response: 0  
Conc: N.D.

Instrument :  
ECD\_S  
ClientSampleId :

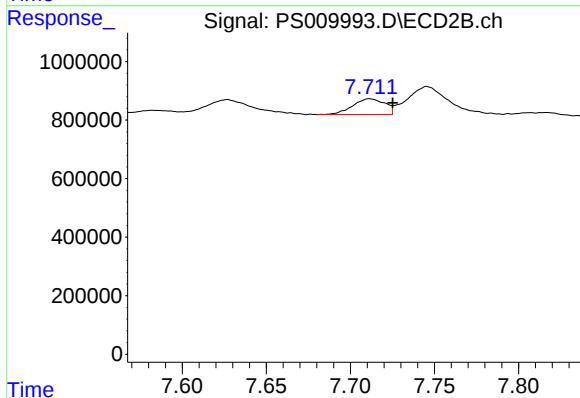


#8 DICHLORPROP

R.T.: 7.712 min  
Delta R.T.: -0.014 min  
Response: 713899  
Conc: 1.42 ng/ml

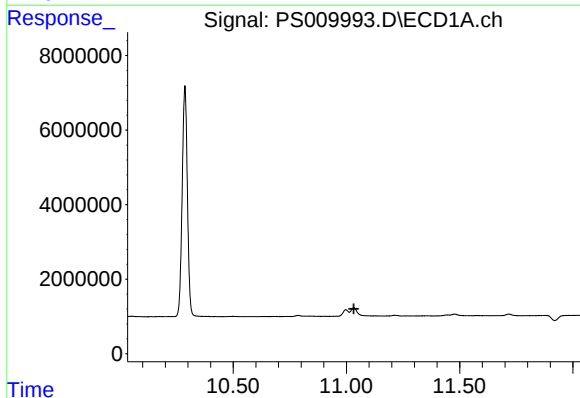

#15 Picloram

R.T.: 0.000 min  
Exp R.T. : 11.033 min  
Response: 0  
Conc: N.D.

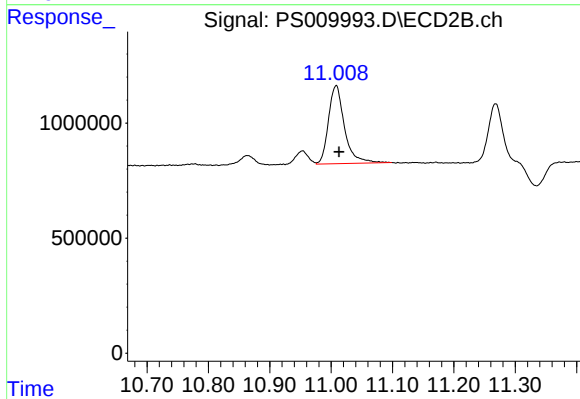

#15 Picloram

R.T.: 11.008 min  
Delta R.T.: -0.005 min  
Response: 6155893  
Conc: 1.81 ng/ml