

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS042420\
 Data File : PS009993.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Apr 2020 07:08
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 24 15:40:54 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS040820.M
 Quant Title : 8080.M
 QLast Update : Thu Apr 09 05:27:48 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.235	6.922	302.8E6	291.6E6	501.474	588.815
Target Compounds							
5) T	DICAMBA	0.000	7.156	0	1875837	N.D.	<MDL
6) T	MCP	0.000	7.156	0	1875837	N.D.	1.140
8) T	DICHLORPROP	0.000	7.712	0	713899	N.D.	1.418
12) T	2,4,5-T	0.000	9.185	0	958639	N.D.	<MDL
15) T	Picloram	0.000	11.008	0	6155893	N.D.	1.810
16) T	DCPA	0.000	10.954	0	860767	N.D.	<MDL



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS042420\
Data File : PS009993.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Apr 2020 07:08
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 24 15:40:54 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS040820.M
Quant Title : 8080.M
QLast Update : Thu Apr 09 05:27:48 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

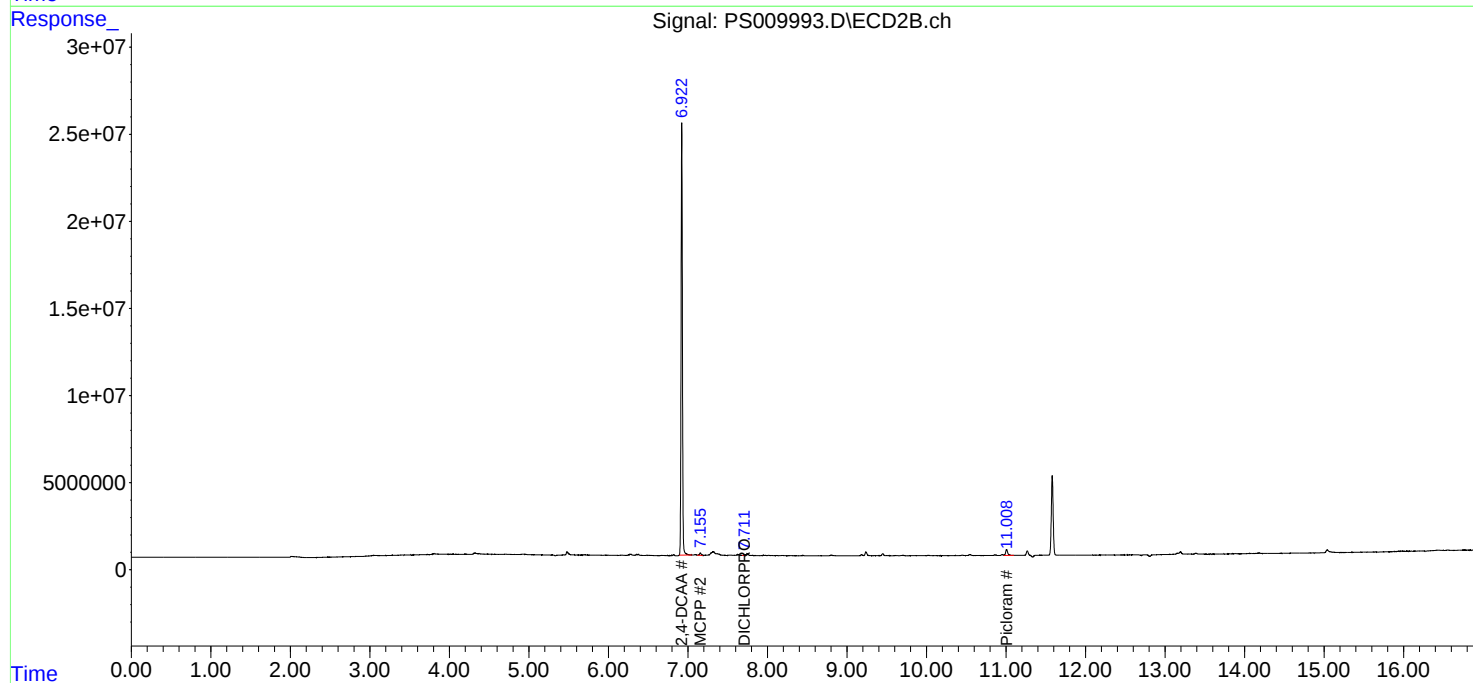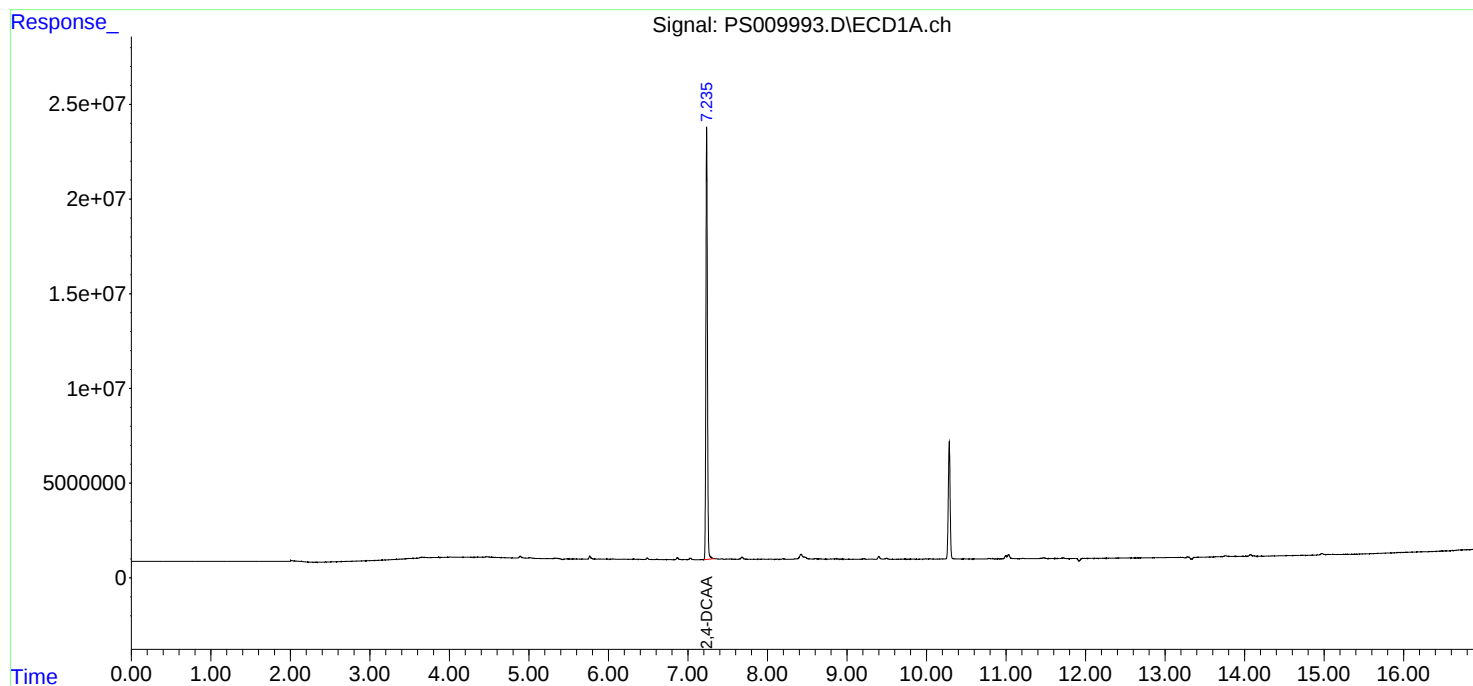


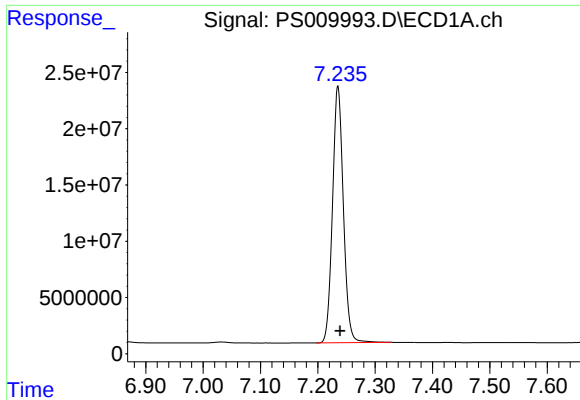

#4 2,4-DCAA


R.T.: 7.235 min
Delta R.T.: -0.004 min
Response: 302797952
Conc: 501.47 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

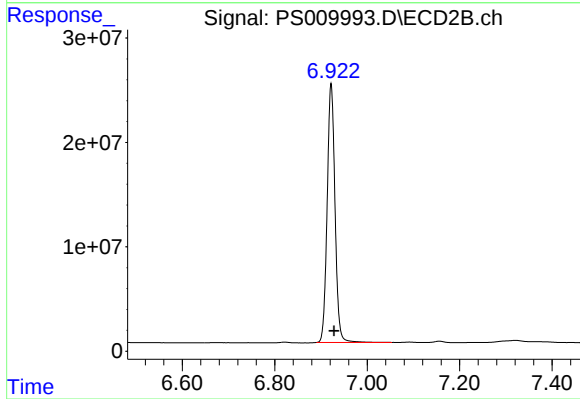


#4 2,4-DCAA

R.T.: 6.922 min
Delta R.T.: -0.006 min
Response: 291610401
Conc: 588.81 ng/ml

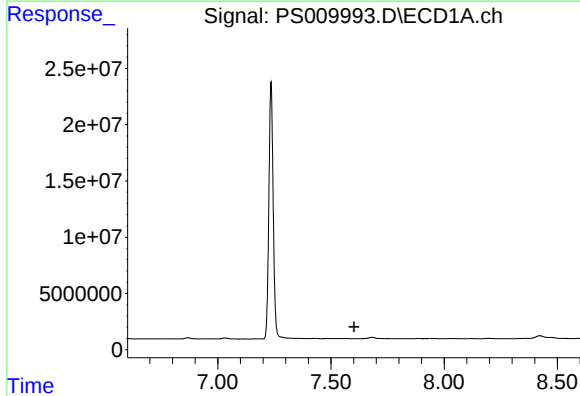


#6 MCP

R.T.: 0.000 min
Exp R.T. : 7.602 min
Response: 0
Conc: N.D.

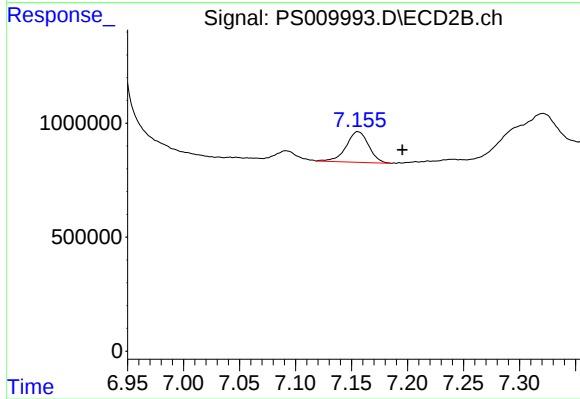

#6 MCP


R.T.: 7.156 min
Delta R.T.: -0.040 min
Response: 1875837
Conc: 1.14 ug/ml

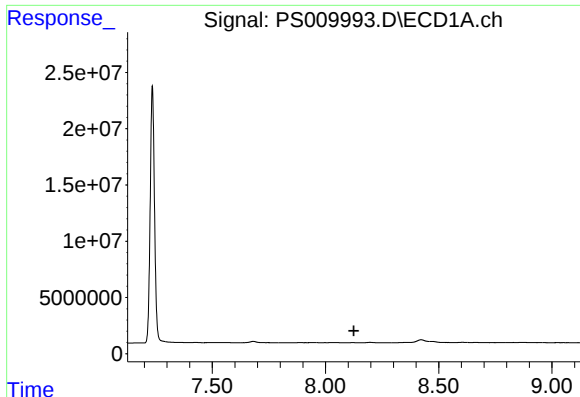

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 8.125 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

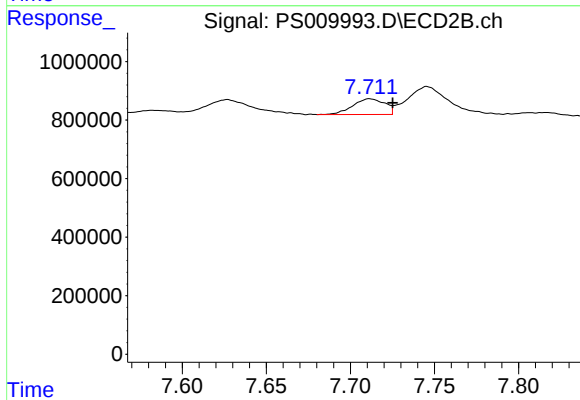


#8 DICHLORPROP

R.T.: 7.712 min
Delta R.T.: -0.014 min
Response: 713899
Conc: 1.42 ng/ml

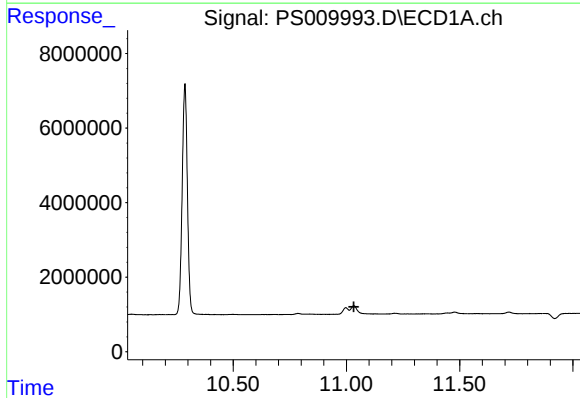

#15 Picloram

R.T.: 0.000 min
Exp R.T.: 11.033 min
Response: 0
Conc: N.D.

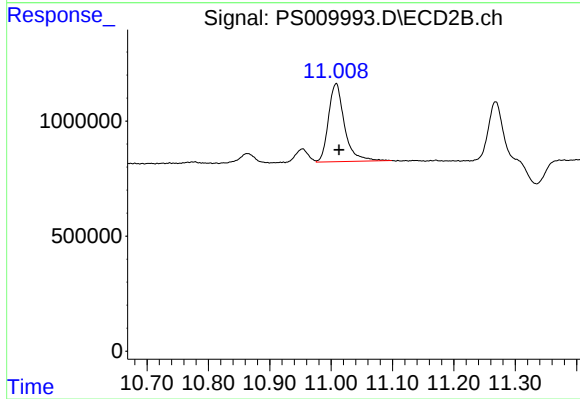

#15 Picloram

R.T.: 11.008 min
Delta R.T.: -0.005 min
Response: 6155893
Conc: 1.81 ng/ml