

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS042420\
 Data File : PS010010.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Apr 2020 19:08
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 25 02:44:02 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS040820.M
 Quant Title : 8080.M
 QLast Update : Thu Apr 09 05:27:48 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.235	6.922	312.8E6	292.6E6	518.065	590.864
Target Compounds							
5) T	DICAMBA	0.000	7.091	0	1151856	N.D.	<MDL
6) T	MCPD	0.000	7.156	0	1178630	N.D.	<MDL
8) T	DICHLORPROP	0.000	7.744	0	3958368	N.D.	7.865
9) T	2,4-D	8.422	0.000	15658966	0	27.272	N.D. #
11) T	2,4,5-TP ...	0.000	8.804	0	1221145	N.D.	<MDL
12) T	2,4,5-T	0.000	9.184	0	1420128	N.D.	<MDL
14) T	DINOSEB	0.000	10.026	0	496863	N.D.	<MDL
15) T	Picloram	0.000	11.007	0	1825714	N.D.	<MDL
16) T	DCPA	0.000	10.952	0	2218991	N.D.	<MDL



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS042420\
Data File : PS010010.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Apr 2020 19:08
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 25 02:44:02 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS040820.M
Quant Title : 8080.M
QLast Update : Thu Apr 09 05:27:48 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

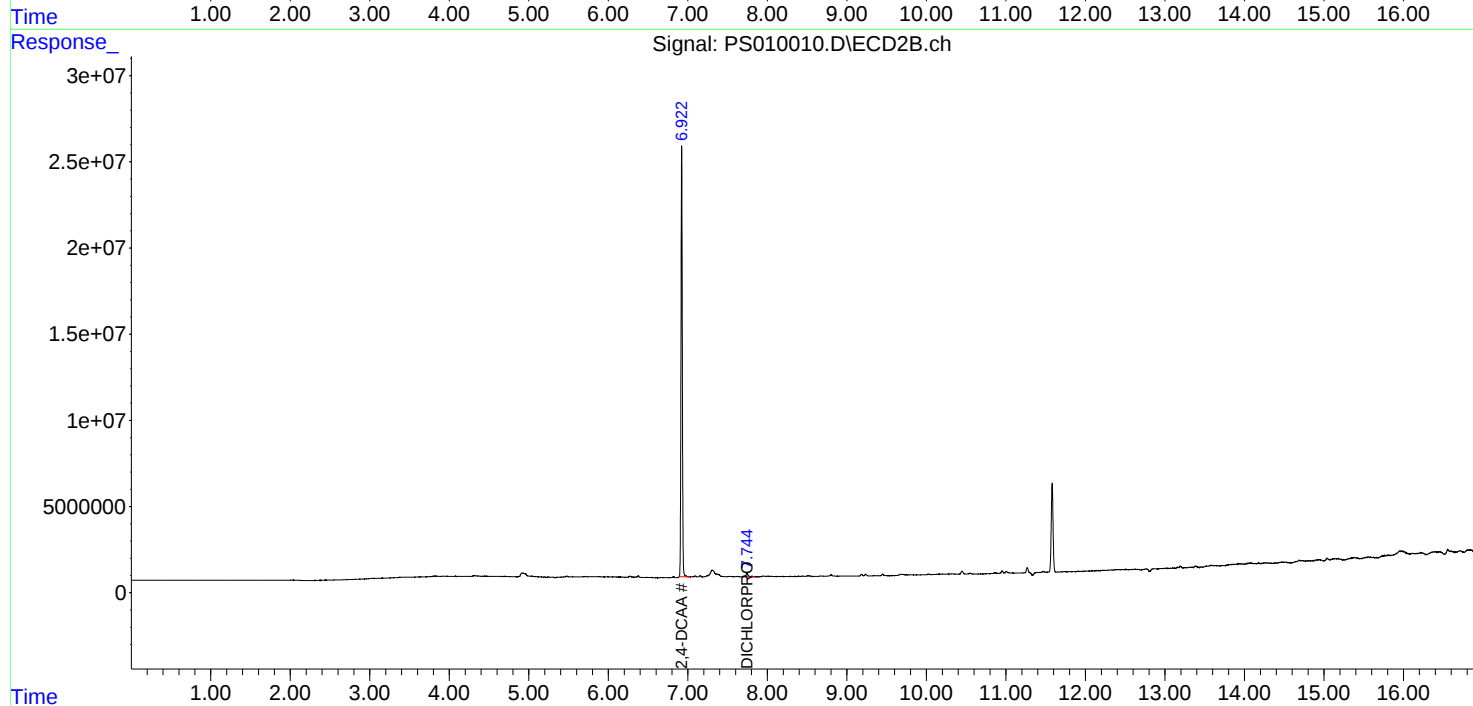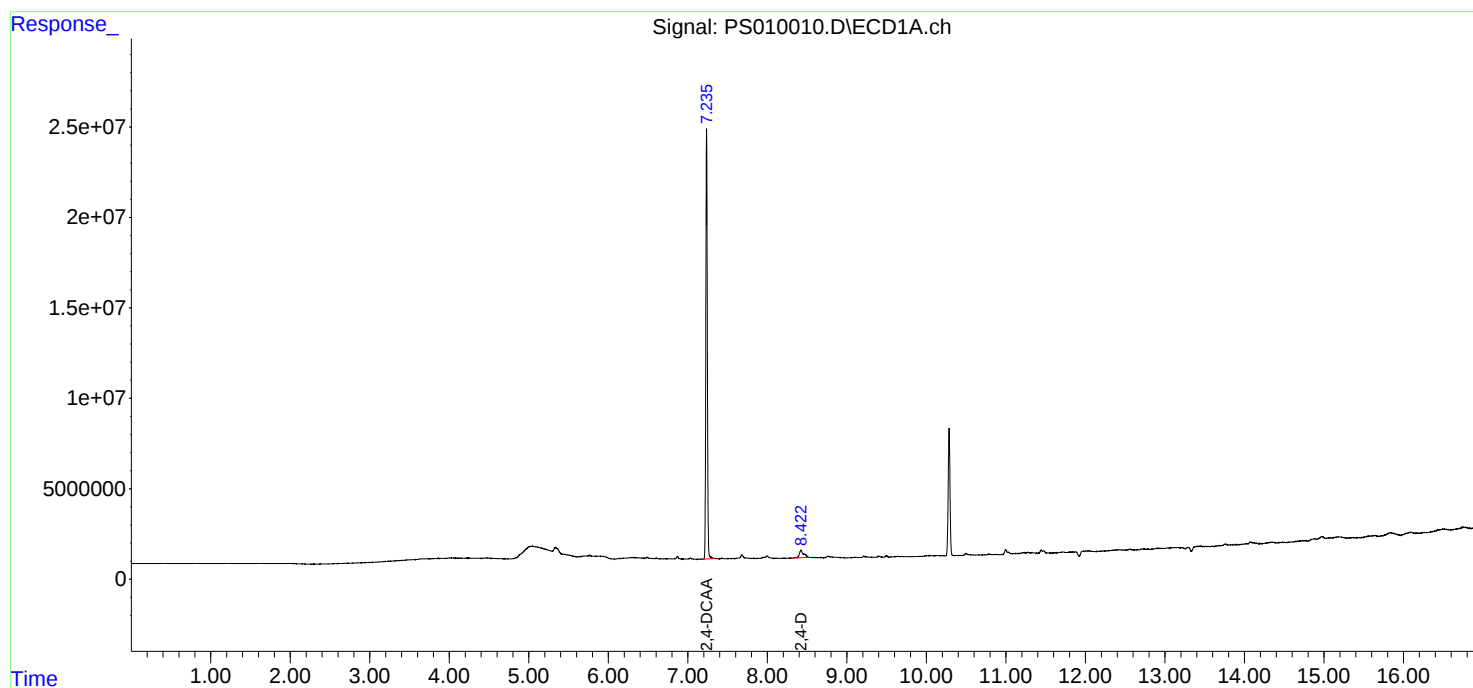


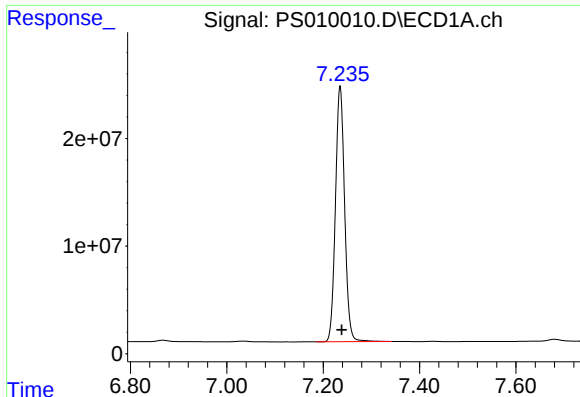

#4 2,4-DCAA


R.T.: 7.235 min
Delta R.T.: -0.004 min
Response: 312815617
Conc: 518.07 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

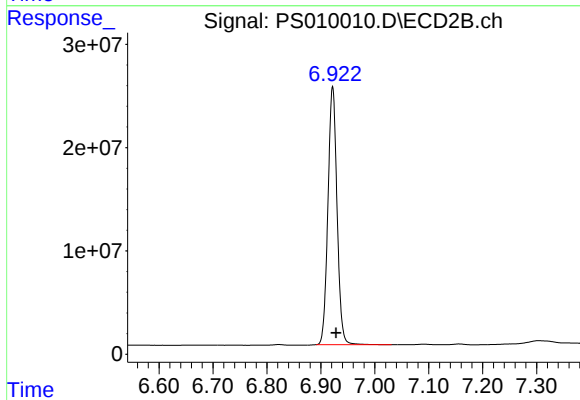


#4 2,4-DCAA

R.T.: 6.922 min
Delta R.T.: -0.006 min
Response: 292625175
Conc: 590.86 ng/ml

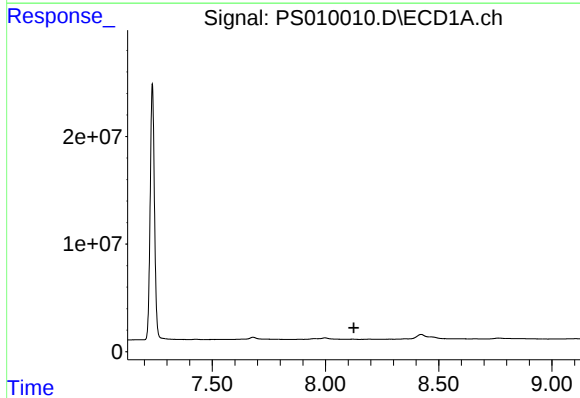


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 8.125 min
Response: 0
Conc: N.D.

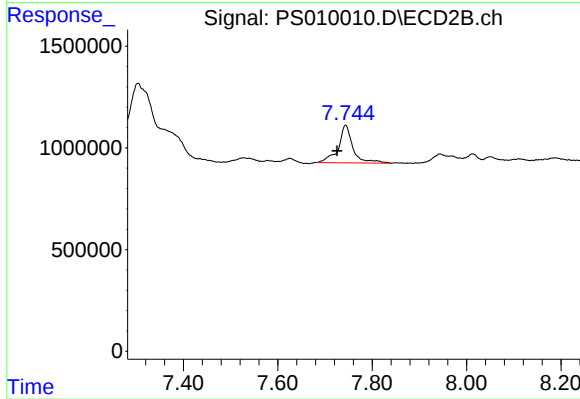

#8 DICHLORPROP


R.T.: 7.744 min
Delta R.T.: 0.019 min
Response: 3958368
Conc: 7.86 ng/ml

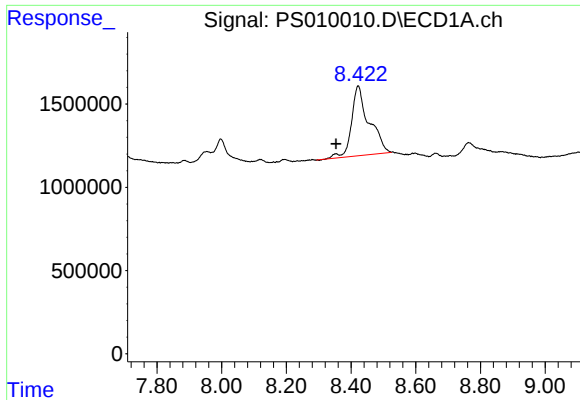

#9 2,4-D

R.T.: 8.422 min
Delta R.T.: 0.068 min
Response: 15658966
Conc: 27.27 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

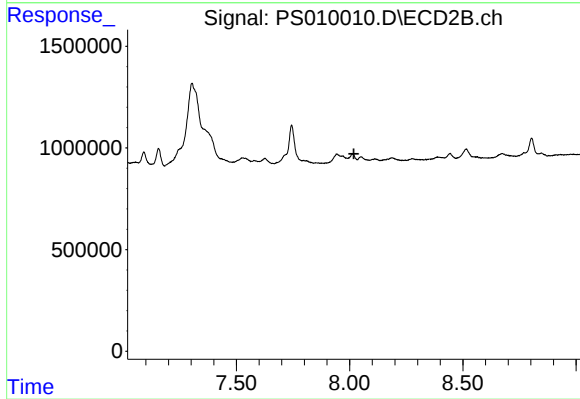

#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 8.019 min
Response: 0
Conc: N.D.