

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Data\PS042420\  
 Data File : PS010029.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 25 Apr 2020 02:24  
 Operator : DD\AJ  
 Sample : I.BLK  
 Misc :  
 ALS Vial : 2 Sample Multiplier: 1

Instrument :  
 ECD\_S  
 ClientSampleId :  
 I.BLK

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Apr 25 02:50:19 2020  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Method\PS040820.M  
 Quant Title : 8080.M  
 QLast Update : Thu Apr 09 05:27:48 2020  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2 µl  
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2  
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

|                             | Compound    | RT#1  | RT#2   | Resp#1  | Resp#2  | ng/ml   | ng/ml   |
|-----------------------------|-------------|-------|--------|---------|---------|---------|---------|
| -----                       |             |       |        |         |         |         |         |
| System Monitoring Compounds |             |       |        |         |         |         |         |
| 4) S                        | 2,4-DCAA    | 7.234 | 6.921  | 315.2E6 | 297.7E6 | 522.082 | 601.170 |
| Target Compounds            |             |       |        |         |         |         |         |
| 5) T                        | DICAMBA     | 0.000 | 7.154  | 0       | 1199042 | N.D.    | <MDL    |
| 6) T                        | MCPD        | 0.000 | 7.154  | 0       | 1199042 | N.D.    | <MDL    |
| 7) T                        | MCPA        | 0.000 | 7.358  | 0       | 138679  | N.D.    | <MDL    |
| 8) T                        | DICHLORPROP | 0.000 | 7.743  | 0       | 3019742 | N.D.    | 6.000   |
| 12) T                       | 2,4,5-T     | 0.000 | 9.184  | 0       | 1125554 | N.D.    | <MDL    |
| 15) T                       | Picloram    | 0.000 | 11.006 | 0       | 3318672 | N.D.    | <MDL    |
| 16) T                       | DCPA        | 0.000 | 10.952 | 0       | 1001039 | N.D.    | <MDL    |
| -----                       |             |       |        |         |         |         |         |



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Data\PS042420\  
Data File : PS010029.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 25 Apr 2020 02:24  
Operator : DD\AJ  
Sample : I.BLK  
Misc :  
ALS Vial : 2 Sample Multiplier: 1

Instrument :  
ECD\_S  
ClientSampleId :  
I.BLK

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Apr 25 02:50:19 2020  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Method\PS040820.M  
Quant Title : 8080.M  
QLast Update : Thu Apr 09 05:27:48 2020  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 2 µl  
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2  
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

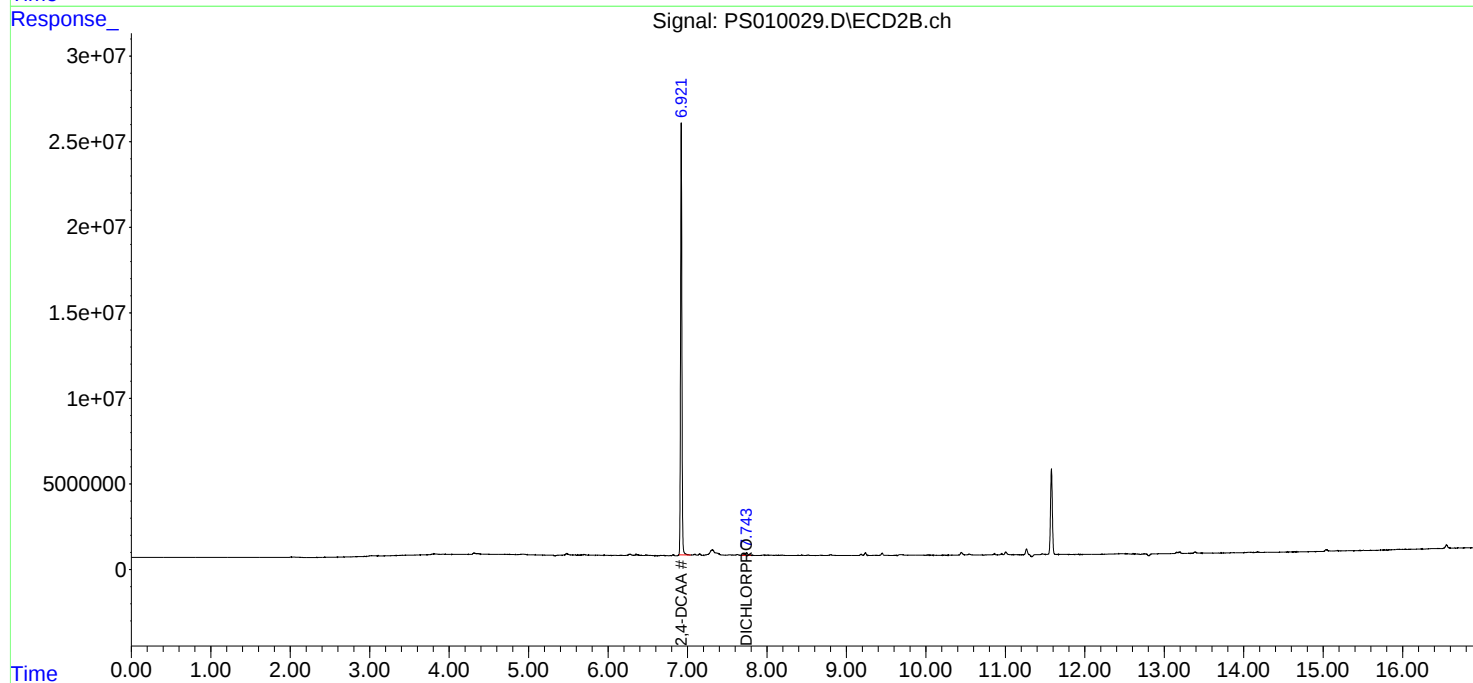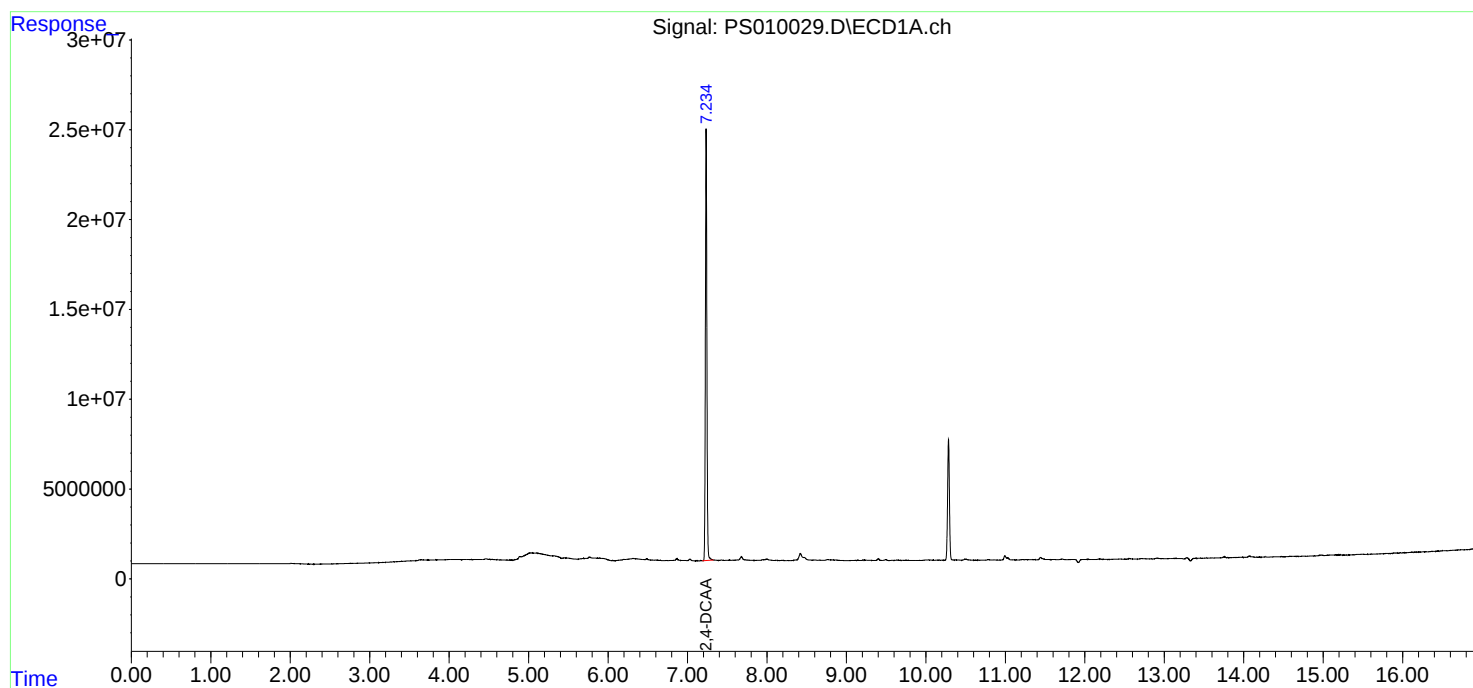


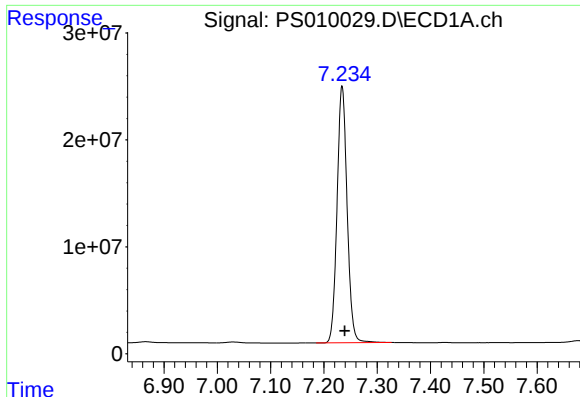

#4 2,4-DCAA


R.T.: 7.234 min  
Delta R.T.: -0.005 min  
Response: 315241295  
Conc: 522.08 ng/ml

Instrument :  
ECD\_S  
ClientSampleId :  
I.BLK

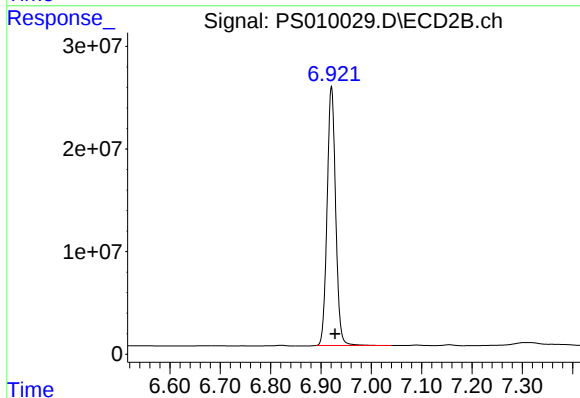


#4 2,4-DCAA

R.T.: 6.921 min  
Delta R.T.: -0.007 min  
Response: 297729374  
Conc: 601.17 ng/ml

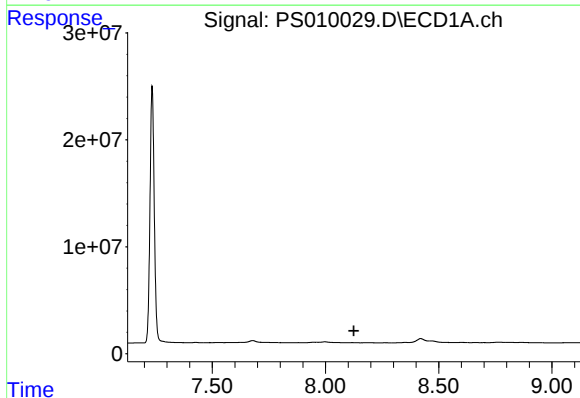

#8 DICHLORPROP

R.T.: 0.000 min  
Exp R.T. : 8.125 min  
Response: 0  
Conc: N.D.

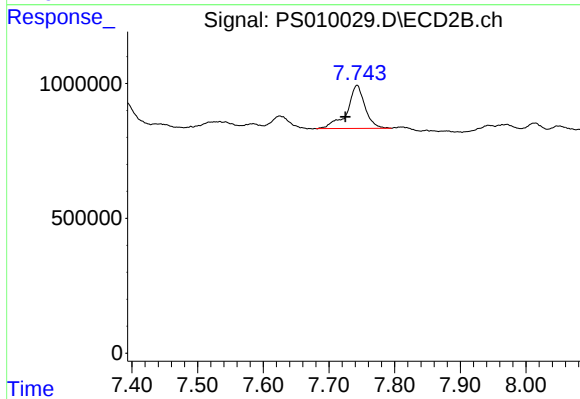

#8 DICHLORPROP

R.T.: 7.743 min  
Delta R.T.: 0.018 min  
Response: 3019742  
Conc: 6.00 ng/ml