

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Data\PS042520\  
 Data File : PS010032.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 25 Apr 2020 10:54  
 Operator : DD\AJ  
 Sample : I.BLK  
 Misc :  
 ALS Vial : 2 Sample Multiplier: 1

Instrument :  
 ECD\_S  
 ClientSampleId :

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Apr 27 00:51:15 2020  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Method\PS040820.M  
 Quant Title : 8080.M  
 QLast Update : Thu Apr 09 05:27:48 2020  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2 µl  
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2  
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

|                             | Compound     | RT#1  | RT#2   | Resp#1  | Resp#2  | ng/ml   | ng/ml   |
|-----------------------------|--------------|-------|--------|---------|---------|---------|---------|
| -----                       |              |       |        |         |         |         |         |
| System Monitoring Compounds |              |       |        |         |         |         |         |
| 4) S                        | 2,4-DCAA     | 7.235 | 6.921  | 323.9E6 | 283.1E6 | 536.459 | 571.557 |
| Target Compounds            |              |       |        |         |         |         |         |
| 5) T                        | DICAMBA      | 0.000 | 7.155  | 0       | 1277913 | N.D.    | <MDL    |
| 6) T                        | MCPD         | 0.000 | 7.155  | 0       | 1277913 | N.D.    | <MDL    |
| 8) T                        | DICHLORPROP  | 0.000 | 7.744  | 0       | 2045515 | N.D.    | 4.064   |
| 11) T                       | 2,4,5-TP ... | 0.000 | 8.803  | 0       | 820042  | N.D.    | <MDL    |
| 12) T                       | 2,4,5-T      | 0.000 | 9.184  | 0       | 1191566 | N.D.    | <MDL    |
| 15) T                       | Picloram     | 0.000 | 11.007 | 0       | 4396527 | N.D.    | 1.293   |
| 16) T                       | DCPA         | 0.000 | 10.951 | 0       | 1297680 | N.D.    | <MDL    |
| -----                       |              |       |        |         |         |         |         |



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Data\PS042520\  
Data File : PS010032.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 25 Apr 2020 10:54  
Operator : DD\AJ  
Sample : I.BLK  
Misc :  
ALS Vial : 2 Sample Multiplier: 1

Instrument :  
ECD\_S  
ClientSampleId :

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Apr 27 00:51:15 2020  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Method\PS040820.M  
Quant Title : 8080.M  
QLast Update : Thu Apr 09 05:27:48 2020  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 2 µl  
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2  
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

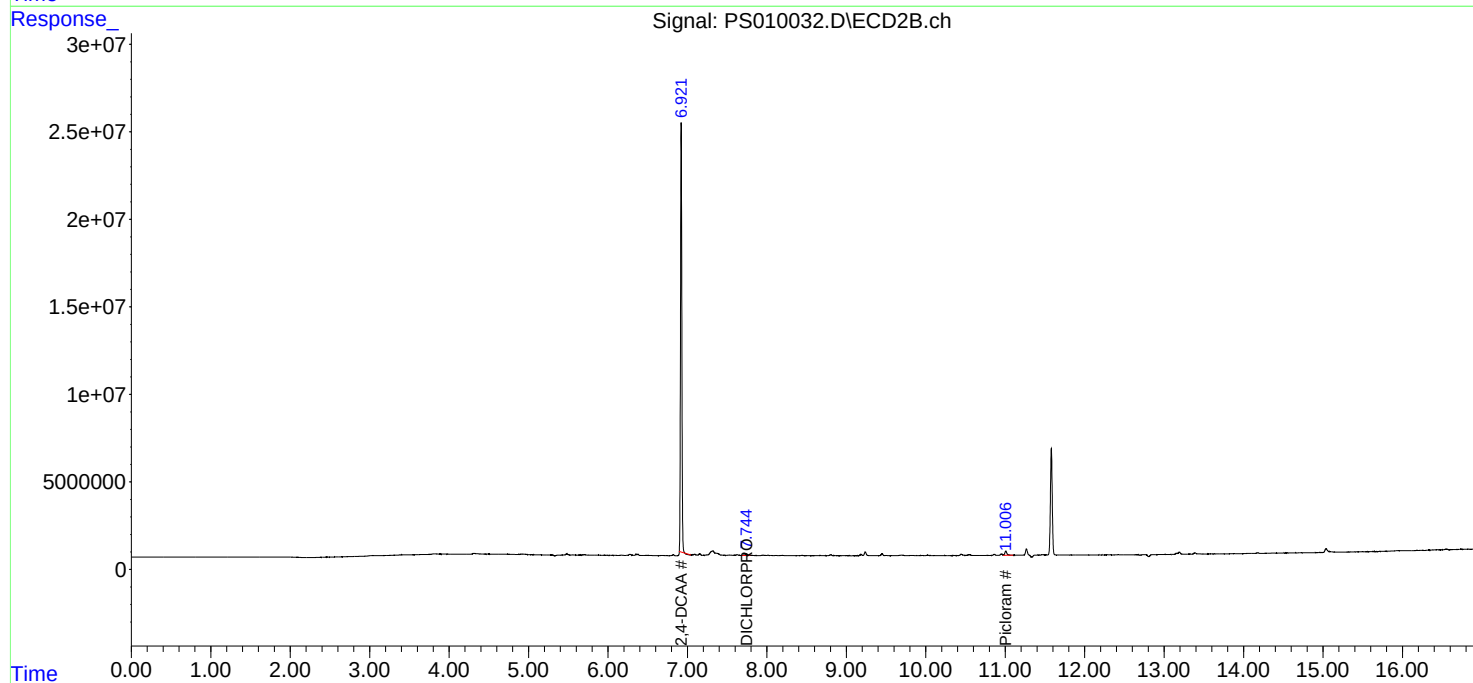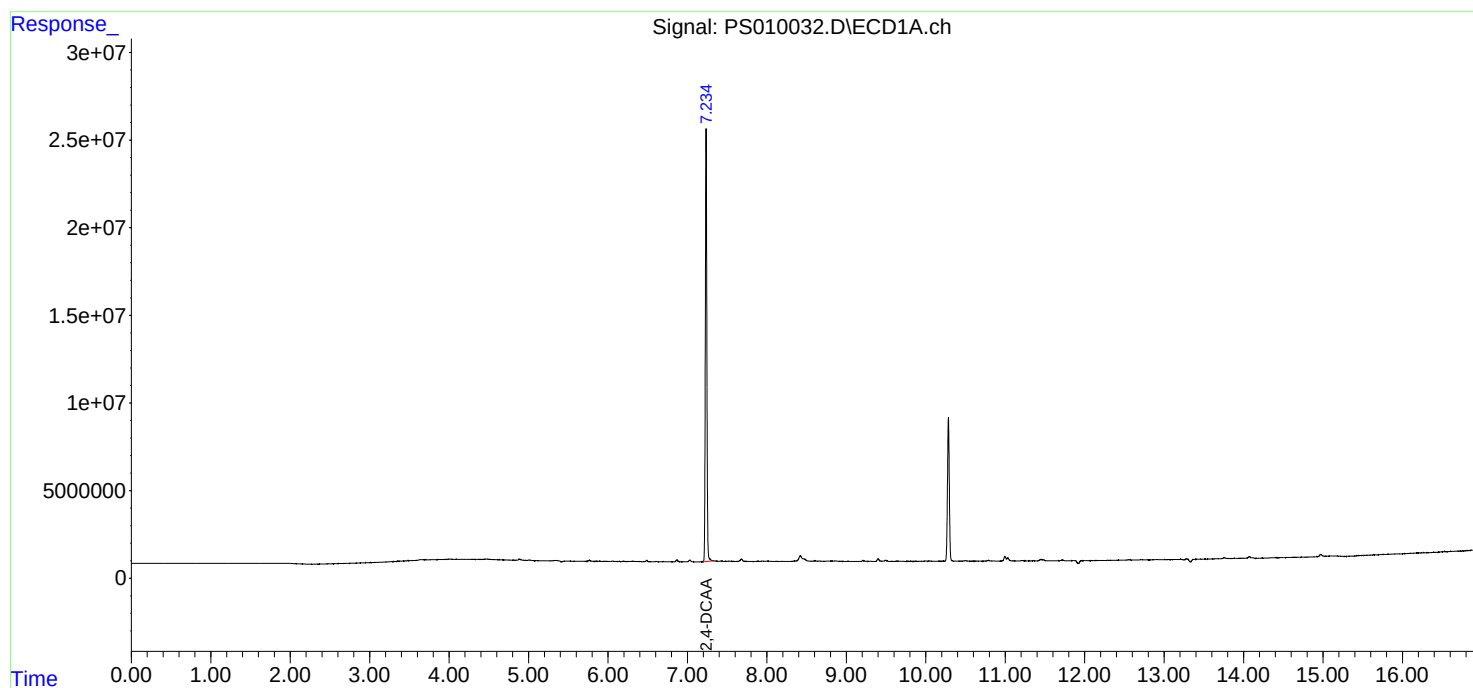


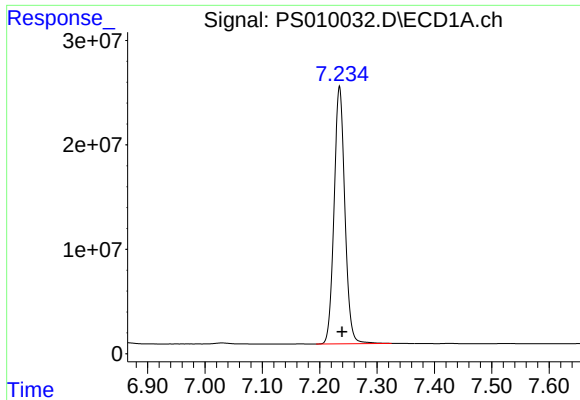

#4 2,4-DCAA


R.T.: 7.235 min  
Delta R.T.: -0.004 min  
Response: 323921841  
Conc: 536.46 ng/ml

Instrument :  
ECD\_S  
ClientSampleId :

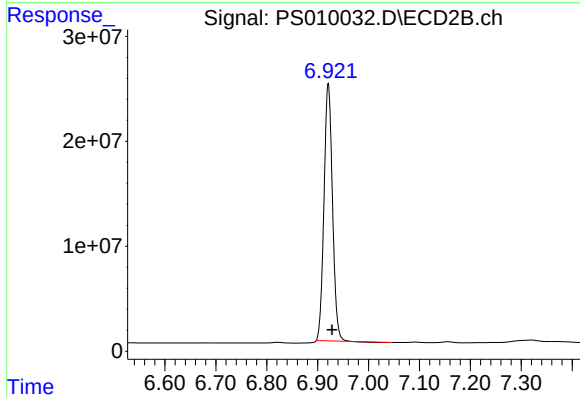


#4 2,4-DCAA

R.T.: 6.921 min  
Delta R.T.: -0.007 min  
Response: 283063716  
Conc: 571.56 ng/ml

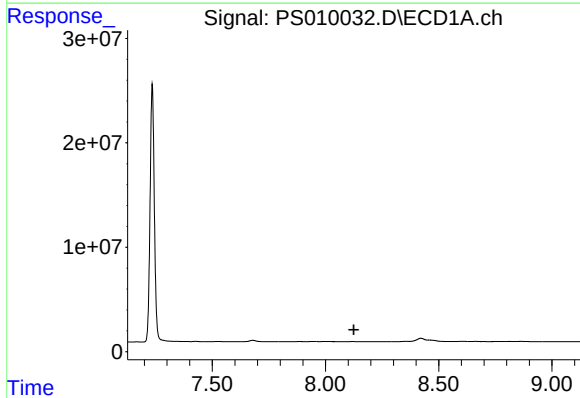


#8 DICHLORPROP

R.T.: 0.000 min  
Exp R.T. : 8.125 min  
Response: 0  
Conc: N.D.

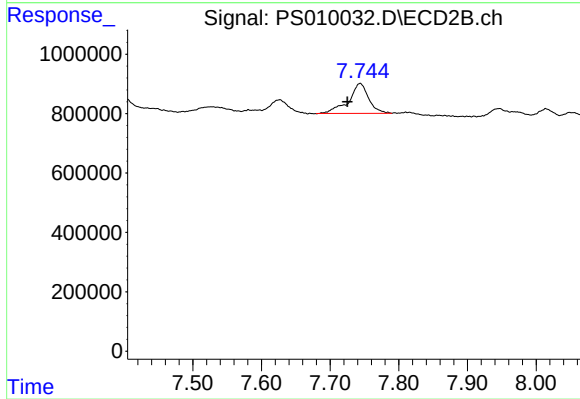

#8 DICHLORPROP


R.T.: 7.744 min  
Delta R.T.: 0.019 min  
Response: 2045515  
Conc: 4.06 ng/ml

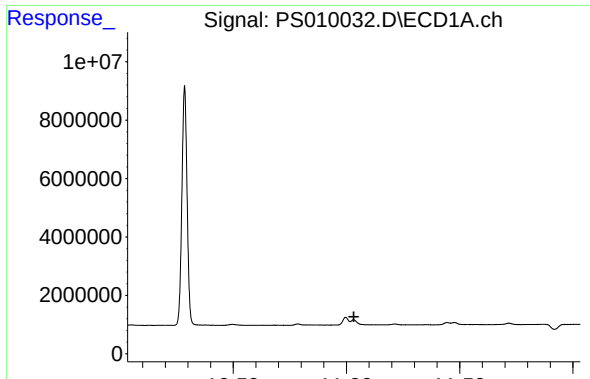

#15 Picloram

R.T.: 0.000 min  
Exp R.T.: 11.033 min  
Response: 0  
Conc: N.D.

Instrument :  
ECD\_S  
ClientSampleId :

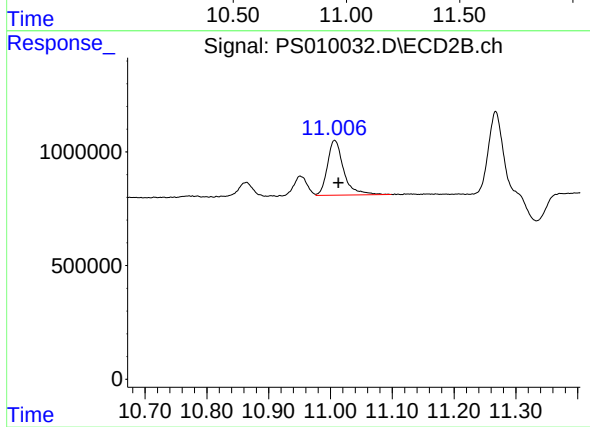

#15 Picloram

R.T.: 11.007 min  
Delta R.T.: -0.006 min  
Response: 4396527  
Conc: 1.29 ng/ml