

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS042619\
 Data File : PS004304.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Apr 2019 15:41
 Operator : EI\SJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 29 10:13:00 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS042619.M
 Quant Title : 8080.M
 QLast Update : Mon Apr 29 10:11:55 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds						
6) T	MCP	0.000	5.975	0	16249846	N.D. 12.123
9) T	2,4-D	7.082	0.000	26375885	0	45.523 N.D. #
15) T	Picloram	9.648	9.529	4738217	3700203	1.081 <MDL #
16) T	DCPA	0.000	9.529	0	3700203	N.D. 1.064



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS042619\
Data File : PS004304.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Apr 2019 15:41
Operator : EI\SJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 29 10:13:00 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS042619.M
Quant Title : 8080.M
QLast Update : Mon Apr 29 10:11:55 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

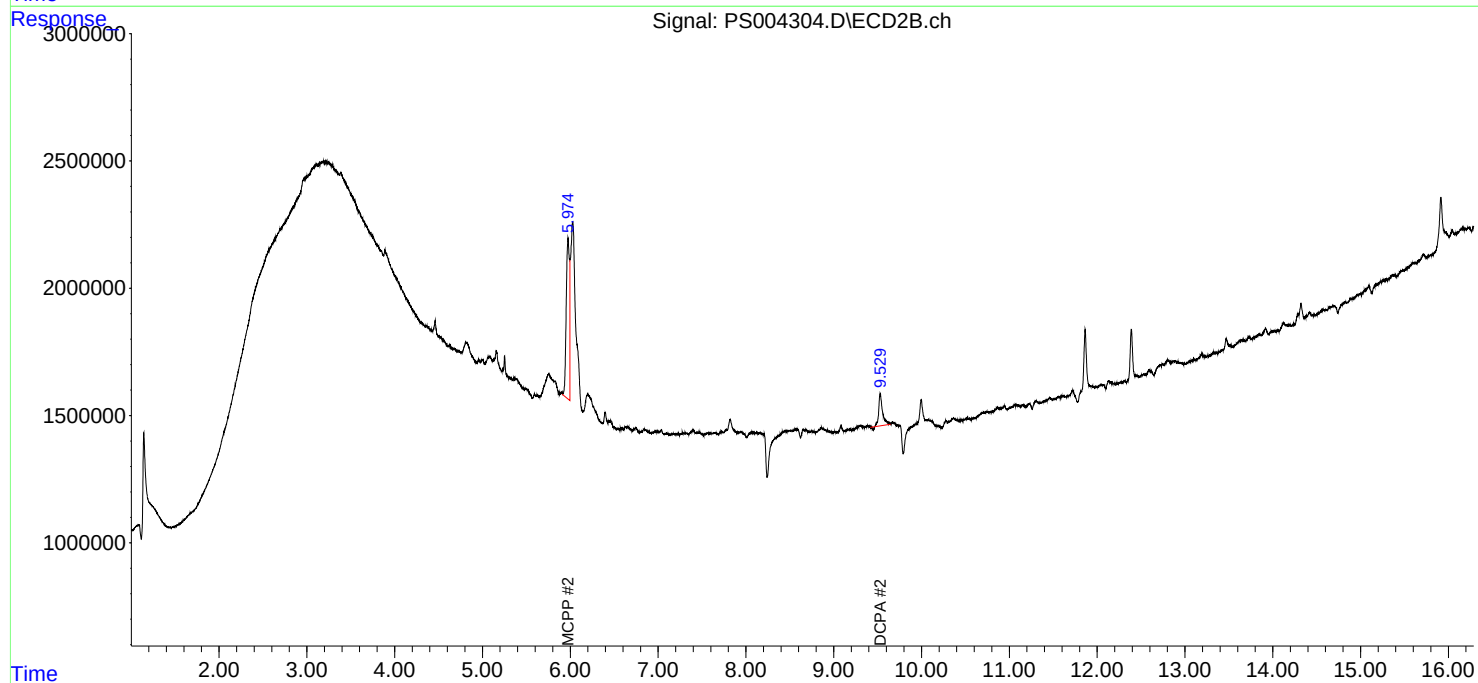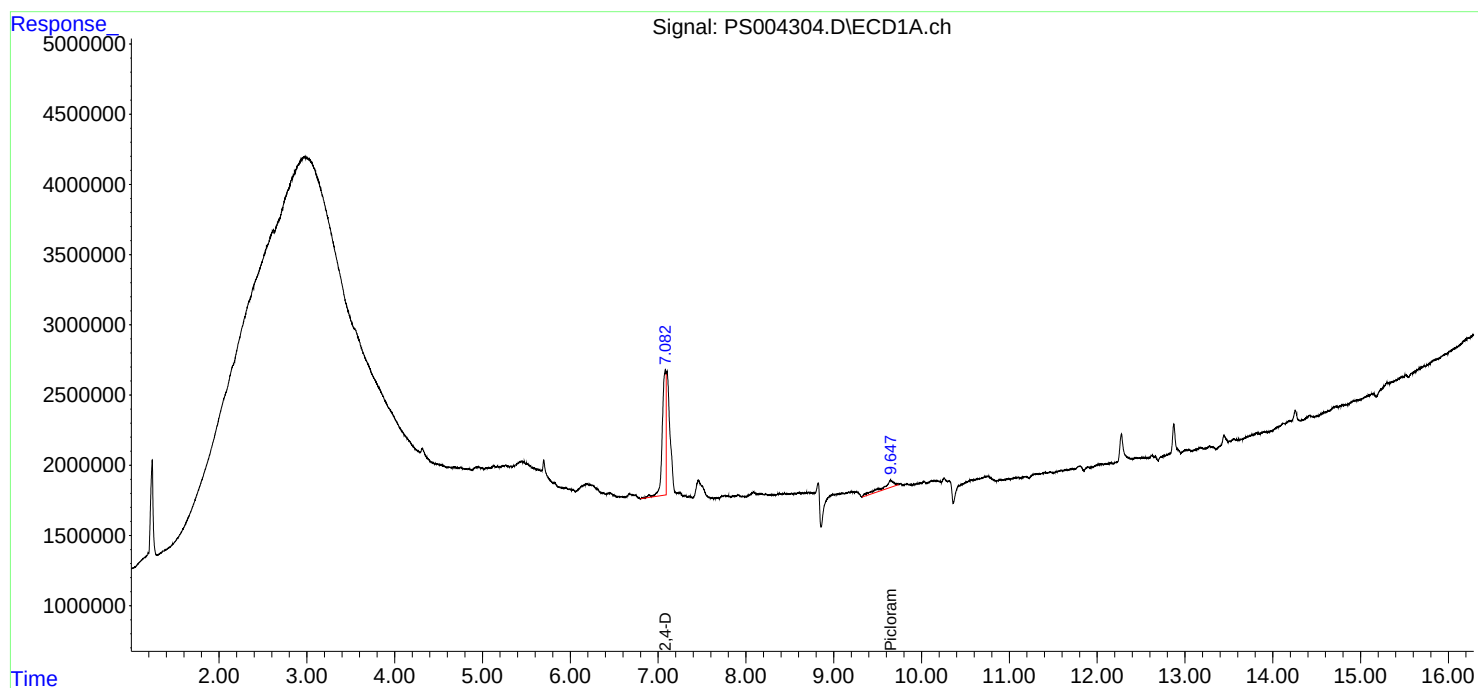


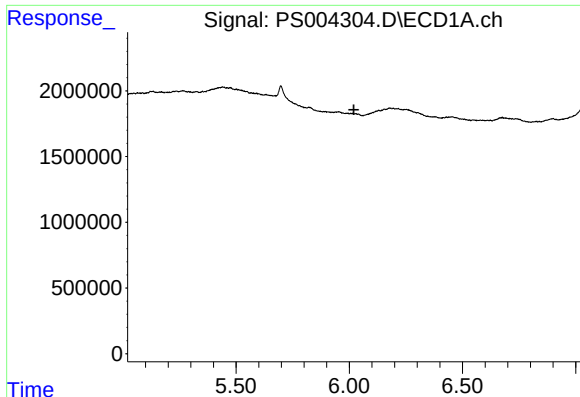

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T. : 6.021 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HEXANE

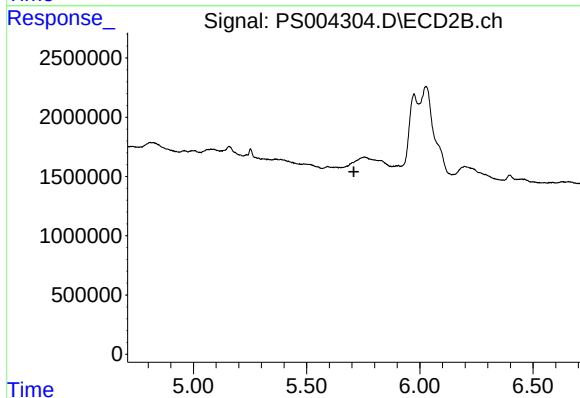


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T. : 5.709 min
Response: 0
Conc: N.D.

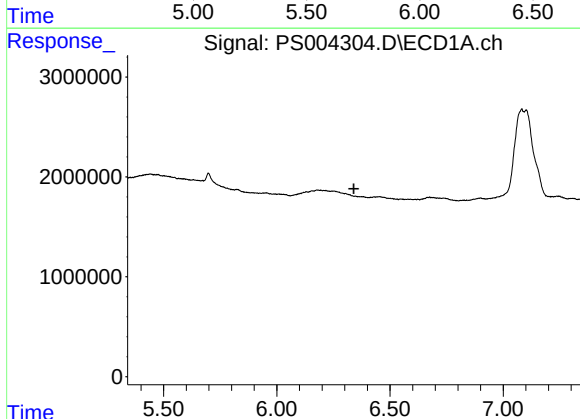


#6 MCPP

R.T.: 0.000 min
Exp R.T. : 6.341 min
Response: 0
Conc: N.D.

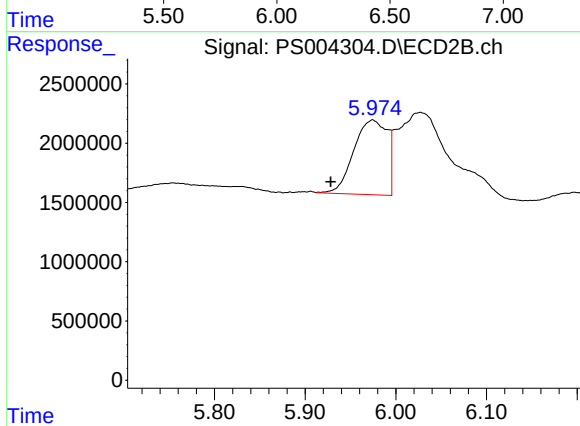

#6 MCPP


R.T.: 5.975 min
Delta R.T.: 0.046 min
Response: 16249846
Conc: 12.12 ug/ml

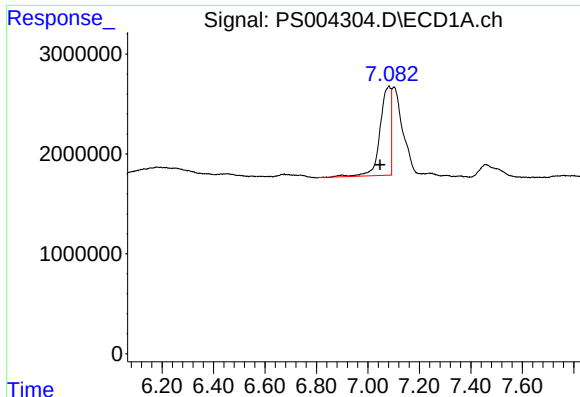

#9 2,4-D


R.T.: 7.082 min
Delta R.T.: 0.035 min
Response: 26375885
Conc: 45.52 ng/ml

Instrument :
ECD_S
ClientSampleId :
HEXANE

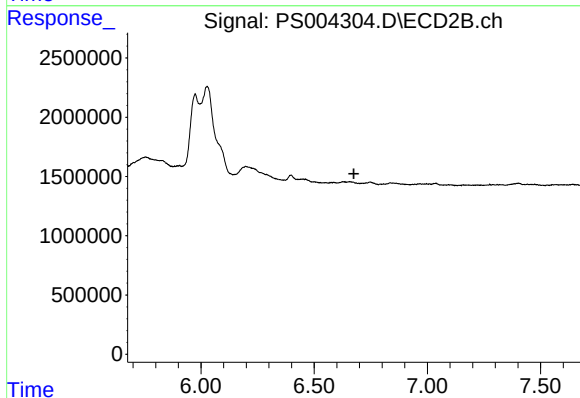


#9 2,4-D

R.T.: 0.000 min
Exp R.T.: 6.675 min
Response: 0
Conc: N.D.

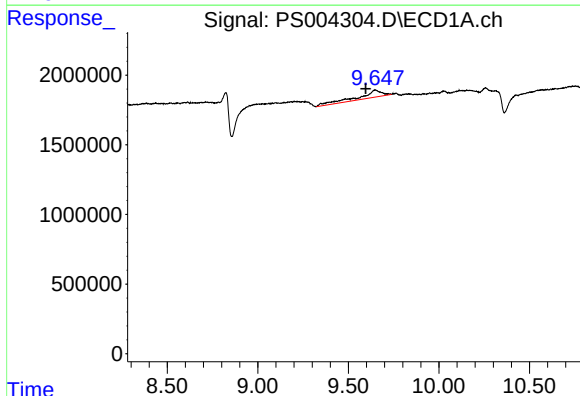


#15 Picloram

R.T.: 9.648 min
Delta R.T.: 0.051 min
Response: 4738217
Conc: 1.08 ng/ml

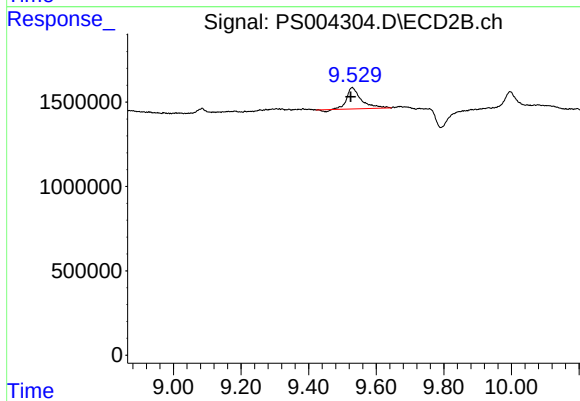

#15 Picloram


R.T.: 9.529 min
Delta R.T.: 0.005 min
Response: 3700203
Conc: N.D.

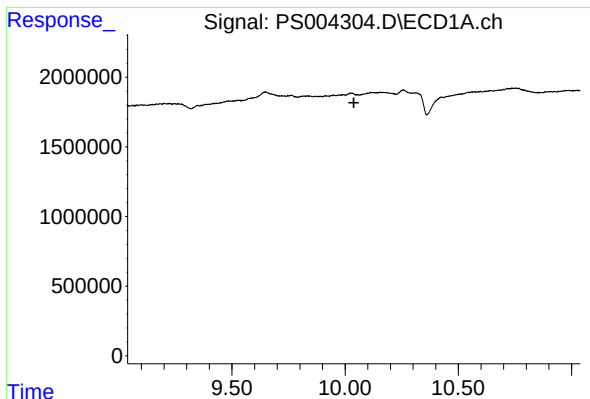

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 10.039 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HEXANE

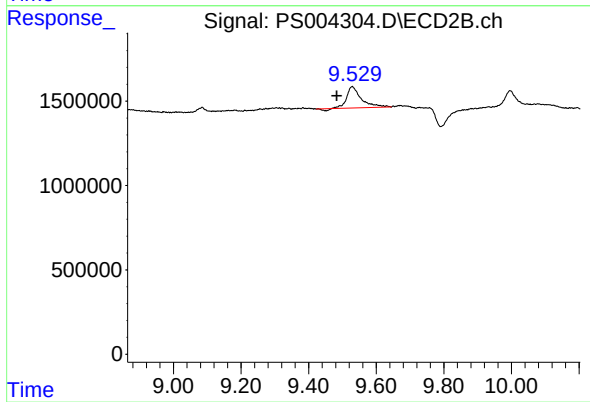

#16 DCPA

R.T.: 9.529 min
Delta R.T.: 0.046 min
Response: 3700203
Conc: 1.06 ng/ml