

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS042619\
 Data File : PS004312.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Apr 2019 19:51
 Operator : EI\SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 29 10:13:36 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS042619.M
 Quant Title : 8080.M
 QLast Update : Mon Apr 29 10:11:55 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.008	5.695	202.1E6	188.1E6	316.626	354.905
Target Compounds							
9) T	2,4-D	7.091	0.000	27677668	0	47.770	N.D. #
15) T	Picloram	0.000	9.536	0	4505870	N.D.	1.206
16) T	DCPA	0.000	9.536	0	4505870	N.D.	1.295



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS042619\
Data File : PS004312.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Apr 2019 19:51
Operator : EI\SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 29 10:13:36 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS042619.M
Quant Title : 8080.M
QLast Update : Mon Apr 29 10:11:55 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

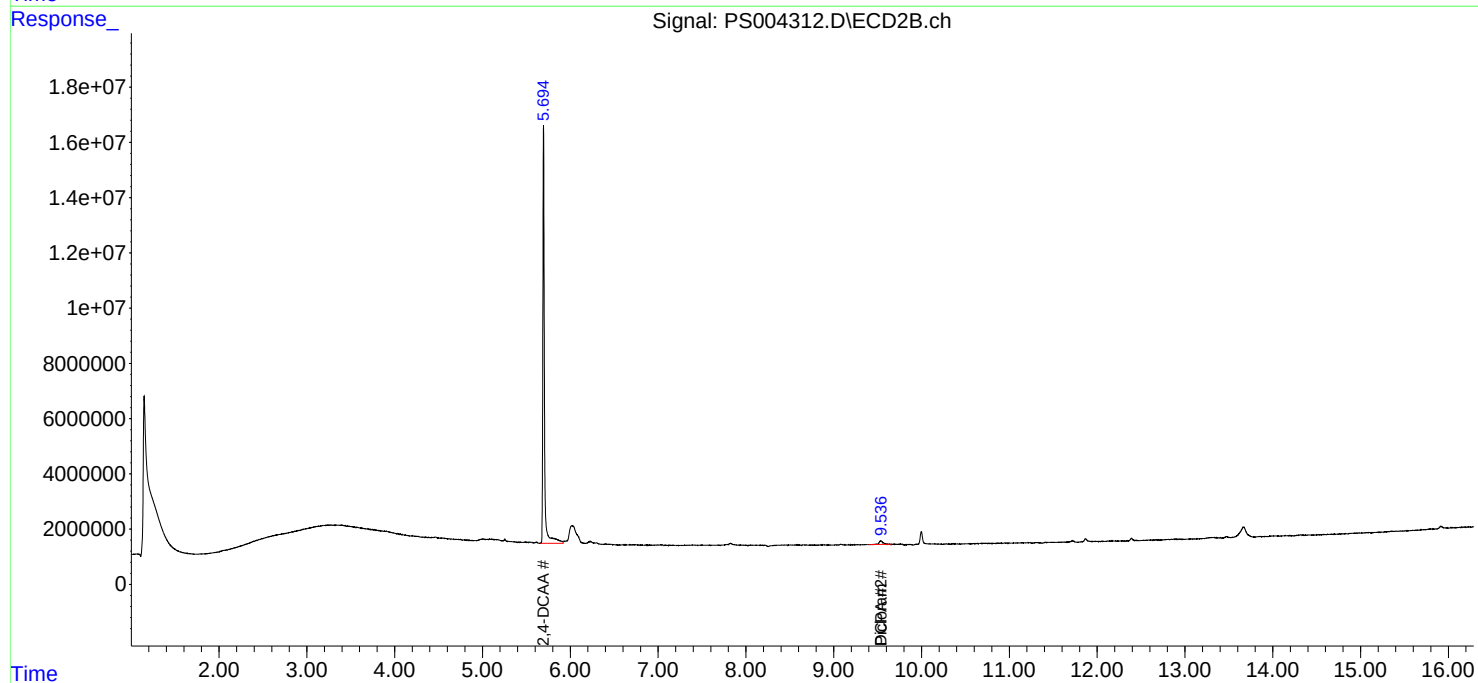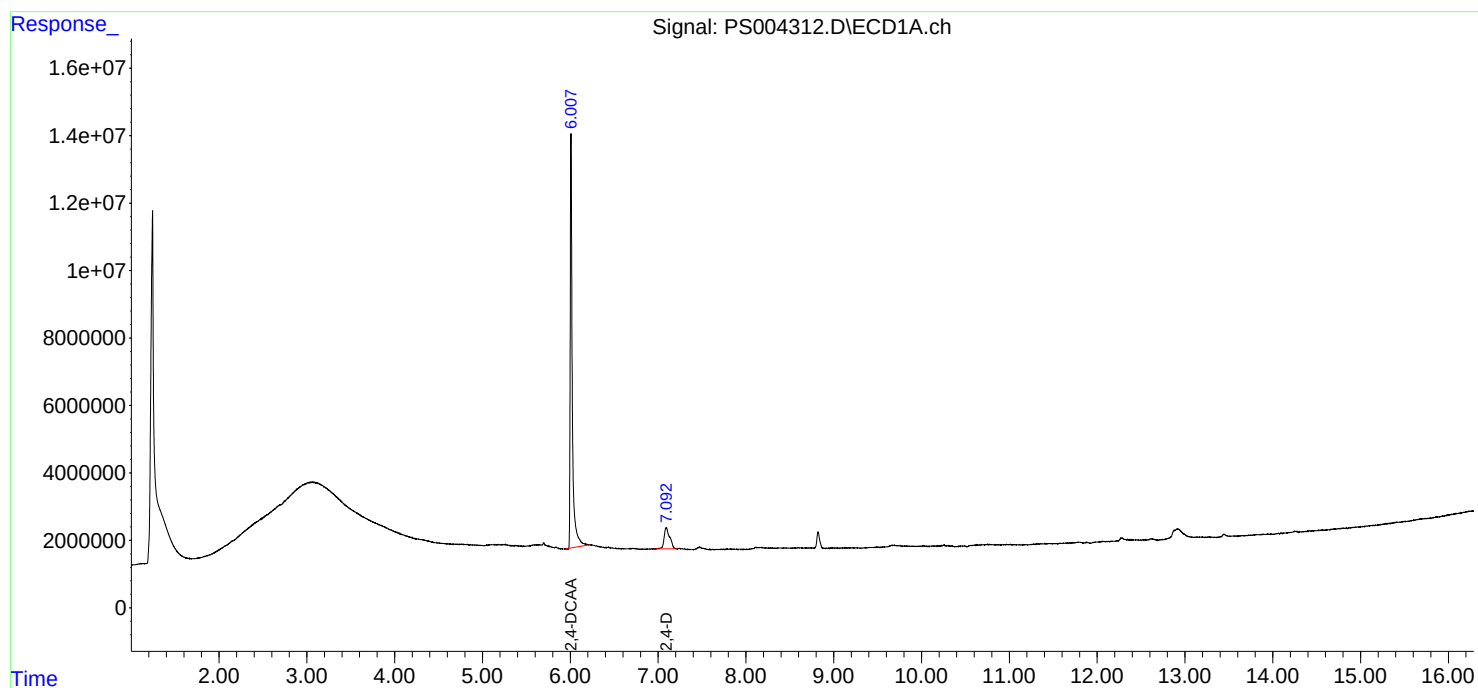


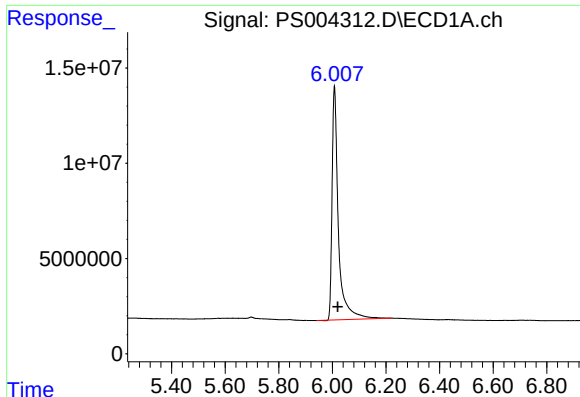

#4 2,4-DCAA


R.T.: 6.008 min
Delta R.T.: -0.013 min
Response: 202055763
Conc: 316.63 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

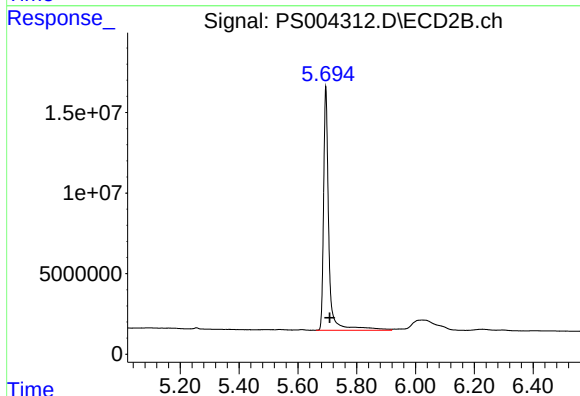


#4 2,4-DCAA

R.T.: 5.695 min
Delta R.T.: -0.013 min
Response: 188064335
Conc: 354.91 ng/ml

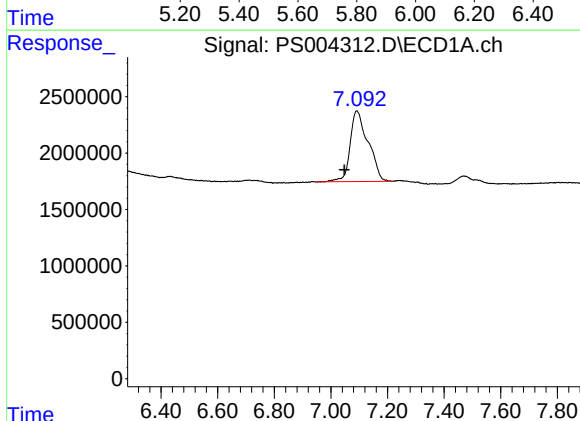


#9 2,4-D

R.T.: 7.091 min
Delta R.T.: 0.044 min
Response: 27677668
Conc: 47.77 ng/ml

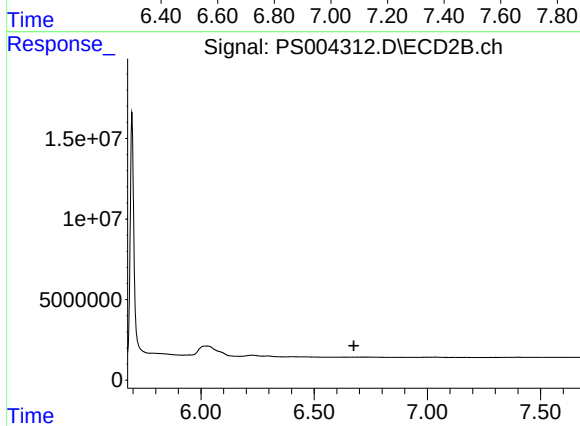

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 6.675 min
Response: 0
Conc: N.D.

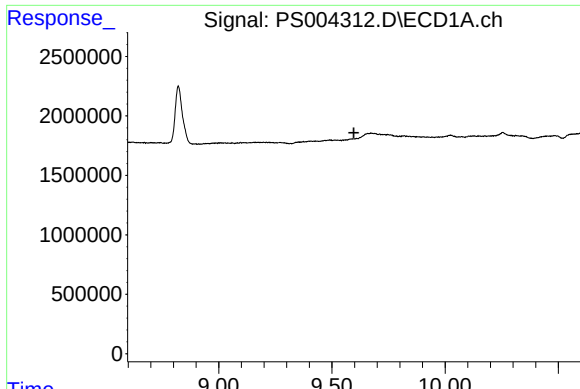

#15 Picloram


R.T.: 0.000 min
Exp R.T. : 9.597 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

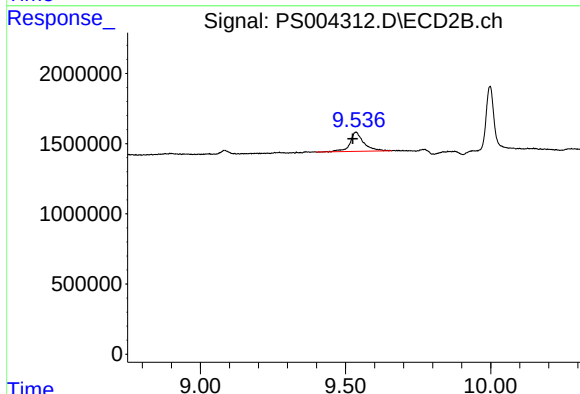


#15 Picloram

R.T.: 9.536 min
Delta R.T.: 0.011 min
Response: 4505870
Conc: 1.21 ng/ml

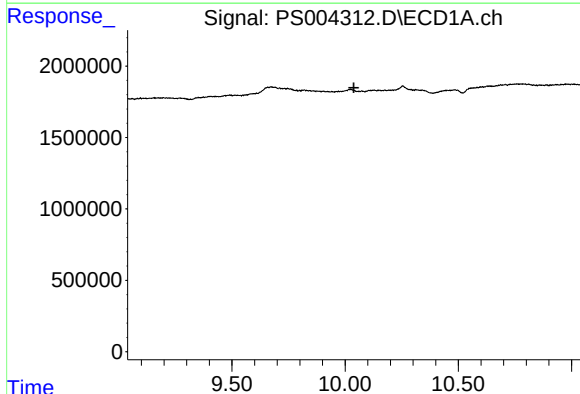

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 10.039 min
Response: 0
Conc: N.D.

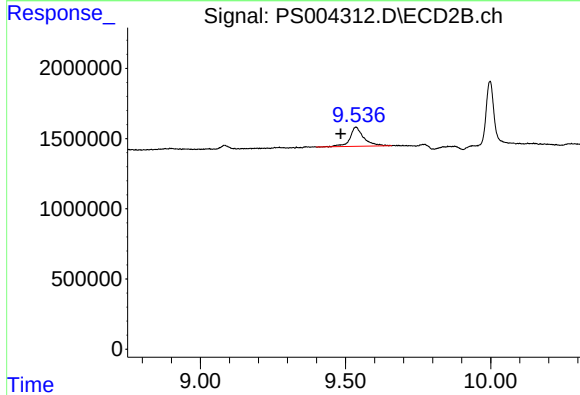

#16 DCPA

R.T.: 9.536 min
Delta R.T.: 0.053 min
Response: 4505870
Conc: 1.30 ng/ml