

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS042619\
 Data File : PS004314.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Apr 2019 20:55
 Operator : EI\SJ
 Sample : PB119241BL
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 PB119241BL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 29 10:14:04 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS042619.M
 Quant Title : 8080.M
 QLast Update : Mon Apr 29 10:11:55 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.996	5.684	214.1E6	184.4E6	335.570	348.055
Target Compounds							
6) T	MCP	0.000	5.998	0	40424257	N.D.	30.158
9) T	2,4-D	7.080	0.000	31134163	0	53.735	N.D. #
15) T	Picloram	0.000	9.527	0	3753544	N.D.	1.005
16) T	DCPA	0.000	9.527	0	3753544	N.D.	1.079



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS042619\
Data File : PS004314.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Apr 2019 20:55
Operator : EI\SJ
Sample : PB119241BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
PB119241BL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 29 10:14:04 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS042619.M
Quant Title : 8080.M
QLast Update : Mon Apr 29 10:11:55 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

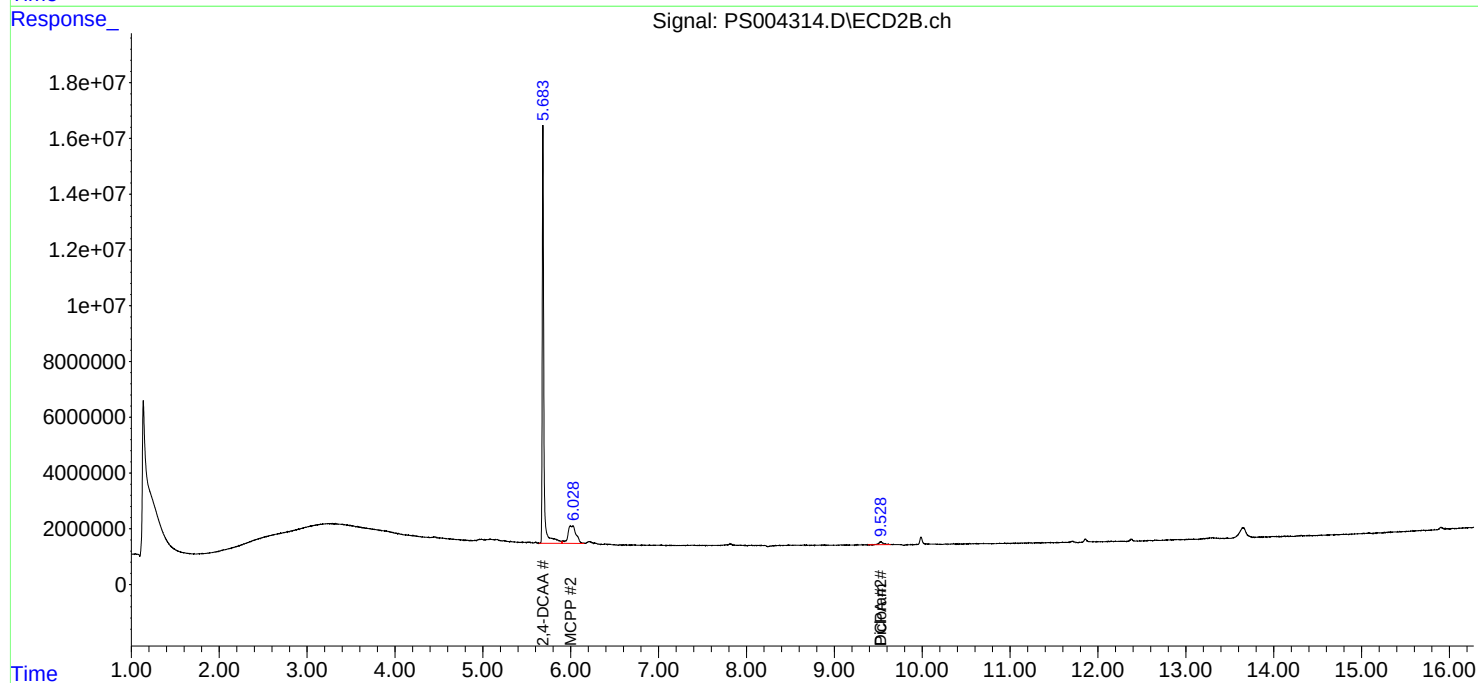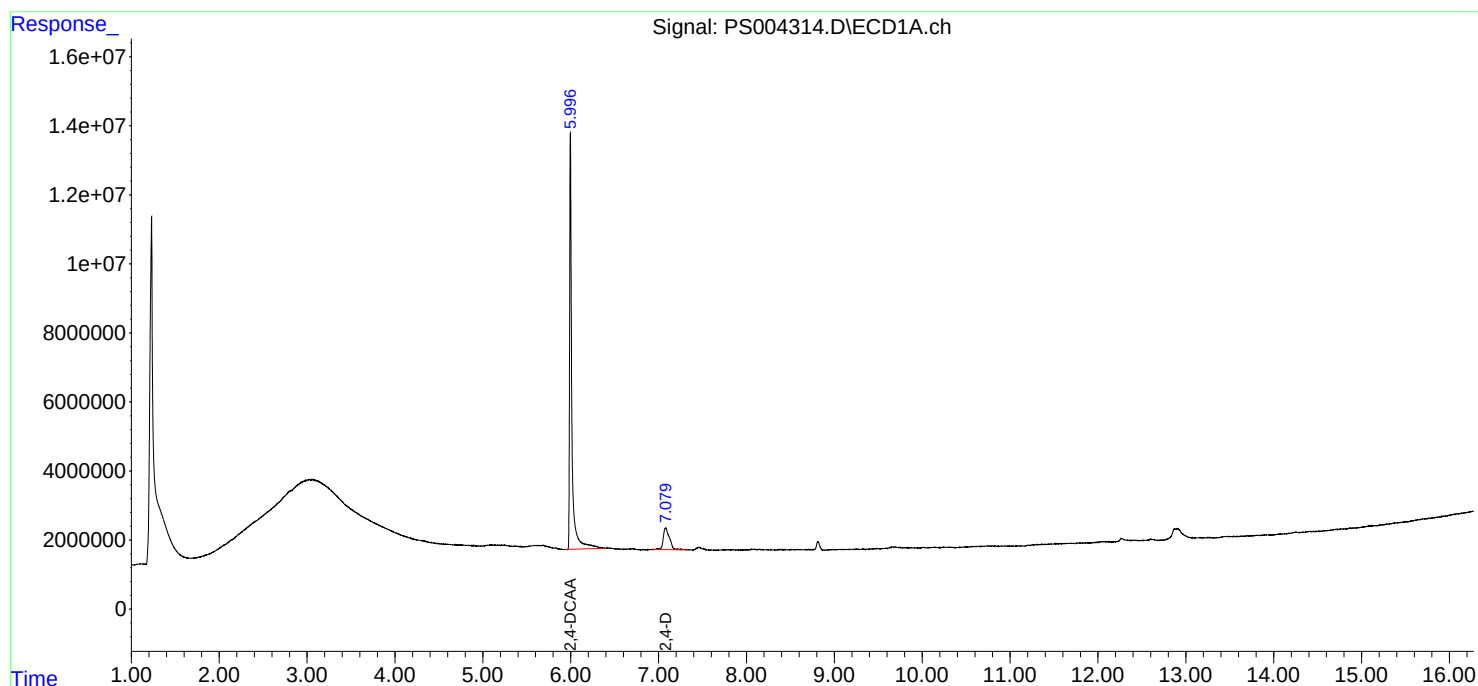


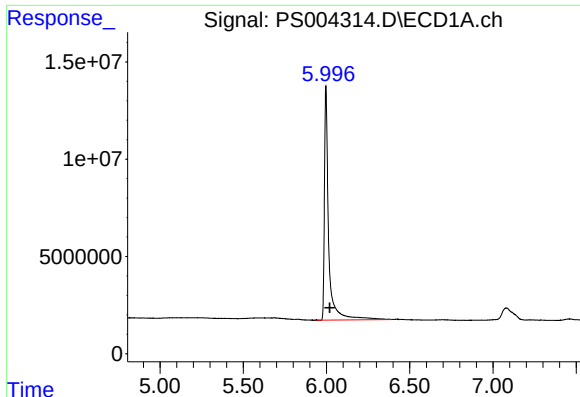

#4 2,4-DCAA


R.T.: 5.996 min
Delta R.T.: -0.024 min
Response: 214145173
Conc: 335.57 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB119241BL

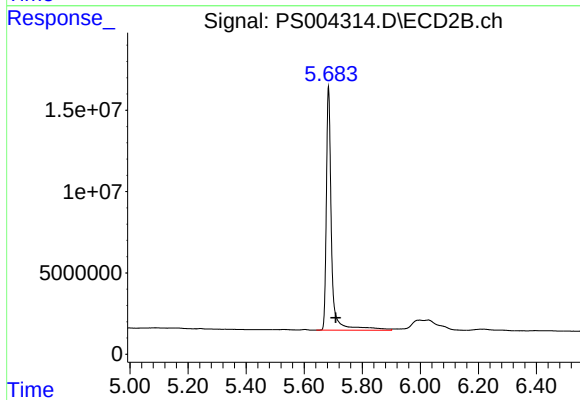


#4 2,4-DCAA

R.T.: 5.684 min
Delta R.T.: -0.024 min
Response: 184434013
Conc: 348.05 ng/ml

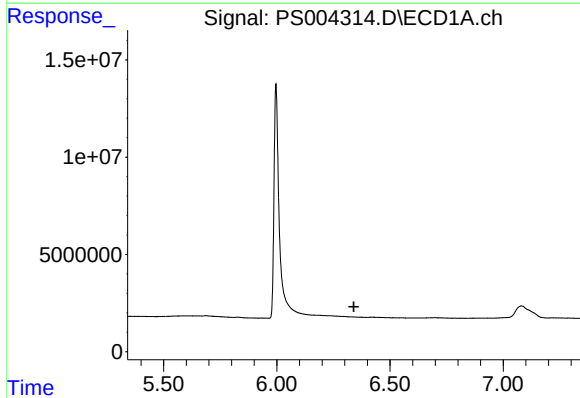


#6 MCP

R.T.: 0.000 min
Exp R.T.: 6.341 min
Response: 0
Conc: N.D.

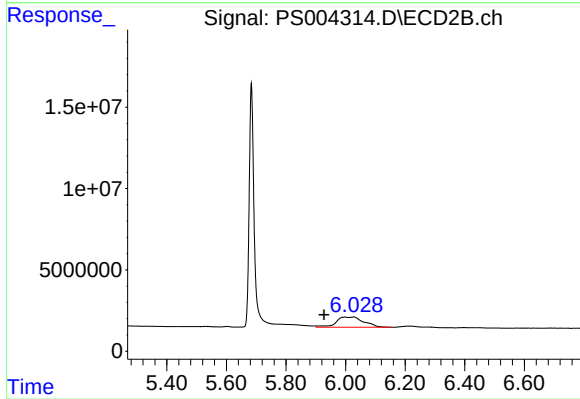

#6 MCP


R.T.: 5.998 min
Delta R.T.: 0.069 min
Response: 40424257
Conc: 30.16 ug/ml

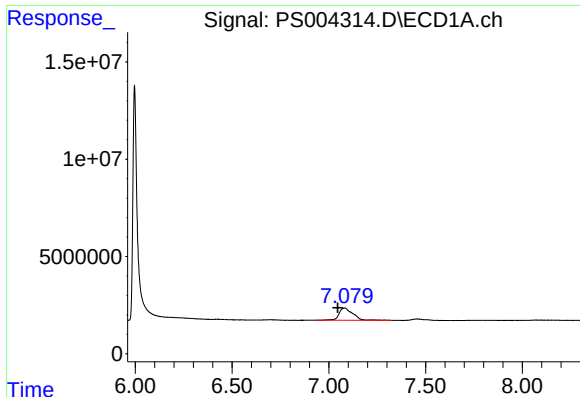

#9 2,4-D


R.T.: 7.080 min
Delta R.T.: 0.033 min
Response: 31134163
Conc: 53.74 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB119241BL

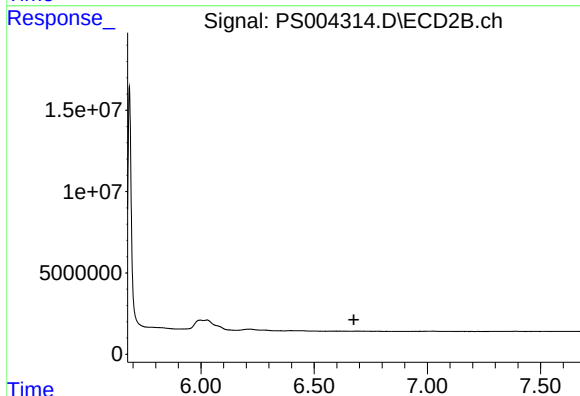


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 6.675 min
Response: 0
Conc: N.D.

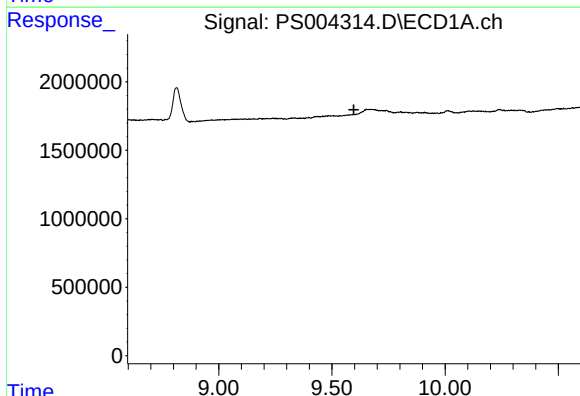


#15 Picloram

R.T.: 0.000 min
Exp R.T. : 9.597 min
Response: 0
Conc: N.D.

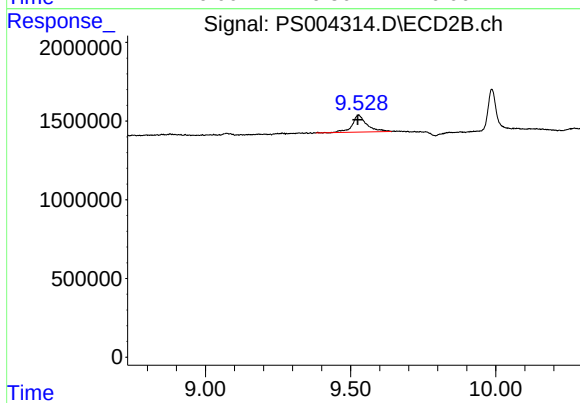

#15 Picloram


R.T.: 9.527 min
Delta R.T.: 0.003 min
Response: 3753544
Conc: 1.00 ng/ml

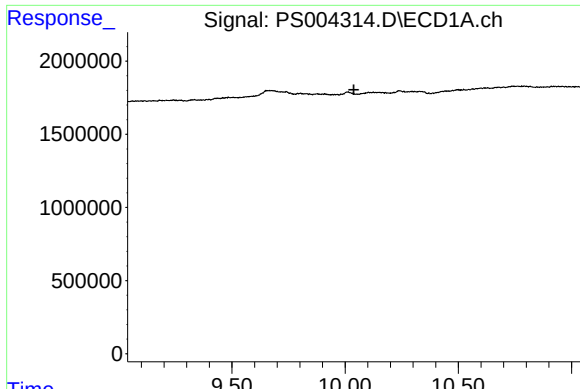

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 10.039 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
PB119241BL

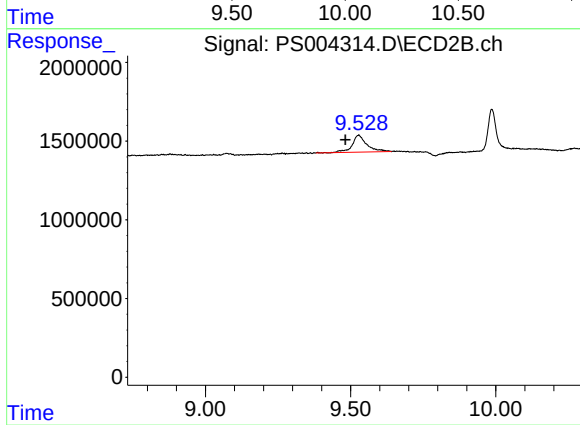

#16 DCPA

R.T.: 9.527 min
Delta R.T.: 0.045 min
Response: 3753544
Conc: 1.08 ng/ml