

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS042619\
 Data File : PS004316.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Apr 2019 21:58
 Operator : EI\SJ
 Sample : PB119241TB
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 29 10:14:35 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS042619.M
 Quant Title : 8080.M
 QLast Update : Mon Apr 29 10:11:55 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.008	5.696	214.2E6	185.2E6	335.694	349.457
Target Compounds							
9) T	2,4-D	7.091	0.000	31142245	0	53.749	N.D. #
15) T	Picloram	0.000	9.535	0	3255859	N.D.	<MDL
16) T	DCPA	0.000	9.535	0	3255859	N.D.	<MDL



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS042619\
Data File : PS004316.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Apr 2019 21:58
Operator : EI\SJ
Sample : PB119241TB
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 29 10:14:35 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS042619.M
Quant Title : 8080.M
QLast Update : Mon Apr 29 10:11:55 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

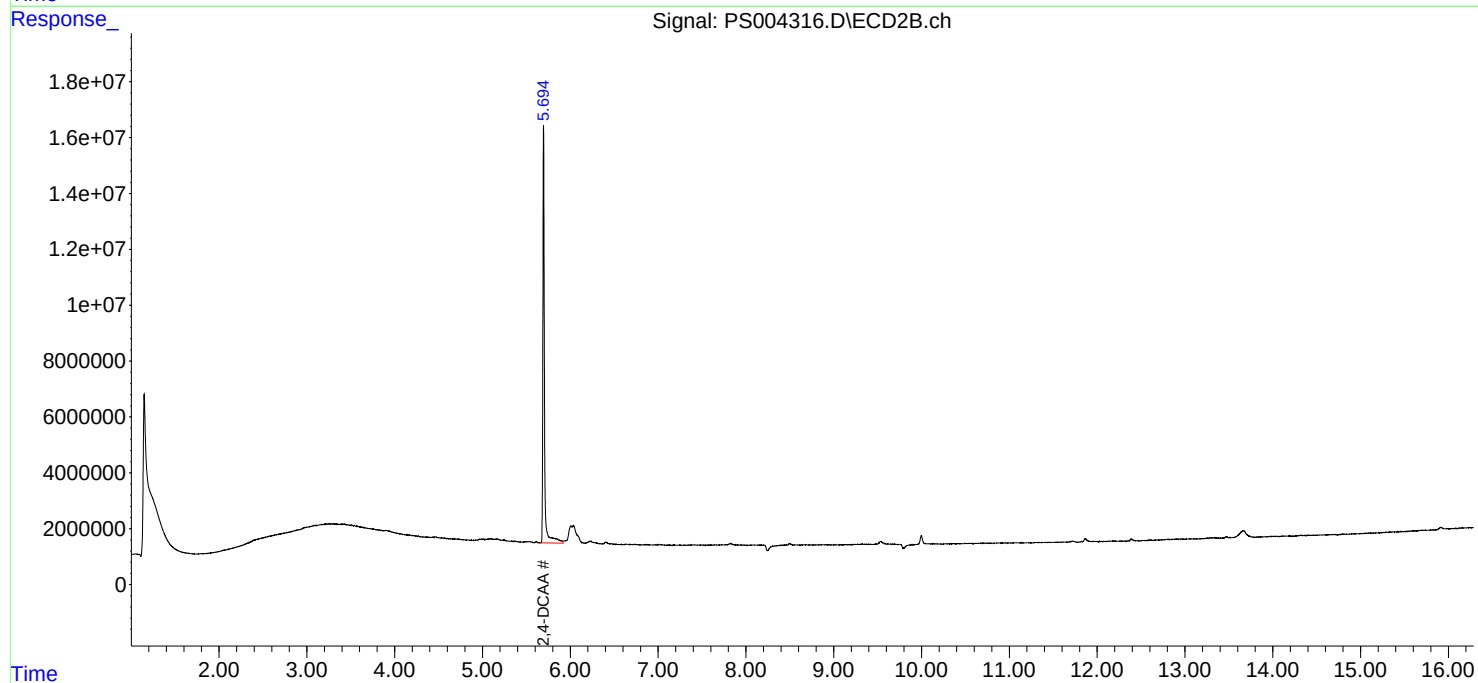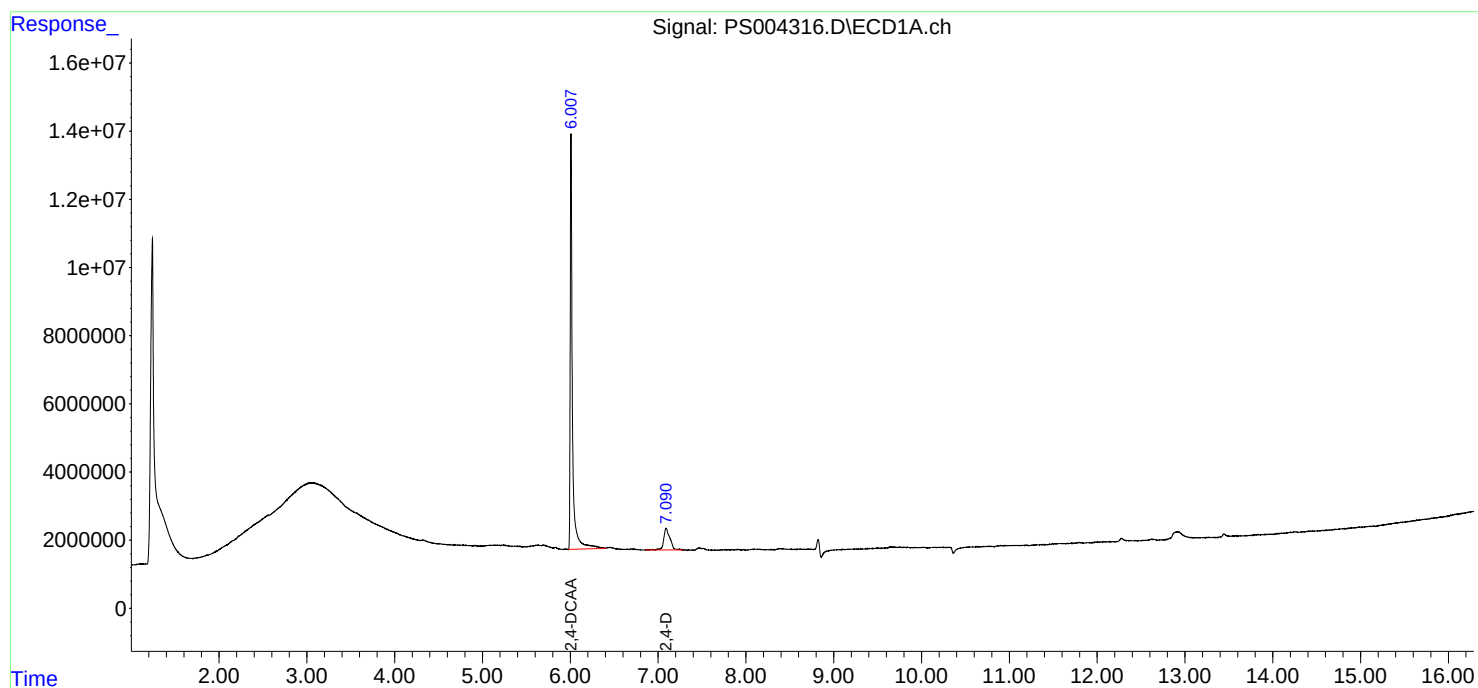


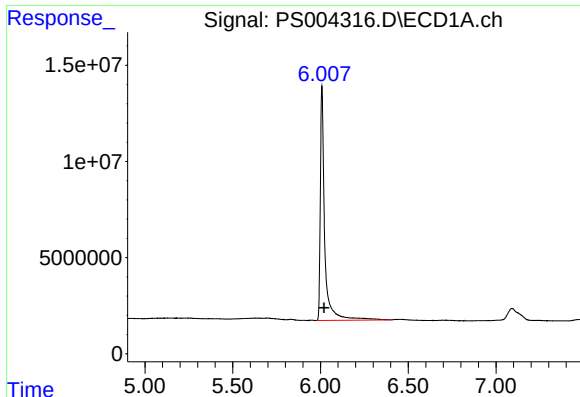

#4 2,4-DCAA


R.T.: 6.008 min
Delta R.T.: -0.012 min
Response: 214224303
Conc: 335.69 ng/ml

Instrument :
ECD_S
ClientSampleId :

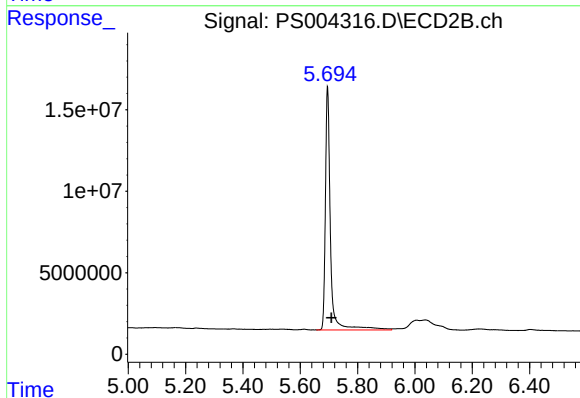


#4 2,4-DCAA

R.T.: 5.696 min
Delta R.T.: -0.013 min
Response: 185177326
Conc: 349.46 ng/ml

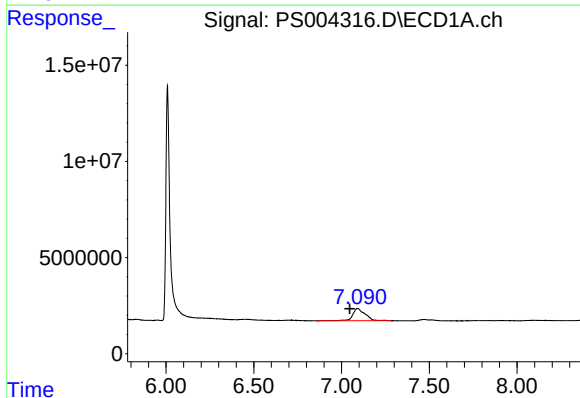

#9 2,4-D

R.T.: 7.091 min
Delta R.T.: 0.043 min
Response: 31142245
Conc: 53.75 ng/ml

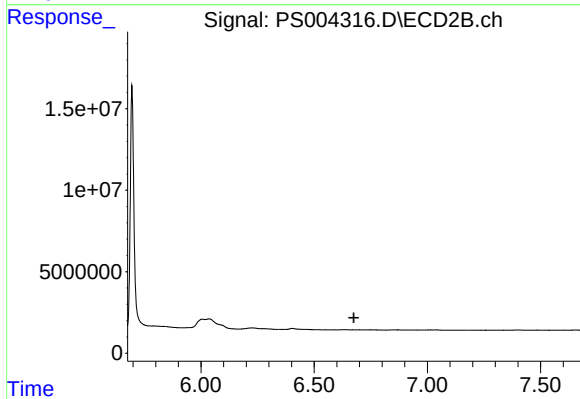

#9 2,4-D

R.T.: 0.000 min
Exp R.T.: 6.675 min
Response: 0
Conc: N.D.