

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS042720\
 Data File : PS010044.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Apr 2020 09:09
 Operator : DD\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 27 14:21:06 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS040820.M
 Quant Title : 8080.M
 QLast Update : Thu Apr 09 05:27:48 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds						
5) T	DICAMBA	0.000	7.152	0	19927602	N.D. 10.019
6) T	MCPP	0.000	7.237	0	12642695	N.D. 7.681
8) T	DICHLORPROP	0.000	7.741	0	1425650	N.D. 2.833
11) T	2,4,5-TP ...	0.000	8.801	0	1633771	N.D. <MDL
12) T	2,4,5-T	0.000	9.236	0	6087165	N.D. 2.333
13) T	2,4-DB	0.000	9.706	0	4336711	N.D. 12.231
15) T	Picloram	11.036	11.005	11680316	16131646	3.770 4.743 #
16) T	DCPA	0.000	10.951	0	1115108	N.D. <MDL



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS042720\
Data File : PS010044.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Apr 2020 09:09
Operator : DD\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 27 14:21:06 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS040820.M
Quant Title : 8080.M
QLast Update : Thu Apr 09 05:27:48 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

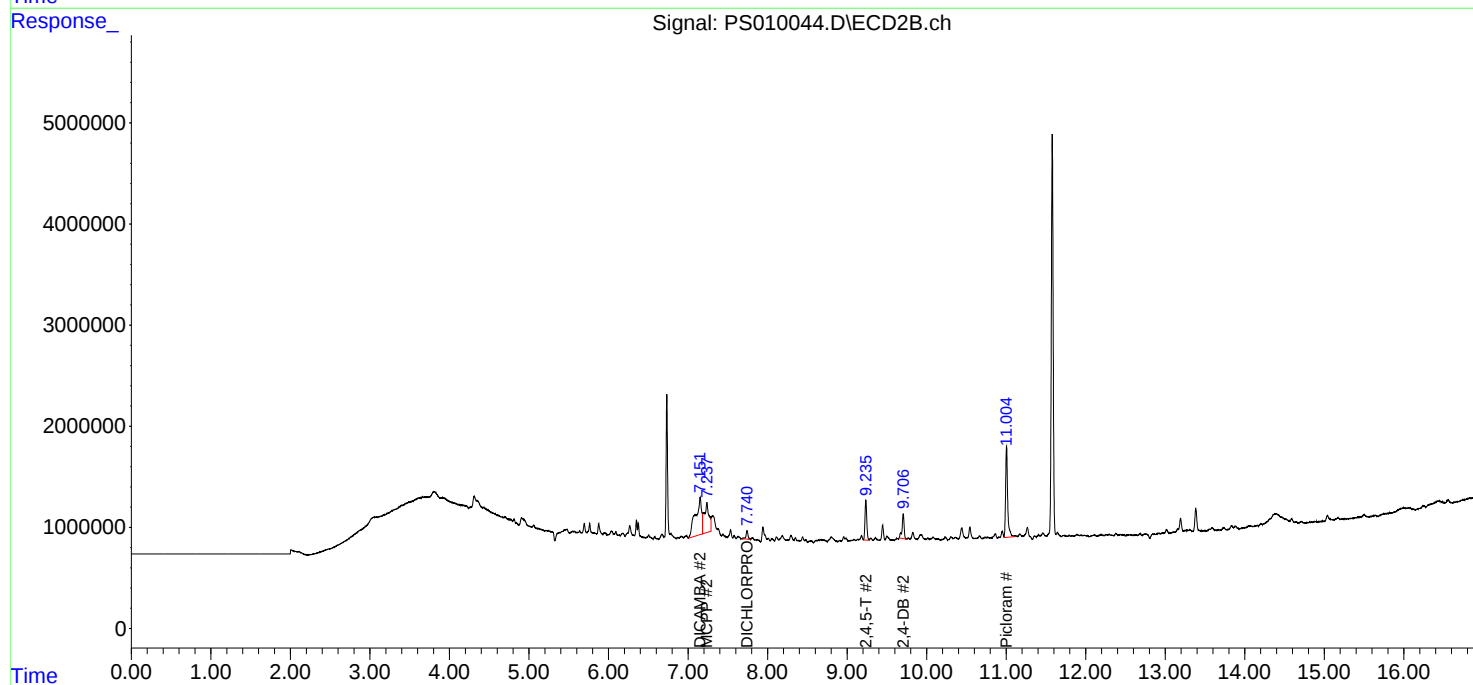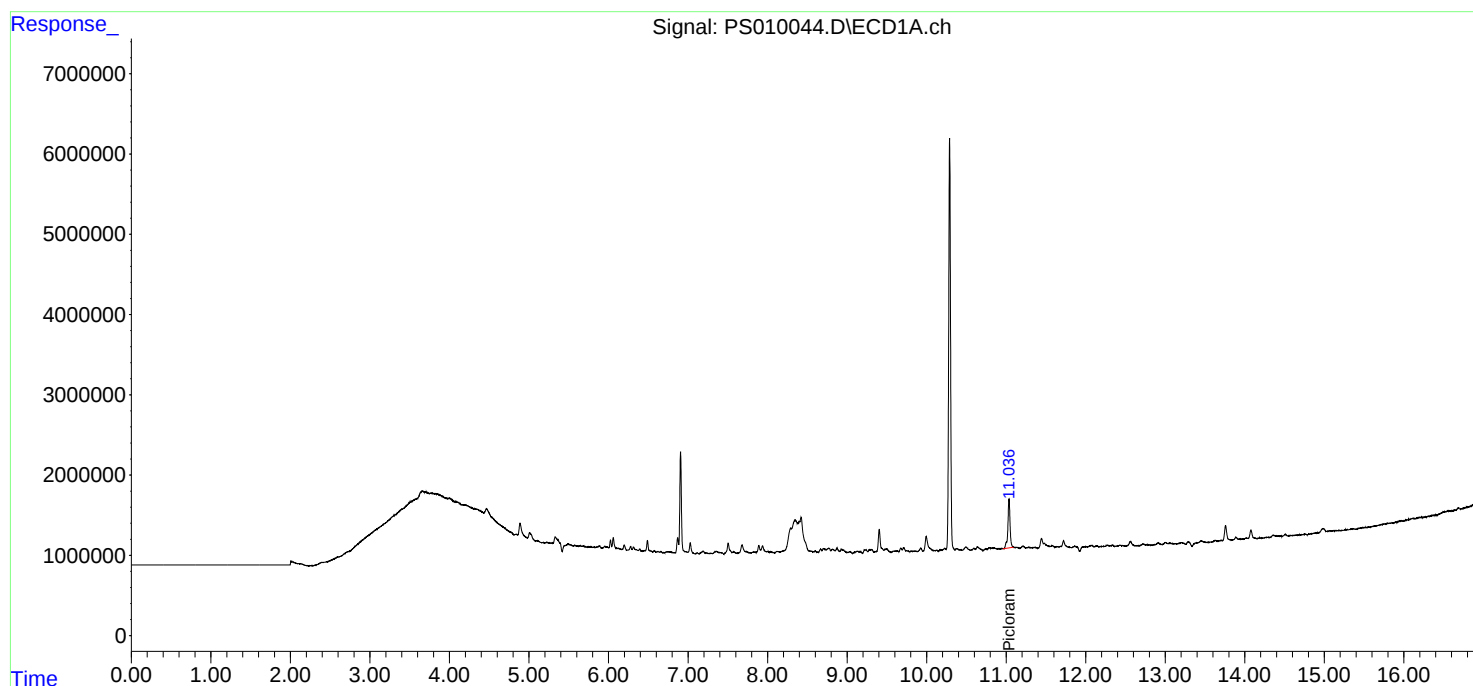


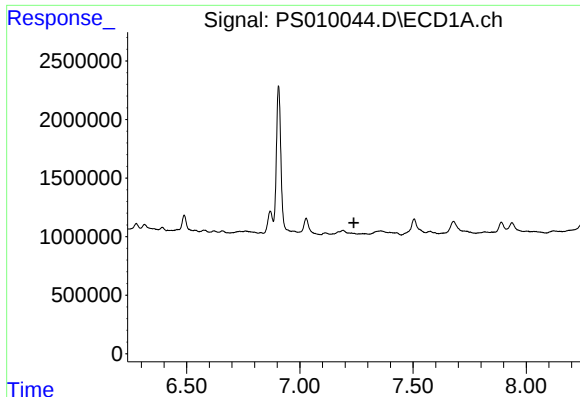

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T. : 7.239 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

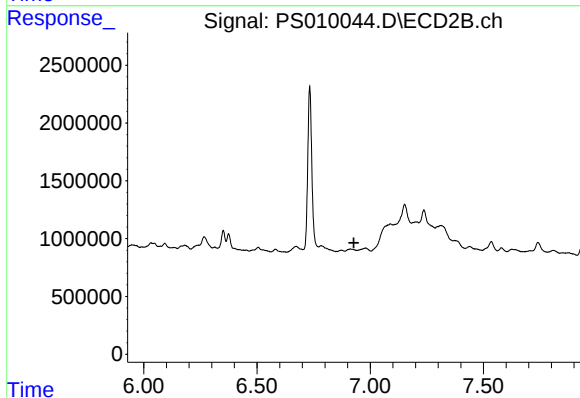


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T. : 6.928 min
Response: 0
Conc: N.D.

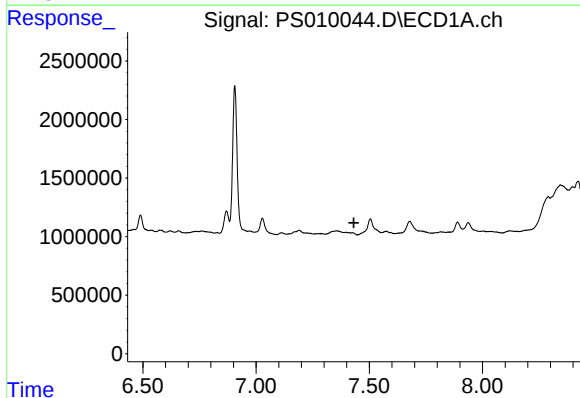


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 7.432 min
Response: 0
Conc: N.D.

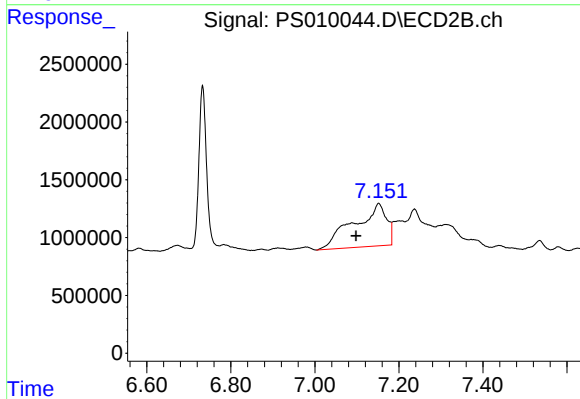

#5 DICAMBA


R.T.: 7.152 min
Delta R.T.: 0.054 min
Response: 19927602
Conc: 10.02 ng/ml

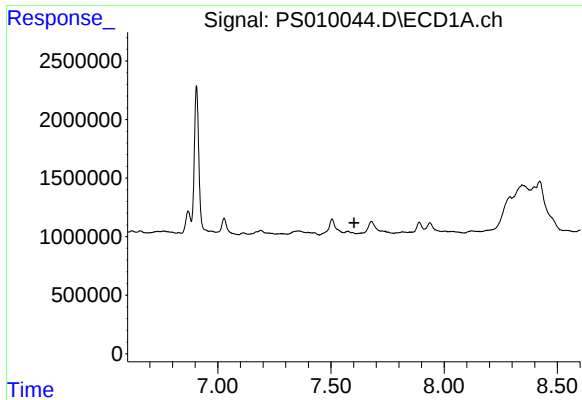

#6 MCP


R.T.: 0.000 min
Exp R.T.: 7.602 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

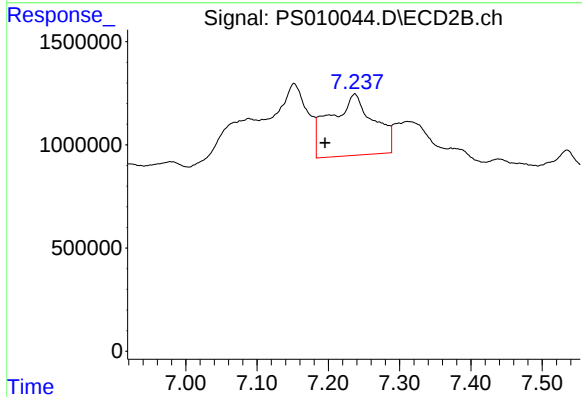


#6 MCP

R.T.: 7.237 min
Delta R.T.: 0.041 min
Response: 12642695
Conc: 7.68 ug/ml

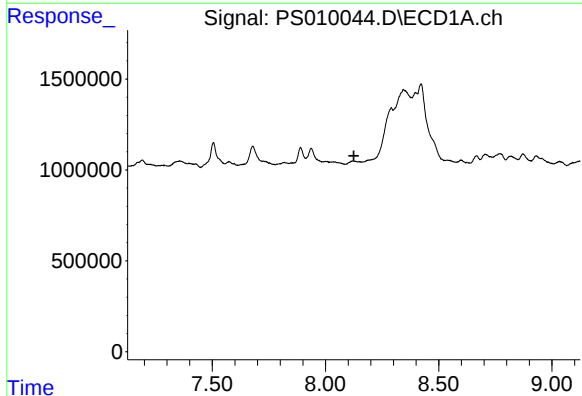


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T.: 8.125 min
Response: 0
Conc: N.D.

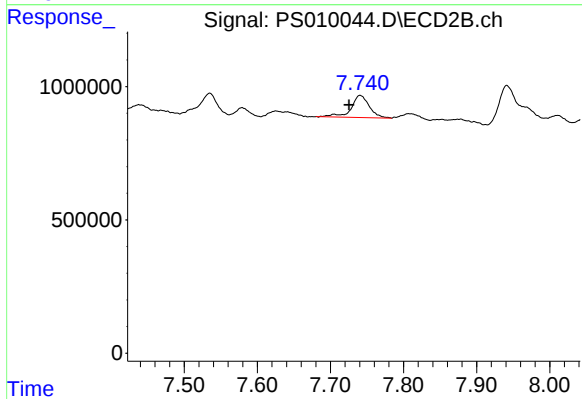

#8 DICHLORPROP


R.T.: 7.741 min
Delta R.T.: 0.016 min
Response: 1425650
Conc: 2.83 ng/ml

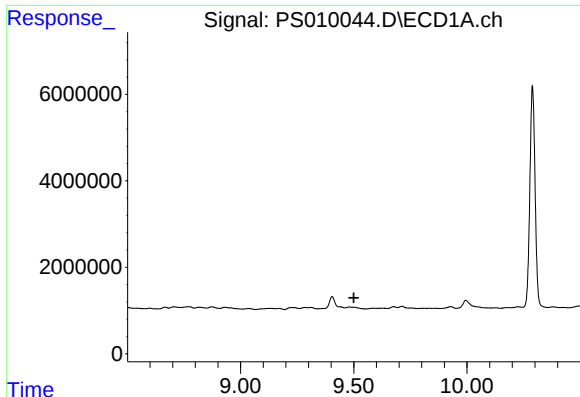

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 9.501 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

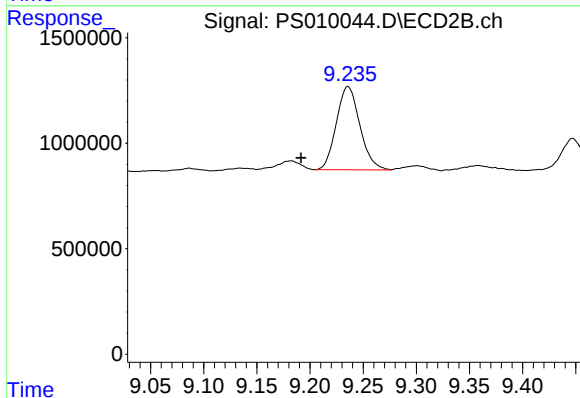


#12 2,4,5-T

R.T.: 9.236 min
Delta R.T.: 0.044 min
Response: 6087165
Conc: 2.33 ng/ml

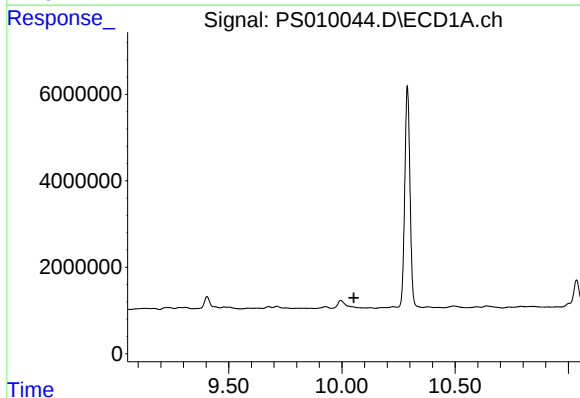


#13 2,4-DB

R.T.: 0.000 min
Exp R.T.: 10.053 min
Response: 0
Conc: N.D.

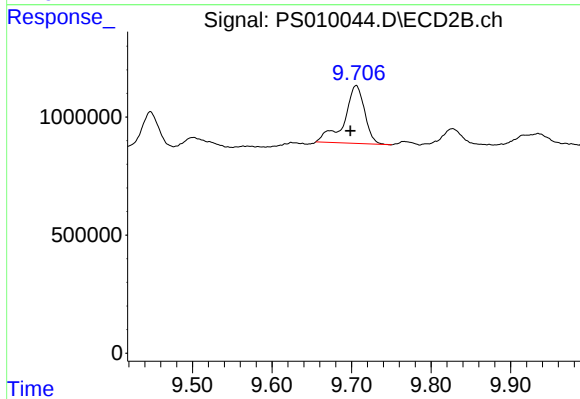

#13 2,4-DB


R.T.: 9.706 min
Delta R.T.: 0.007 min
Response: 4336711
Conc: 12.23 ng/ml

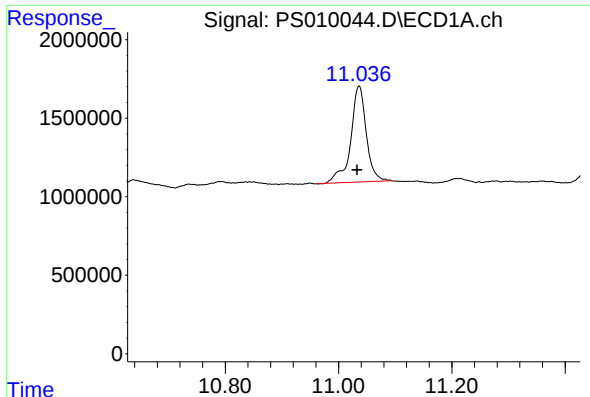

#15 Picloram

R.T.: 11.036 min
Delta R.T.: 0.004 min
Response: 11680316
Conc: 3.77 ng/ml

Instrument :
ECD_S
ClientSampleId :

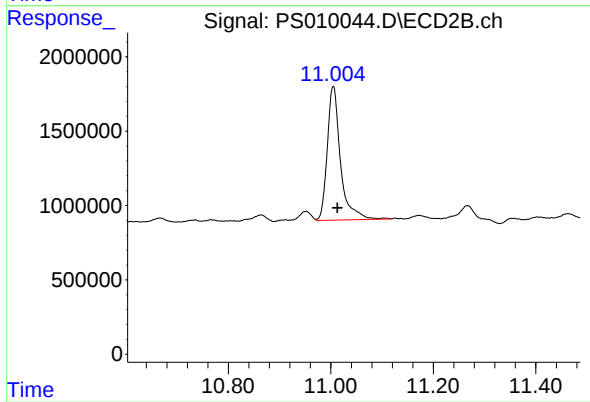

#15 Picloram

R.T.: 11.005 min
Delta R.T.: -0.008 min
Response: 16131646
Conc: 4.74 ng/ml