

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS042721\
 Data File : PS014786.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Apr 2021 08:20
 Operator : DD\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 27 10:52:53 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS040821.M
 Quant Title : 8080.M
 QLast Update : Thu Apr 08 14:34:06 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds						
6) T	MCP	0.000	7.195f	0	1156409	N.D. <MDL
8) T	DICHLORPROP	0.000	7.703	0	7306891	N.D. 14.474
9) T	2,4-D	8.330f	0.000	8225247	0	5.173 N.D. #
11) T	2,4,5-TP ...	0.000	8.734	0	3437208	N.D. 1.258
12) T	2,4,5-T	9.416	0.000	5757360	0	<MDL N.D. #
13) T	2,4-DB	9.921	9.590f	6415185	2576461	4.216 7.428 #
15) T	Picloram	10.947	10.974	93014264	39612797	8.314 10.564 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS042721\
Data File : PS014786.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Apr 2021 08:20
Operator : DD\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 27 10:52:53 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS040821.M
Quant Title : 8080.M
QLast Update : Thu Apr 08 14:34:06 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

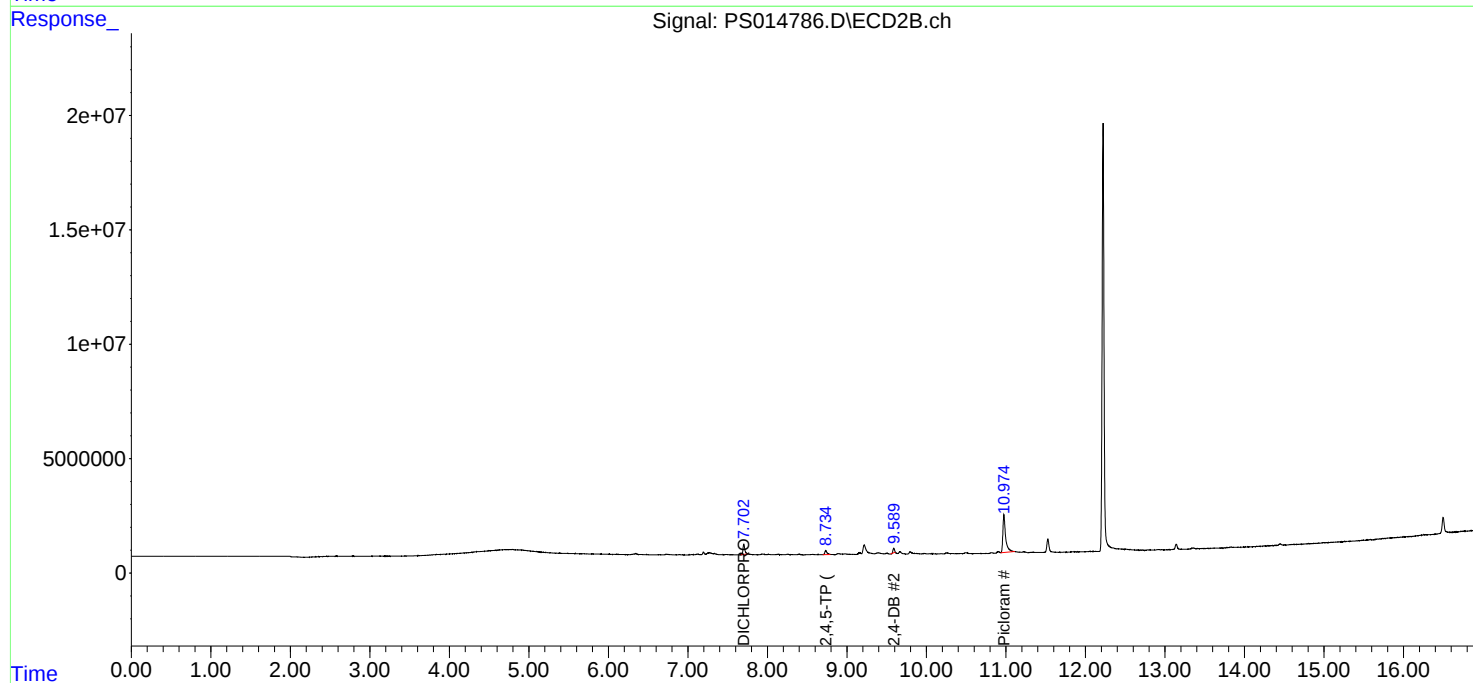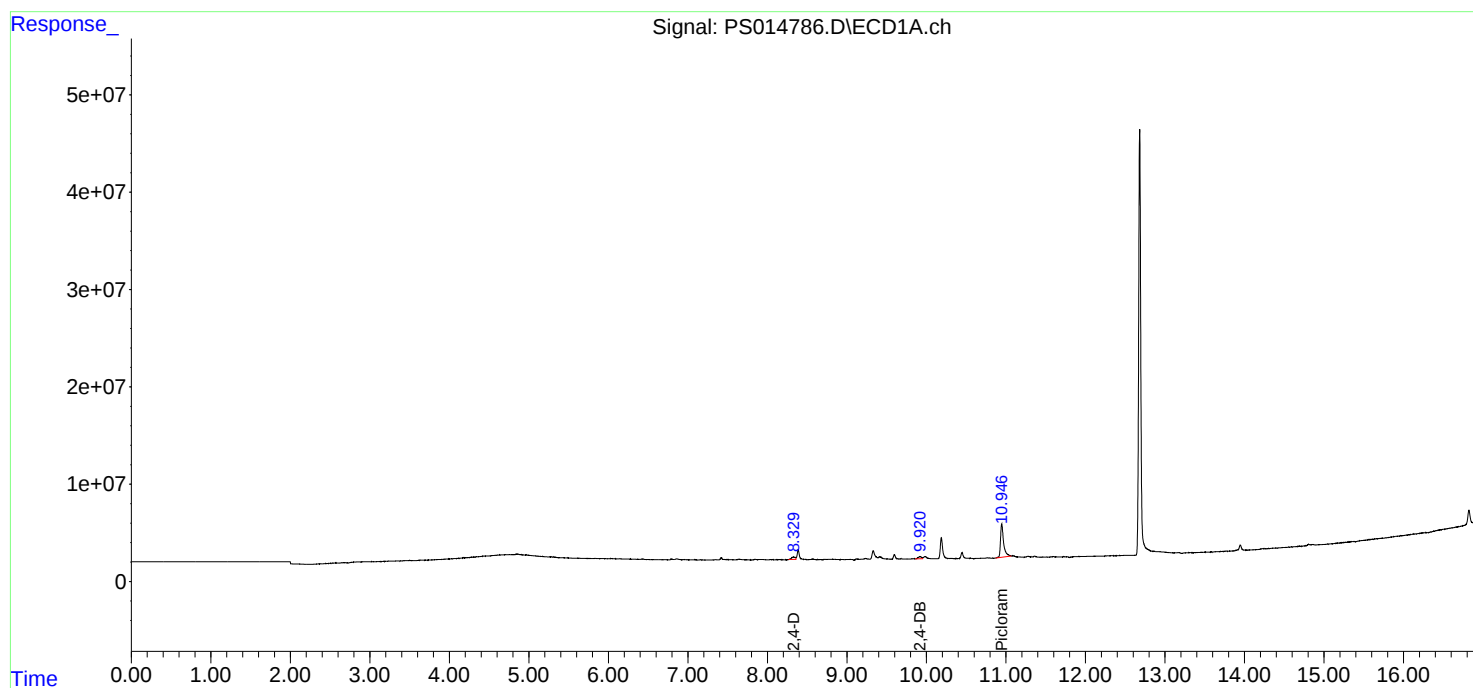


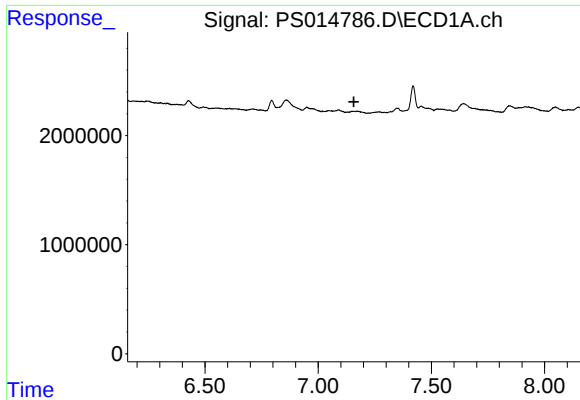

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T. : 7.158 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

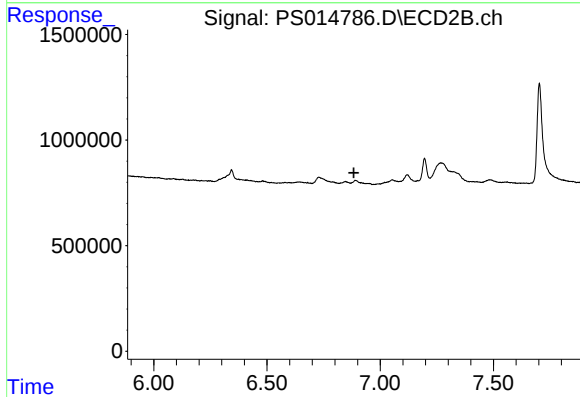


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T. : 6.884 min
Response: 0
Conc: N.D.

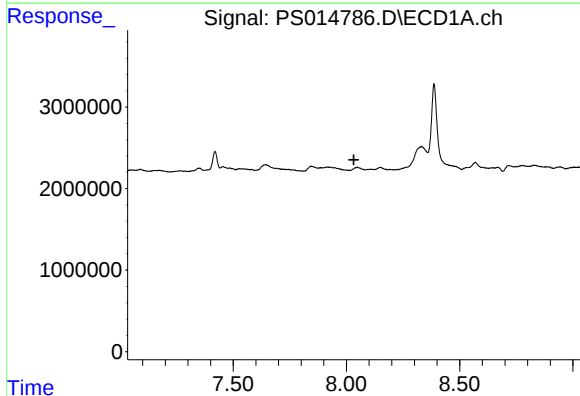


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 8.033 min
Response: 0
Conc: N.D.

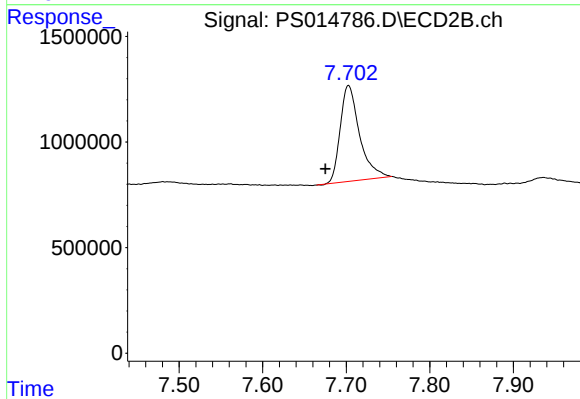

#8 DICHLORPROP


R.T.: 7.703 min
Delta R.T.: 0.028 min
Response: 7306891
Conc: 14.47 ng/ml

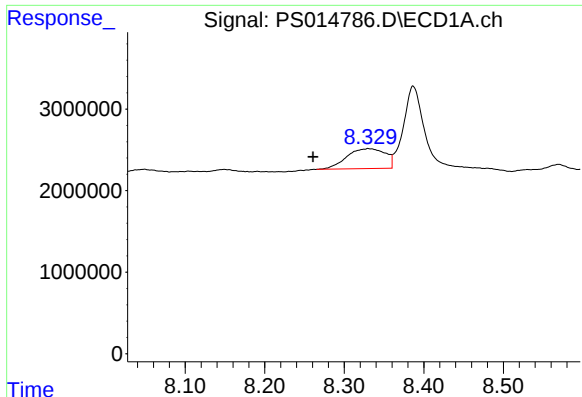

#9 2,4-D


R.T.: 8.330 min
Delta R.T.: 0.069 min
Response: 8225247
Conc: 5.17 ng/ml

Instrument :
ECD_S
ClientSampleId :

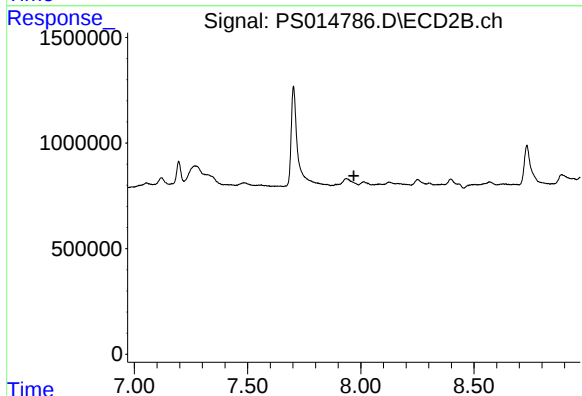


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 7.970 min
Response: 0
Conc: N.D.

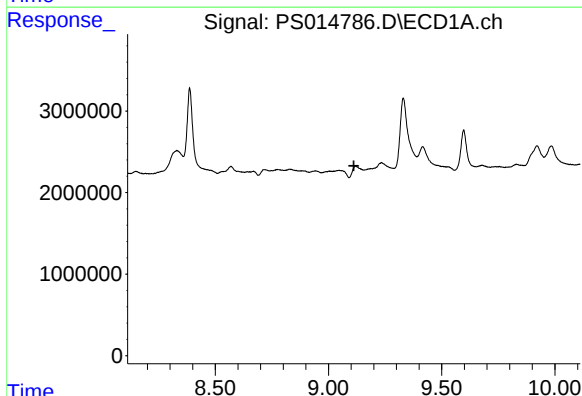


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T. : 9.112 min
Response: 0
Conc: N.D.

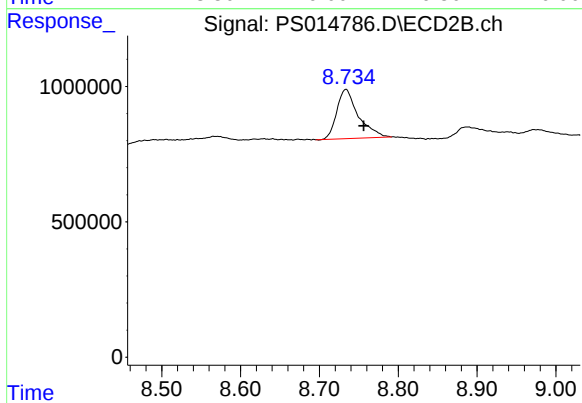

#11 2,4,5-TP (SILVEX)


R.T.: 8.734 min
Delta R.T.: -0.022 min
Response: 3437208
Conc: 1.26 ng/ml

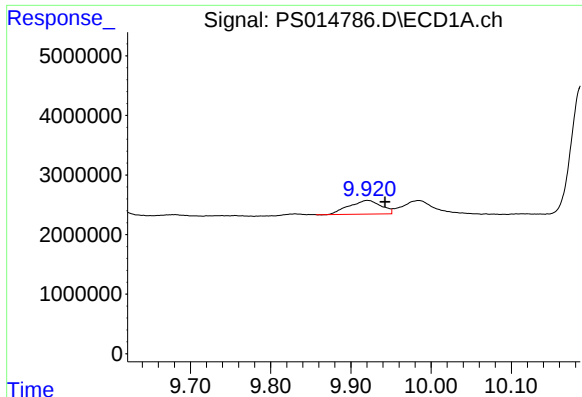

#13 2,4-DB


R.T.: 9.921 min
Delta R.T.: -0.022 min
Response: 6415185
Conc: 4.22 ng/ml

Instrument :
ECD_S
ClientSampleId :

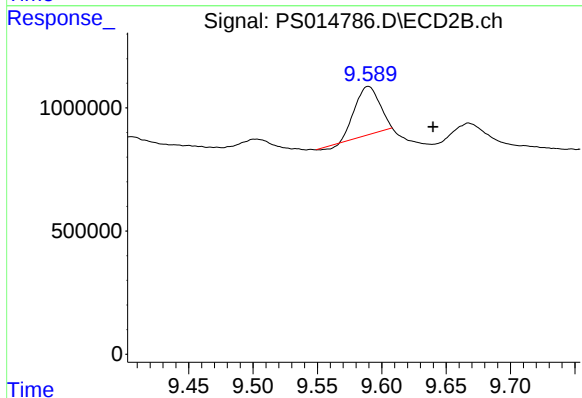


#13 2,4-DB

R.T.: 9.590 min
Delta R.T.: -0.050 min
Response: 2576461
Conc: 7.43 ng/ml

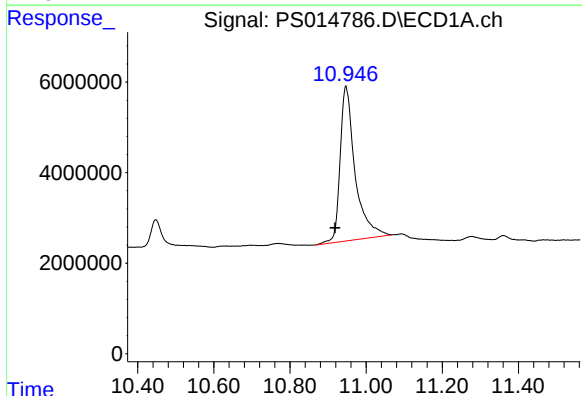

#15 Picloram

R.T.: 10.947 min
Delta R.T.: 0.028 min
Response: 93014264
Conc: 8.31 ng/ml

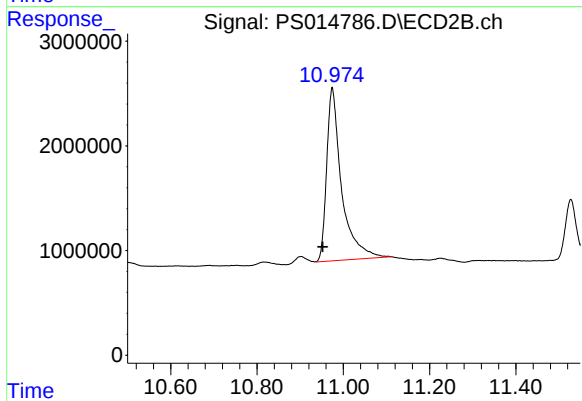

#15 Picloram

R.T.: 10.974 min
Delta R.T.: 0.022 min
Response: 39612797
Conc: 10.56 ng/ml