

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS042820\
 Data File : PS010058.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Apr 2020 07:54
 Operator : DD\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 28 15:56:01 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS040820.M
 Quant Title : 8080.M
 QLast Update : Thu Apr 09 05:27:48 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds						
5) T	DICAMBA	0.000	7.155	0	3133798	N.D. 1.576
6) T	MCPP	0.000	7.155	0	3133798	N.D. 1.904
8) T	DICHLORPROP	0.000	7.743	0	1256201	N.D. 2.496
9) T	2,4-D	8.419	0.000	5717326	0	9.957 N.D. #
12) T	2,4,5-T	0.000	9.239	0	5046458	N.D. 1.934
13) T	2,4-DB	0.000	9.708	0	4533805	N.D. 12.787
15) T	Picloram	11.032	11.007	11466151	15461460	3.701 4.546
16) T	DCPA	0.000	10.952	0	1102098	N.D. <MDL



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS042820\
Data File : PS010058.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Apr 2020 07:54
Operator : DD\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 28 15:56:01 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS040820.M
Quant Title : 8080.M
QLast Update : Thu Apr 09 05:27:48 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

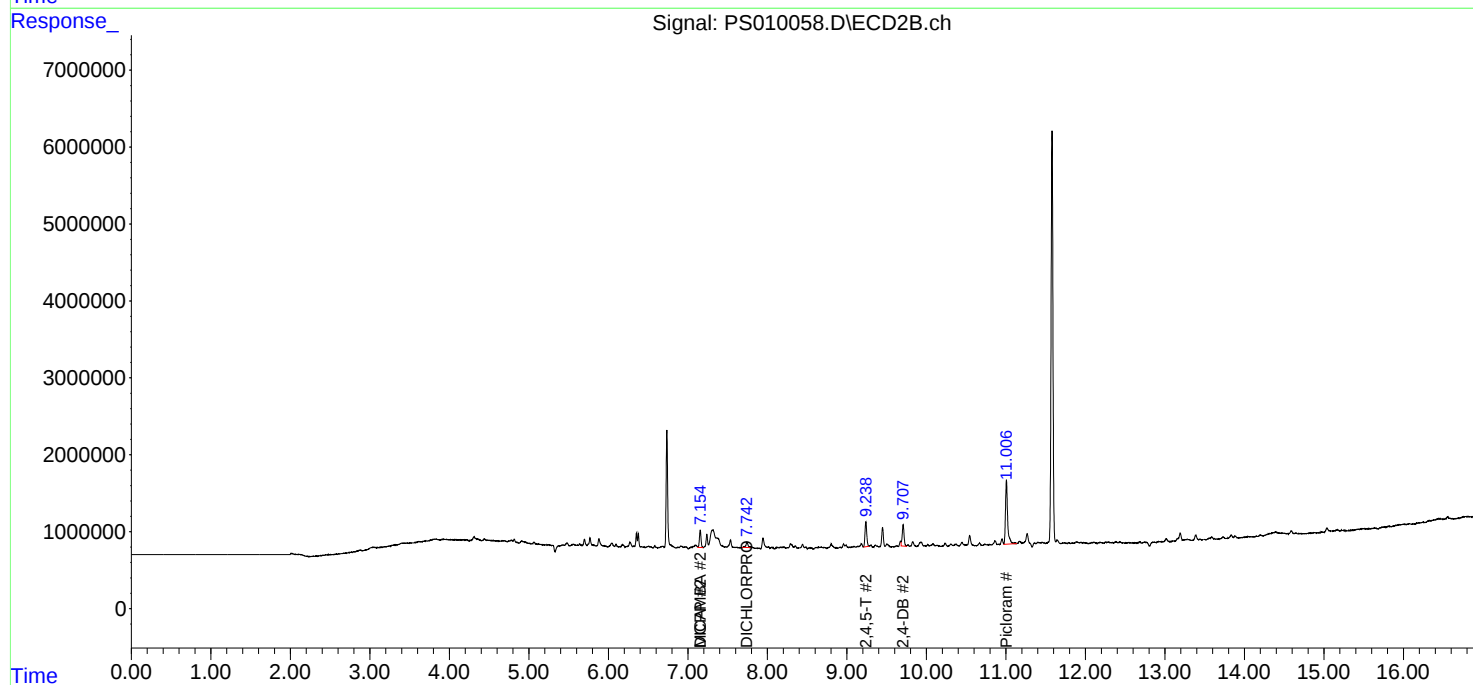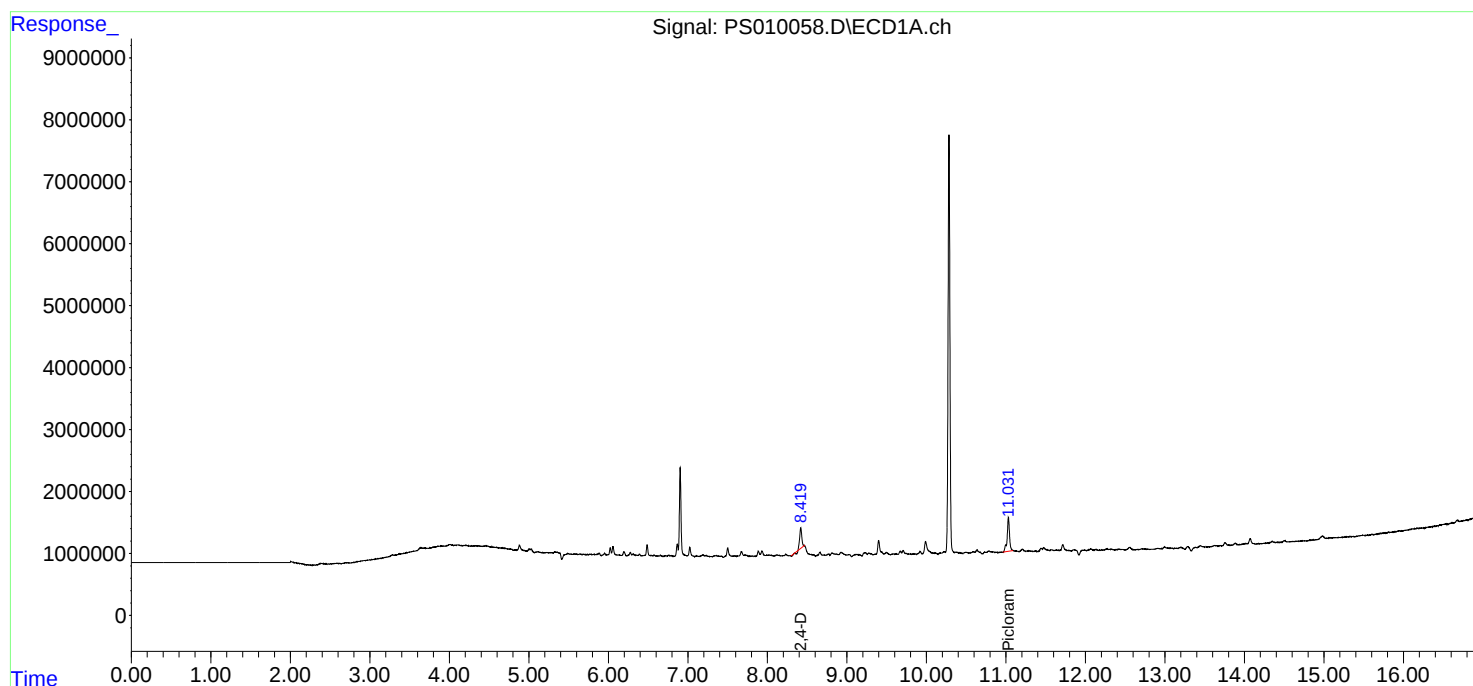


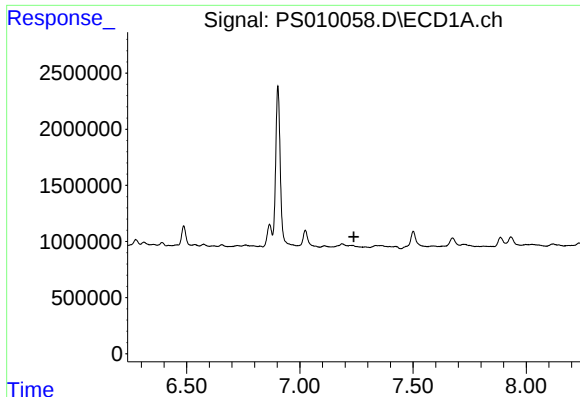

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T. : 7.239 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

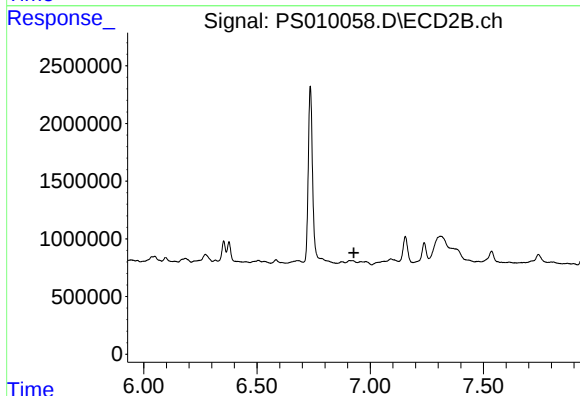


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T. : 6.928 min
Response: 0
Conc: N.D.

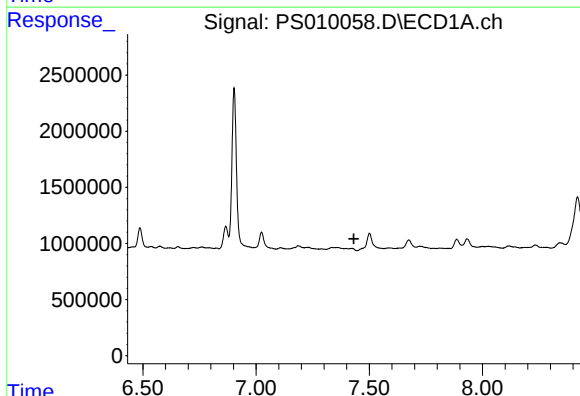


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 7.432 min
Response: 0
Conc: N.D.

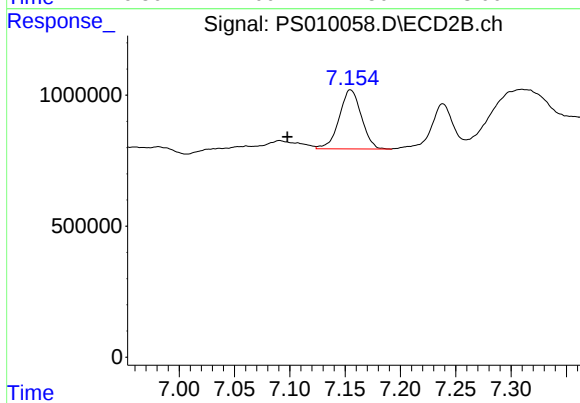

#5 DICAMBA


R.T.: 7.155 min
Delta R.T.: 0.057 min
Response: 3133798
Conc: 1.58 ng/ml

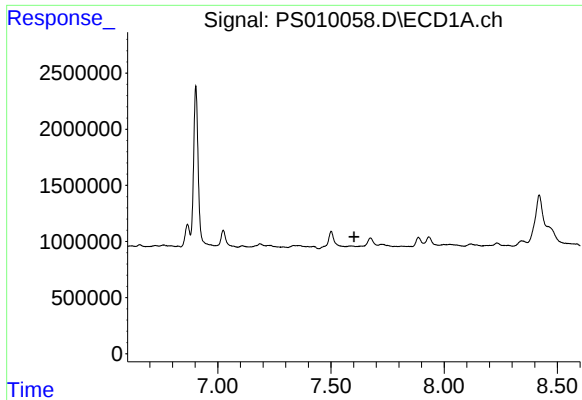

#6 MCP


R.T.: 0.000 min
Exp R.T.: 7.602 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

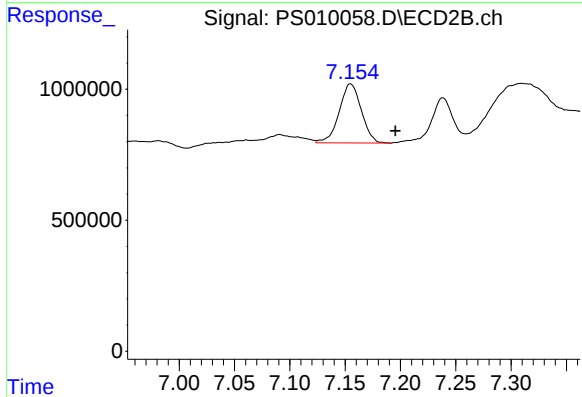


#6 MCP

R.T.: 7.155 min
Delta R.T.: -0.041 min
Response: 3133798
Conc: 1.90 ug/ml

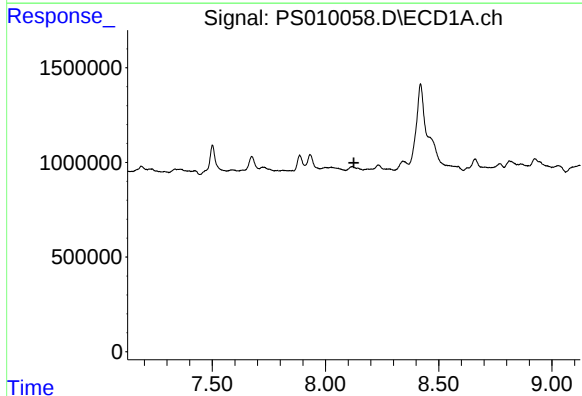


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T.: 8.125 min
Response: 0
Conc: N.D.

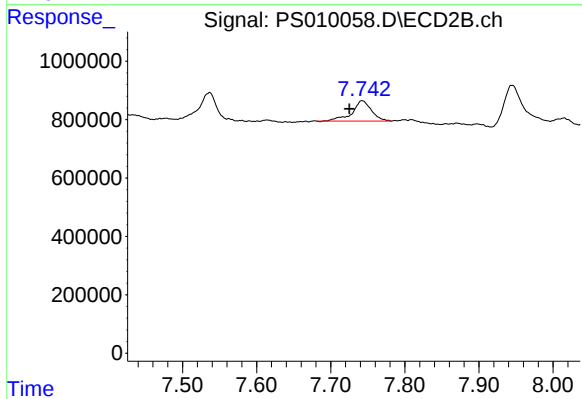

#8 DICHLORPROP


R.T.: 7.743 min
Delta R.T.: 0.017 min
Response: 1256201
Conc: 2.50 ng/ml

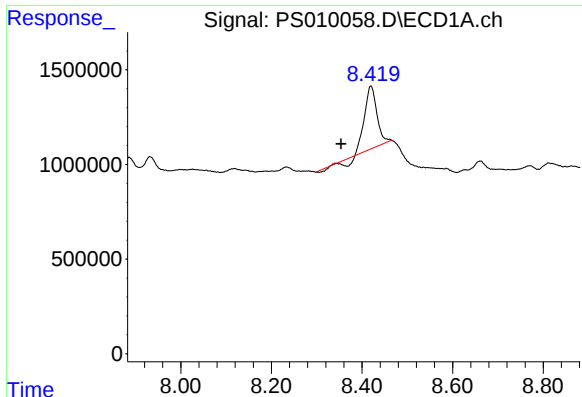

#9 2,4-D


R.T.: 8.419 min
Delta R.T.: 0.065 min
Response: 5717326
Conc: 9.96 ng/ml

Instrument :
ECD_S
ClientSampleId :

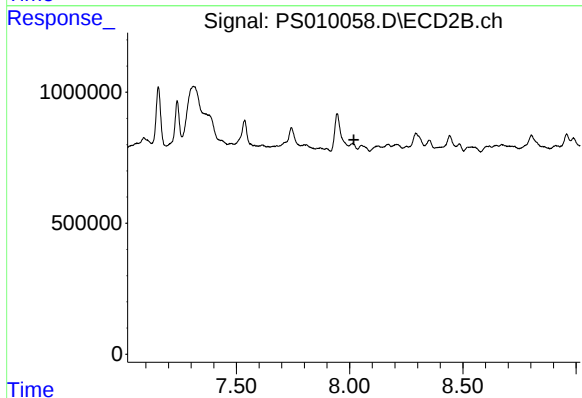


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 8.019 min
Response: 0
Conc: N.D.

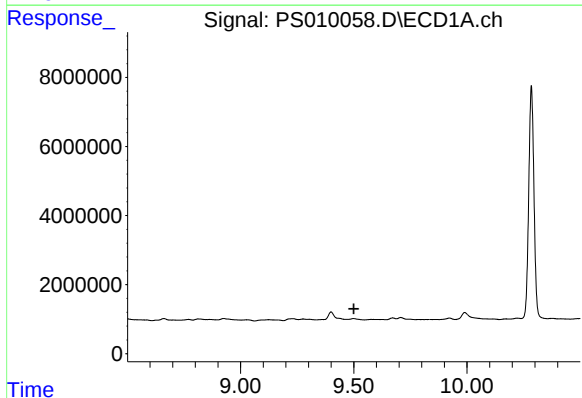


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 9.501 min
Response: 0
Conc: N.D.

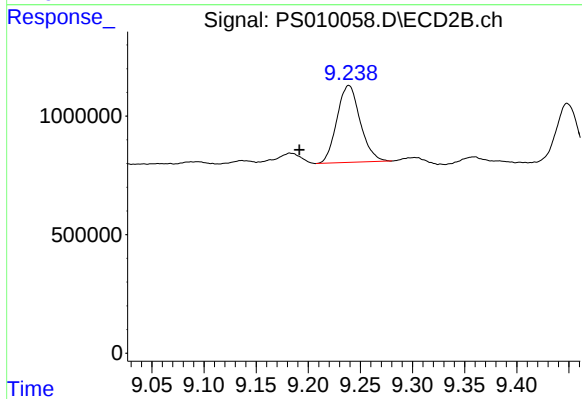

#12 2,4,5-T


R.T.: 9.239 min
Delta R.T.: 0.048 min
Response: 5046458
Conc: 1.93 ng/ml

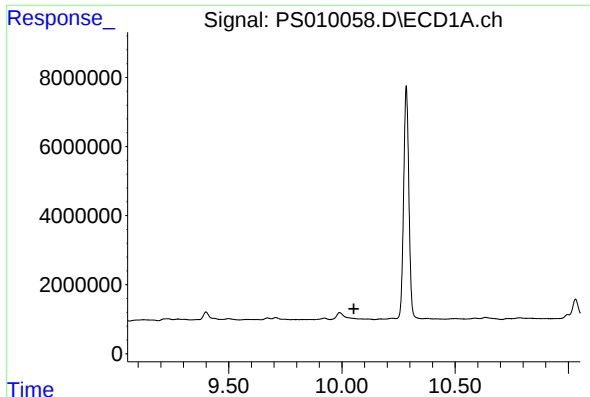

#13 2,4-DB


R.T.: 0.000 min
Exp R.T.: 10.053 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

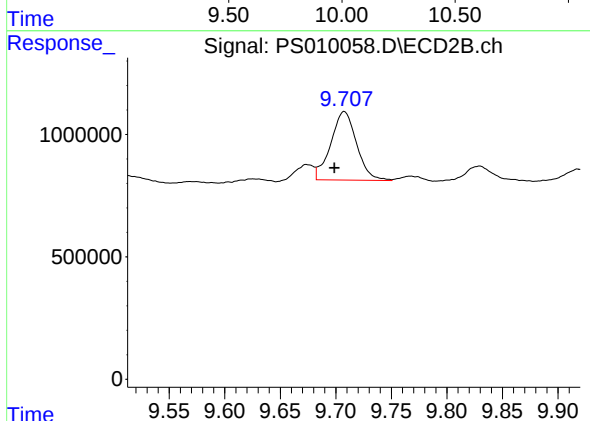


#13 2,4-DB

R.T.: 9.708 min
Delta R.T.: 0.009 min
Response: 4533805
Conc: 12.79 ng/ml

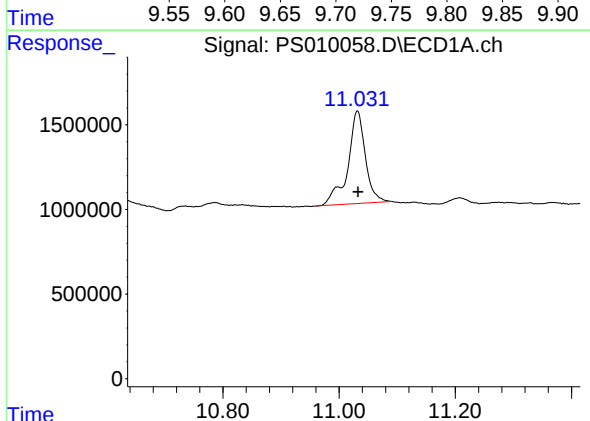

#15 Picloram

R.T.: 11.032 min
Delta R.T.: -0.001 min
Response: 11466151
Conc: 3.70 ng/ml

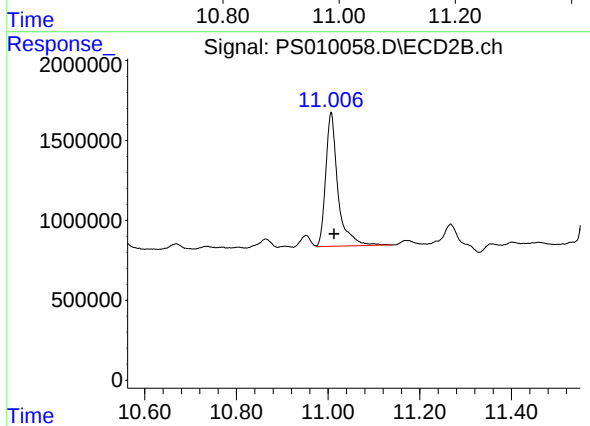

#15 Picloram

R.T.: 11.007 min
Delta R.T.: -0.006 min
Response: 15461460
Conc: 4.55 ng/ml