

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS042821\
 Data File : PS014835.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Apr 2021 10:50
 Operator : DD\AJ
 Sample : M2176-04
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 STOCKPILE-COMP-1

Manual Integrations
 APPROVED

Ankita
 4/29/2021 11:52:16 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 28 13:15:00 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS040821.M
 Quant Title : 8080.M
 QLast Update : Thu Apr 08 14:34:06 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
4) S 2,4-DCAA	7.157	6.884	911.0E6	321.5E6	598.866m	690.630m

Target Compounds

 (f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS042821\
Data File : PS014835.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Apr 2021 10:50
Operator : DD\AJ
Sample : M2176-04
Misc :
ALS Vial : 8 Sample Multiplier: 1



Instrument :
ECD_S
ClientSampleId :
STOCKPILE-COMP-1


Manual Integrations
APPROVED

Ankita
4/29/2021 11:52:16 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 28 13:15:00 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS040821.M
Quant Title : 8080.M
QLast Update : Thu Apr 08 14:34:06 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

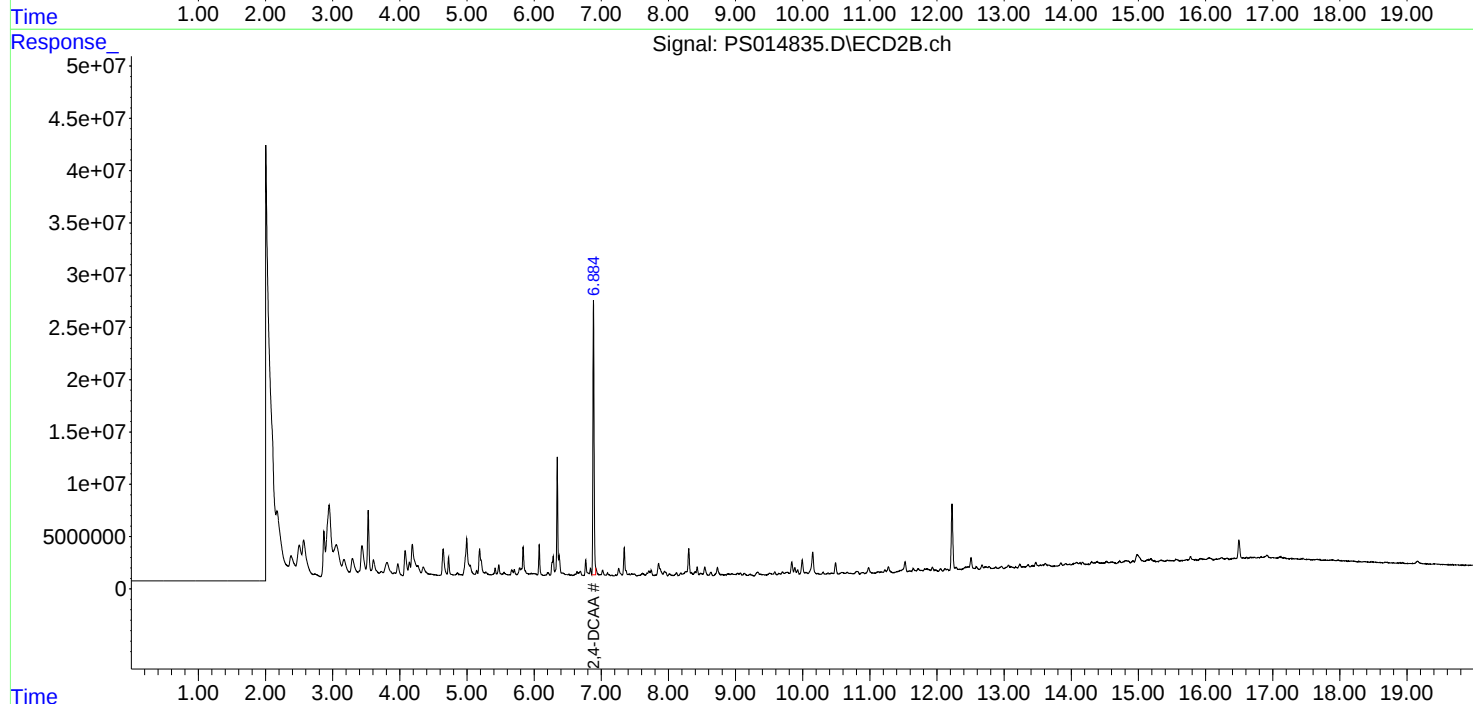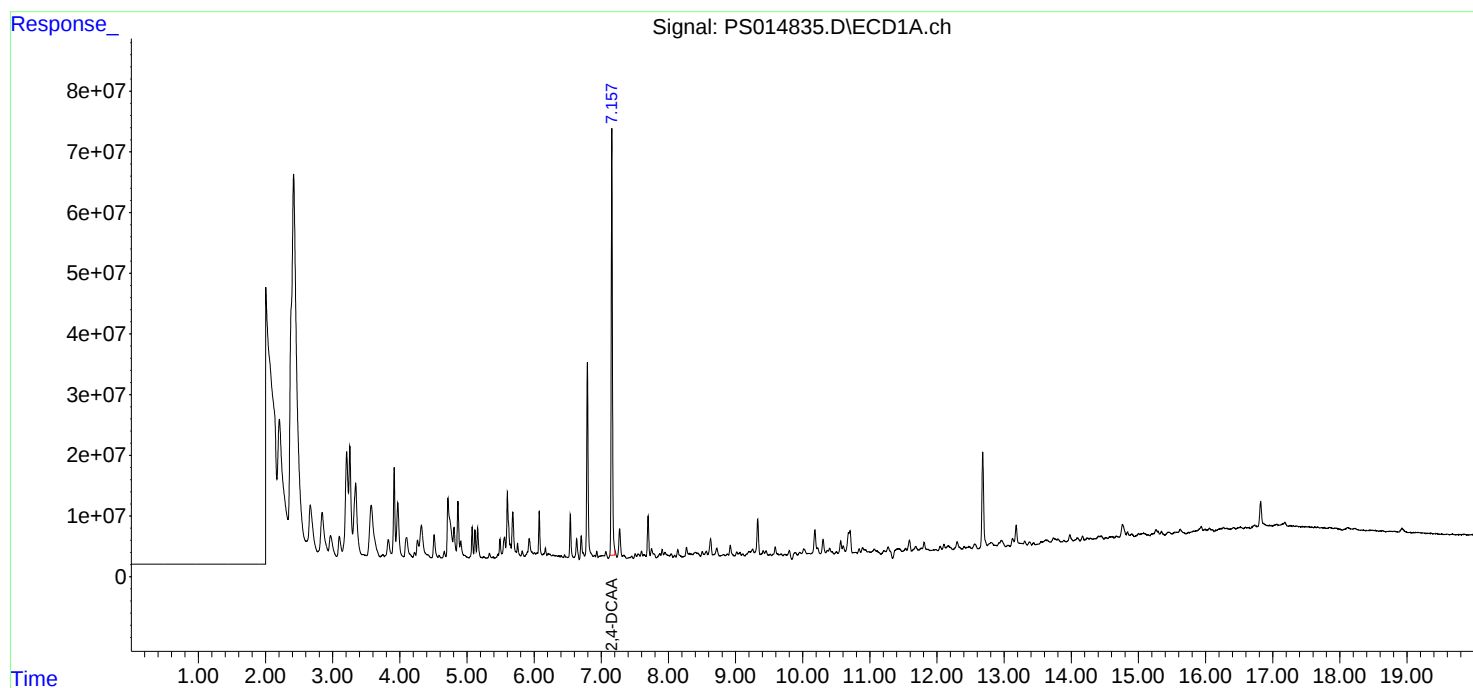

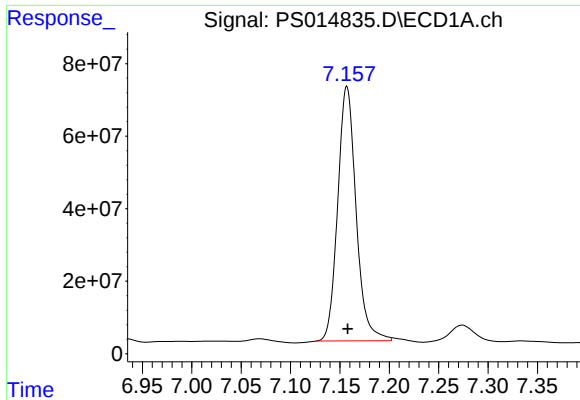


#4 2,4-DCAA

R.T.: 7.157 min
Delta R.T.: -0.001 min
Response: 910991699
Conc: 598.87 ng/ml m

Instrument :
ECD_S
ClientSampleId :
STOCKPILE-COMP-1

Manual Integrations
APPROVED

Ankita
4/29/2021 11:52:16 AM

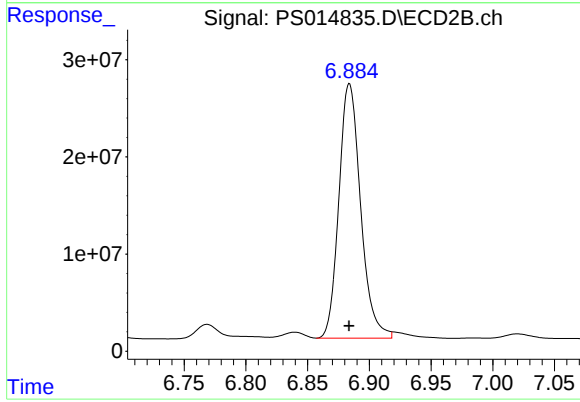

#4 2,4-DCAA

R.T.: 6.884 min
Delta R.T.: 0.000 min
Response: 321457061
Conc: 690.63 ng/ml m