

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS042822\
 Data File : PS019164.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Sep 2021 04:59
 Operator : AJ\MA
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 29 01:09:20 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS041822.M
 Quant Title : 8080.M
 QLast Update : Mon Apr 18 17:28:16 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds							
3) T	4-Nitroph...	7.012	0.000	446598	0	<MDL	N.D. #
12) T	2,4,5-T	9.414f	9.115f	16413889	3047436	<MDL	<MDL #
14) T	DINOSEB	11.125f	0.000	14797366	0	<MDL	N.D. #
15) T	Picloram	10.995	10.883	19325472	15075435	<MDL	2.546 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS042822\
Data File : PS019164.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Sep 2021 04:59
Operator : AJ\MA
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 29 01:09:20 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS041822.M
Quant Title : 8080.M
QLast Update : Mon Apr 18 17:28:16 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

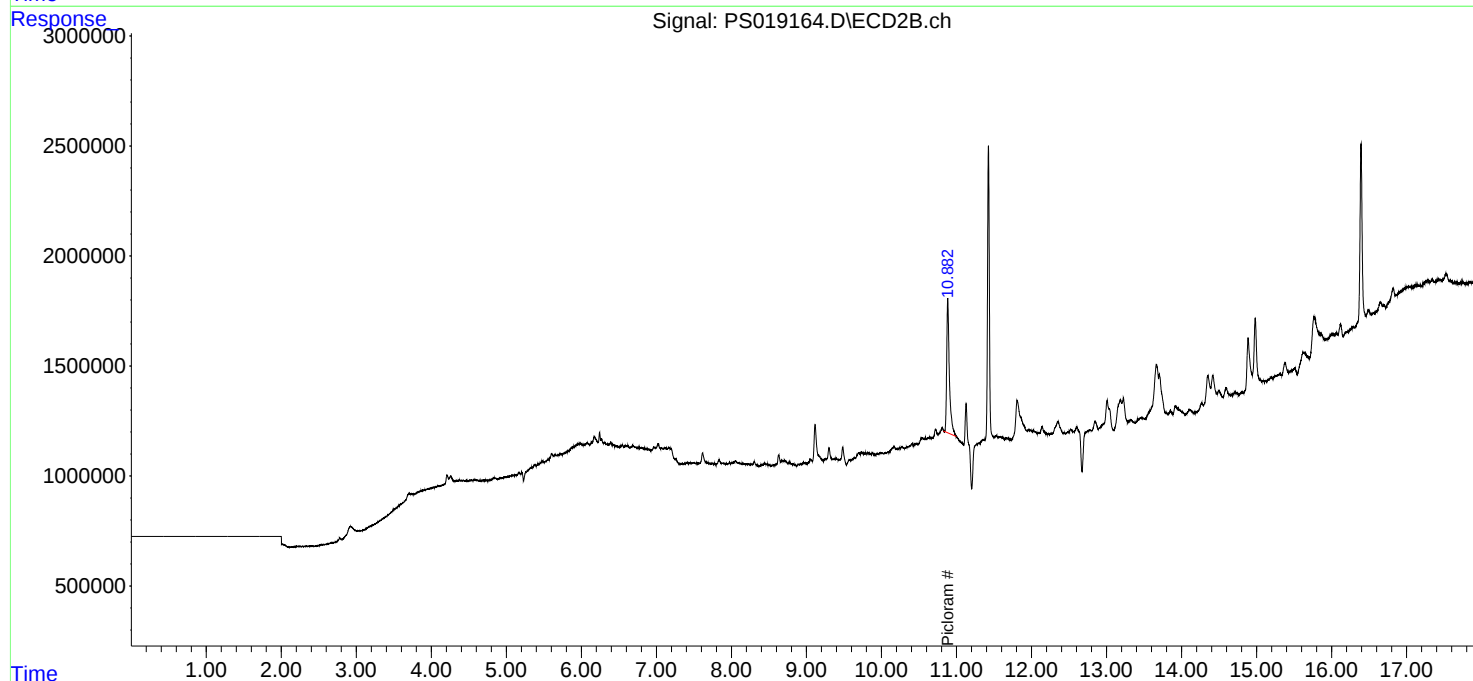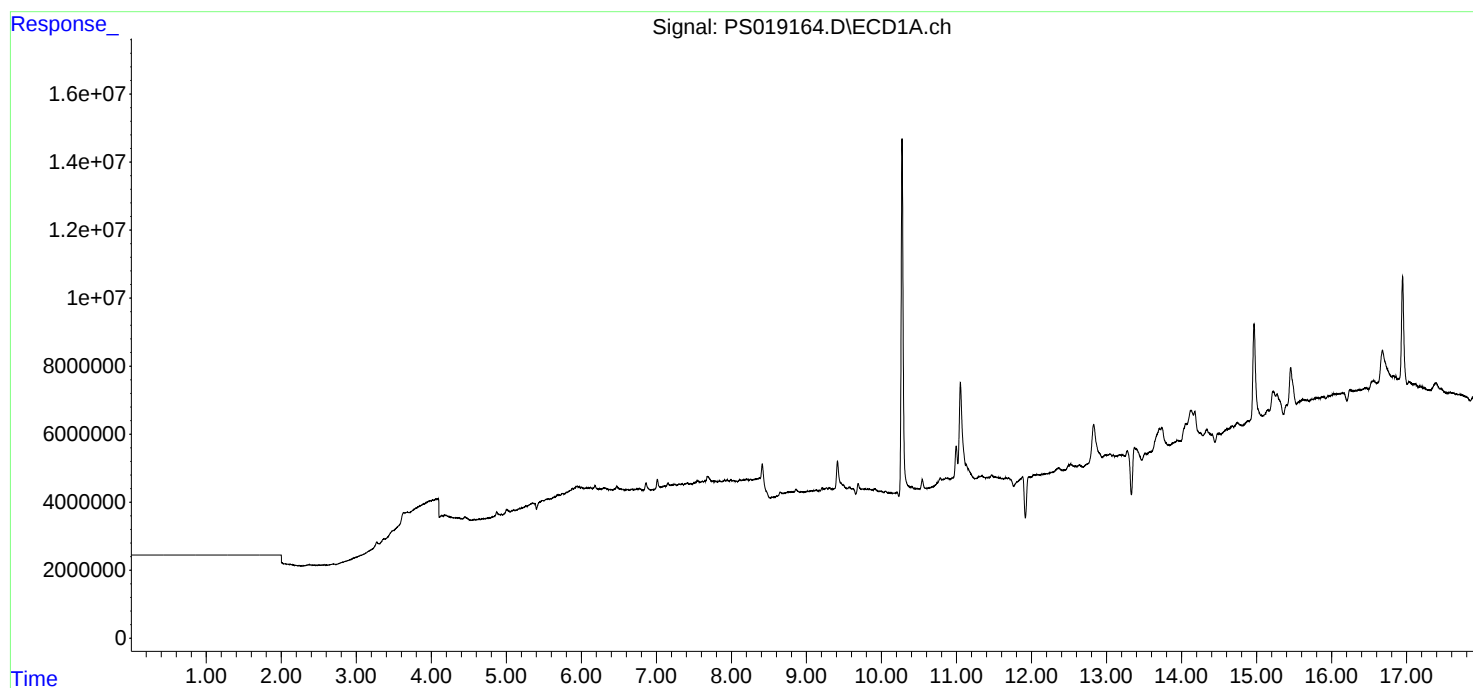


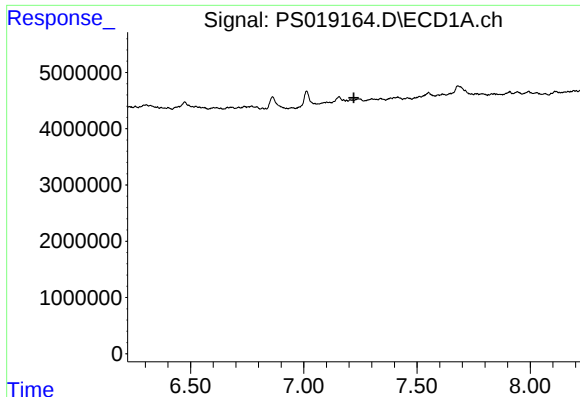

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T.: 7.221 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

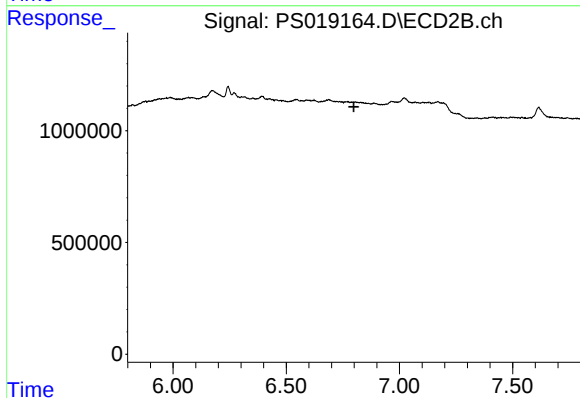


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T.: 6.799 min
Response: 0
Conc: N.D.

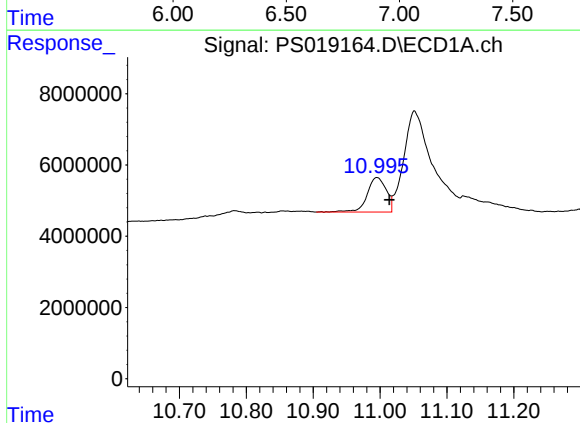

#15 Picloram

R.T.: 10.995 min
Delta R.T.: -0.019 min
Response: 19325472
Conc: N.D.

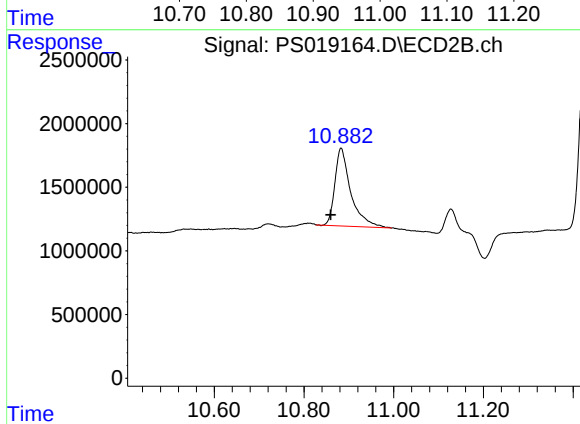

#15 Picloram

R.T.: 10.883 min
Delta R.T.: 0.023 min
Response: 15075435
Conc: 2.55 ng/ml