

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS042822\
 Data File : PS019189.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Sep 2021 17:38
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 29 01:15:54 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS041822.M
 Quant Title : 8080.M
 QLast Update : Mon Apr 18 17:28:16 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.221	6.798	1492.1E6	364.4E6	398.940	501.965 #
Target Compounds							
7) T	MCPA	7.709	0.000	20613283	0	1.368	N.D. #
8) T	DICHLORPROP	0.000	7.631f	0	5424426	N.D.	6.491
11) T	2,4,5-TP ...	9.264f	8.633	4734112	1565470	<MDL	<MDL #
12) T	2,4,5-T	9.501	0.000	10636171	0	<MDL	N.D. #
13) T	2,4-DB	0.000	9.488f	0	3023379	N.D.	5.454
15) T	Picloram	11.009	10.904f	8346508	27938288	<MDL	4.719 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS042822\
Data File : PS019189.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Sep 2021 17:38
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 29 01:15:54 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS041822.M
Quant Title : 8080.M
QLast Update : Mon Apr 18 17:28:16 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

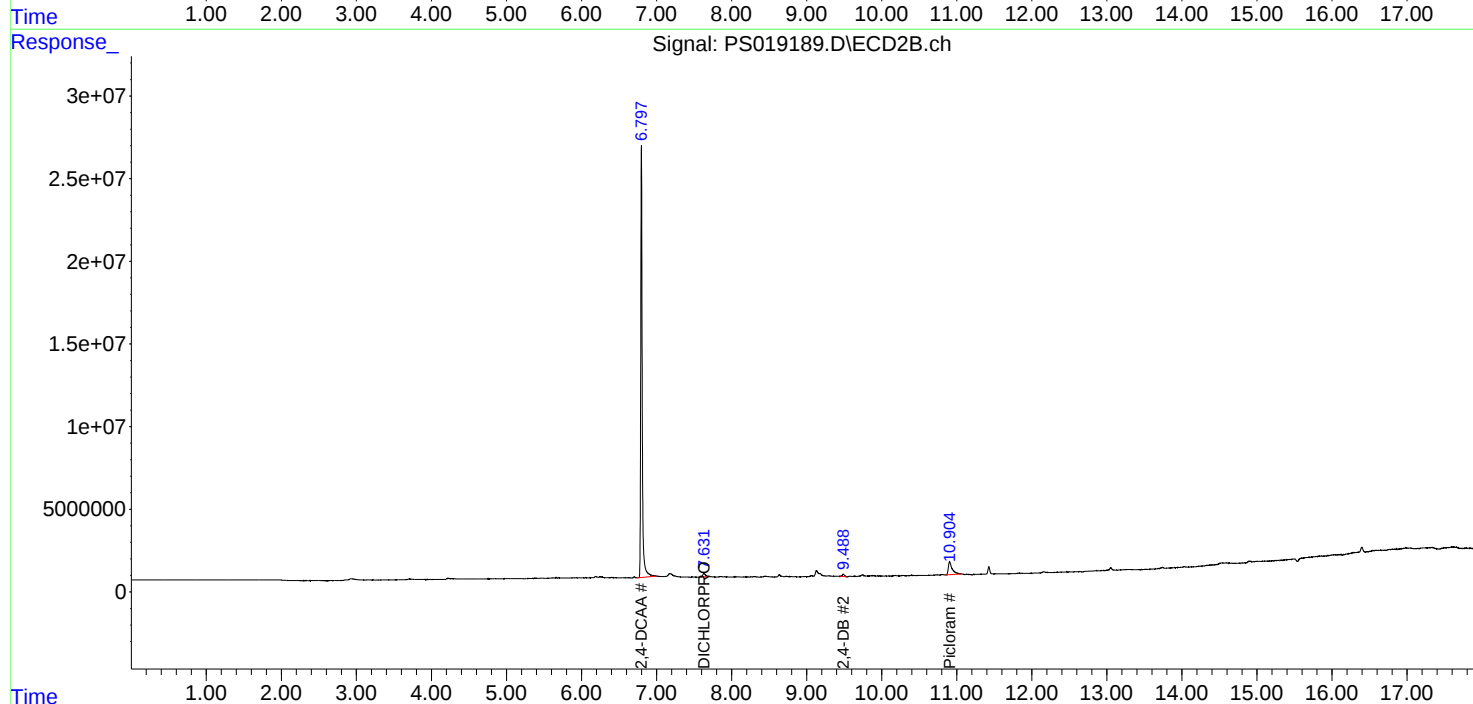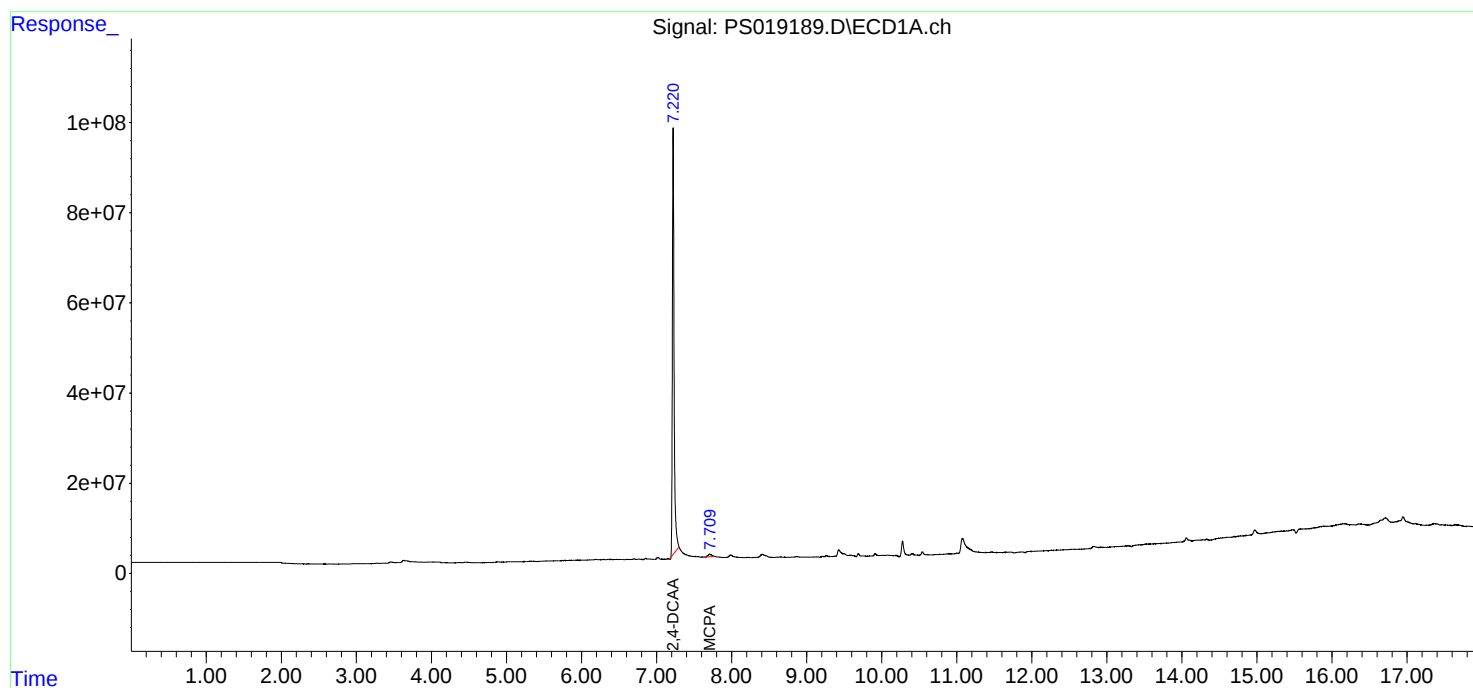


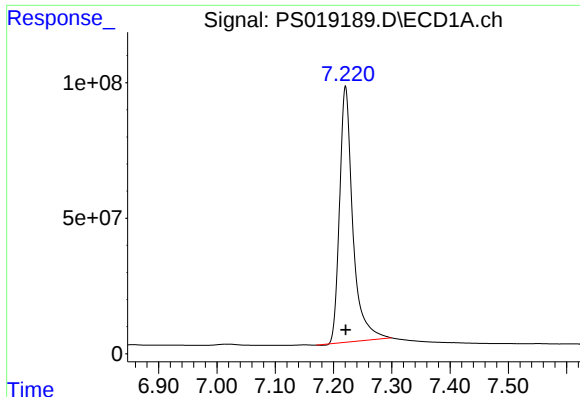

#4 2,4-DCAA


R.T.: 7.221 min
Delta R.T.: 0.000 min
Response: 1492058115
Conc: 398.94 ng/ml

Instrument :
ECD_S
ClientSampleId :

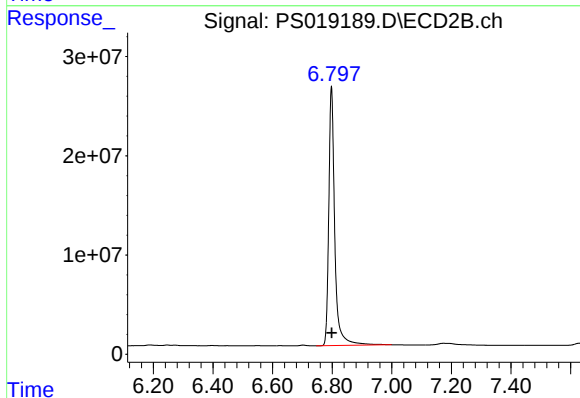


#4 2,4-DCAA

R.T.: 6.798 min
Delta R.T.: -0.001 min
Response: 364365009
Conc: 501.97 ng/ml

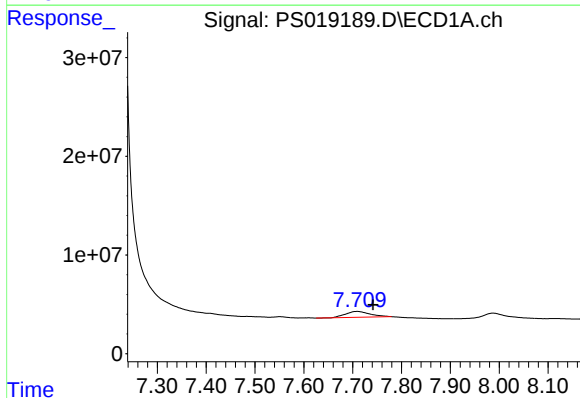


#7 MCPA

R.T.: 7.709 min
Delta R.T.: -0.032 min
Response: 20613283
Conc: 1.37 ug/ml

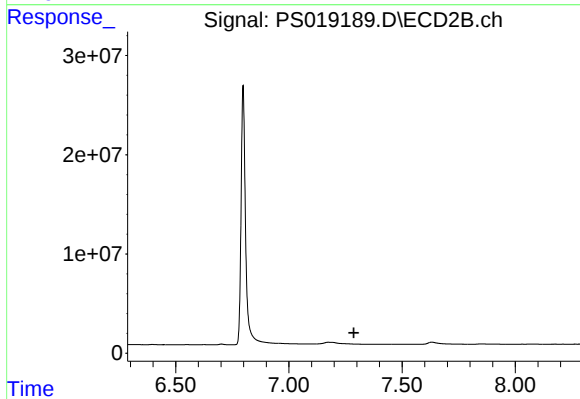

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 7.287 min
Response: 0
Conc: N.D.

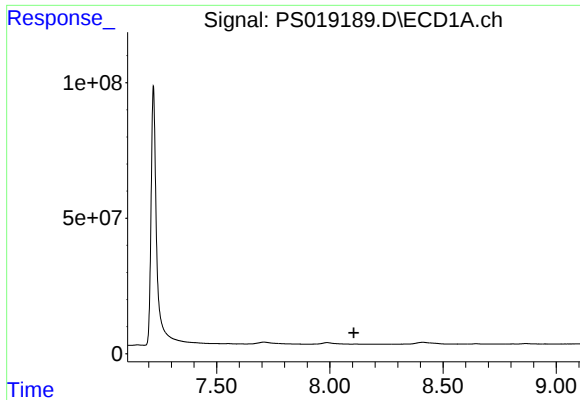

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 8.106 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

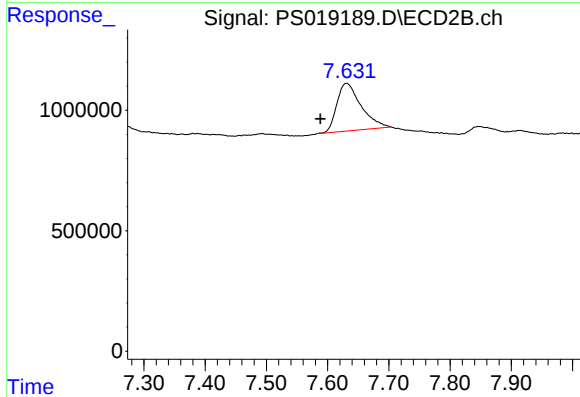


#8 DICHLORPROP

R.T.: 7.631 min
Delta R.T.: 0.043 min
Response: 5424426
Conc: 6.49 ng/ml

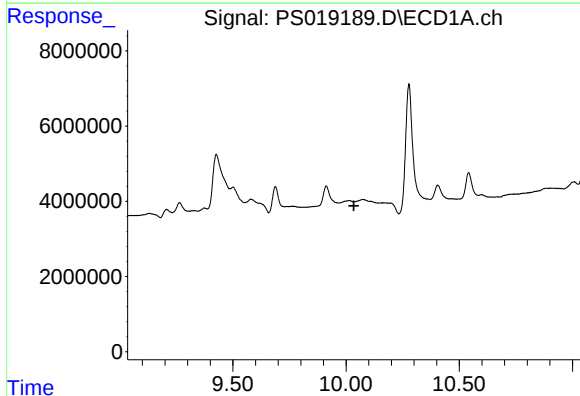


#13 2,4-DB

R.T.: 0.000 min
Exp R.T.: 10.034 min
Response: 0
Conc: N.D.

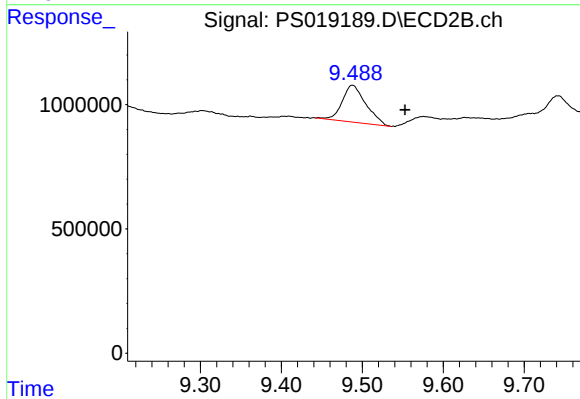

#13 2,4-DB


R.T.: 9.488 min
Delta R.T.: -0.065 min
Response: 3023379
Conc: 5.45 ng/ml

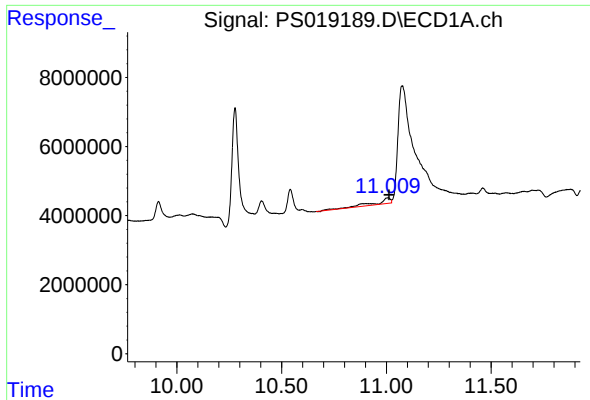

#15 Picloram

R.T.: 11.009 min
Delta R.T.: -0.005 min
Response: 8346508
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

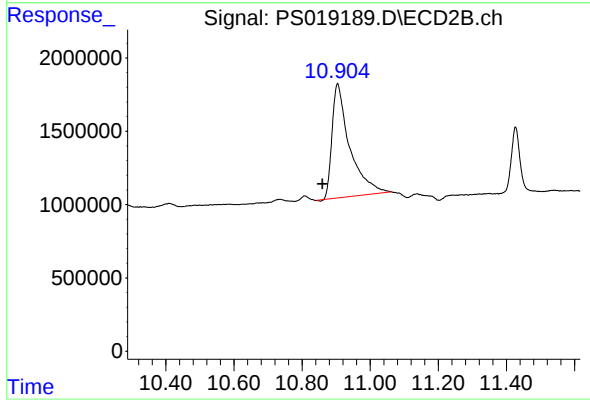

#15 Picloram

R.T.: 10.904 min
Delta R.T.: 0.044 min
Response: 27938288
Conc: 4.72 ng/ml