

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS042919\
 Data File : PS004347.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Apr 2019 01:53
 Operator : EI\SJ
 Sample : MDL-BL-WATER-02
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 MDL-BL-WATER-02

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 30 09:18:50 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS042919.M
 Quant Title : 8080.M
 QLast Update : Tue Apr 30 08:27:54 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.003	5.692	282.1E6	227.4E6	448.162	471.429
Target Compounds							
9) T	2,4-D	7.090	0.000	24215492	0	37.775	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS042919\
Data File : PS004347.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Apr 2019 01:53
Operator : EI\SJ
Sample : MDL-BL-WATER-02
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
MDL-BL-WATER-02

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 30 09:18:50 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS042919.M
Quant Title : 8080.M
QLast Update : Tue Apr 30 08:27:54 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

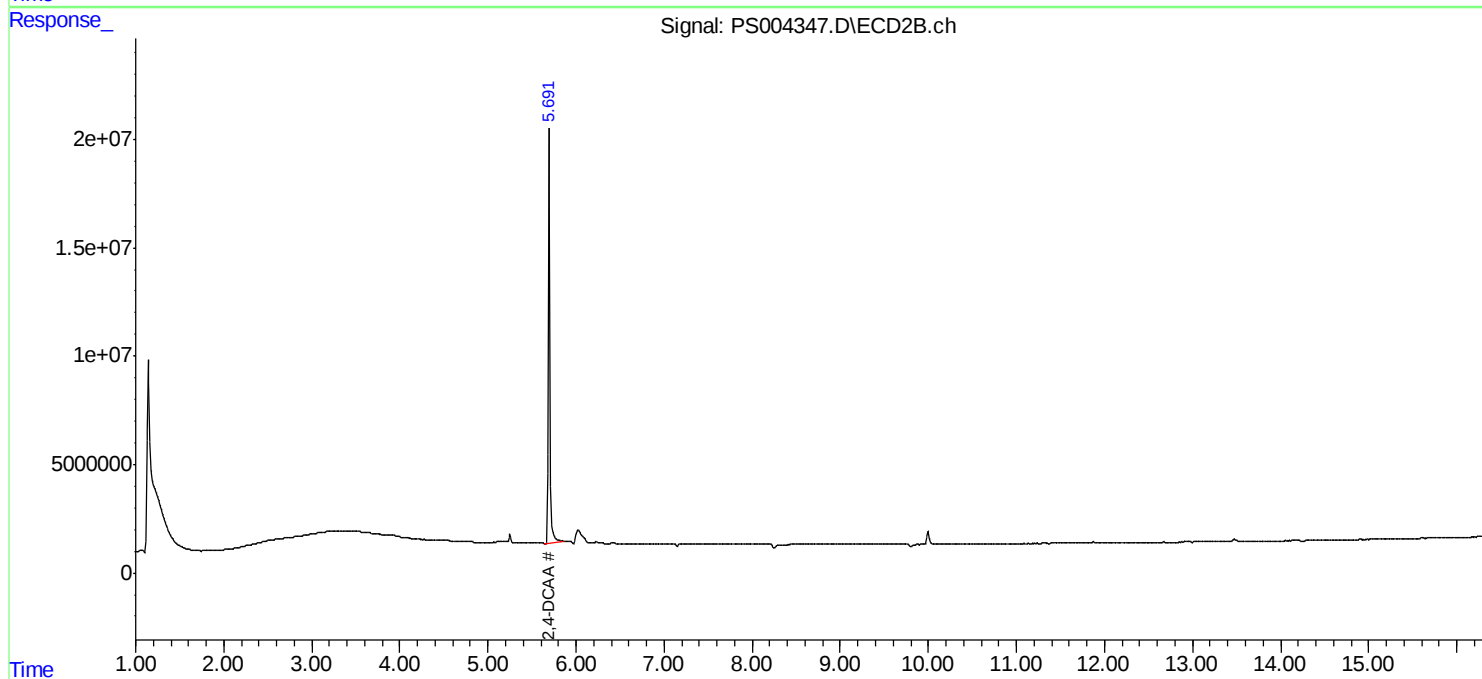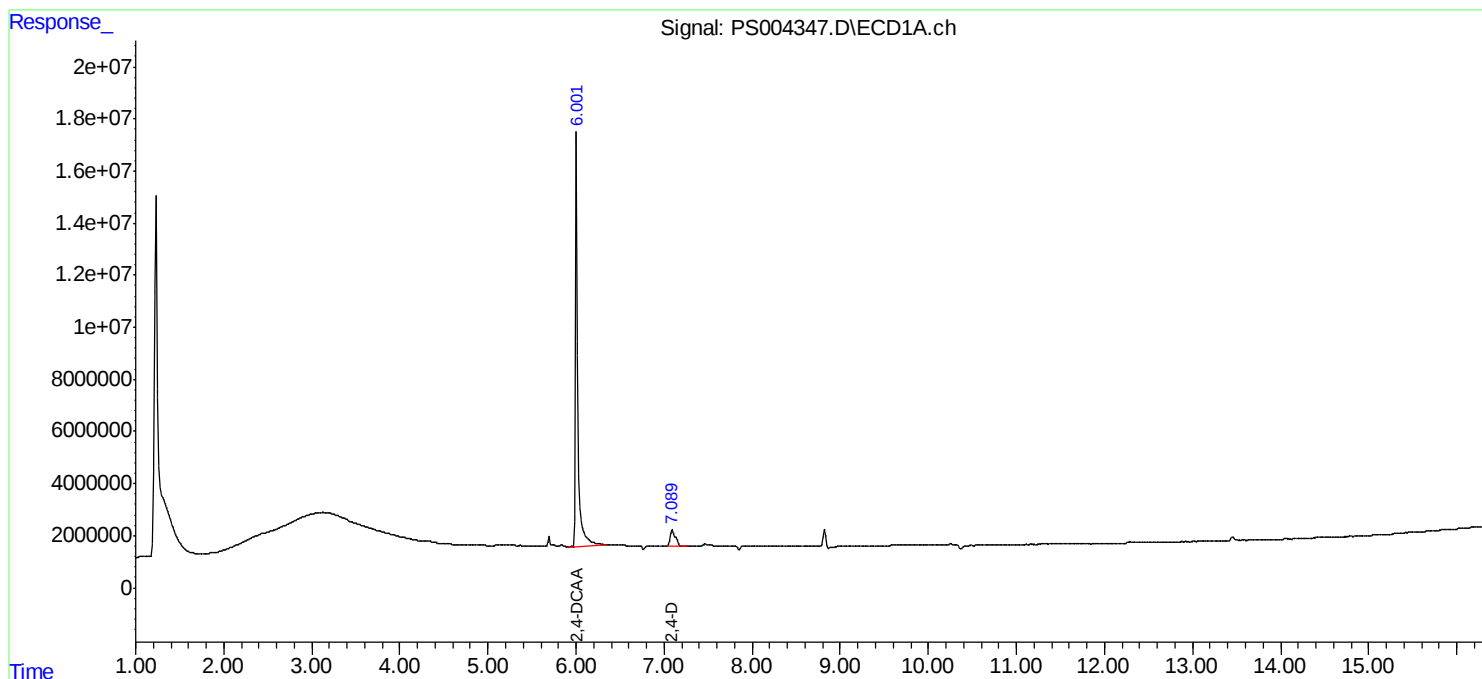


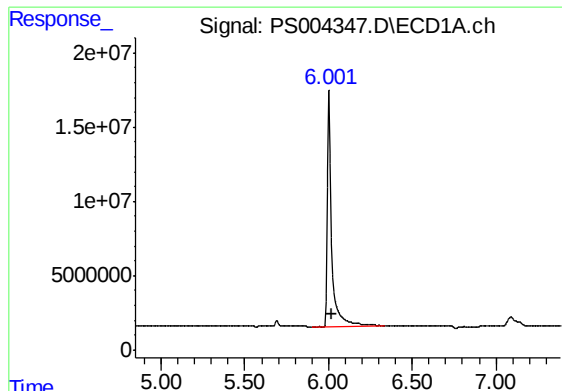

#4 2,4-DCAA


R.T.: 6.003 min
Delta R.T.: -0.015 min
Response: 282098954
Conc: 448.16 ng/ml

Instrument :
ECD_S
ClientSampleId :
MDL-BL-WATER-02

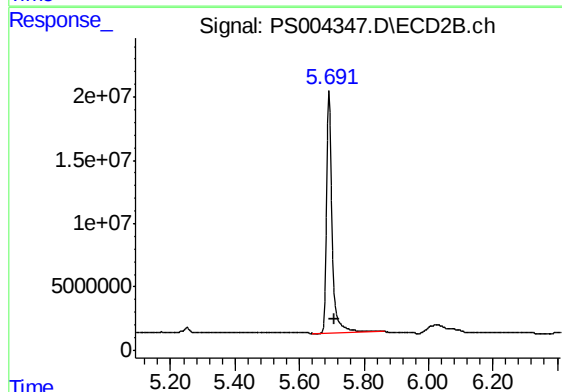


#4 2,4-DCAA

R.T.: 5.692 min
Delta R.T.: -0.017 min
Response: 227362428
Conc: 471.43 ng/ml

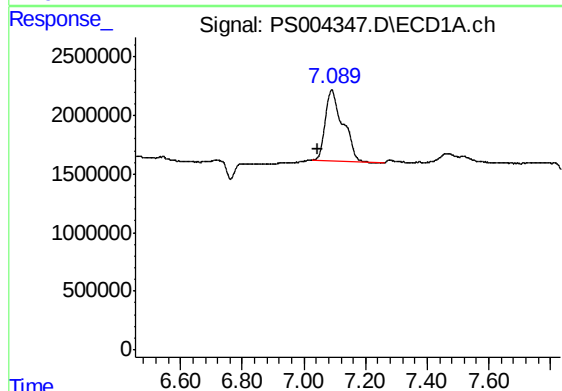

#9 2,4-D

R.T.: 7.090 min
Delta R.T.: 0.045 min
Response: 24215492
Conc: 37.78 ng/ml

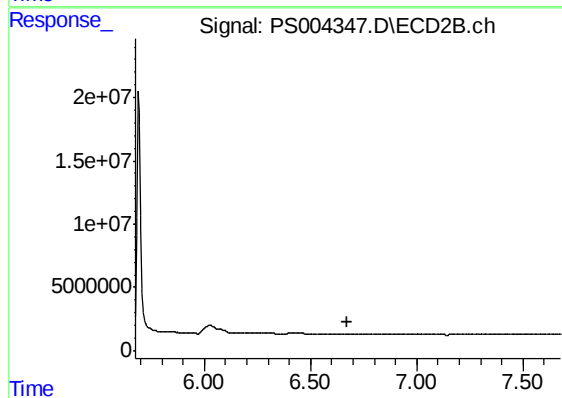

#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 6.676 min
Response: 0
Conc: N.D.