

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS042919\
 Data File : PS004348.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Apr 2019 02:23
 Operator : EI\SJ
 Sample : MDL-BL-WATER-03
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 MDL-BL-WATER-03

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 30 09:19:05 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS042919.M
 Quant Title : 8080.M
 QLast Update : Tue Apr 30 08:27:54 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.045	5.735	286.5E6	231.2E6	455.208	479.321
Target Compounds							
7) T	MCPA	0.000	6.070	0	30436360	N.D.	15.321



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS042919\
Data File : PS004348.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Apr 2019 02:23
Operator : EI\SJ
Sample : MDL-BL-WATER-03
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
MDL-BL-WATER-03

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 30 09:19:05 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS042919.M
Quant Title : 8080.M
QLast Update : Tue Apr 30 08:27:54 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

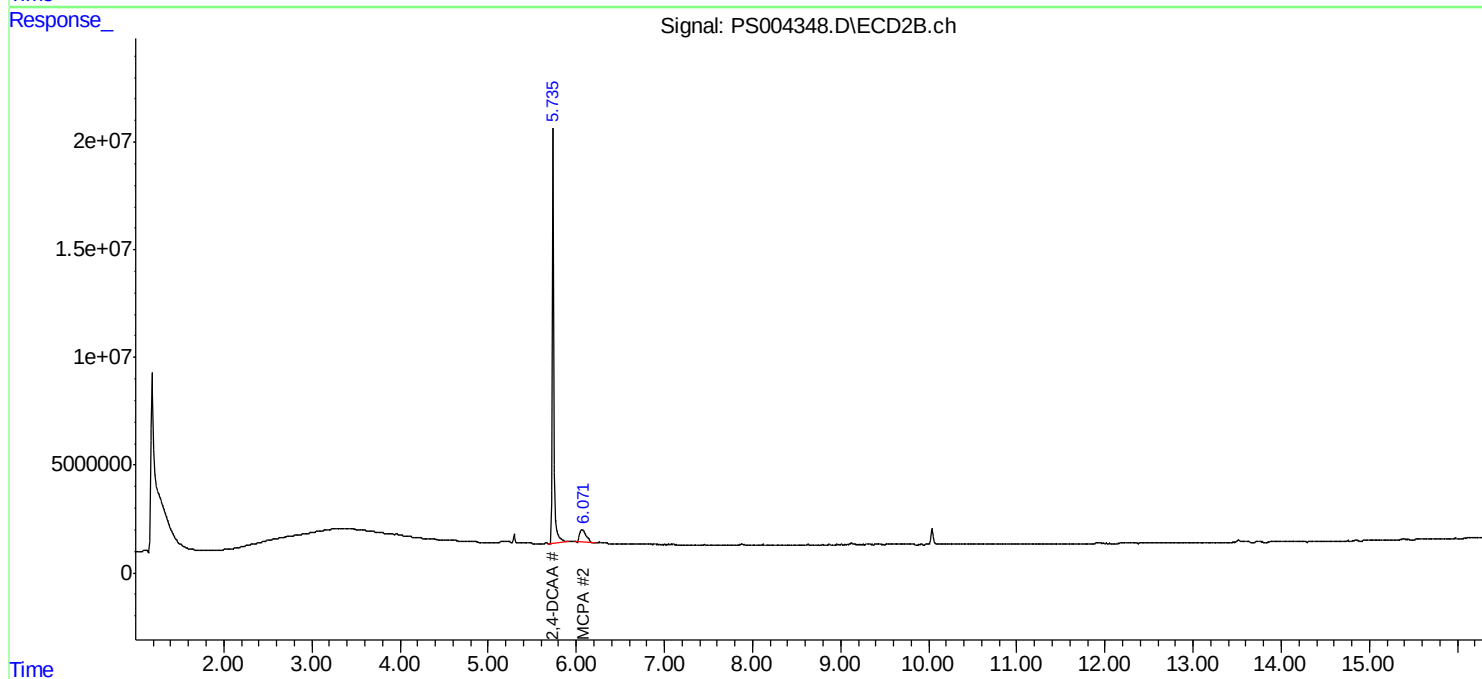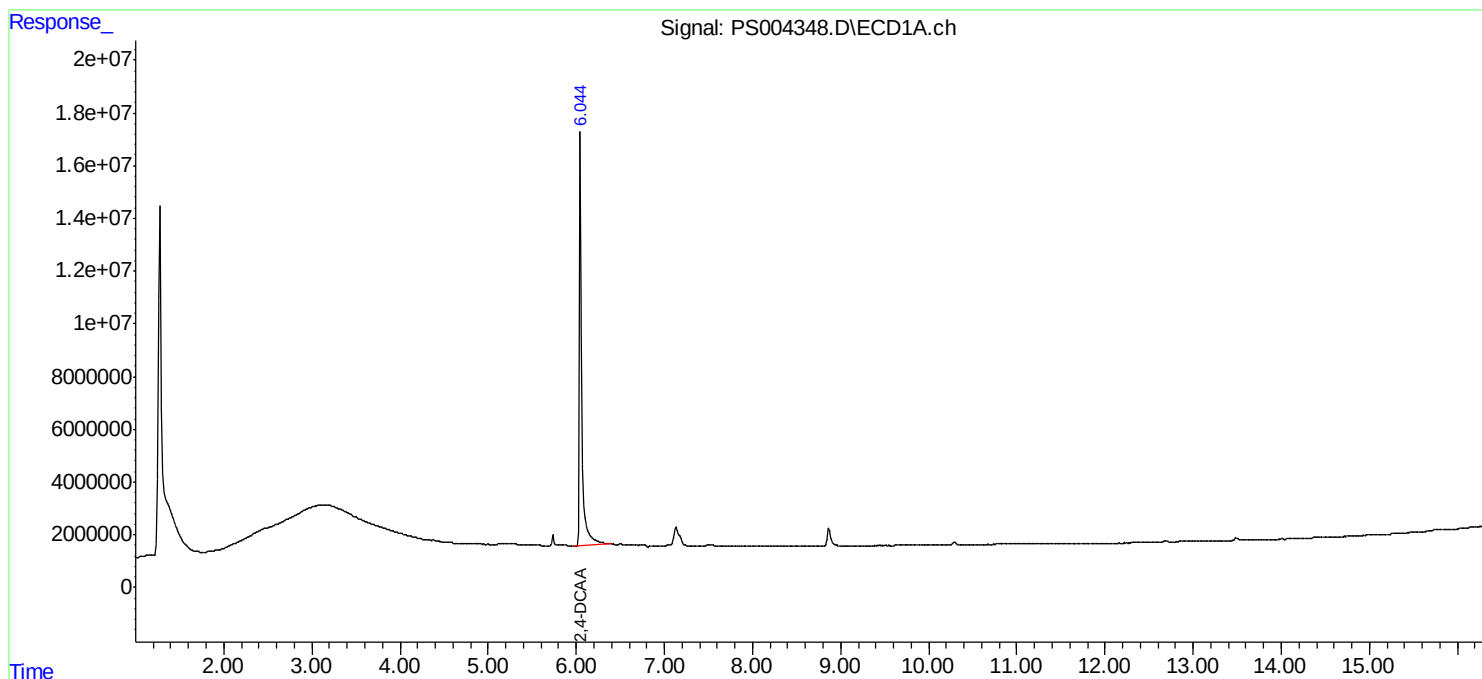


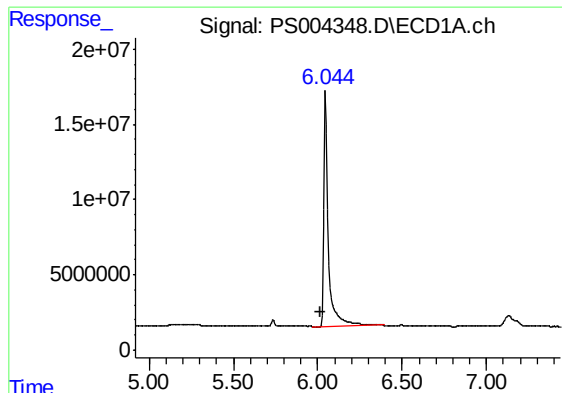

#4 2,4-DCAA


R.T.: 6.045 min
Delta R.T.: 0.027 min
Response: 286534157
Conc: 455.21 ng/ml

Instrument :
ECD_S
ClientSampleId :
MDL-BL-WATER-03

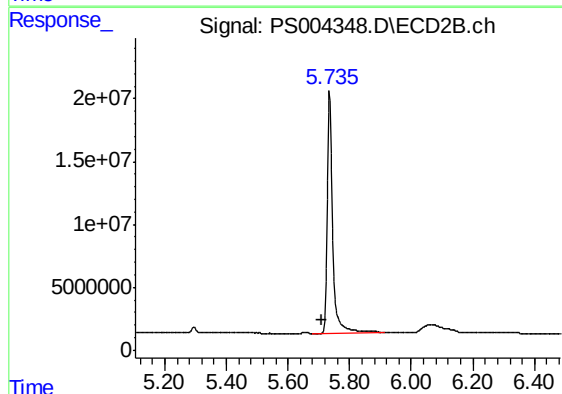


#4 2,4-DCAA

R.T.: 5.735 min
Delta R.T.: 0.026 min
Response: 231168702
Conc: 479.32 ng/ml

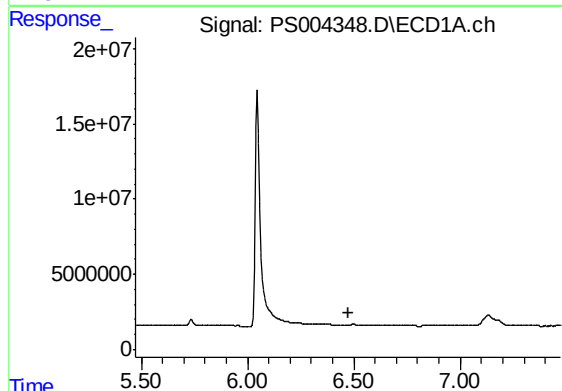

#7 MCPA

R.T.: 0.000 min
Exp R.T. : 6.472 min
Response: 0
Conc: N.D.

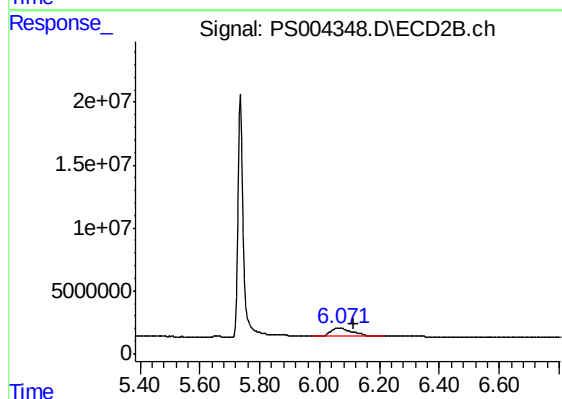

#7 MCPA

R.T.: 6.070 min
Delta R.T.: -0.044 min
Response: 30436360
Conc: 15.32 ug/ml