

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS042921\
 Data File : PS014847.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Apr 2021 09:18
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 29 16:03:53 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS040821.M
 Quant Title : 8080.M
 QLast Update : Thu Apr 08 14:34:06 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.162	6.888	712.4E6	236.0E6	468.344	507.022
Target Compounds							
2) T	3,5-DICHL...	6.440f	0.000	10789842	0	5.207	N.D. #
6) T	MCP	0.000	7.127	0	4625822	N.D.	2.747
12) T	2,4,5-T	9.392	0.000	5712606	0	<MDL	N.D. #
15) T	Picloram	10.926	11.013f	9030792	16851109	<MDL	4.494 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS042921\
Data File : PS014847.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Apr 2021 09:18
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 29 16:03:53 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS040821.M
Quant Title : 8080.M
QLast Update : Thu Apr 08 14:34:06 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

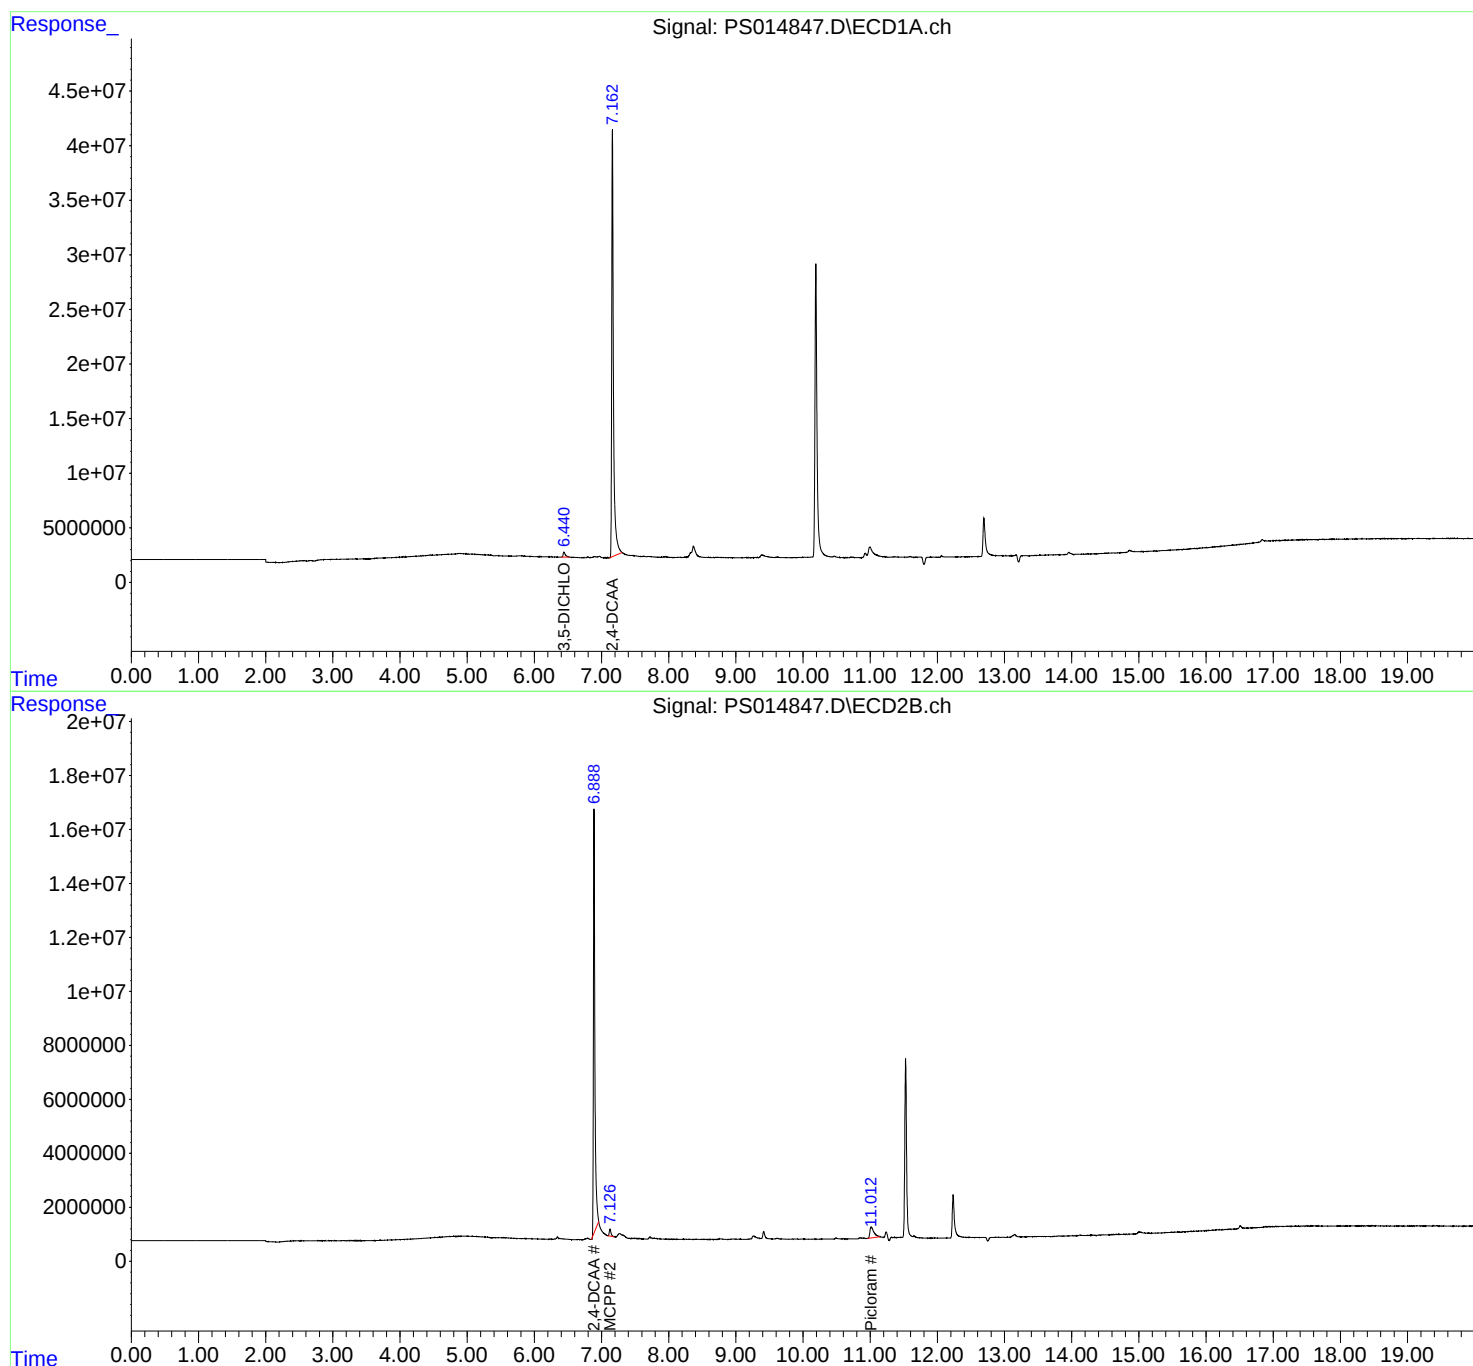


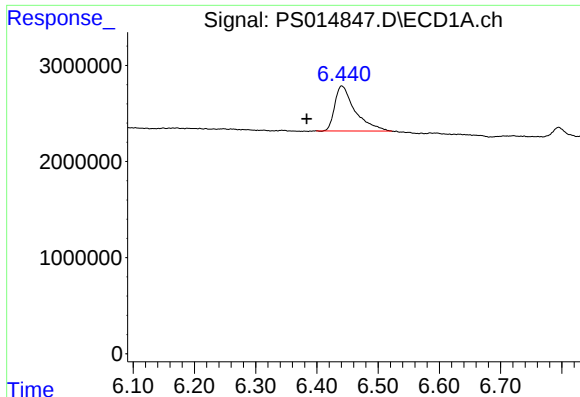

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.440 min
Delta R.T.: 0.057 min
Response: 10789842
Conc: 5.21 ng/ml

Instrument :
ECD_S
ClientSampleId :

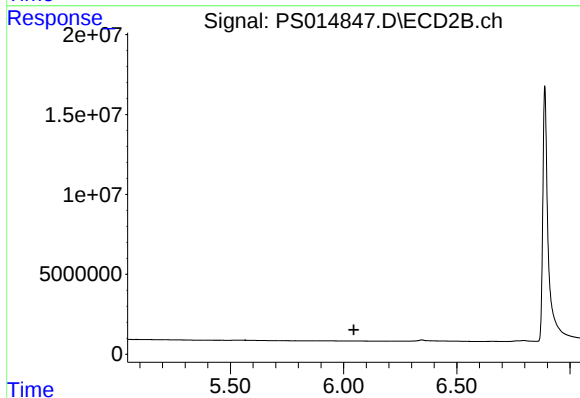


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.045 min
Response: 0
Conc: N.D.

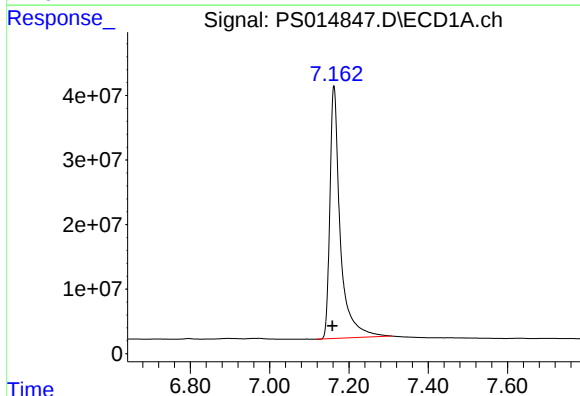


#4 2,4-DCAA

R.T.: 7.162 min
Delta R.T.: 0.004 min
Response: 712443212
Conc: 468.34 ng/ml

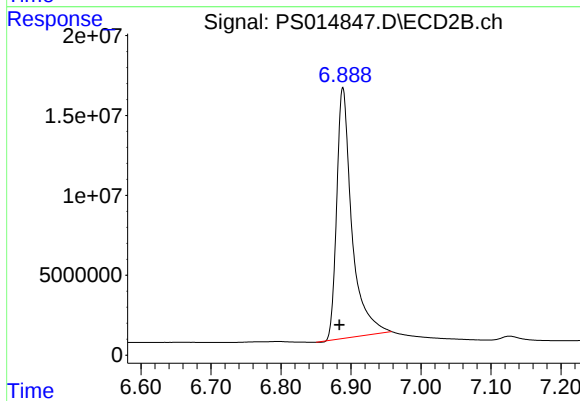

#4 2,4-DCAA


R.T.: 6.888 min
Delta R.T.: 0.005 min
Response: 235995937
Conc: 507.02 ng/ml

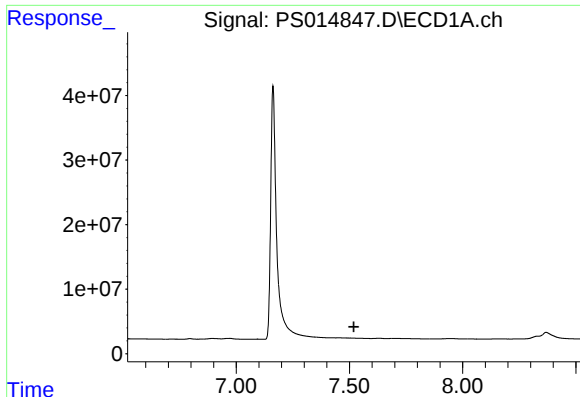

#6 MCPP


R.T.: 0.000 min
Exp R.T.: 7.520 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

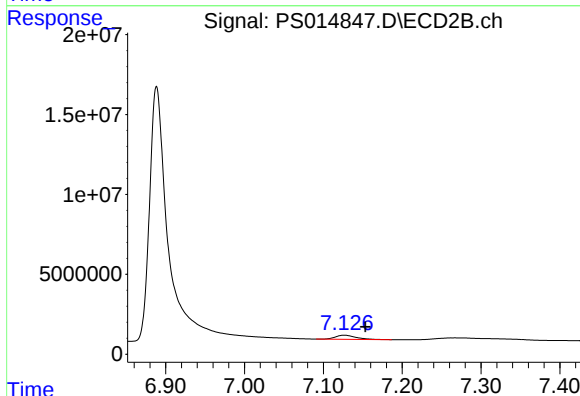


#6 MCPP

R.T.: 7.127 min
Delta R.T.: -0.027 min
Response: 4625822
Conc: 2.75 ug/ml

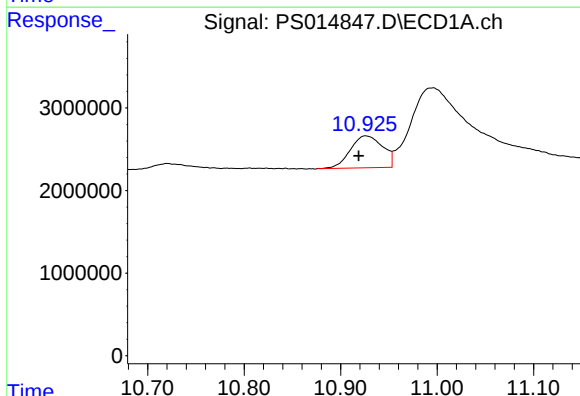

#15 Picloram

R.T.: 10.926 min
Delta R.T.: 0.007 min
Response: 9030792
Conc: N.D.

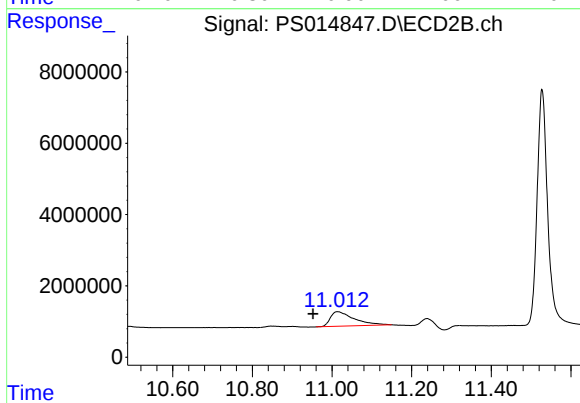

#15 Picloram

R.T.: 11.013 min
Delta R.T.: 0.060 min
Response: 16851109
Conc: 4.49 ng/ml