

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS042921\
 Data File : PS014850.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Apr 2021 12:05
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 29 16:05:01 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS040821.M
 Quant Title : 8080.M
 QLast Update : Thu Apr 08 14:34:06 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.161	6.888	718.8E6	243.2E6	472.554	522.495
Target Compounds							
2) T	3,5-DICHL...	6.441f	0.000	12556573	0	6.060	N.D. #
5) T	DICAMBA	7.352	0.000	4542091	0	<MDL	N.D. #
6) T	MCP	0.000	7.125	0	4476691	N.D.	2.658
10) T	Pentachlo...	8.577	8.405	9654600	3941588	<MDL	<MDL #
11) T	2,4,5-TP ...	9.135	8.779	6091379	3173215	<MDL	1.162 #
12) T	2,4,5-T	9.370	9.187f	42626985	2922390	5.182	1.117 #
14) T	DINOSEB	11.098	9.980	30672960	2325574	4.760	1.208 #
15) T	Picloram	10.923	10.999f	9613561	63484696	<MDL	16.930 #
16) T	DCPA	11.363	10.901	13031414	7050962	1.058	1.736 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS042921\
Data File : PS014850.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Apr 2021 12:05
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 29 16:05:01 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS040821.M
Quant Title : 8080.M
QLast Update : Thu Apr 08 14:34:06 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

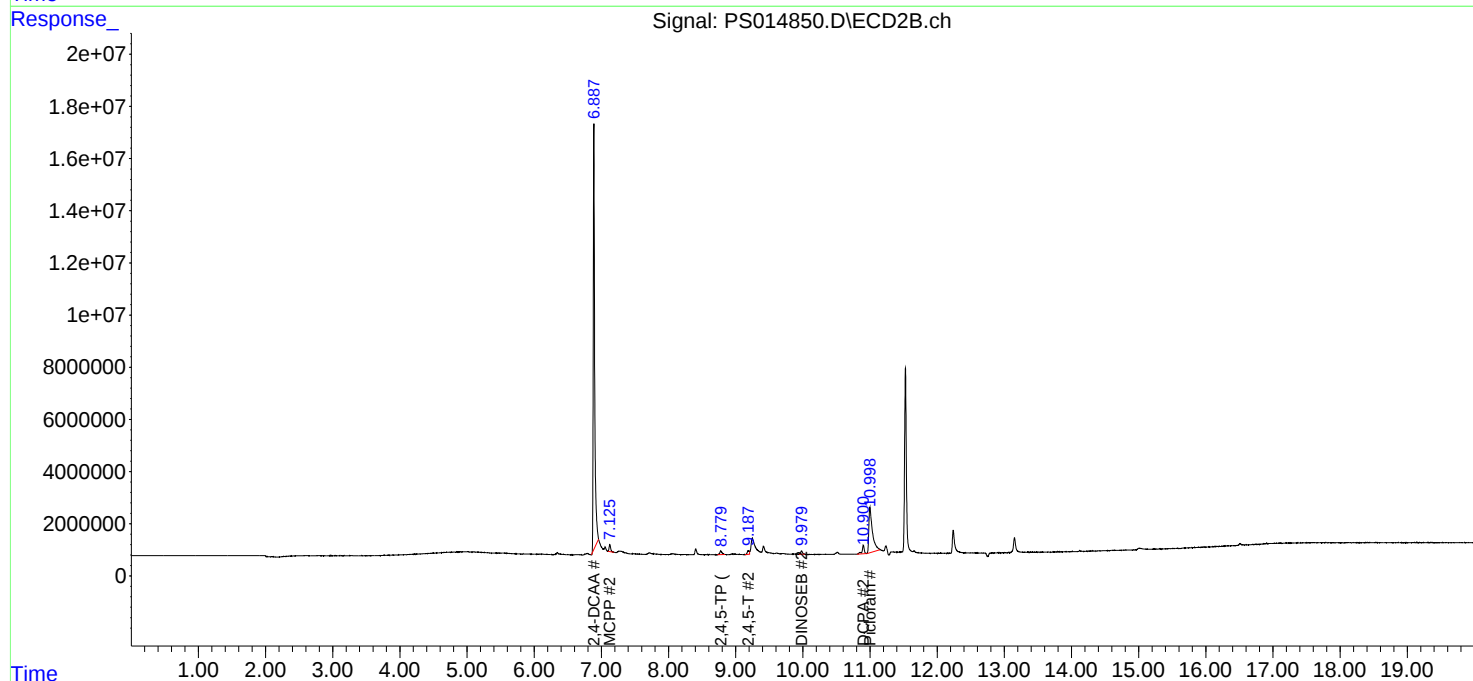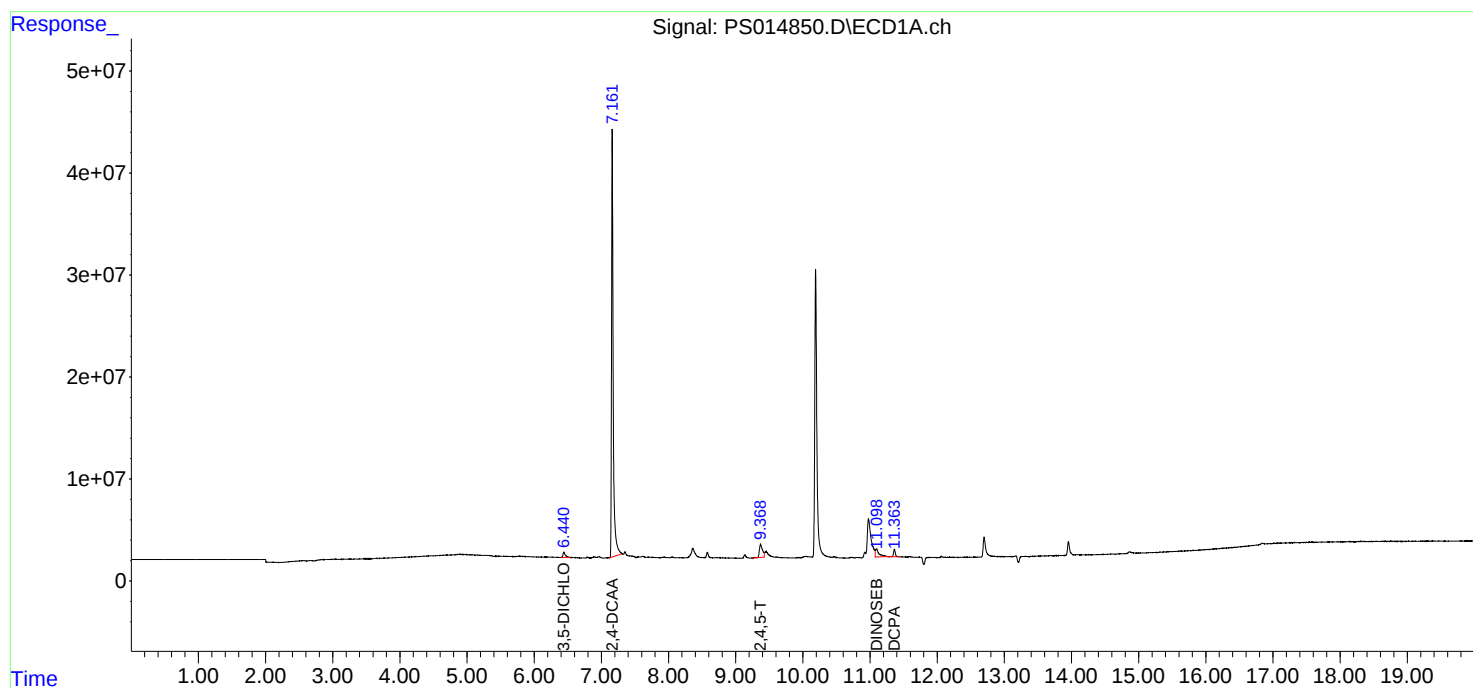


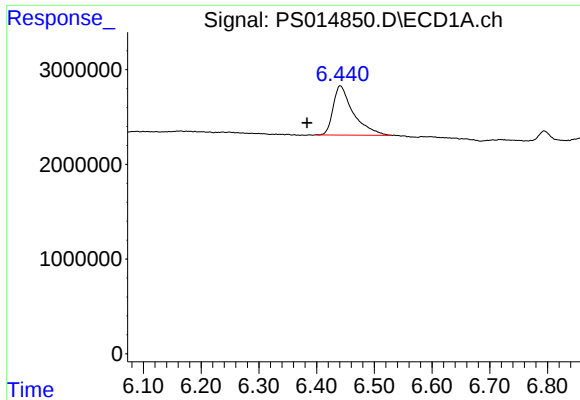

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.441 min
Delta R.T.: 0.057 min
Response: 12556573
Conc: 6.06 ng/ml

Instrument :
ECD_S
ClientSampleId :

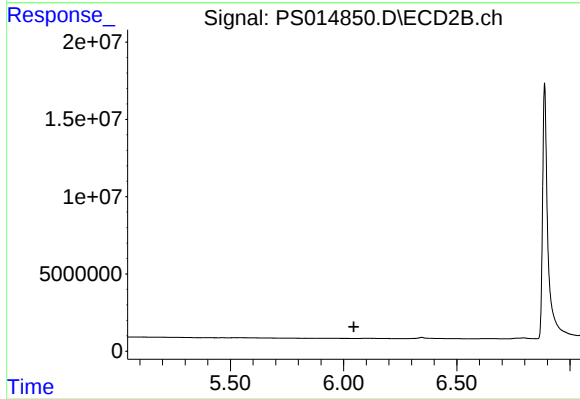


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.045 min
Response: 0
Conc: N.D.

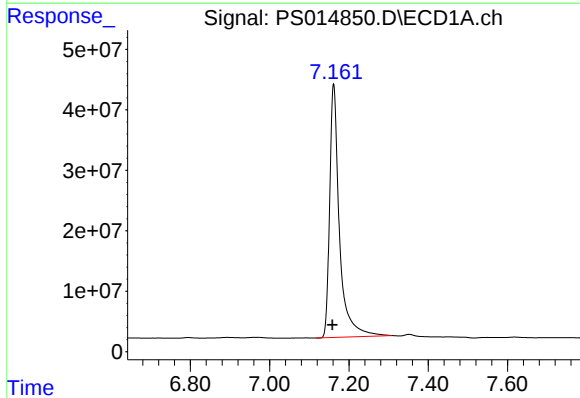


#4 2,4-DCAA

R.T.: 7.161 min
Delta R.T.: 0.004 min
Response: 718847723
Conc: 472.55 ng/ml

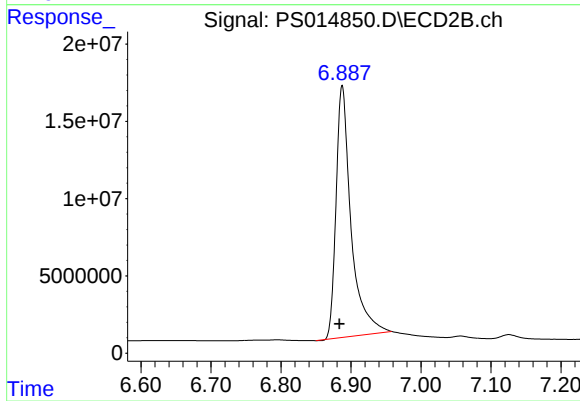

#4 2,4-DCAA


R.T.: 6.888 min
Delta R.T.: 0.004 min
Response: 243197866
Conc: 522.50 ng/ml

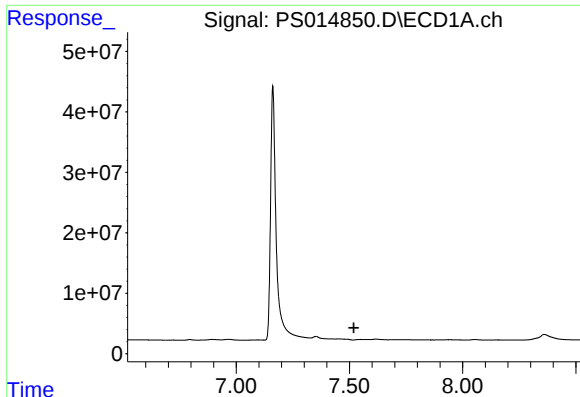

#6 MCP


R.T.: 0.000 min
Exp R.T.: 7.520 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

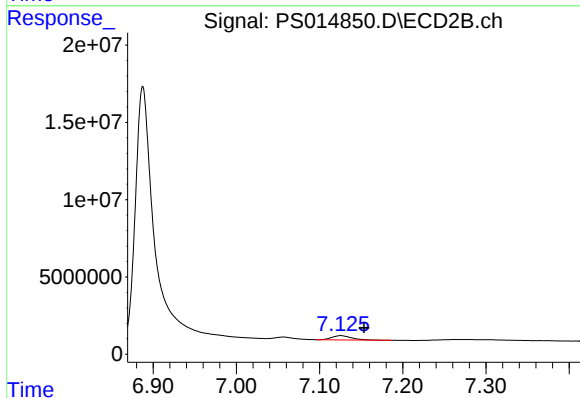


#6 MCP

R.T.: 7.125 min
Delta R.T.: -0.028 min
Response: 4476691
Conc: 2.66 ug/ml

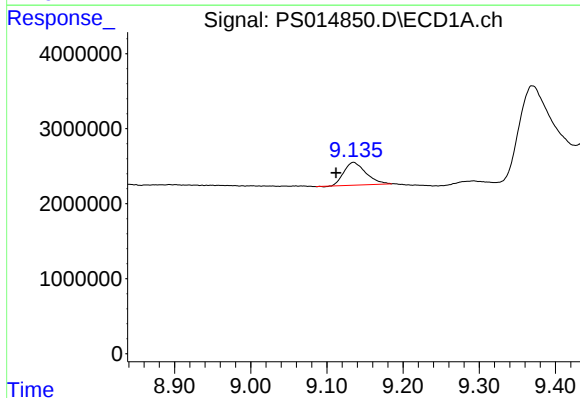


#11 2,4,5-TP (SILVEX)

R.T.: 9.135 min
Delta R.T.: 0.023 min
Response: 6091379
Conc: N.D.

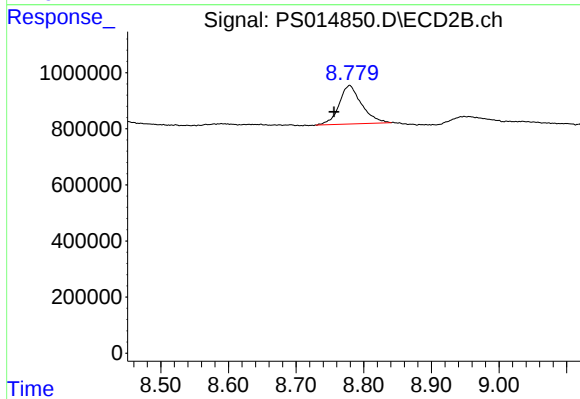

#11 2,4,5-TP (SILVEX)


R.T.: 8.779 min
Delta R.T.: 0.023 min
Response: 3173215
Conc: 1.16 ng/ml

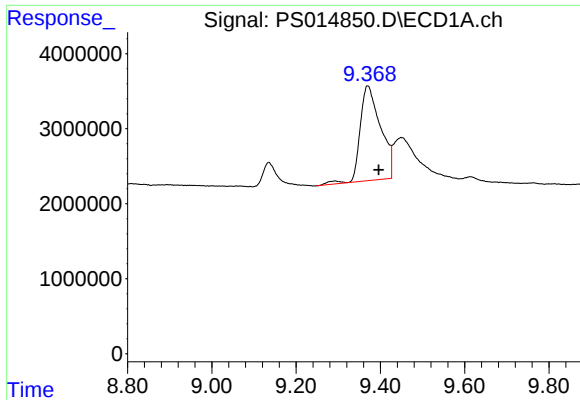

#12 2,4,5-T


R.T.: 9.370 min
Delta R.T.: -0.027 min
Response: 42626985
Conc: 5.18 ng/ml

Instrument :
ECD_S
ClientSampleId :

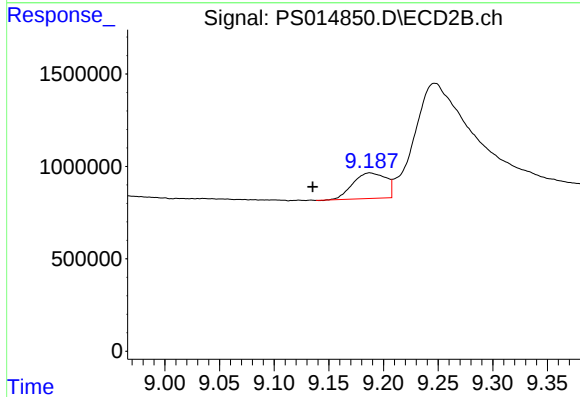


#12 2,4,5-T

R.T.: 9.187 min
Delta R.T.: 0.052 min
Response: 2922390
Conc: 1.12 ng/ml

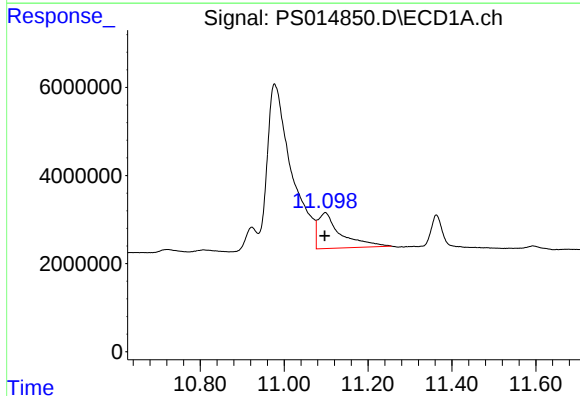


#14 DINOSEB

R.T.: 11.098 min
Delta R.T.: 0.001 min
Response: 30672960
Conc: 4.76 ng/ml

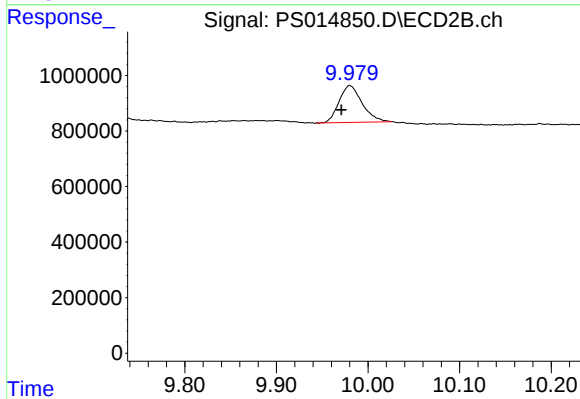

#14 DINOSEB


R.T.: 9.980 min
Delta R.T.: 0.009 min
Response: 2325574
Conc: 1.21 ng/ml

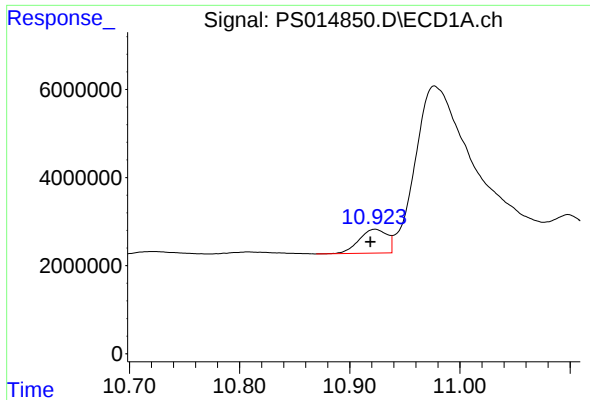

#15 Picloram


R.T.: 10.923 min
Delta R.T.: 0.004 min
Response: 9613561
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

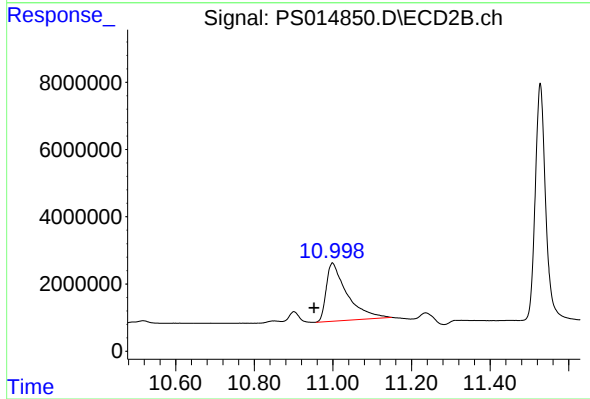


#15 Picloram

R.T.: 10.999 min
Delta R.T.: 0.046 min
Response: 63484696
Conc: 16.93 ng/ml

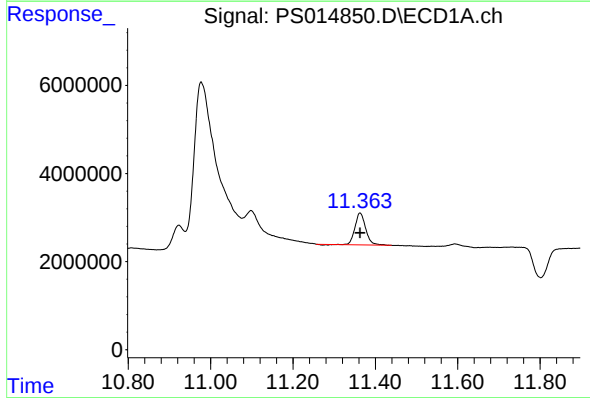

#16 DCPA

R.T.: 11.363 min
Delta R.T.: 0.000 min
Response: 13031414
Conc: 1.06 ng/ml

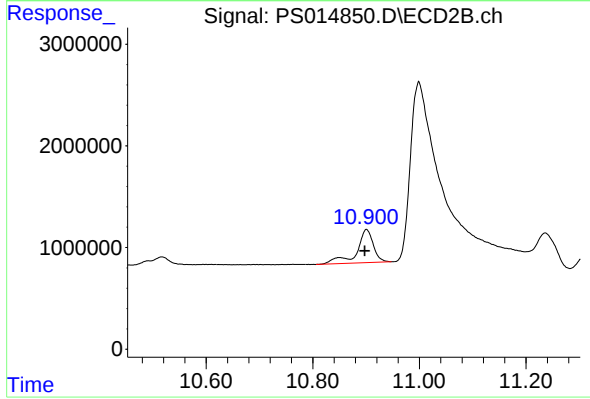

#16 DCPA

R.T.: 10.901 min
Delta R.T.: 0.003 min
Response: 7050962
Conc: 1.74 ng/ml