

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS042921\
 Data File : PS014856.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Apr 2021 19:13
 Operator : DD\AJ
 Sample : M2196-02MS
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 WALL-D-4075-AMS

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 30 02:12:25 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS040821.M
 Quant Title : 8080.M
 QLast Update : Thu Apr 08 14:34:06 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.157	6.885	877.2E6	320.9E6	576.622	689.488
Target Compounds							
1) T	Dalapon	3.007	2.606	799.0E6	339.3E6	443.117	521.303
2) T	3,5-DICHL...	6.383	6.048	1269.2E6	380.0E6	612.555	518.175
3) T	4-Nitroph...	7.020	0.000	6908197	0	8.501	N.D. #
5) T	DICAMBA	7.345	7.050	3185.7E6	1128.2E6	547.525	557.814
6) T	MCPD	7.509	7.144	252.2E6	100.5E6	57.915	59.696
7) T	MCPA	7.657	7.358	372.5E6	298.3E6	59.857	122.819 #
8) T	DICHLORPROP	8.031	7.676	807.2E6	310.0E6	576.818	614.008
9) T	2,4-D	8.261	7.973	993.7E6	395.4E6	624.949	711.006
10) T	Pentachlo...	8.565	8.395	12466.3E6	4132.6E6	593.160	614.740
11) T	2,4,5-TP ...	9.110	8.756	5123.8E6	1715.7E6	625.890	628.075
12) T	2,4,5-T	9.396	9.136	4674.5E6	1544.8E6	568.249	590.641
13) T	2,4-DB	9.945	9.643	599.1E6	194.8E6	393.696	561.538 #
14) T	DINOSEB	11.092	9.971	3459.5E6	1065.8E6	536.887	553.456
15) T	Picloram	10.924	10.958	4571.7E6	1638.4E6	408.619	436.920
16) T	DCPA	11.358	10.896	5474.3E6	2052.0E6	444.266	505.324



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS042921\
Data File : PS014856.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Apr 2021 19:13
Operator : DD\AJ
Sample : M2196-02MS
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
WALL-D-4075-AMS

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 30 02:12:25 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS040821.M
Quant Title : 8080.M
QLast Update : Thu Apr 08 14:34:06 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

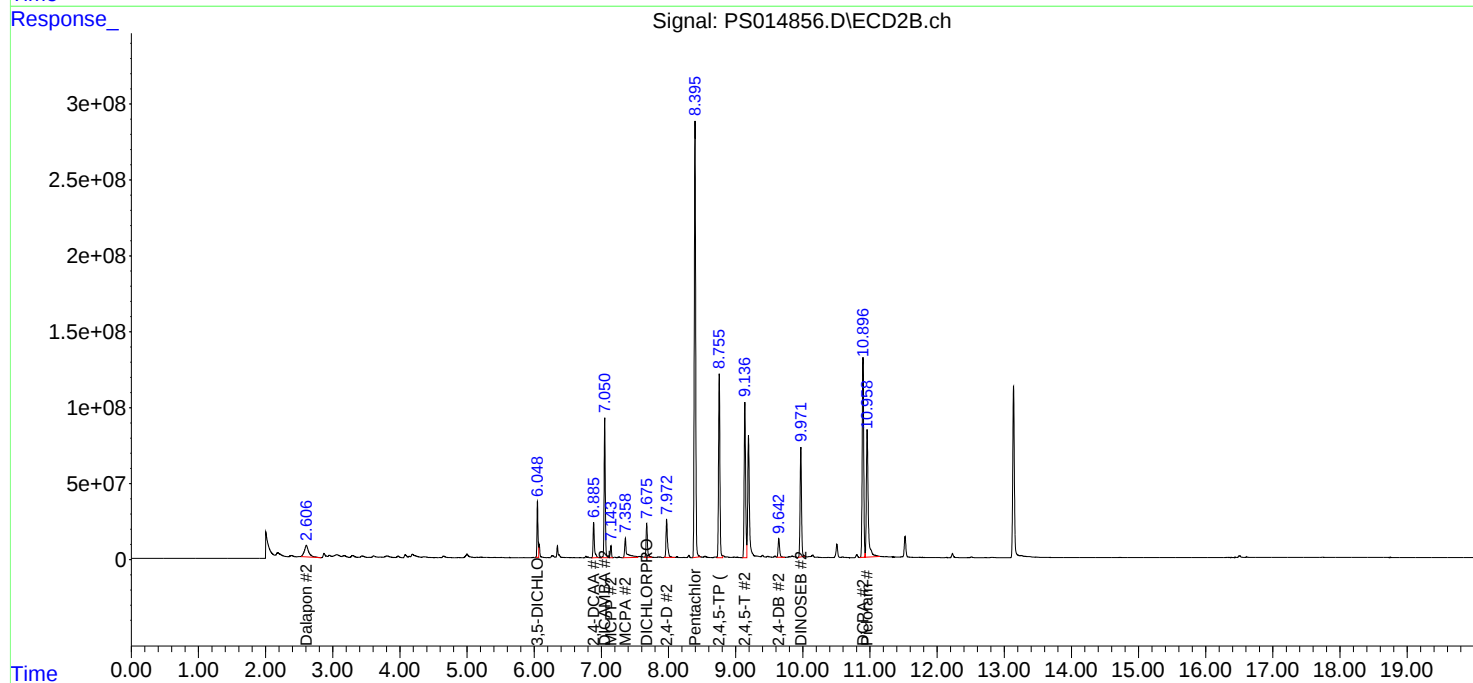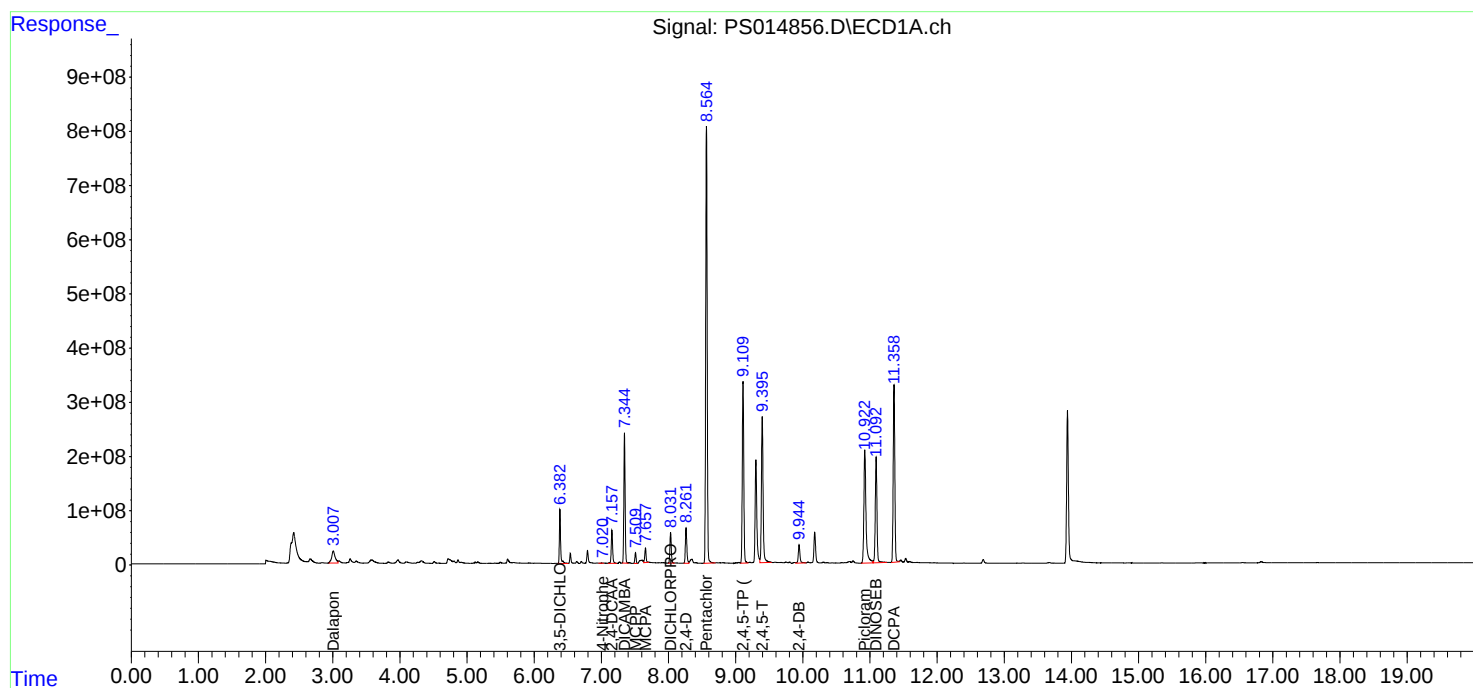


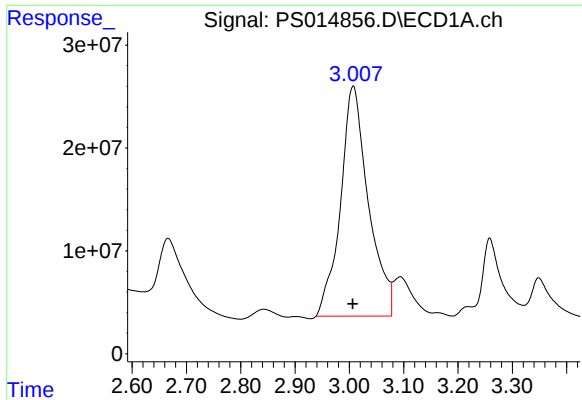

#1 Dalapon


R.T.: 3.007 min
Delta R.T.: 0.001 min
Response: 799016154
Conc: 443.12 ng/ml

Instrument :
ECD_S
ClientSampleId :
WALL-D-4075-AMS

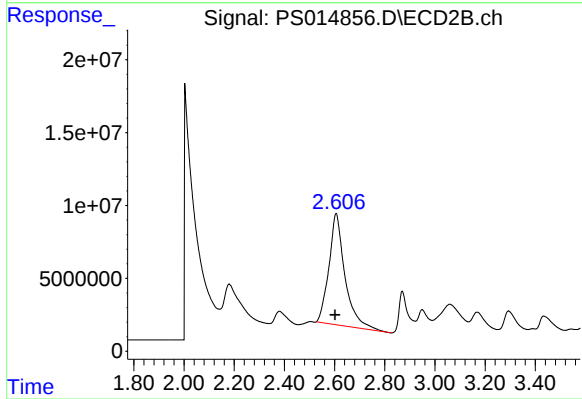


#1 Dalapon

R.T.: 2.606 min
Delta R.T.: 0.004 min
Response: 339276964
Conc: 521.30 ng/ml

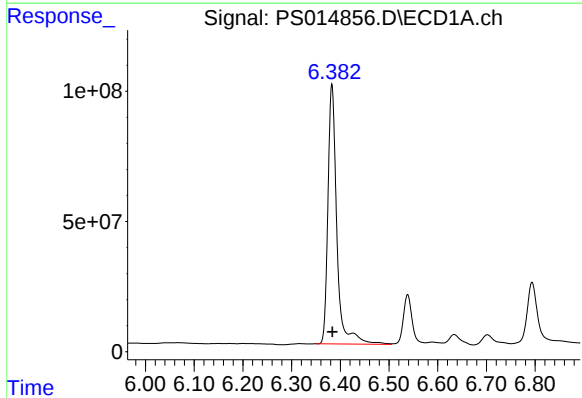


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.383 min
Delta R.T.: 0.000 min
Response: 1269216513
Conc: 612.56 ng/ml

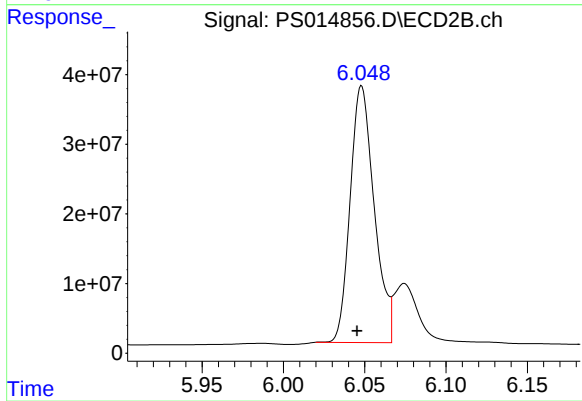

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.048 min
Delta R.T.: 0.003 min
Response: 379976279
Conc: 518.18 ng/ml

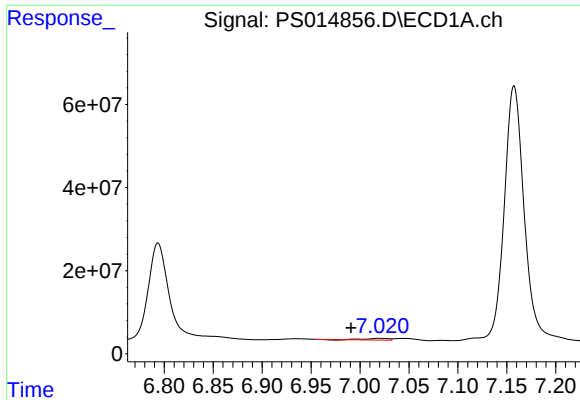

#3 4-Nitrophenol


R.T.: 7.020 min
Delta R.T.: 0.029 min
Response: 6908197
Conc: 8.50 ng/ml

Instrument :
ECD_S
ClientSampleId :
WALL-D-4075-AMS

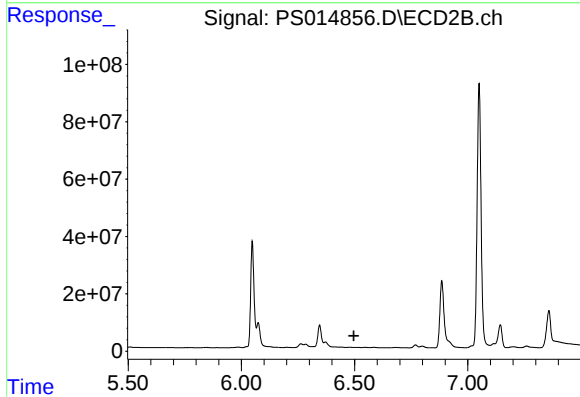


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T.: 6.497 min
Response: 0
Conc: N.D.

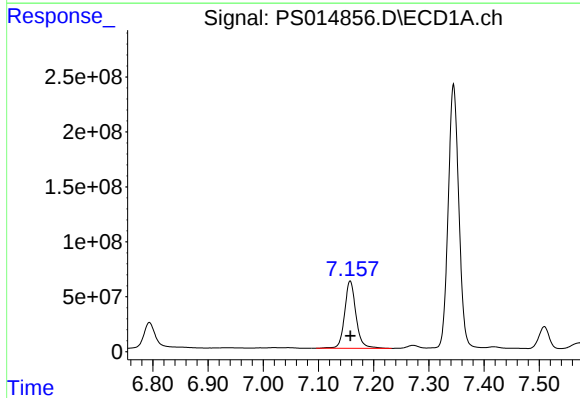


#4 2,4-DCAA

R.T.: 7.157 min
Delta R.T.: 0.000 min
Response: 877154320
Conc: 576.62 ng/ml

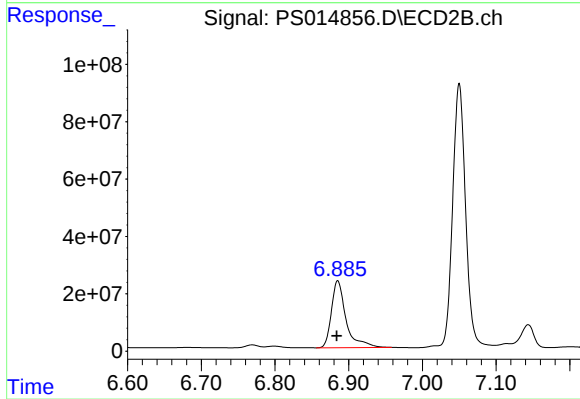

#4 2,4-DCAA


R.T.: 6.885 min
Delta R.T.: 0.002 min
Response: 320925612
Conc: 689.49 ng/ml

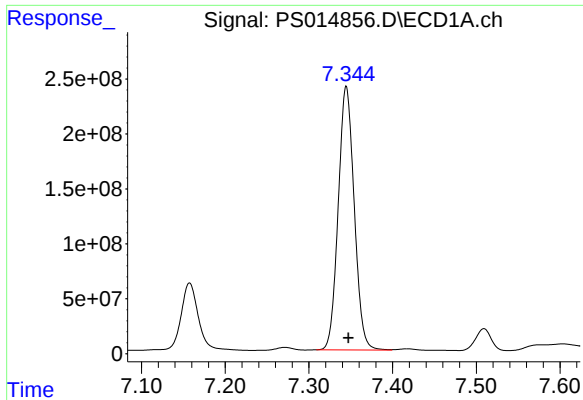

#5 DICAMBA


R.T.: 7.345 min
Delta R.T.: -0.002 min
Response: 3185696430
Conc: 547.53 ng/ml

Instrument :
ECD_S
ClientSampleId :
WALL-D-4075-AMS

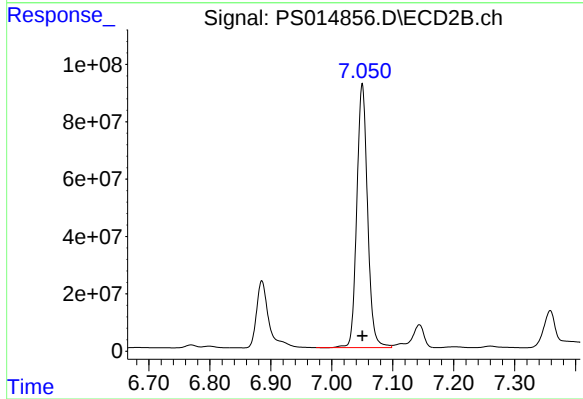


#5 DICAMBA

R.T.: 7.050 min
Delta R.T.: 0.000 min
Response: 1128193104
Conc: 557.81 ng/ml

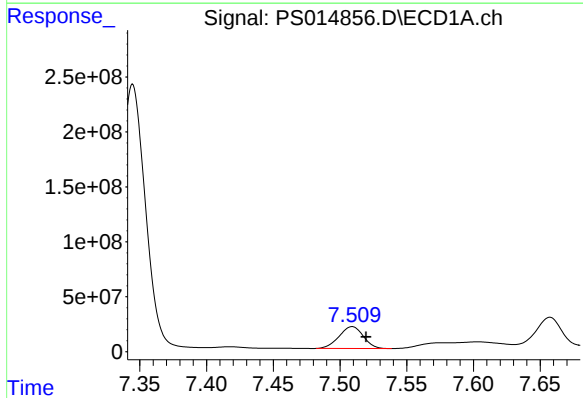


#6 MCP

R.T.: 7.509 min
Delta R.T.: -0.011 min
Response: 252175461
Conc: 57.92 ug/ml

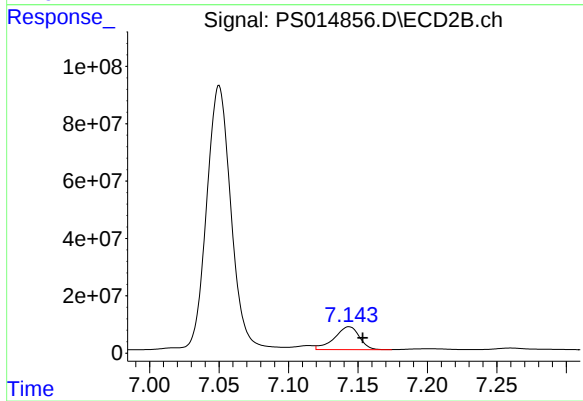

#6 MCP


R.T.: 7.144 min
Delta R.T.: -0.010 min
Response: 100531537
Conc: 59.70 ug/ml

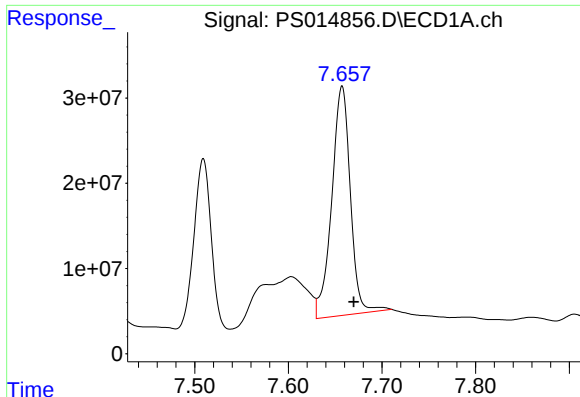

#7 MCPA


R.T.: 7.657 min
Delta R.T.: -0.013 min
Response: 372487385
Conc: 59.86 ug/ml

Instrument :
ECD_S
ClientSampleId :
WALL-D-4075-AMS

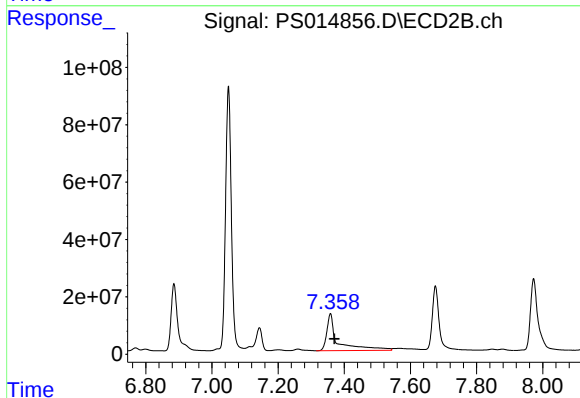


#7 MCPA

R.T.: 7.358 min
Delta R.T.: -0.012 min
Response: 298268093
Conc: 122.82 ug/ml

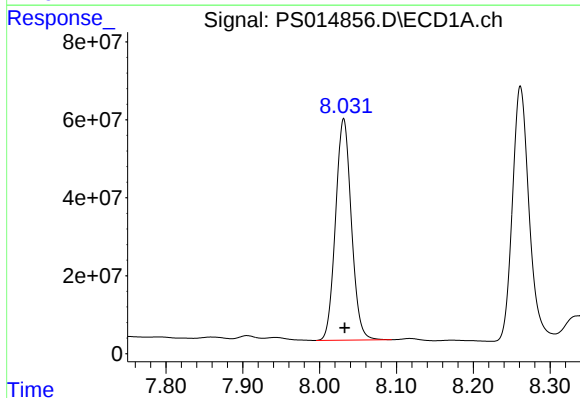


#8 DICHLORPROP

R.T.: 8.031 min
Delta R.T.: -0.001 min
Response: 807160091
Conc: 576.82 ng/ml

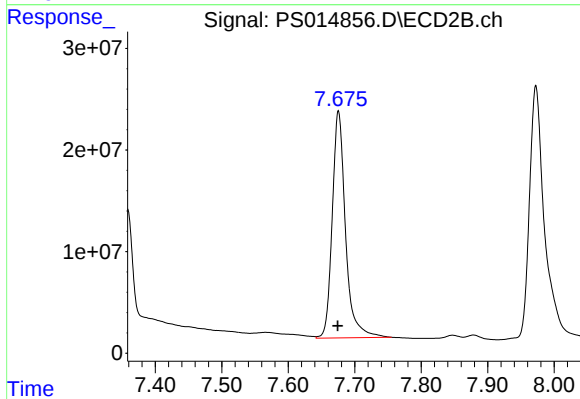

#8 DICHLORPROP


R.T.: 7.676 min
Delta R.T.: 0.000 min
Response: 309963836
Conc: 614.01 ng/ml

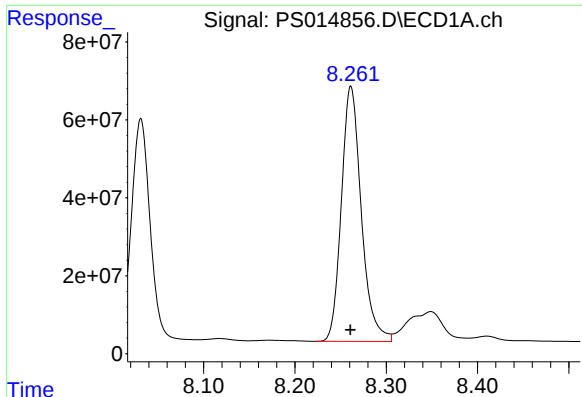

#9 2,4-D


R.T.: 8.261 min
Delta R.T.: 0.000 min
Response: 993659475
Conc: 624.95 ng/ml

Instrument :
ECD_S
ClientSampleId :
WALL-D-4075-AMS

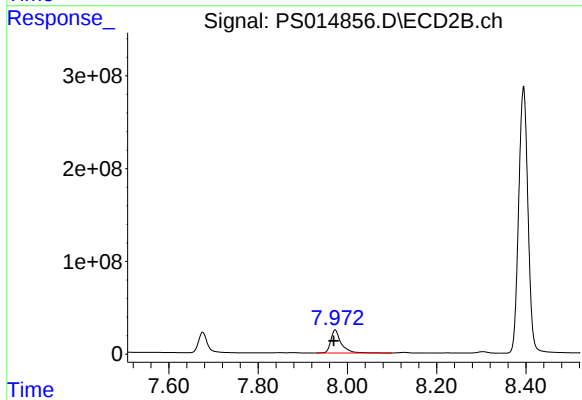


#9 2,4-D

R.T.: 7.973 min
Delta R.T.: 0.003 min
Response: 395386476
Conc: 711.01 ng/ml

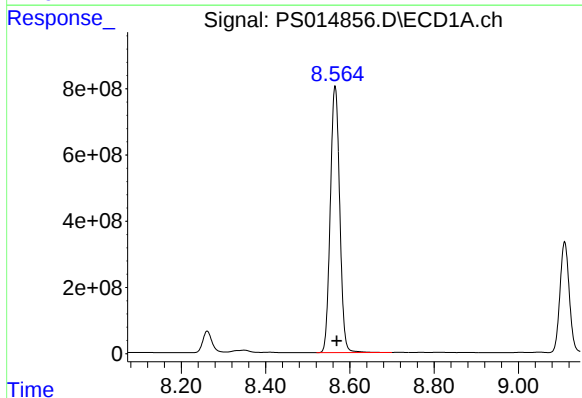


#10 Pentachlorophenol

R.T.: 8.565 min
Delta R.T.: -0.004 min
Response: 12466291108
Conc: 593.16 ng/ml

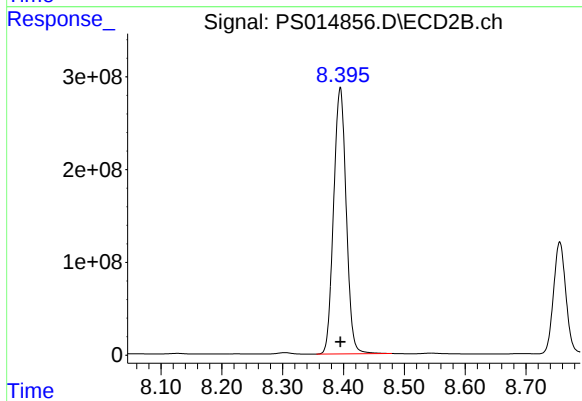

#10 Pentachlorophenol


R.T.: 8.395 min
Delta R.T.: 0.000 min
Response: 4132618392
Conc: 614.74 ng/ml

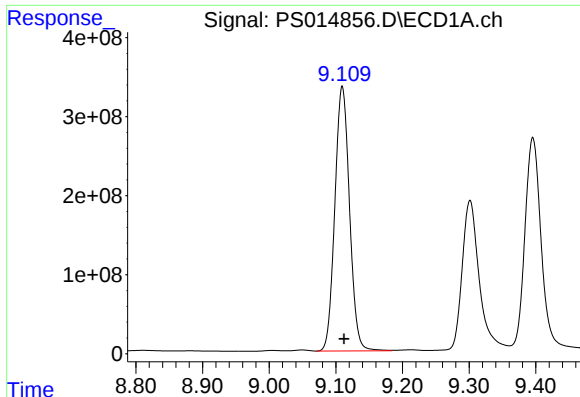

#11 2,4,5-TP (SILVEX)


R.T.: 9.110 min
Delta R.T.: -0.002 min
Response: 5123799169
Conc: 625.89 ng/ml

Instrument :
ECD_S
ClientSampleId :
WALL-D-4075-AMS

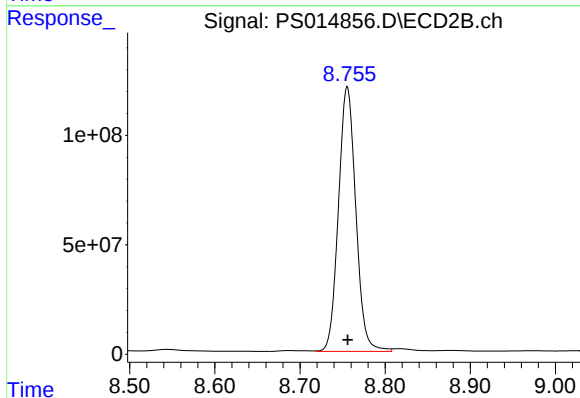


#11 2,4,5-TP (SILVEX)

R.T.: 8.756 min
Delta R.T.: 0.000 min
Response: 1715692354
Conc: 628.07 ng/ml

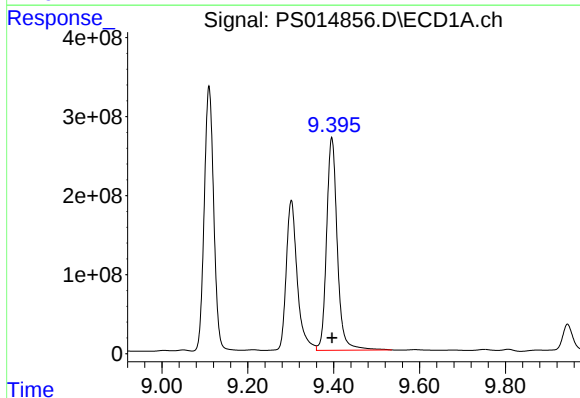


#12 2,4,5-T

R.T.: 9.396 min
Delta R.T.: 0.000 min
Response: 4674474482
Conc: 568.25 ng/ml

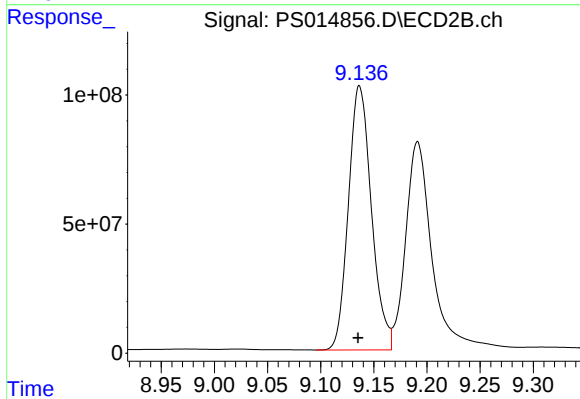

#12 2,4,5-T


R.T.: 9.136 min
Delta R.T.: 0.001 min
Response: 1544846472
Conc: 590.64 ng/ml

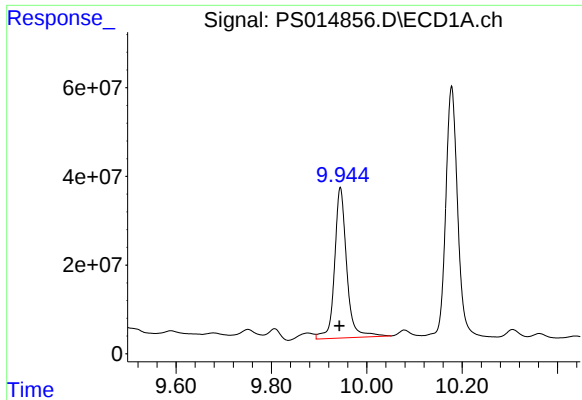

#13 2,4-DB


R.T.: 9.945 min
Delta R.T.: 0.002 min
Response: 599108913
Conc: 393.70 ng/ml

Instrument :
ECD_S
ClientSampleId :
WALL-D-4075-AMS

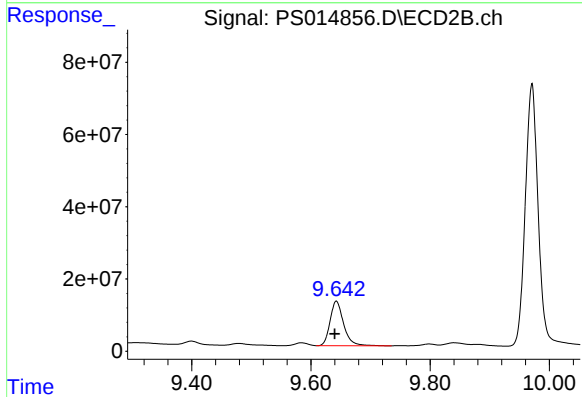


#13 2,4-DB

R.T.: 9.643 min
Delta R.T.: 0.003 min
Response: 194781778
Conc: 561.54 ng/ml

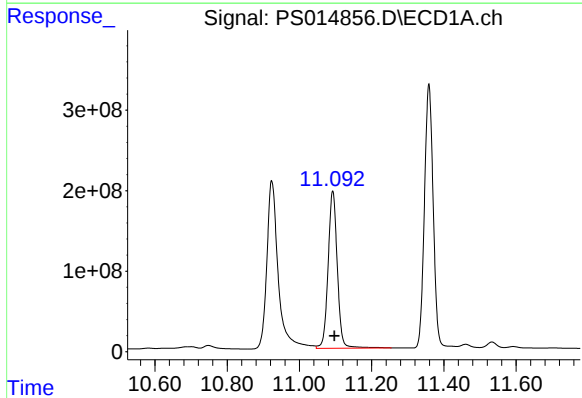


#14 DINOSEB

R.T.: 11.092 min
Delta R.T.: -0.004 min
Response: 3459507871
Conc: 536.89 ng/ml

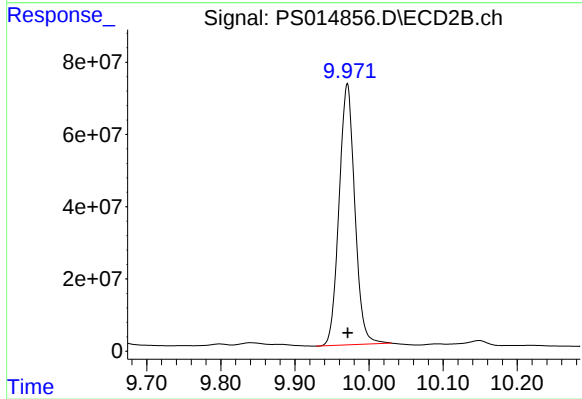

#14 DINOSEB


R.T.: 9.971 min
Delta R.T.: 0.000 min
Response: 1065776913
Conc: 553.46 ng/ml

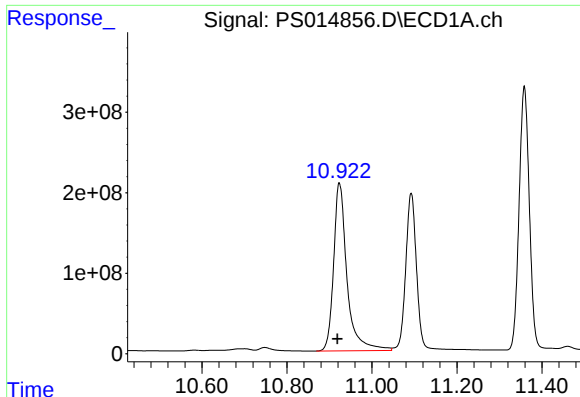

#15 Picloram


R.T.: 10.924 min
Delta R.T.: 0.005 min
Response: 4571748361
Conc: 408.62 ng/ml

Instrument :
ECD_S
ClientSampleId :
WALL-D-4075-AMS

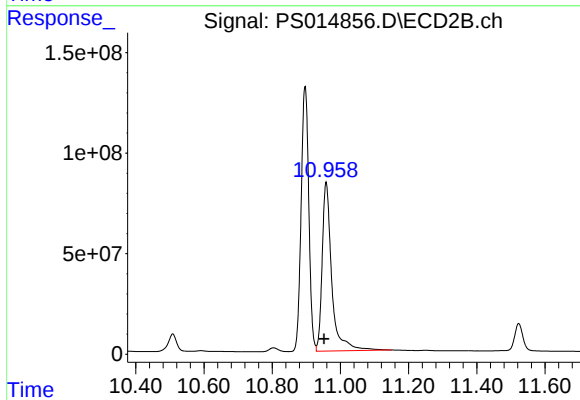


#15 Picloram

R.T.: 10.958 min
Delta R.T.: 0.006 min
Response: 1638406942
Conc: 436.92 ng/ml

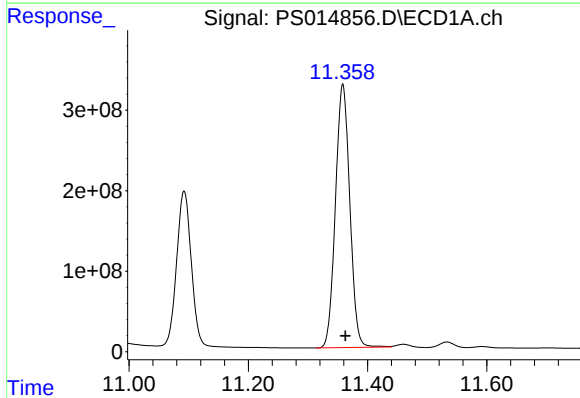

#16 DCPA

R.T.: 11.358 min
Delta R.T.: -0.004 min
Response: 5474260754
Conc: 444.27 ng/ml

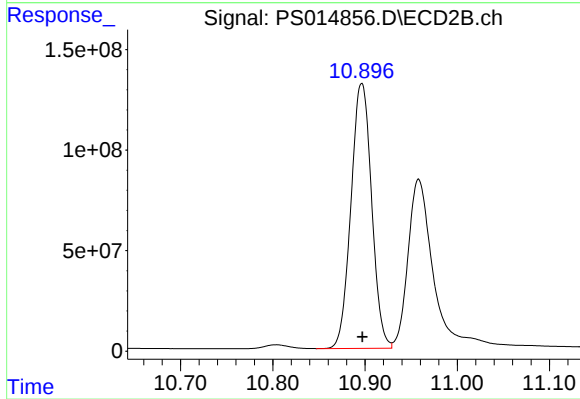

#16 DCPA

R.T.: 10.896 min
Delta R.T.: 0.000 min
Response: 2051959212
Conc: 505.32 ng/ml