

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS042921\
 Data File : PS014858.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Apr 2021 20:06
 Operator : DD\AJ
 Sample : M2196-06
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 WALL-D-4075-B

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 30 02:12:48 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS040821.M
 Quant Title : 8080.M
 QLast Update : Thu Apr 08 14:34:06 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.159	6.885	785.4E6	283.9E6	516.307	609.904
Target Compounds							
1) T	Dalapon	2.967	2.569	70694359	50429147	39.206	77.485 #
2) T	3,5-DICHL...	6.429f	6.076	29537351	69223418	14.255	94.400 #
3) T	4-Nitroph...	7.047f	6.478	9413929	5847175	11.585	20.710 #
5) T	DICAMBA	7.333	7.020	19961324	7811822	3.431	3.862
6) T	MCP	7.506	7.117	4416227	17198282	1.014	10.212 #
7) T	MCPA	7.699	0.000	2811166	0	<MDL	N.D. #
8) T	DICHLORPROP	0.000	7.727f	0	5598687	N.D.	11.090
10) T	Pentachlo...	8.570	8.398	7951913	3619972	<MDL	<MDL #
11) T	2,4,5-TP ...	9.112	8.733	8982068	4328763	1.097	1.585 #
12) T	2,4,5-T	9.456f	0.000	7732420	0	<MDL	N.D. #
13) T	2,4-DB	9.913	0.000	39532187	0	25.978	N.D. #
14) T	DINOSEB	11.076	10.011f	18169263	4699939	2.820	2.441
15) T	Picloram	10.920	10.994f	8461838	4308451	<MDL	1.149 #
16) T	DCPA	11.367	10.896	7037855	7154969	<MDL	1.762 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS042921\
Data File : PS014858.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Apr 2021 20:06
Operator : DD\AJ
Sample : M2196-06
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleID :
WALL-D-4075-B

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 30 02:12:48 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS040821.M
Quant Title : 8080.M
QLast Update : Thu Apr 08 14:34:06 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

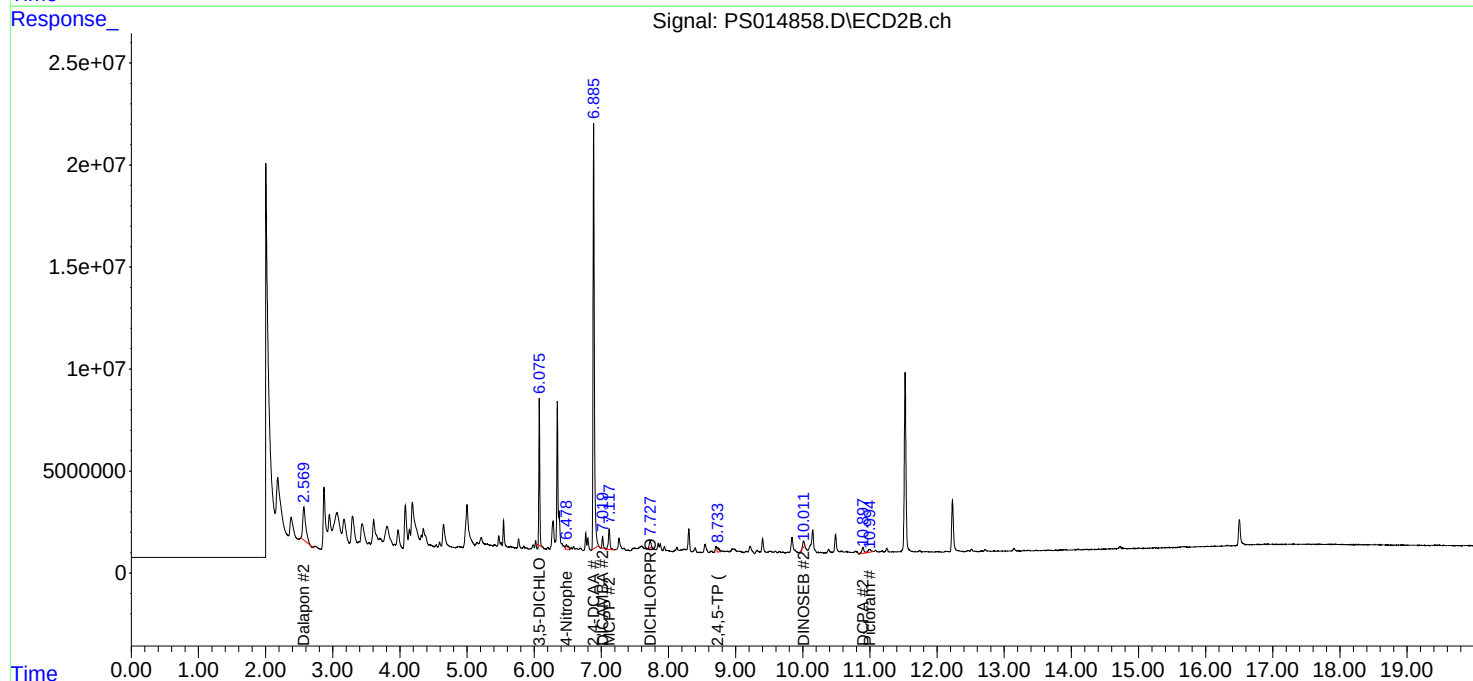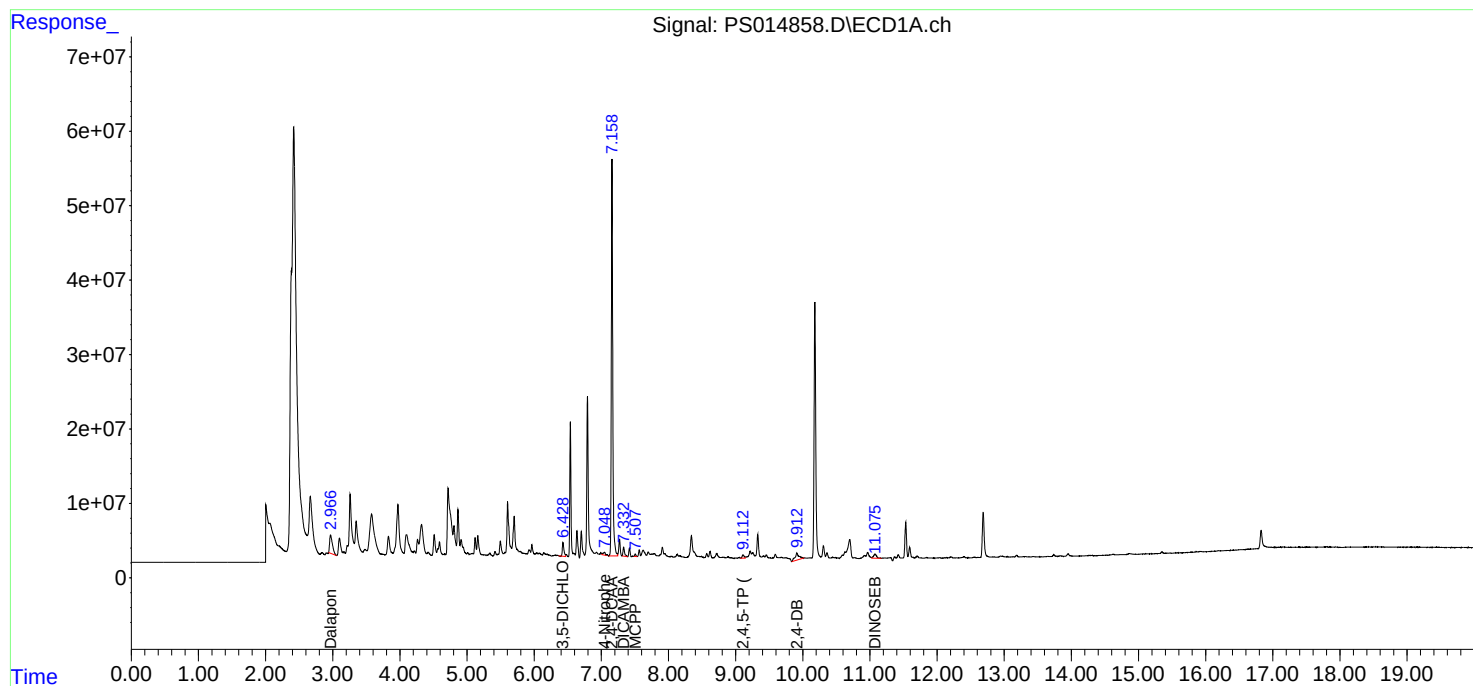


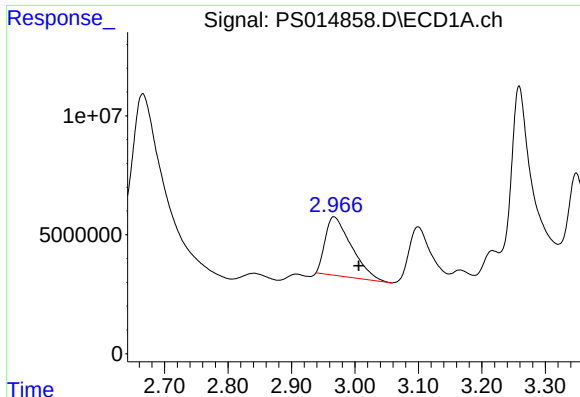

#1 Dalapon


R.T.: 2.967 min
Delta R.T.: -0.039 min
Response: 70694359
Conc: 39.21 ng/ml

Instrument :
ECD_S
ClientSampleId :
WALL-D-4075-B

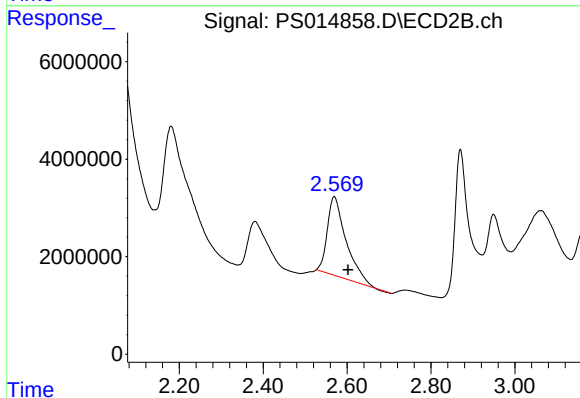


#1 Dalapon

R.T.: 2.569 min
Delta R.T.: -0.033 min
Response: 50429147
Conc: 77.48 ng/ml

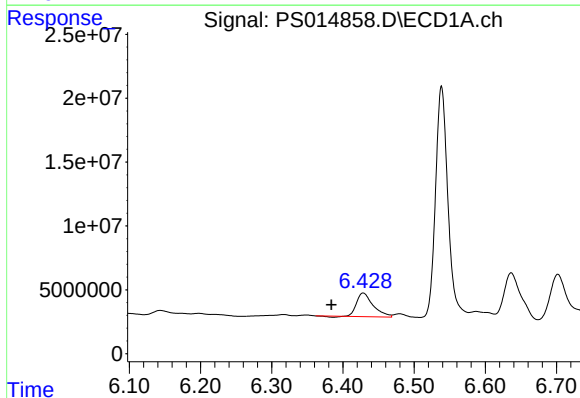


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.429 min
Delta R.T.: 0.045 min
Response: 29537351
Conc: 14.26 ng/ml

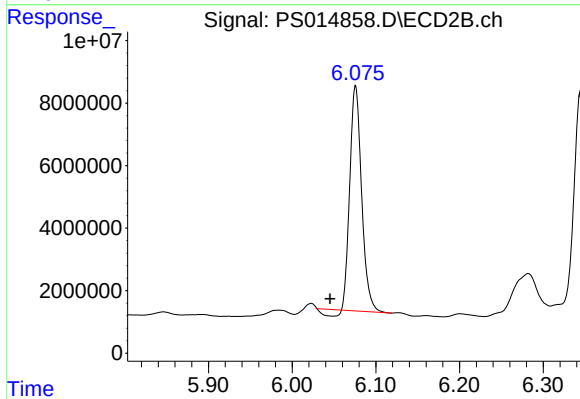

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.076 min
Delta R.T.: 0.030 min
Response: 69223418
Conc: 94.40 ng/ml

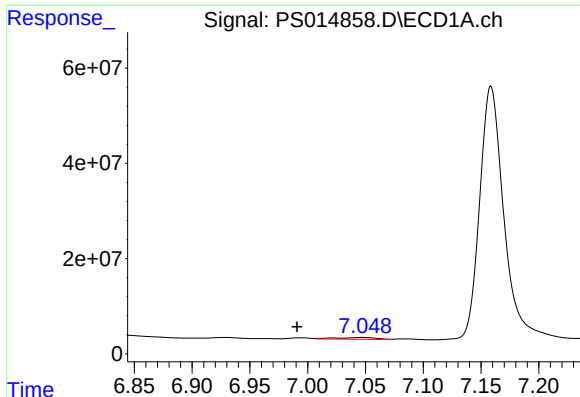

#3 4-Nitrophenol


R.T.: 7.047 min
Delta R.T.: 0.056 min
Response: 9413929
Conc: 11.58 ng/ml

Instrument :
ECD_S
ClientSampleId :
WALL-D-4075-B

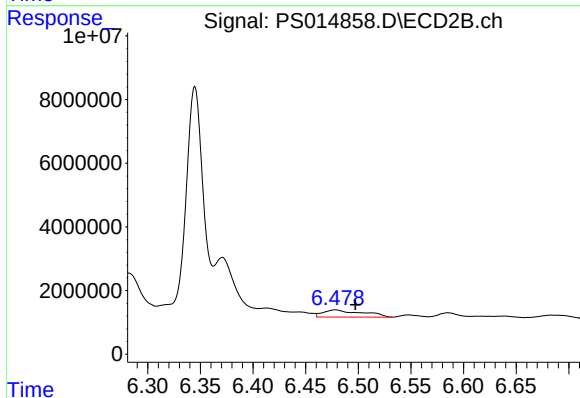


#3 4-Nitrophenol

R.T.: 6.478 min
Delta R.T.: -0.019 min
Response: 5847175
Conc: 20.71 ng/ml

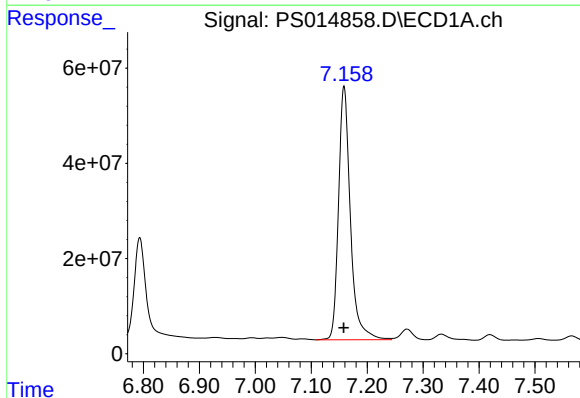


#4 2,4-DCAA

R.T.: 7.159 min
Delta R.T.: 0.000 min
Response: 785403203
Conc: 516.31 ng/ml

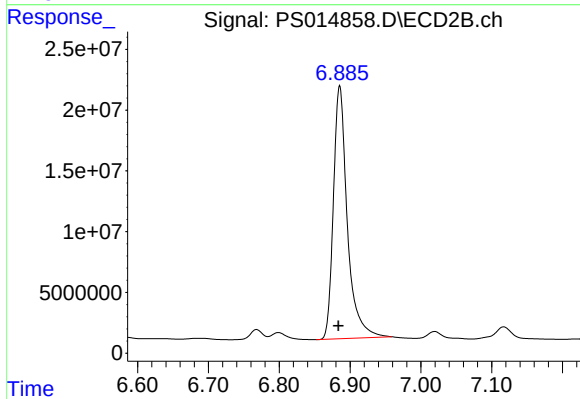

#4 2,4-DCAA


R.T.: 6.885 min
Delta R.T.: 0.002 min
Response: 283882925
Conc: 609.90 ng/ml

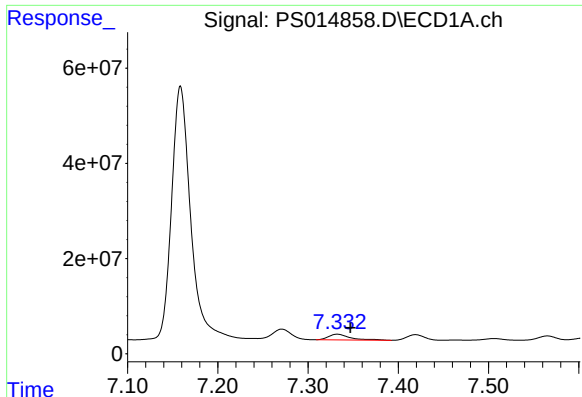

#5 DICAMBA


R.T.: 7.333 min
Delta R.T.: -0.014 min
Response: 19961324
Conc: 3.43 ng/ml

Instrument :
ECD_S
ClientSampleId :
WALL-D-4075-B

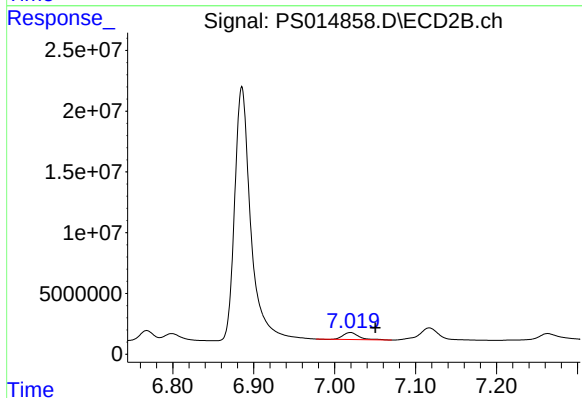


#5 DICAMBA

R.T.: 7.020 min
Delta R.T.: -0.031 min
Response: 7811822
Conc: 3.86 ng/ml

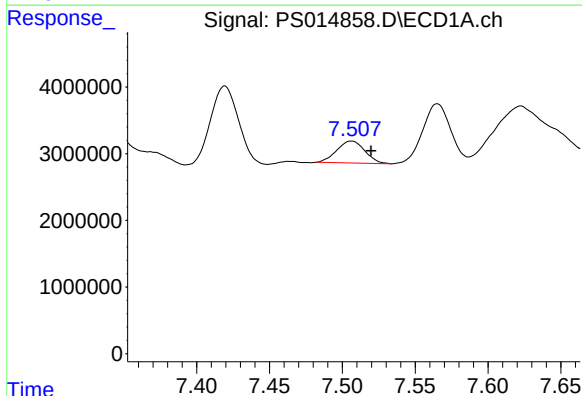


#6 MCP

R.T.: 7.506 min
Delta R.T.: -0.013 min
Response: 4416227
Conc: 1.01 ug/ml

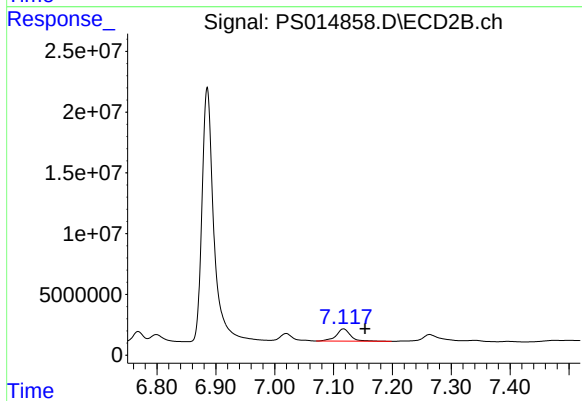

#6 MCP


R.T.: 7.117 min
Delta R.T.: -0.037 min
Response: 17198282
Conc: 10.21 ug/ml

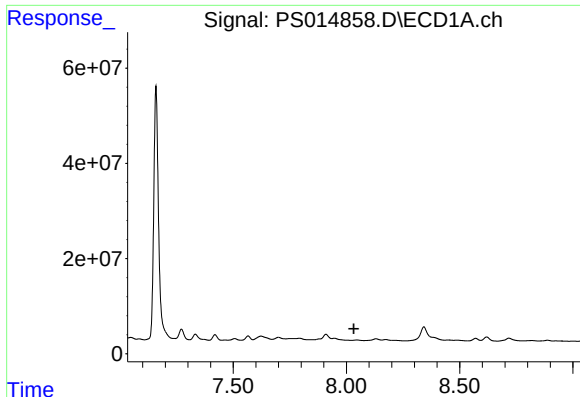

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 8.033 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
WALL-D-4075-B

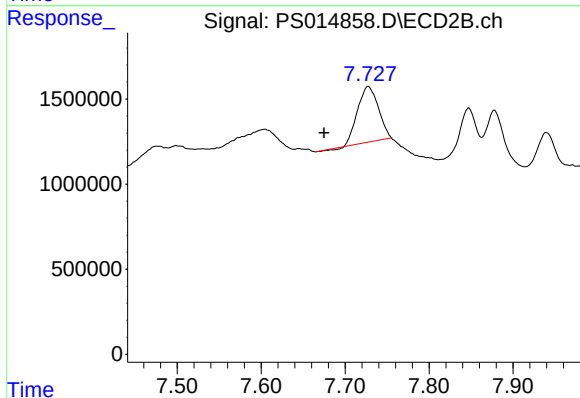


#8 DICHLORPROP

R.T.: 7.727 min
Delta R.T.: 0.053 min
Response: 5598687
Conc: 11.09 ng/ml

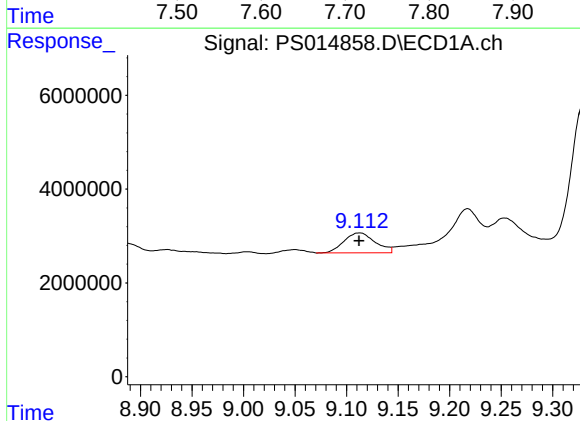


#11 2,4,5-TP (SILVEX)

R.T.: 9.112 min
Delta R.T.: 0.000 min
Response: 8982068
Conc: 1.10 ng/ml

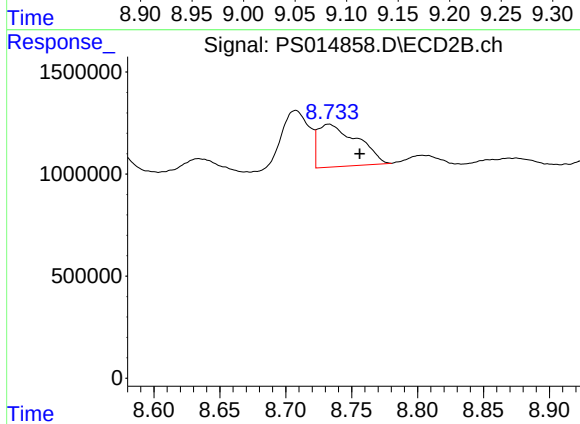

#11 2,4,5-TP (SILVEX)


R.T.: 8.733 min
Delta R.T.: -0.024 min
Response: 4328763
Conc: 1.58 ng/ml

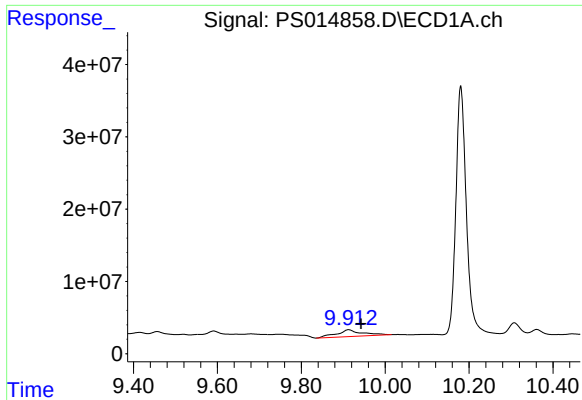

#13 2,4-DB


R.T.: 9.913 min
Delta R.T.: -0.030 min
Response: 39532187
Conc: 25.98 ng/ml

Instrument :
ECD_S
ClientSampleId :
WALL-D-4075-B

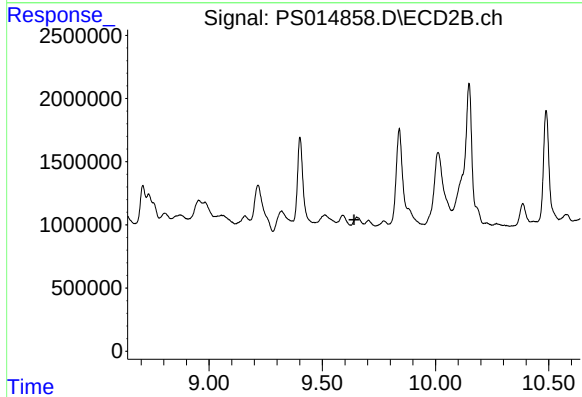


#13 2,4-DB

R.T.: 0.000 min
Exp R.T. : 9.640 min
Response: 0
Conc: N.D.

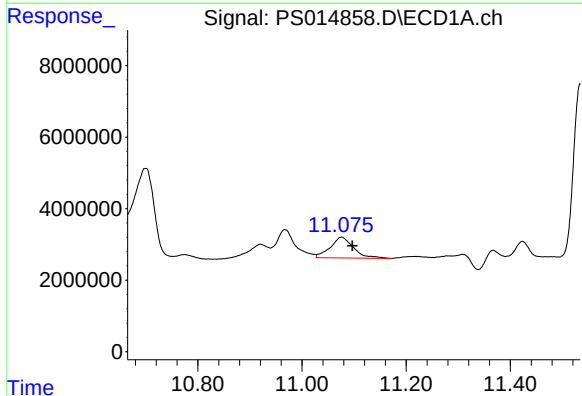


#14 DINOSEB

R.T.: 11.076 min
Delta R.T.: -0.021 min
Response: 18169263
Conc: 2.82 ng/ml

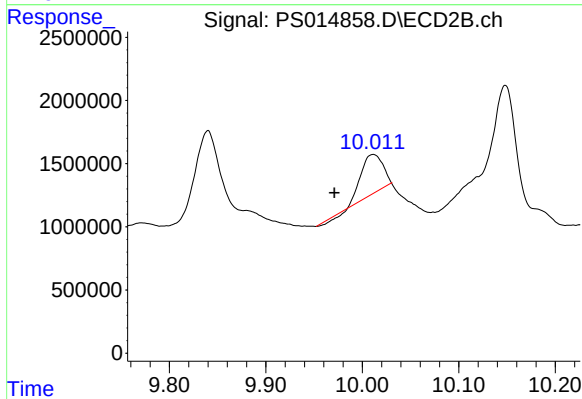

#14 DINOSEB


R.T.: 10.011 min
Delta R.T.: 0.040 min
Response: 4699939
Conc: 2.44 ng/ml

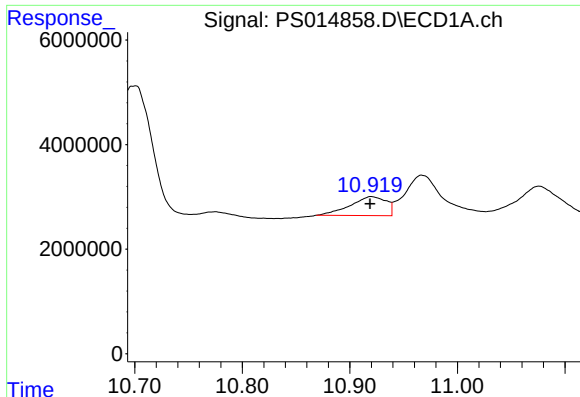

#15 Picloram


R.T.: 10.920 min
Delta R.T.: 0.001 min
Response: 8461838
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
WALL-D-4075-B

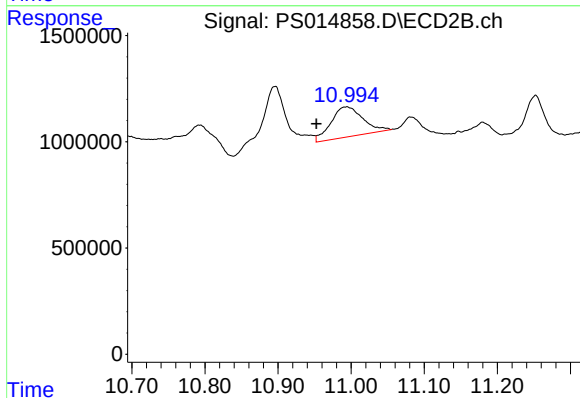


#15 Picloram

R.T.: 10.994 min
Delta R.T.: 0.042 min
Response: 4308451
Conc: 1.15 ng/ml

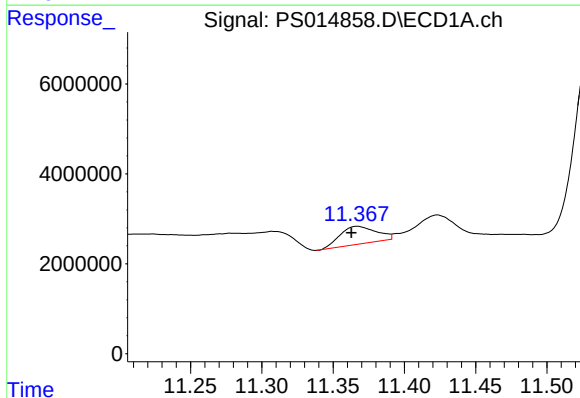

#16 DCPA

R.T.: 11.367 min
Delta R.T.: 0.004 min
Response: 7037855
Conc: N.D.

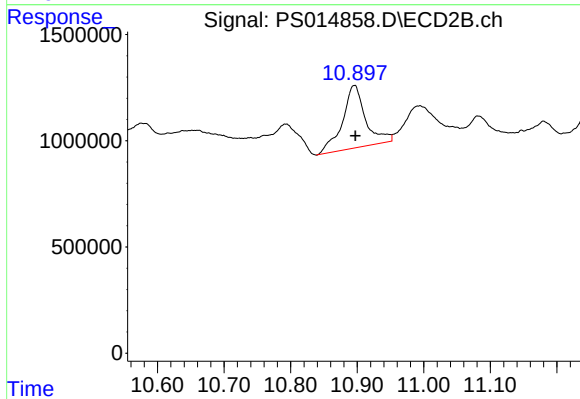

#16 DCPA

R.T.: 10.896 min
Delta R.T.: -0.001 min
Response: 7154969
Conc: 1.76 ng/ml