

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS042921\
 Data File : PS014865.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Apr 2021 23:09
 Operator : DD\AJ
 Sample : M2187-03
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 TEST-PIT-II

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 30 02:14:07 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS040821.M
 Quant Title : 8080.M
 QLast Update : Thu Apr 08 14:34:06 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.159	6.888	258.0E6	88022565	169.615	189.111
Target Compounds							
1) T	Dalapon	2.965f	2.568	71722700	79934519	39.776	122.820 #
2) T	3,5-DICHL...	0.000	6.076	0	35742446	N.D.	48.742
3) T	4-Nitroph...	7.045f	6.519	19779768	1080103	24.341	3.826 #
5) T	DICAMBA	7.355	7.021	5329232	5987988	<MDL	2.961 #
6) T	MCP	7.506	7.117	9236989	2884393	2.121	1.713
7) T	MCPA	7.646	7.343	13683600	41774380	2.199	17.202 #
8) T	DICHLORPROP	0.000	7.682	0	1061969	N.D.	2.104
9) T	2,4-D	8.218f	7.941	7948249	1430542	4.999	2.572 #
10) T	Pentachlo...	8.622f	8.396	28653085	2657654	1.363	<MDL #
11) T	2,4,5-TP ...	9.105	8.731	10467816	21501090	1.279	7.871 #
12) T	2,4,5-T	9.411	9.139	25128541	12511657	3.055	4.784 #
13) T	2,4-DB	9.954	0.000	8723983	0	5.733	N.D. #
14) T	DINOSEB	11.074	9.997	29825444	17537879	4.629	9.107 #
15) T	Picloram	10.915	10.985	7778032	11414444	<MDL	3.044 #
16) T	DCPA	11.431f	10.896	12760300	2744000	1.036	<MDL #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS042921\
Data File : PS014865.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Apr 2021 23:09
Operator : DD\AJ
Sample : M2187-03
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
TEST-PIT-II

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 30 02:14:07 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS040821.M
Quant Title : 8080.M
QLast Update : Thu Apr 08 14:34:06 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

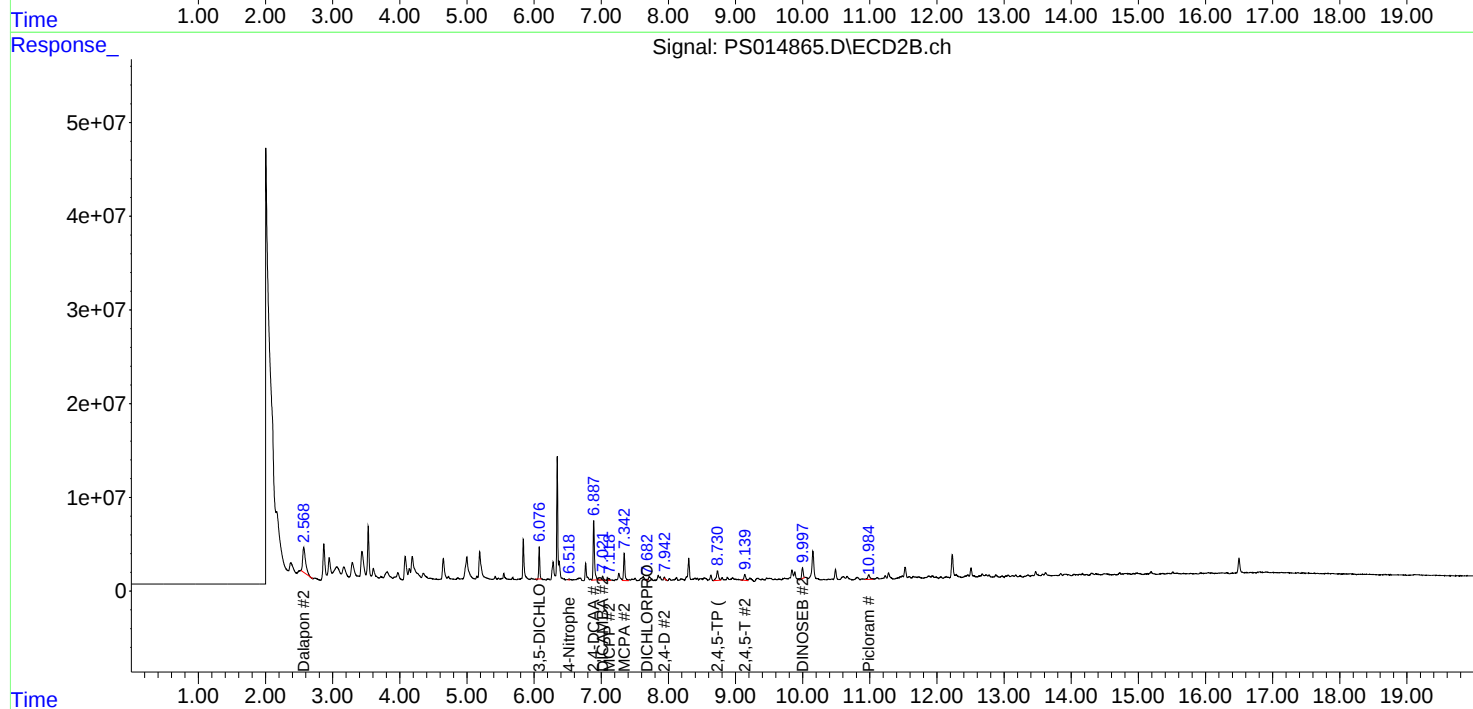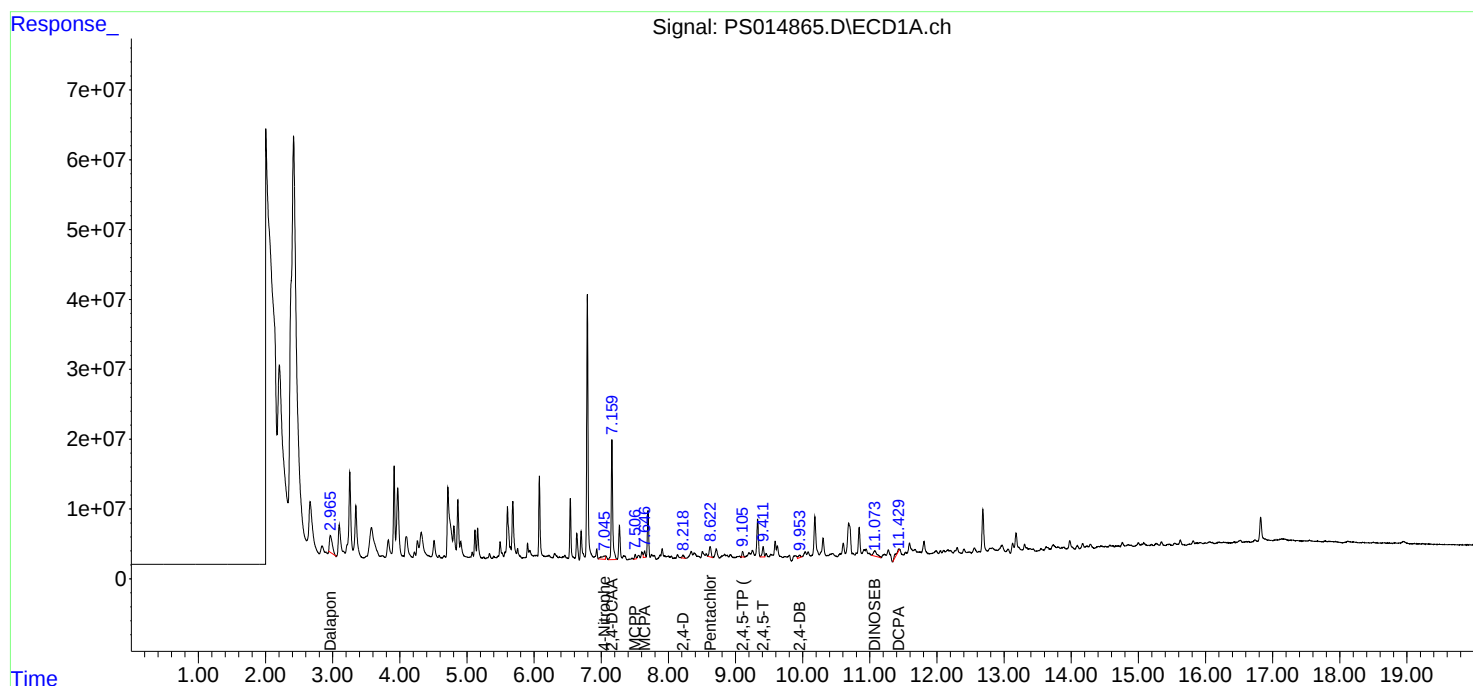


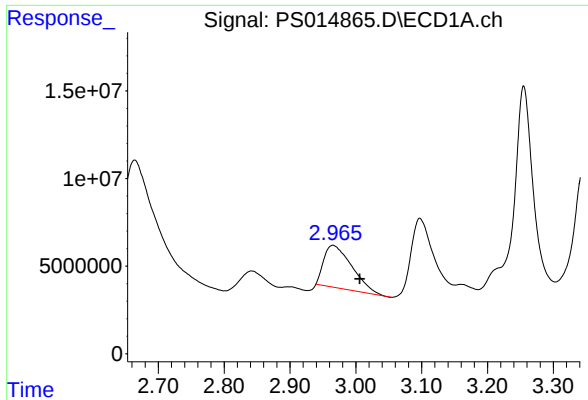

#1 Dalapon


R.T.: 2.965 min
Delta R.T.: -0.041 min
Response: 71722700
Conc: 39.78 ng/ml

Instrument :
ECD_S
ClientSampleId :
TEST-PIT-II

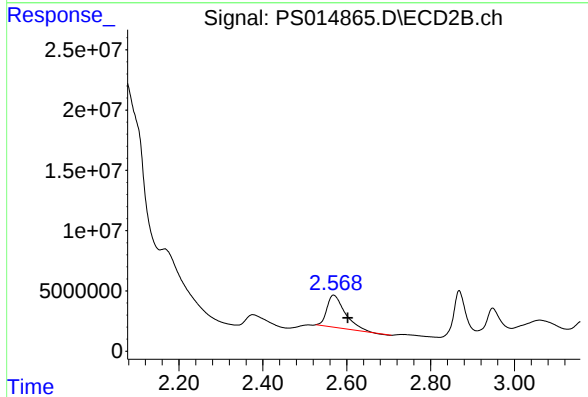


#1 Dalapon

R.T.: 2.568 min
Delta R.T.: -0.035 min
Response: 79934519
Conc: 122.82 ng/ml

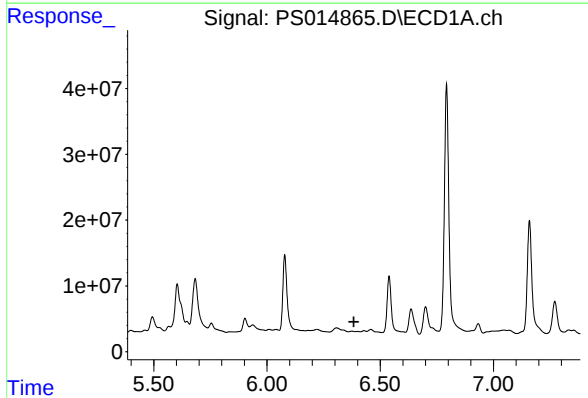


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.384 min
Response: 0
Conc: N.D.

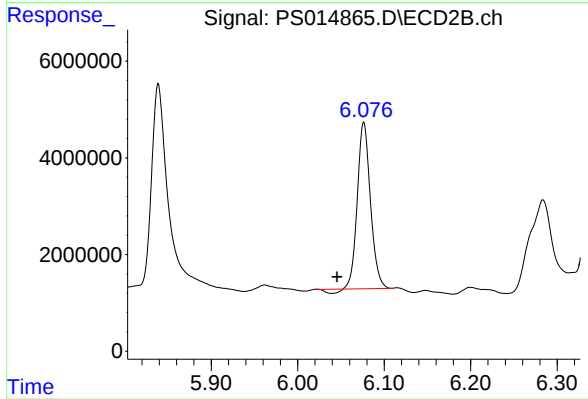

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.076 min
Delta R.T.: 0.031 min
Response: 35742446
Conc: 48.74 ng/ml

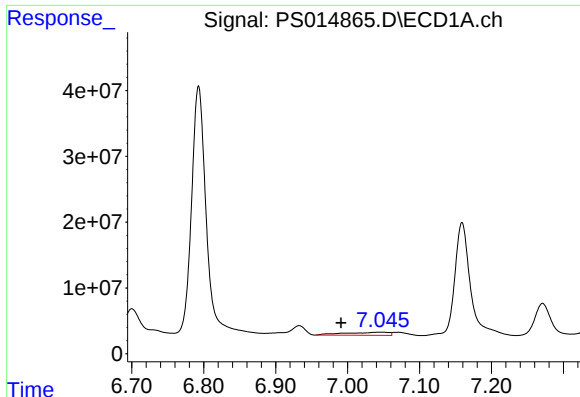

#3 4-Nitrophenol


R.T.: 7.045 min
Delta R.T.: 0.055 min
Response: 19779768
Conc: 24.34 ng/ml

Instrument :
ECD_S
ClientSampleId :
TEST-PIT-II

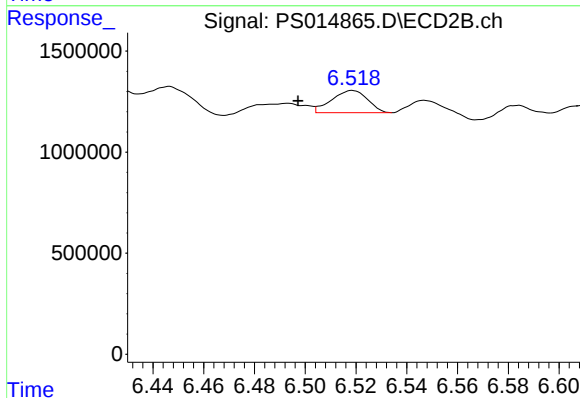


#3 4-Nitrophenol

R.T.: 6.519 min
Delta R.T.: 0.021 min
Response: 1080103
Conc: 3.83 ng/ml

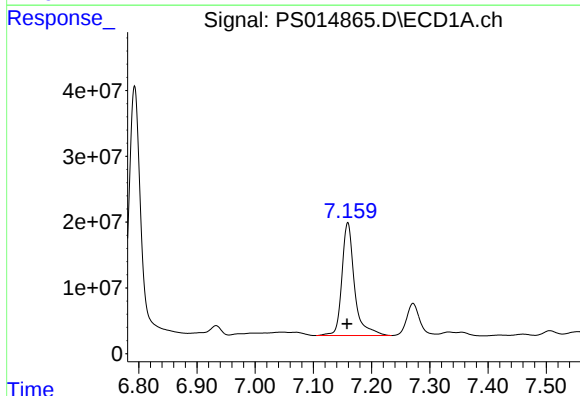


#4 2,4-DCAA

R.T.: 7.159 min
Delta R.T.: 0.001 min
Response: 258016916
Conc: 169.61 ng/ml

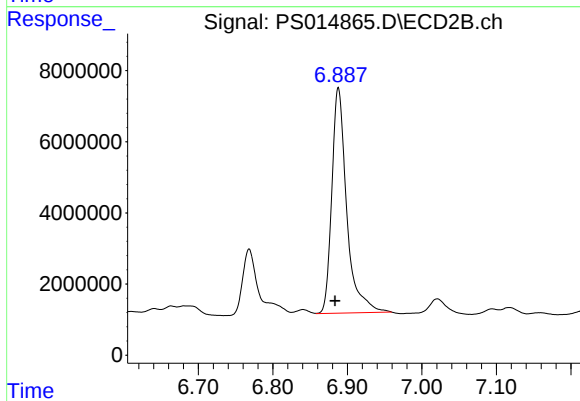

#4 2,4-DCAA


R.T.: 6.888 min
Delta R.T.: 0.004 min
Response: 88022565
Conc: 189.11 ng/ml

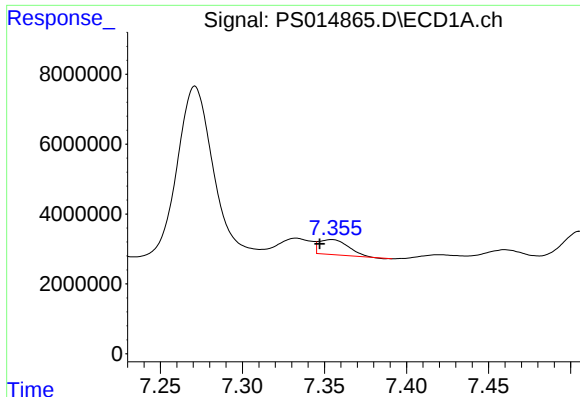

#5 DICAMBA


R.T.: 7.355 min
Delta R.T.: 0.008 min
Response: 5329232
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
TEST-PIT-II

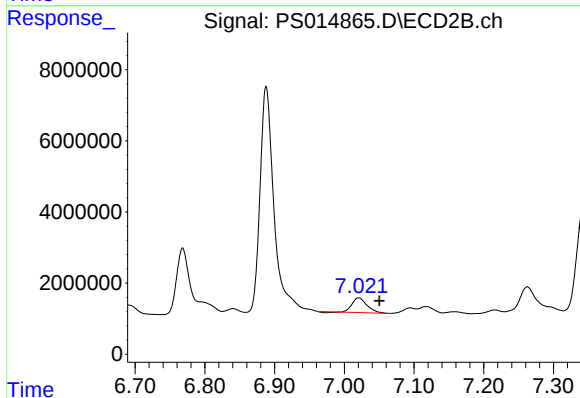


#5 DICAMBA

R.T.: 7.021 min
Delta R.T.: -0.029 min
Response: 5987988
Conc: 2.96 ng/ml

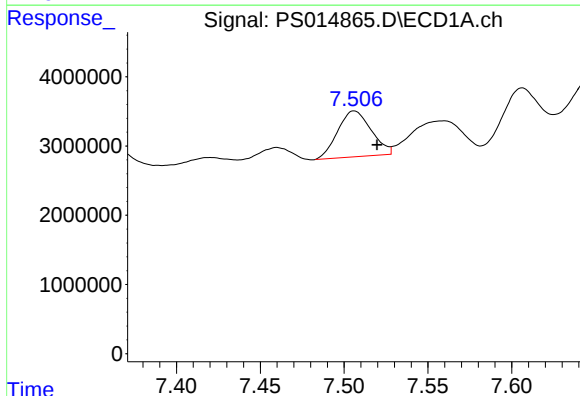


#6 MCP

R.T.: 7.506 min
Delta R.T.: -0.014 min
Response: 9236989
Conc: 2.12 ug/ml

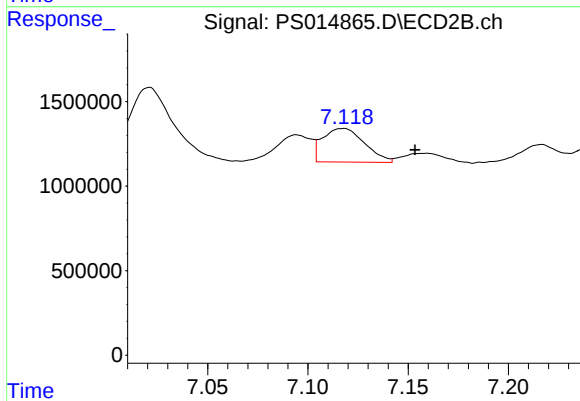

#6 MCP


R.T.: 7.117 min
Delta R.T.: -0.036 min
Response: 2884393
Conc: 1.71 ug/ml

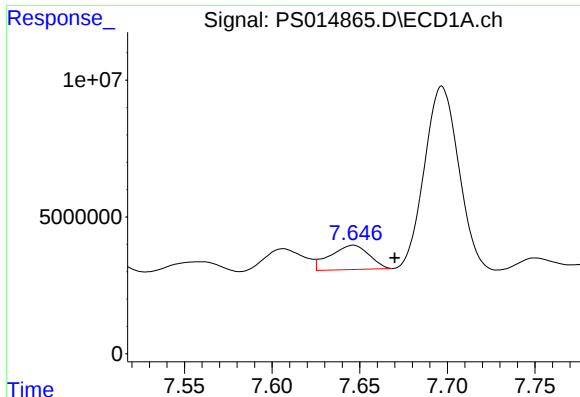

#7 MCPA


R.T.: 7.646 min
Delta R.T.: -0.024 min
Response: 13683600
Conc: 2.20 ug/ml

Instrument :
ECD_S
ClientSampleId :
TEST-PIT-II

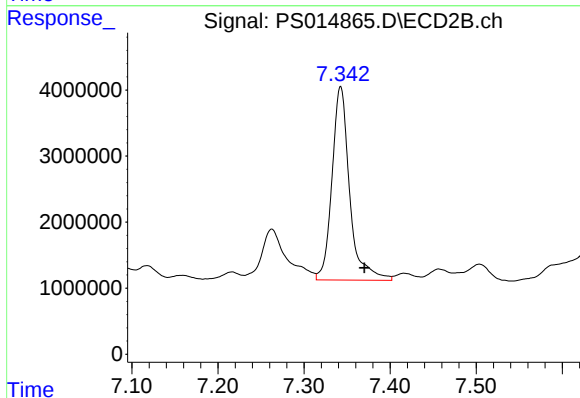


#7 MCPA

R.T.: 7.343 min
Delta R.T.: -0.028 min
Response: 41774380
Conc: 17.20 ug/ml

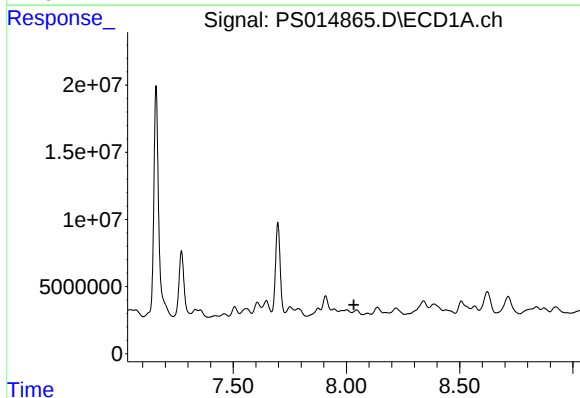


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 8.033 min
Response: 0
Conc: N.D.

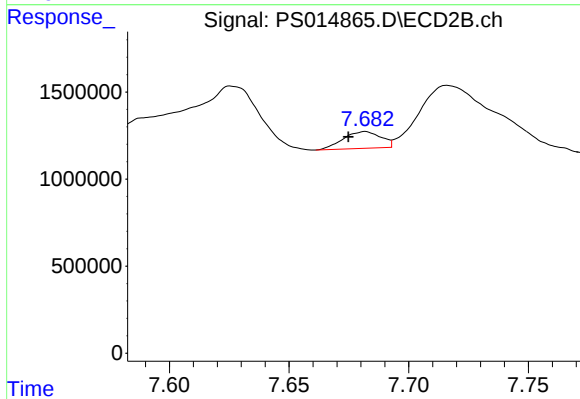

#8 DICHLORPROP


R.T.: 7.682 min
Delta R.T.: 0.007 min
Response: 1061969
Conc: 2.10 ng/ml

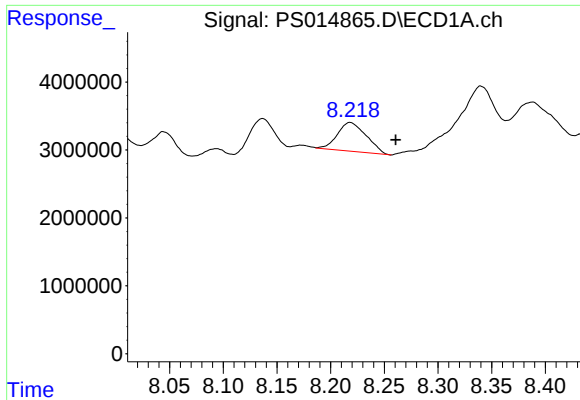

#9 2,4-D


R.T.: 8.218 min
Delta R.T.: -0.042 min
Response: 7948249
Conc: 5.00 ng/ml

Instrument :
ECD_S
ClientSampleId :
TEST-PIT-II

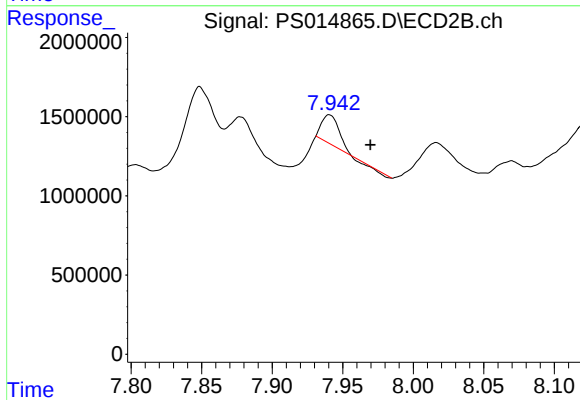


#9 2,4-D

R.T.: 7.941 min
Delta R.T.: -0.029 min
Response: 1430542
Conc: 2.57 ng/ml

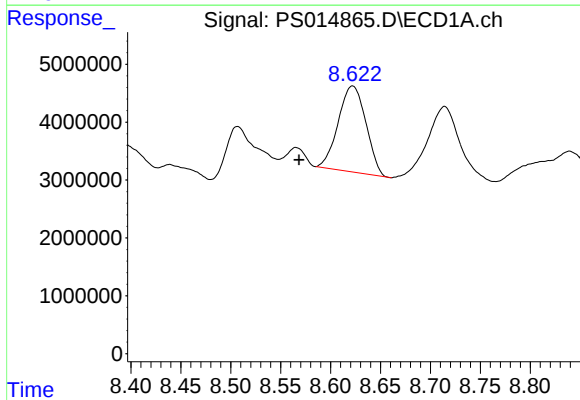


#10 Pentachlorophenol

R.T.: 8.622 min
Delta R.T.: 0.053 min
Response: 28653085
Conc: 1.36 ng/ml

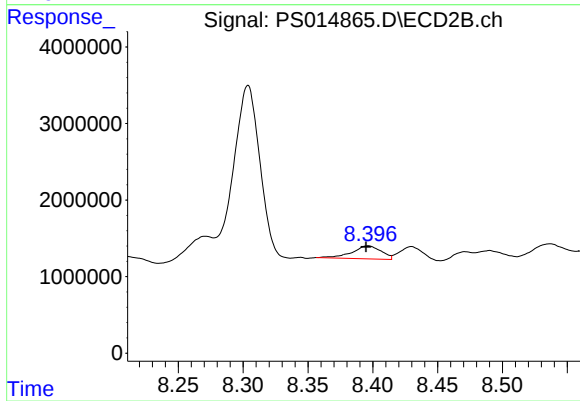

#10 Pentachlorophenol


R.T.: 8.396 min
Delta R.T.: 0.002 min
Response: 2657654
Conc: N.D.

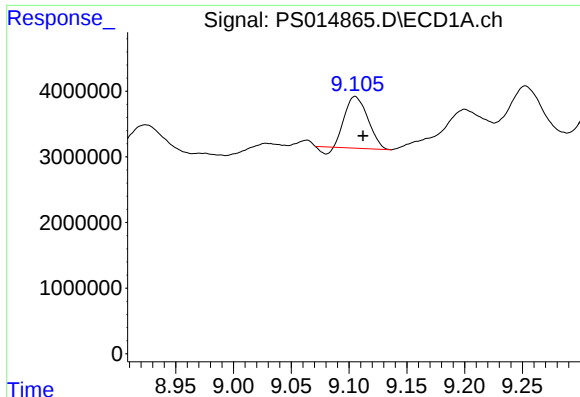

#11 2,4,5-TP (SILVEX)


R.T.: 9.105 min
Delta R.T.: -0.007 min
Response: 10467816
Conc: 1.28 ng/ml

Instrument :
ECD_S
ClientSampleId :
TEST-PIT-II

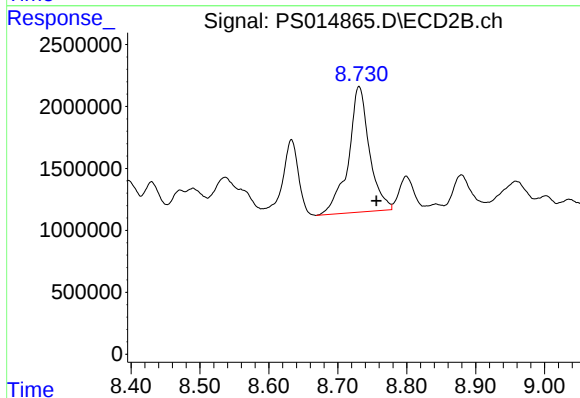


#11 2,4,5-TP (SILVEX)

R.T.: 8.731 min
Delta R.T.: -0.025 min
Response: 21501090
Conc: 7.87 ng/ml

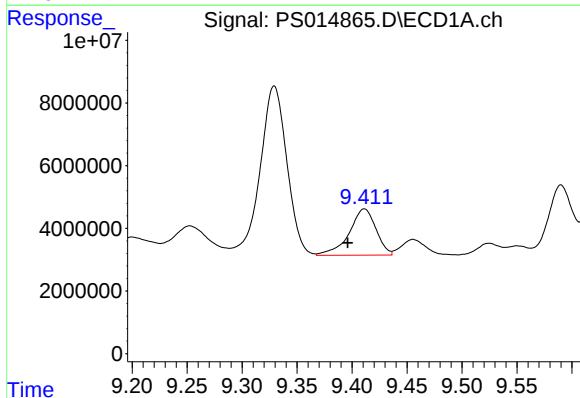


#12 2,4,5-T

R.T.: 9.411 min
Delta R.T.: 0.015 min
Response: 25128541
Conc: 3.05 ng/ml

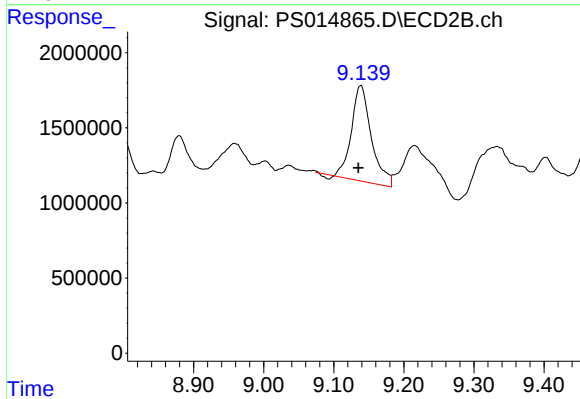

#12 2,4,5-T


R.T.: 9.139 min
Delta R.T.: 0.003 min
Response: 12511657
Conc: 4.78 ng/ml

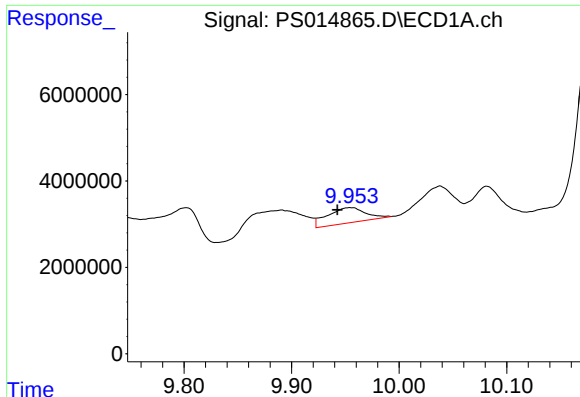

#13 2,4-DB


R.T.: 9.954 min
Delta R.T.: 0.012 min
Response: 8723983
Conc: 5.73 ng/ml

Instrument :
ECD_S
ClientSampleId :
TEST-PIT-II

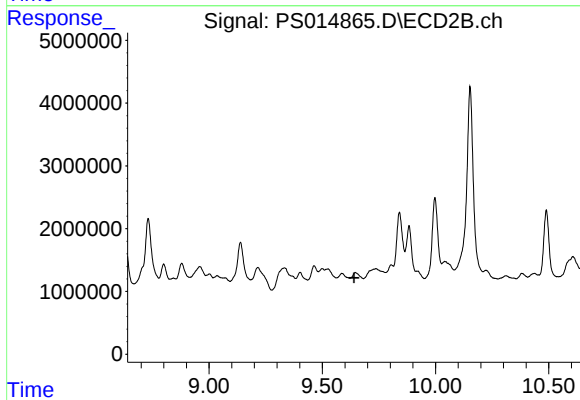


#13 2,4-DB

R.T.: 0.000 min
Exp R.T. : 9.640 min
Response: 0
Conc: N.D.

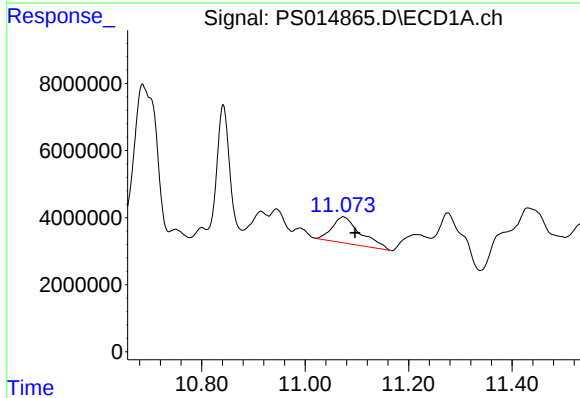


#14 DINOSEB

R.T.: 11.074 min
Delta R.T.: -0.023 min
Response: 29825444
Conc: 4.63 ng/ml

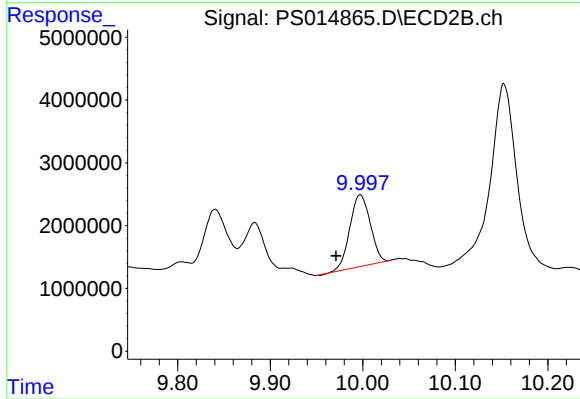

#14 DINOSEB


R.T.: 9.997 min
Delta R.T.: 0.026 min
Response: 17537879
Conc: 9.11 ng/ml

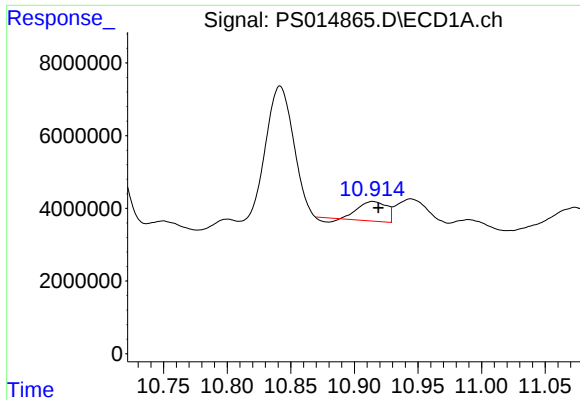

#15 Picloram


R.T.: 10.915 min
Delta R.T.: -0.004 min
Response: 7778032
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
TEST-PIT-II

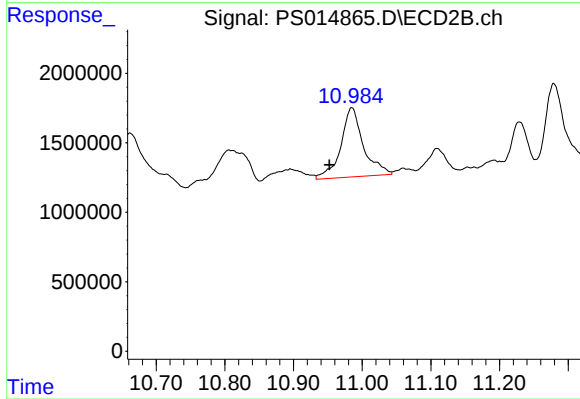


#15 Picloram

R.T.: 10.985 min
Delta R.T.: 0.032 min
Response: 11414444
Conc: 3.04 ng/ml

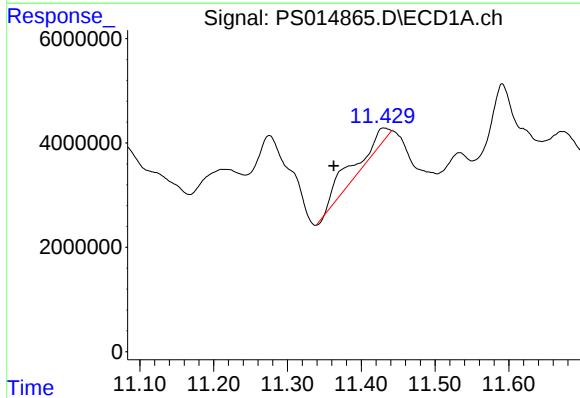

#16 DCPA

R.T.: 11.431 min
Delta R.T.: 0.068 min
Response: 12760300
Conc: 1.04 ng/ml

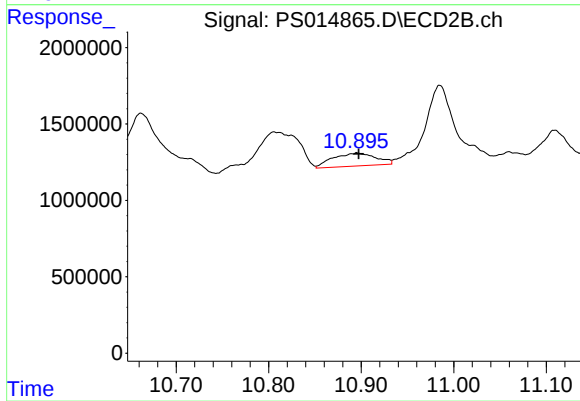

#16 DCPA

R.T.: 10.896 min
Delta R.T.: -0.002 min
Response: 2744000
Conc: N.D.