

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Data\PS043019\  
 Data File : PS004360.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 30 Apr 2019 12:35  
 Operator : EI\SJ  
 Sample : MDL-BL-WATER-04  
 Misc :  
 ALS Vial : 10 Sample Multiplier: 1

Instrument :  
 ECD\_S  
 ClientSampleId :  
 MDL-BL-WATER-04

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: May 01 03:11:10 2019  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Method\PS042919.M  
 Quant Title : 8080.M  
 QLast Update : Tue Apr 30 08:27:54 2019  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2 µl  
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2  
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

|                             | Compound | RT#1  | RT#2  | Resp#1   | Resp#2  | ng/ml   | ng/ml   |
|-----------------------------|----------|-------|-------|----------|---------|---------|---------|
| -----                       |          |       |       |          |         |         |         |
| System Monitoring Compounds |          |       |       |          |         |         |         |
| 4) S                        | 2,4-DCAA | 5.985 | 5.674 | 305.2E6  | 248.7E6 | 484.884 | 515.599 |
| Target Compounds            |          |       |       |          |         |         |         |
| 9) T                        | 2,4-D    | 7.070 | 0.000 | 34508306 | 0       | 60.653  | N.D. #  |
| -----                       |          |       |       |          |         |         |         |



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Data\PS043019\  
Data File : PS004360.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 30 Apr 2019 12:35  
Operator : EI\SJ  
Sample : MDL-BL-WATER-04  
Misc :  
ALS Vial : 10 Sample Multiplier: 1

Instrument :  
ECD\_S  
ClientSampleId :  
MDL-BL-WATER-04

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: May 01 03:11:10 2019  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Method\PS042919.M  
Quant Title : 8080.M  
QLast Update : Tue Apr 30 08:27:54 2019  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 2 µl  
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2  
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

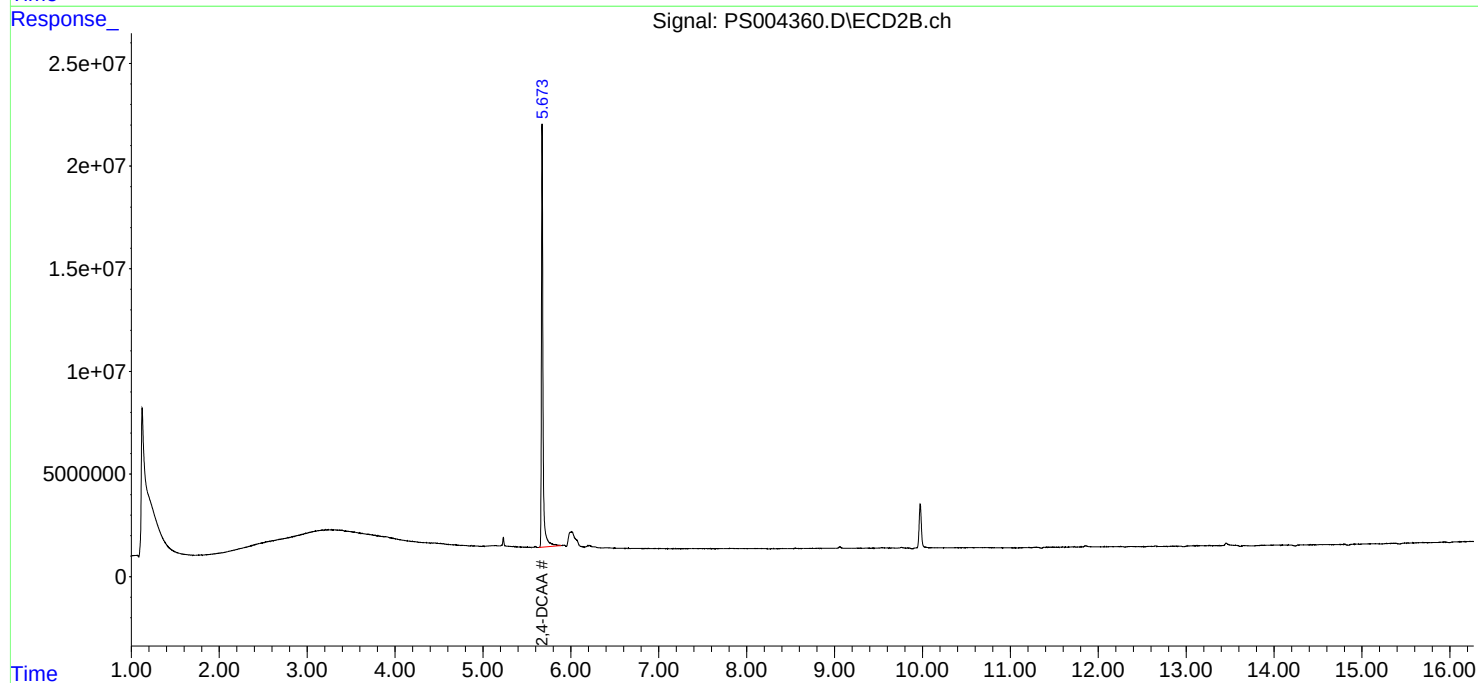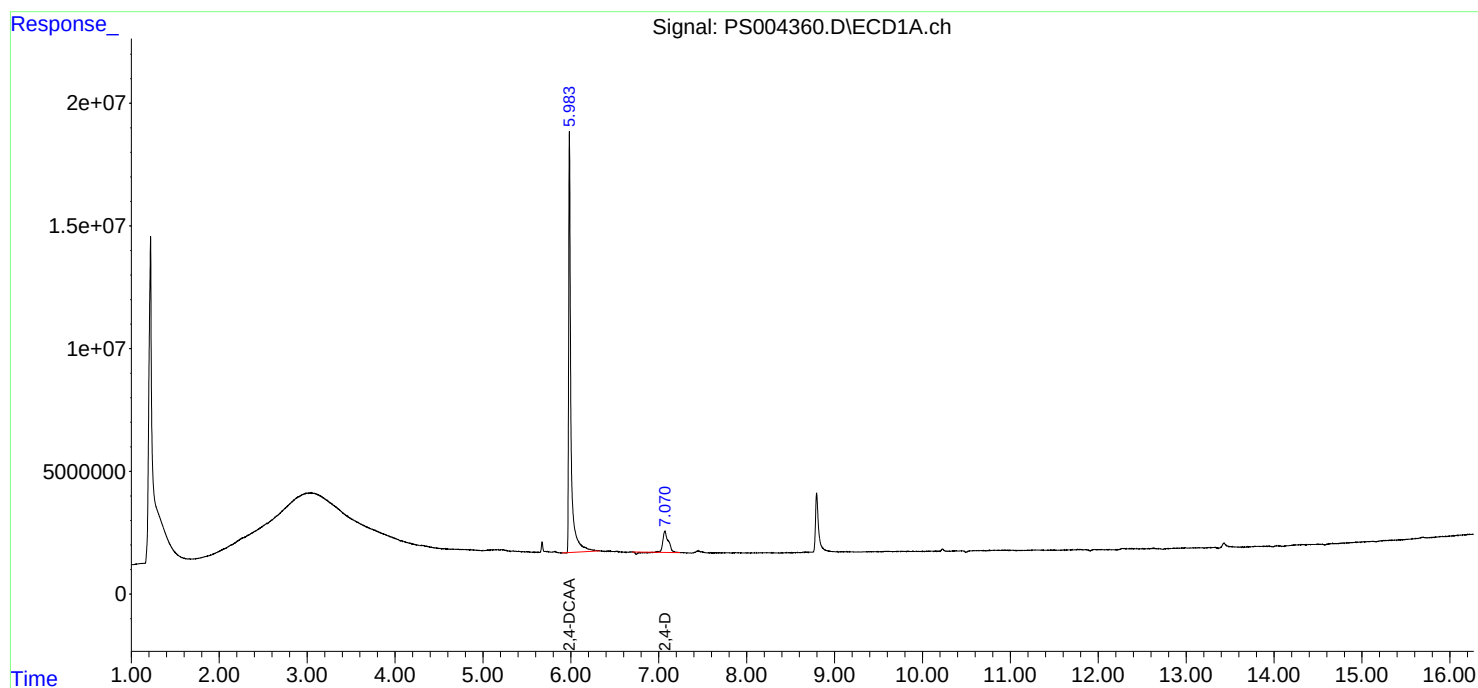


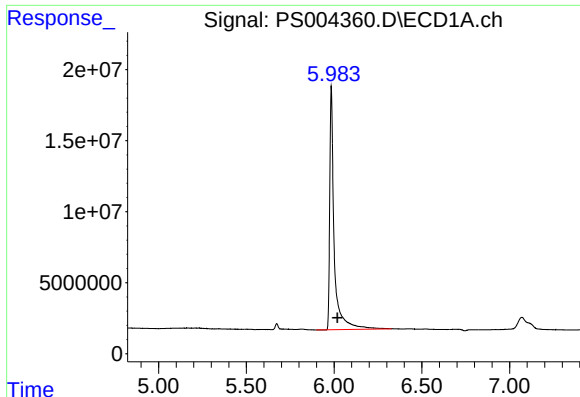

#4 2,4-DCAA


R.T.: 5.985 min  
Delta R.T.: -0.033 min  
Response: 305213522  
Conc: 484.88 ng/ml

Instrument :  
ECD\_S  
ClientSampleId :  
MDL-BL-WATER-04

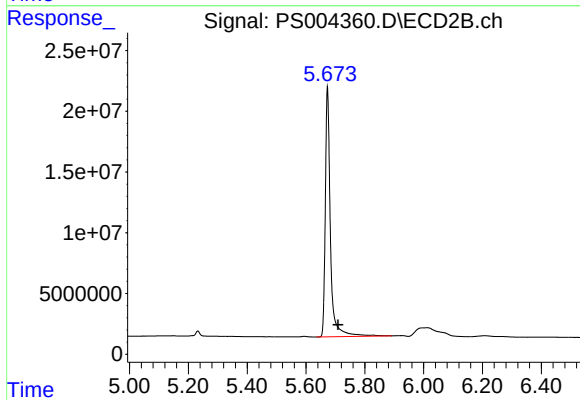


#4 2,4-DCAA

R.T.: 5.674 min  
Delta R.T.: -0.035 min  
Response: 248664788  
Conc: 515.60 ng/ml

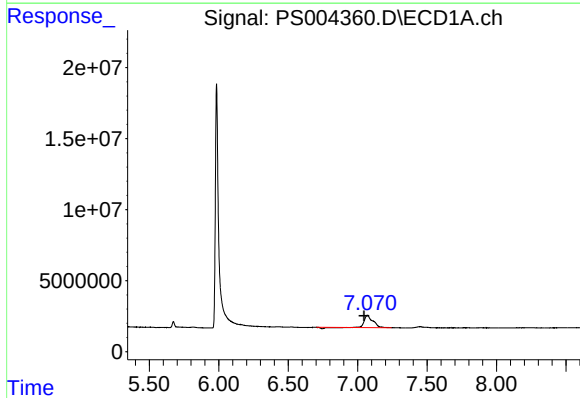

#9 2,4-D

R.T.: 7.070 min  
Delta R.T.: 0.025 min  
Response: 34508306  
Conc: 60.65 ng/ml

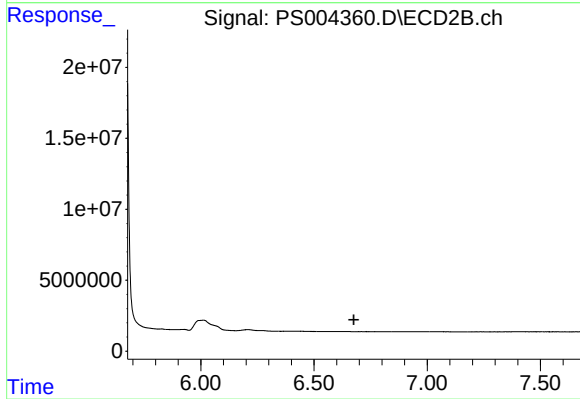

#9 2,4-D

R.T.: 0.000 min  
Exp R.T.: 6.676 min  
Response: 0  
Conc: N.D.