

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS043019\
Data File : PS004360.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Apr 2019 12:35
Operator : EI\SJ
Sample : MDL-BL-WATER-04
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
MDL-BL-WATER-04

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 01 03:11:10 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS042919.M
Quant Title : 8080.M
QLast Update : Tue Apr 30 08:27:54 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.985	5.674	305.2E6	248.7E6	484.884	515.599

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS043019\
Data File : PS004360.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Apr 2019 12:35
Operator : EI\SJ
Sample : MDL-BL-WATER-04
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
MDL-BL-WATER-04

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 01 03:11:10 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS042919.M
Quant Title : 8080.M
QLast Update : Tue Apr 30 08:27:54 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

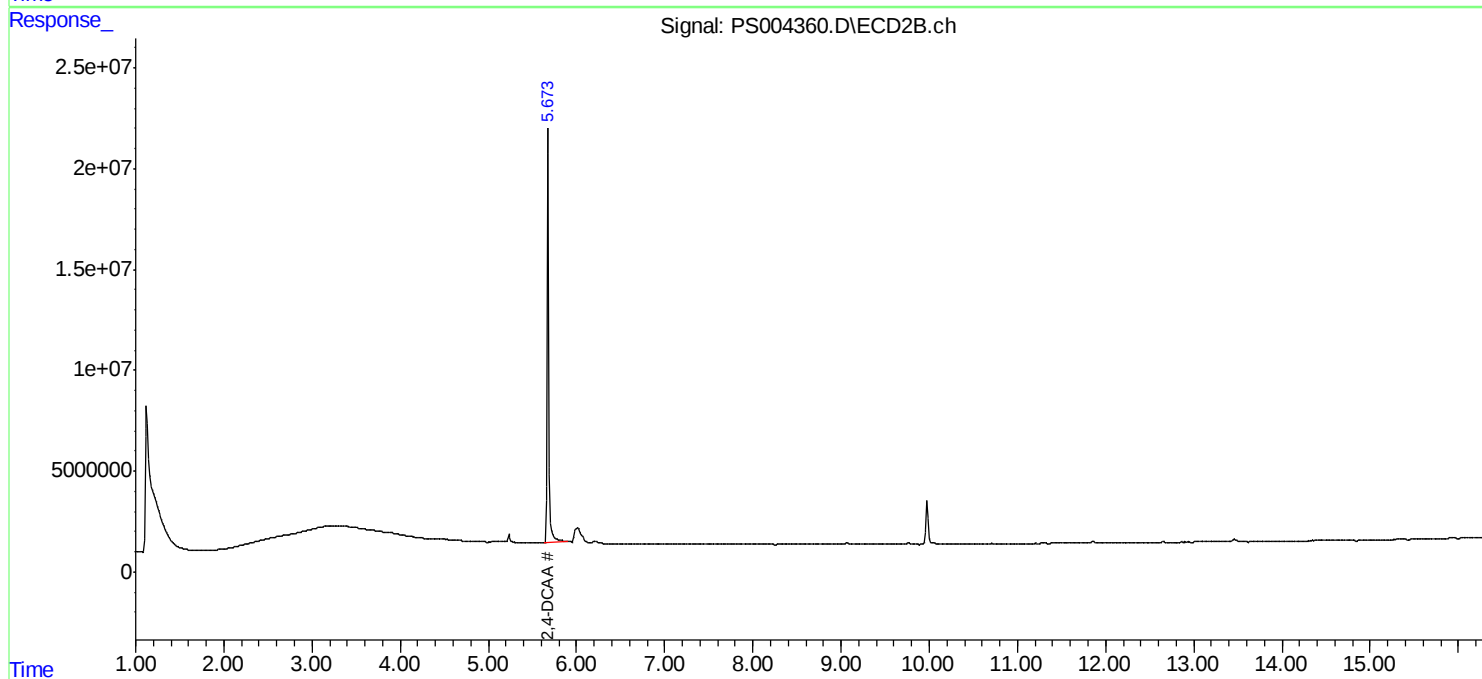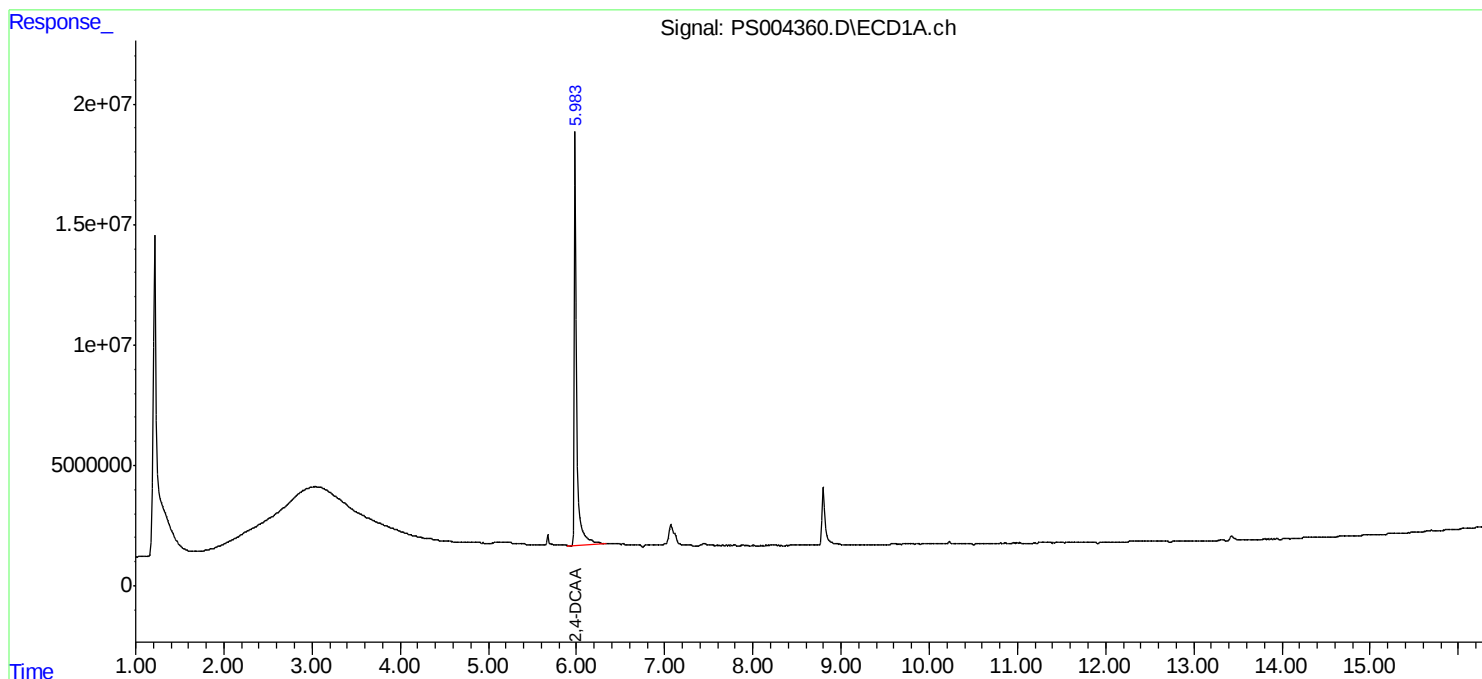


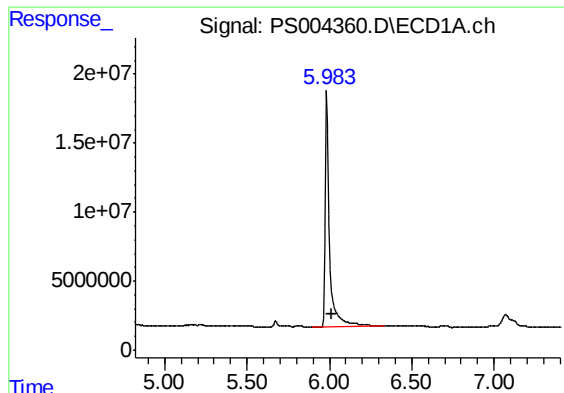

#4 2,4-DCAA

R.T.: 5.985 min
Delta R.T.: -0.033 min
Response: 305213522
Conc: 484.88 ng/ml

Instrument :
ECD_S
ClientSampleId :
MDL-BL-WATER-04

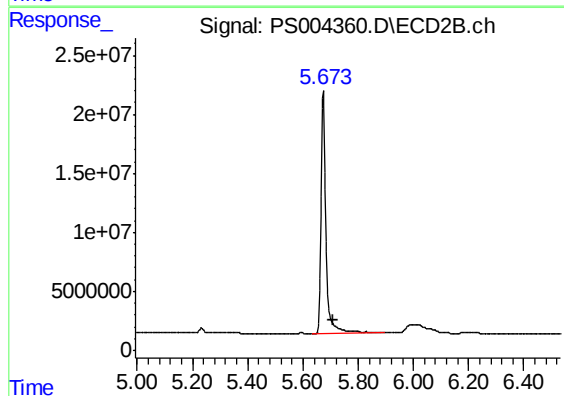

#4 2,4-DCAA

R.T.: 5.674 min
Delta R.T.: -0.035 min
Response: 248664788
Conc: 515.60 ng/ml