

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS043021\
 Data File : PS014871.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Apr 2021 08:15
 Operator : DD\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampled :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 30 11:57:35 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS040821.M
 Quant Title : 8080.M
 QLast Update : Thu Apr 08 14:34:06 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds

2) T	3,5-DICHL...	6.442f	0.000	13703967	0	6.614	N.D.	#
6) T	MCPP	0.000	7.128	0	5412011	N.D.	3.214	
12) T	2,4,5-T	9.387	0.000	7312055	0	<MDL	N.D.	#
15) T	Picloram	10.927	11.016f	8658830	24046490	<MDL	6.413	#



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS043021\
 Data File : PS014871.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Apr 2021 08:15
 Operator : DD\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 30 11:57:35 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS040821.M
 Quant Title : 8080.M
 QLast Update : Thu Apr 08 14:34:06 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

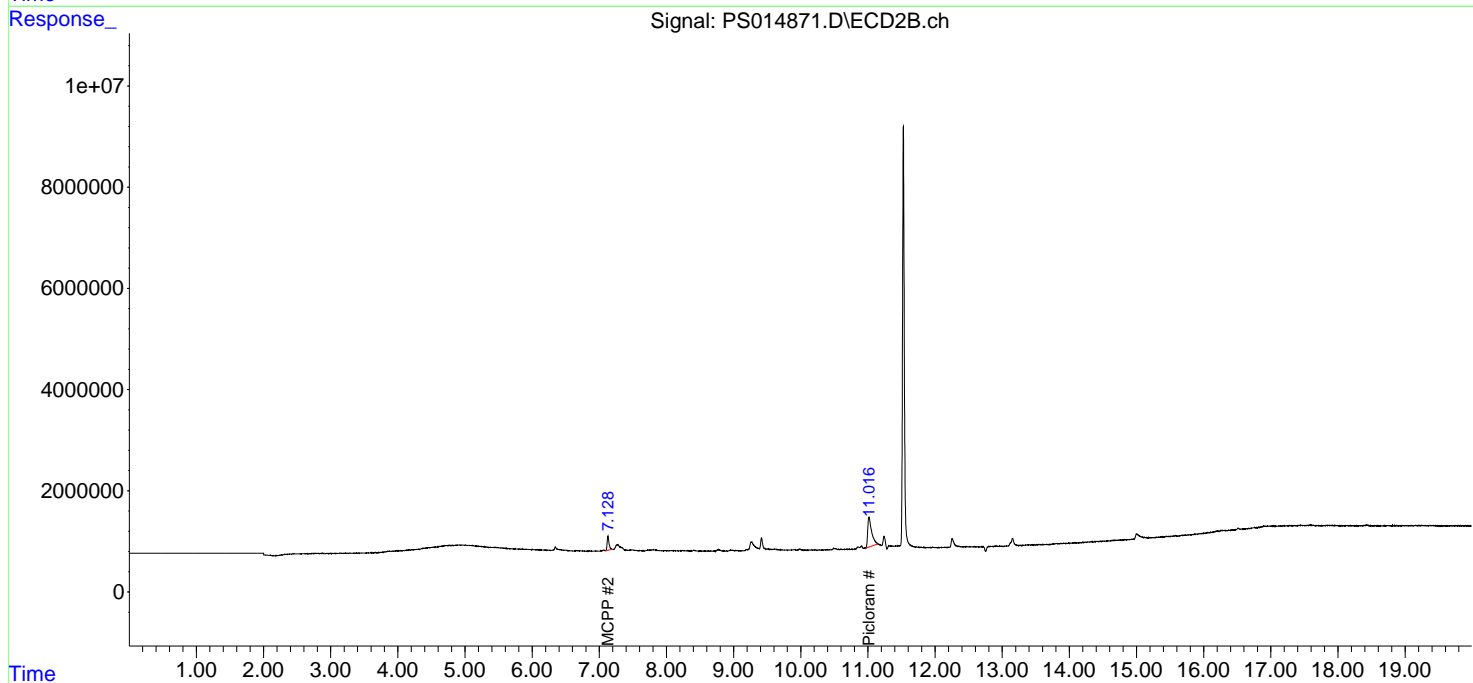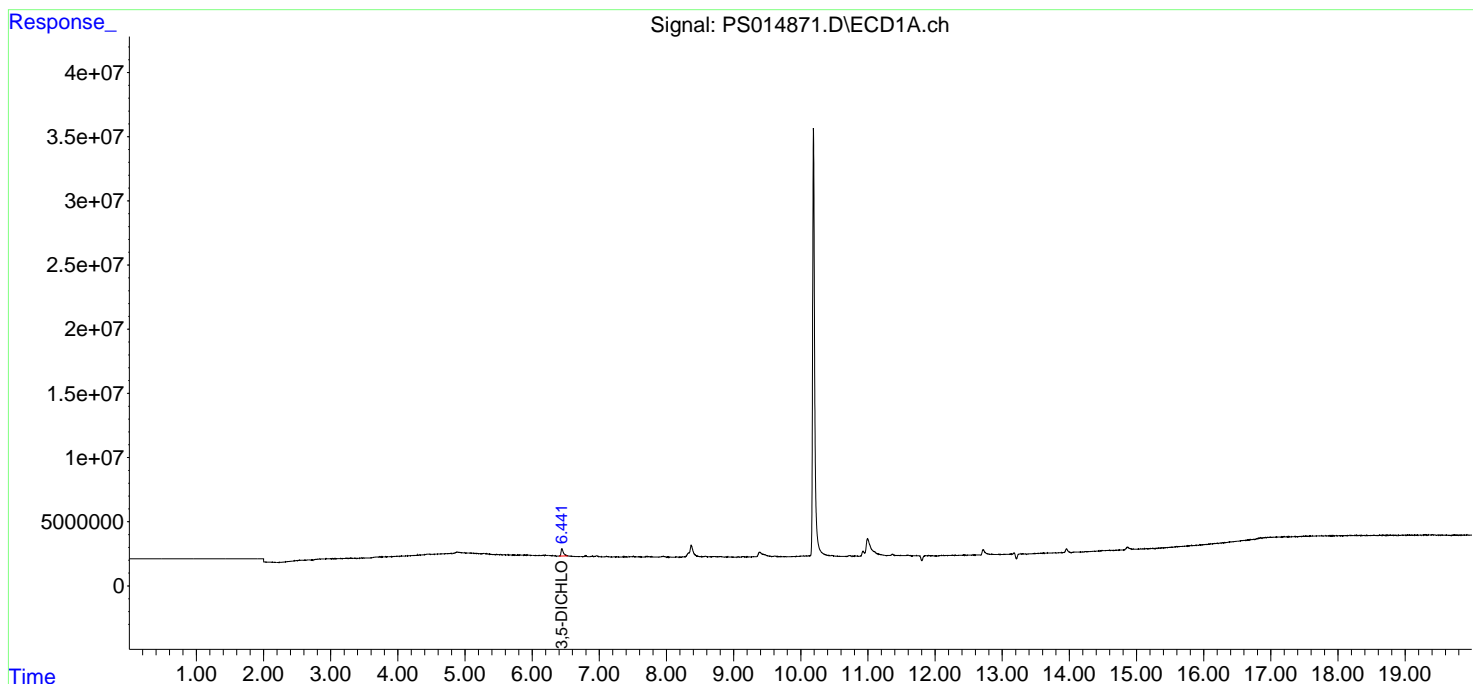


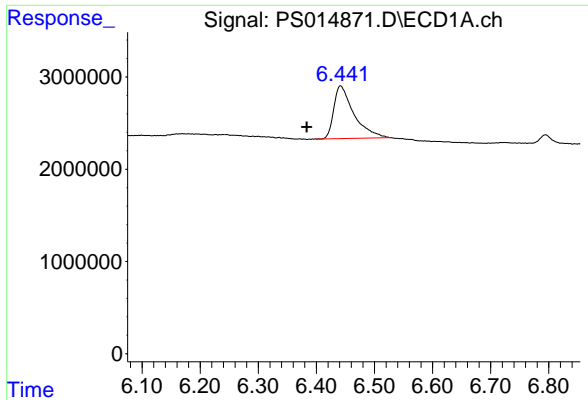

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.442 min
 Delta R.T.: 0.058 min
 Response: 13703967
 Conc: 6.61 ng/ml

Instrument :
 ECD_S
 ClientSampleId :
 HEXANE

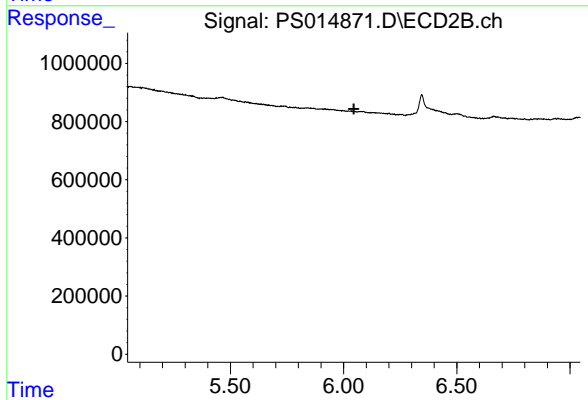


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
 Exp R.T. : 6.045 min
 Response: 0
 Conc: N.D.

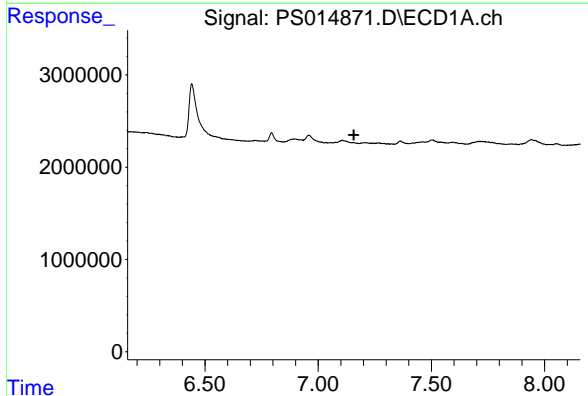


#4 2,4-DCAA

R.T.: 0.000 min
 Exp R.T. : 7.158 min
 Response: 0
 Conc: N.D.

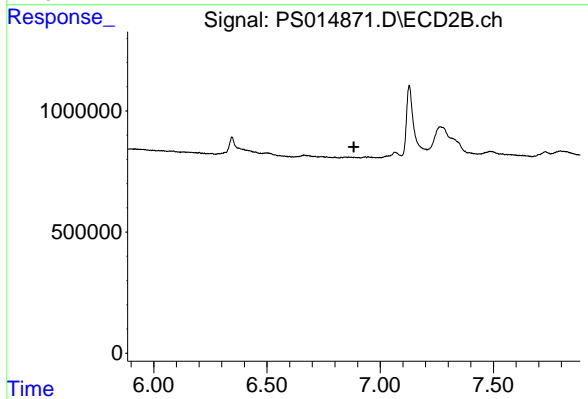


#4 2,4-DCAA

R.T.: 0.000 min
 Exp R.T. : 6.884 min
 Response: 0
 Conc: N.D.

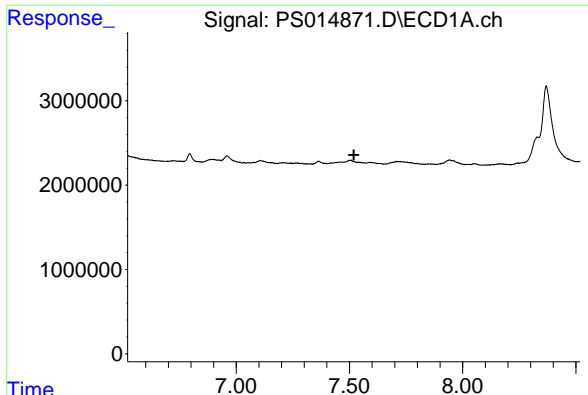


#6 MCP
 R.T.: 0.000 min
 Exp R.T.: 7.520 min
 Response: 0
 Conc: N.D.


Instrument :
 ECD_S
 ClientSampleId :
 HEXANE

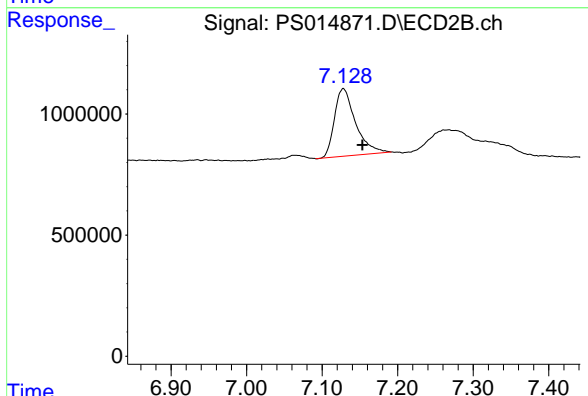

#6 MCP
 R.T.: 7.128 min
 Delta R.T.: -0.025 min
 Response: 5412011
 Conc: 3.21 ug/ml

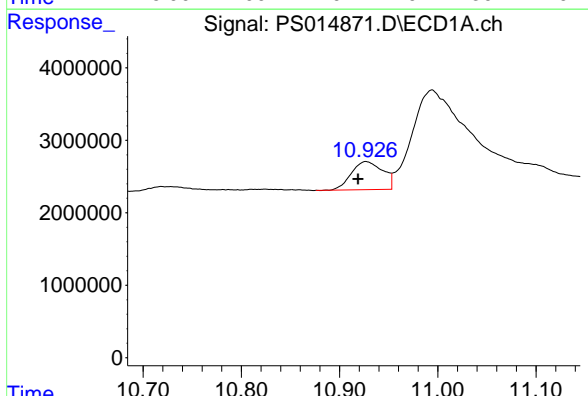

#15 Picloram
 R.T.: 10.927 min
 Delta R.T.: 0.008 min
 Response: 8658830
 Conc: N.D.

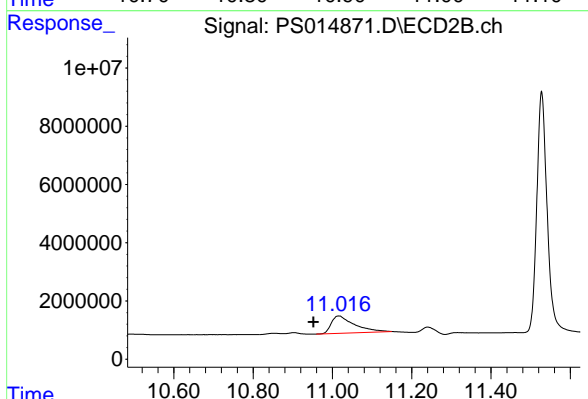

#15 Picloram
 R.T.: 11.016 min
 Delta R.T.: 0.063 min
 Response: 24046490
 Conc: 6.41 ng/ml