

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS043021\
 Data File : PS014879.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Apr 2021 13:28
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 30 14:23:32 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS040821.M
 Quant Title : 8080.M
 QLast Update : Thu Apr 08 14:34:06 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.160	6.887	713.8E6	240.0E6	469.227	515.619
Target Compounds							
5) T	DICAMBA	7.349	0.000	4668539	0	<MDL	N.D. #
9) T	2,4-D	8.330f	0.000	2728428	0	1.716	N.D. #
10) T	Pentachlo...	8.576	8.403	7544232	3139325	<MDL	<MDL #
11) T	2,4,5-TP ...	9.131	8.774	6535817	3022186	<MDL	1.106 #
12) T	2,4,5-T	9.364	9.182f	49404545	3005156	6.006	1.149 #
14) T	DINOSEB	11.097	9.979	28431074	2984577	4.412	1.550 #
15) T	Picloram	10.917	10.999f	3841257	55708884	<MDL	14.856 #
16) T	DCPA	11.361	10.900	16395401	7516397	1.331	1.851 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS043021\
Data File : PS014879.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Apr 2021 13:28
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 30 14:23:32 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS040821.M
Quant Title : 8080.M
QLast Update : Thu Apr 08 14:34:06 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

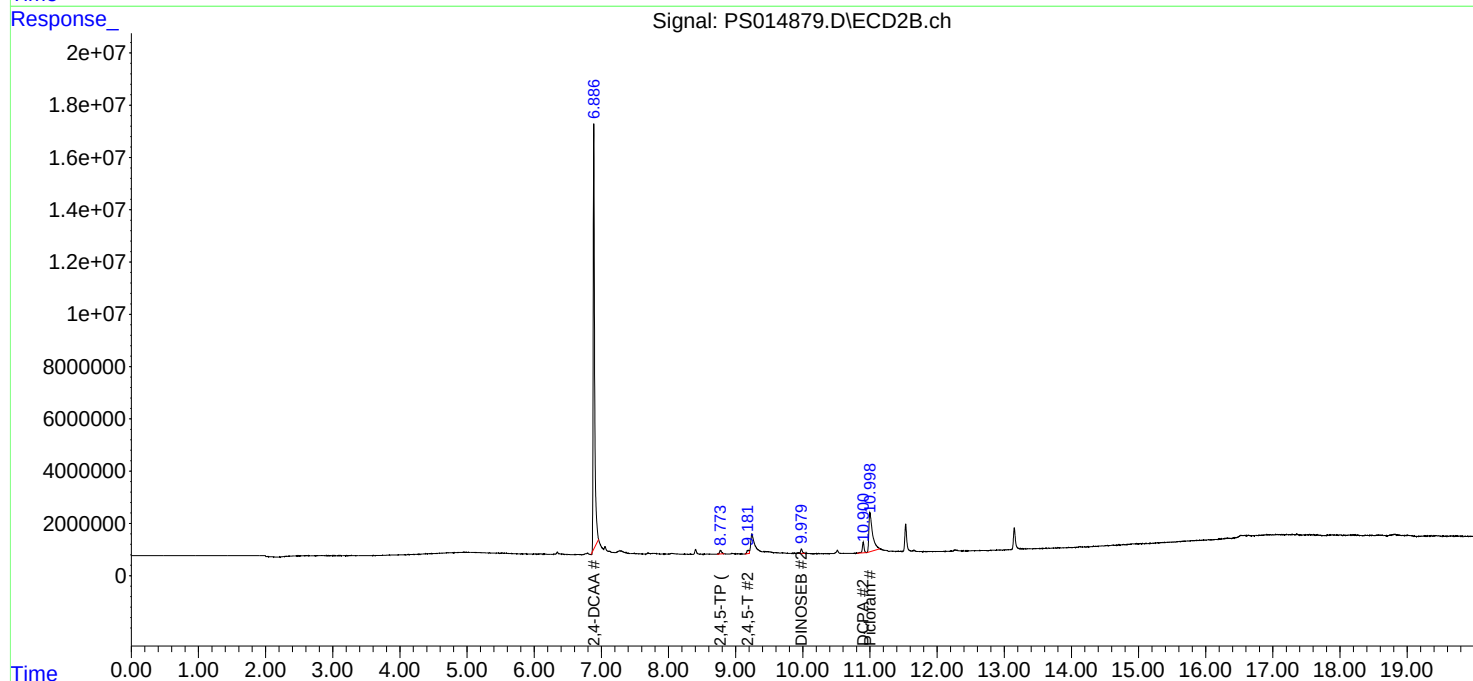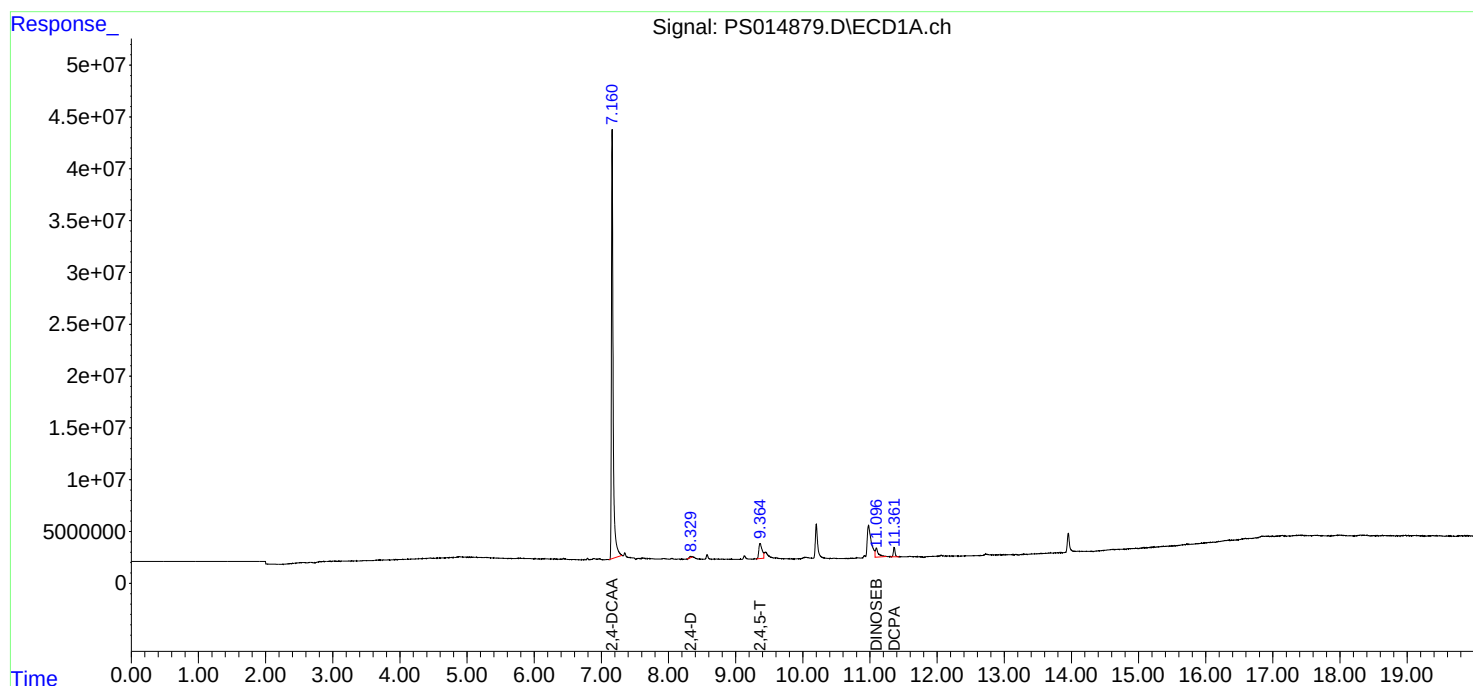


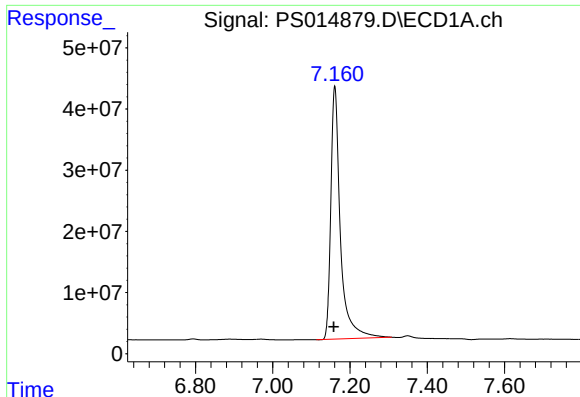

#4 2,4-DCAA


R.T.: 7.160 min
Delta R.T.: 0.003 min
Response: 713786068
Conc: 469.23 ng/ml

Instrument :
ECD_S
ClientSampleId :

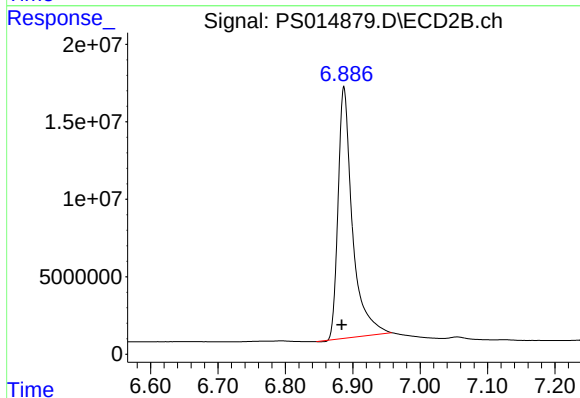


#4 2,4-DCAA

R.T.: 6.887 min
Delta R.T.: 0.003 min
Response: 239997502
Conc: 515.62 ng/ml

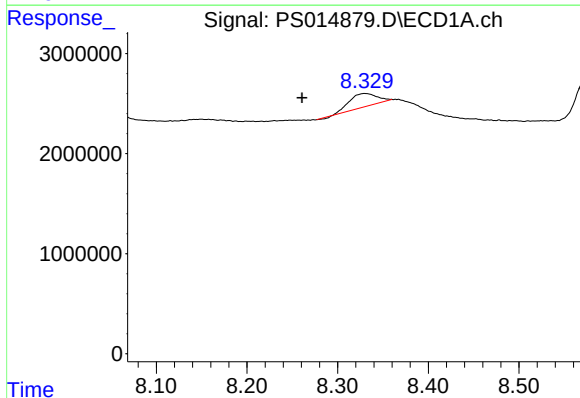


#9 2,4-D

R.T.: 8.330 min
Delta R.T.: 0.069 min
Response: 2728428
Conc: 1.72 ng/ml

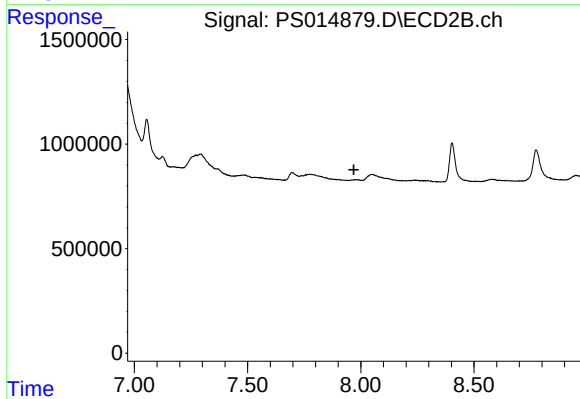

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 7.970 min
Response: 0
Conc: N.D.

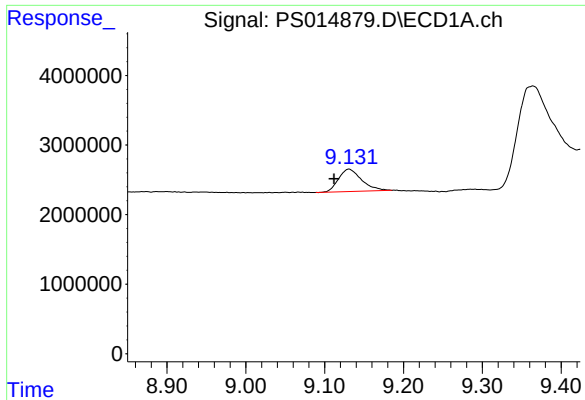

#11 2,4,5-TP (SILVEX)


R.T.: 9.131 min
Delta R.T.: 0.019 min
Response: 6535817
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

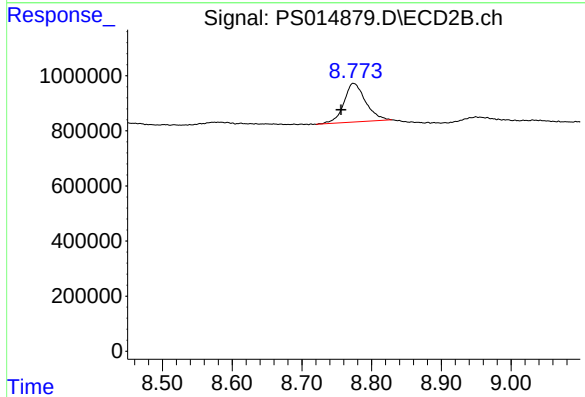


#11 2,4,5-TP (SILVEX)

R.T.: 8.774 min
Delta R.T.: 0.018 min
Response: 3022186
Conc: 1.11 ng/ml

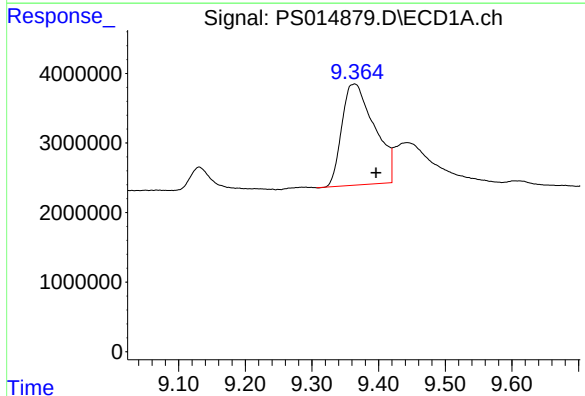


#12 2,4,5-T

R.T.: 9.364 min
Delta R.T.: -0.032 min
Response: 49404545
Conc: 6.01 ng/ml

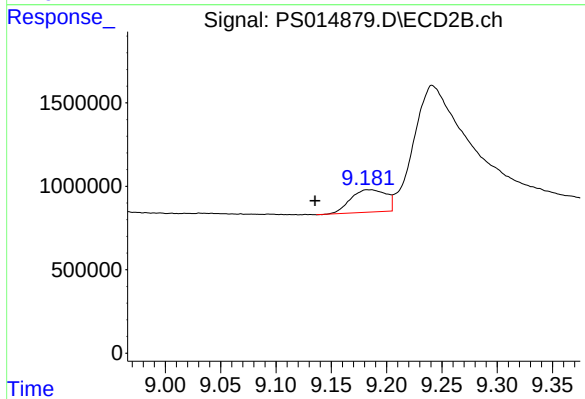

#12 2,4,5-T


R.T.: 9.182 min
Delta R.T.: 0.047 min
Response: 3005156
Conc: 1.15 ng/ml

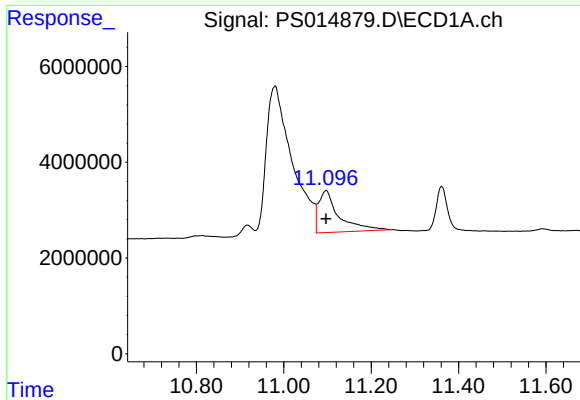

#14 DINOSEB


R.T.: 11.097 min
Delta R.T.: 0.000 min
Response: 28431074
Conc: 4.41 ng/ml

Instrument :
ECD_S
ClientSampleId :

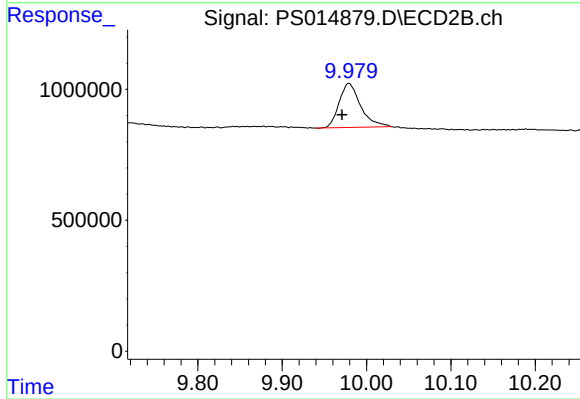


#14 DINOSEB

R.T.: 9.979 min
Delta R.T.: 0.008 min
Response: 2984577
Conc: 1.55 ng/ml

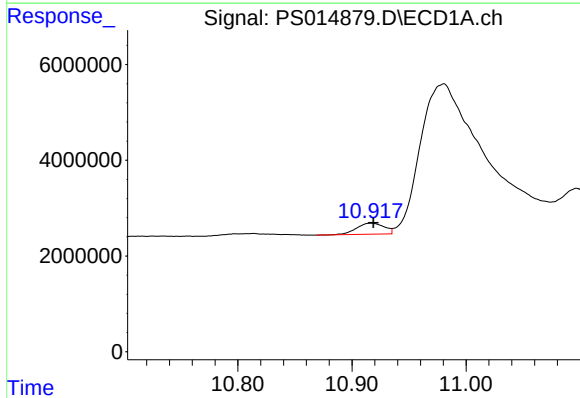


#15 Picloram

R.T.: 10.917 min
Delta R.T.: -0.002 min
Response: 3841257
Conc: N.D.

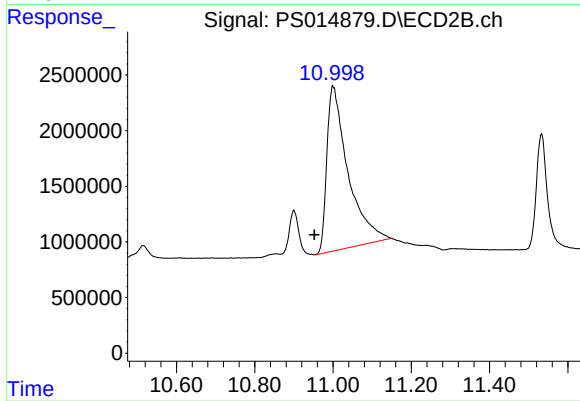

#15 Picloram


R.T.: 10.999 min
Delta R.T.: 0.046 min
Response: 55708884
Conc: 14.86 ng/ml

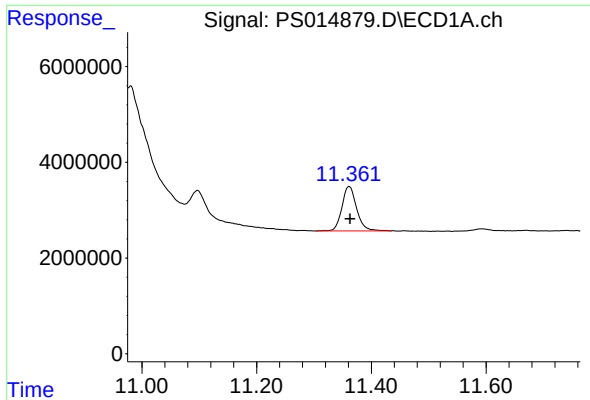

#16 DCPA

R.T.: 11.361 min
Delta R.T.: -0.002 min
Response: 16395401
Conc: 1.33 ng/ml

Instrument :
ECD_S
ClientSampleId :

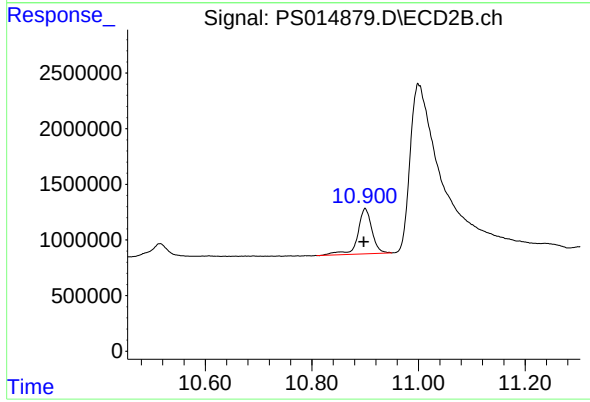

#16 DCPA

R.T.: 10.900 min
Delta R.T.: 0.003 min
Response: 7516397
Conc: 1.85 ng/ml