

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS043025\
 Data File : PS029992.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 May 2025 01:46
 Operator : AR\AJ
 Sample : PB167796BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 PB167796BL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 01 02:20:33 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS042325.M
 Quant Title : 8080.M
 QLast Update : Wed Apr 23 12:57:40 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.954	0.000	1430101	0	<MDL	N.D. #
Target Compounds							
1) T	Dalapon	2.450	0.000	1956949	0	<MDL	N.D. #
2) T	3,5-DICHL...	6.146	0.000	376281	0	<MDL	N.D. #
3) T	4-Nitroph...	6.749	0.000	1177996	0	<MDL	N.D. #
5) T	DICAMBA	7.127	0.000	313744	0	<MDL	N.D. #
6) T	MCPD	7.303	7.728f	-91464	2907905	N.D.	1.663
7) T	MCPA	7.445	7.952f	315873	69744017	<MDL	29.480 #
8) T	DICHLORPROP	7.799	0.000	1158204	0	<MDL	N.D. #
9) T	2,4-D	7.994	0.000	6495853	0	2.309	N.D. #
10) T	Pentachlo...	8.318	0.000	2005704	0	<MDL	N.D. #
11) T	2,4,5-TP ...	8.896f	0.000	3968003	0	<MDL	N.D. #
12) T	2,4,5-T	9.185f	0.000	2111390	0	<MDL	N.D. #
14) T	DINOSEB	10.905f	0.000	985883	0	<MDL	N.D. #
15) T	Picloram	10.659	0.000	118.5E6	0	6.464	N.D. #
16) T	DCPA	11.141	0.000	7837776	0	<MDL	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS043025\
Data File : PS029992.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 May 2025 01:46
Operator : AR\AJ
Sample : PB167796BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
PB167796BL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 01 02:20:33 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS042325.M
Quant Title : 8080.M
QLast Update : Wed Apr 23 12:57:40 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

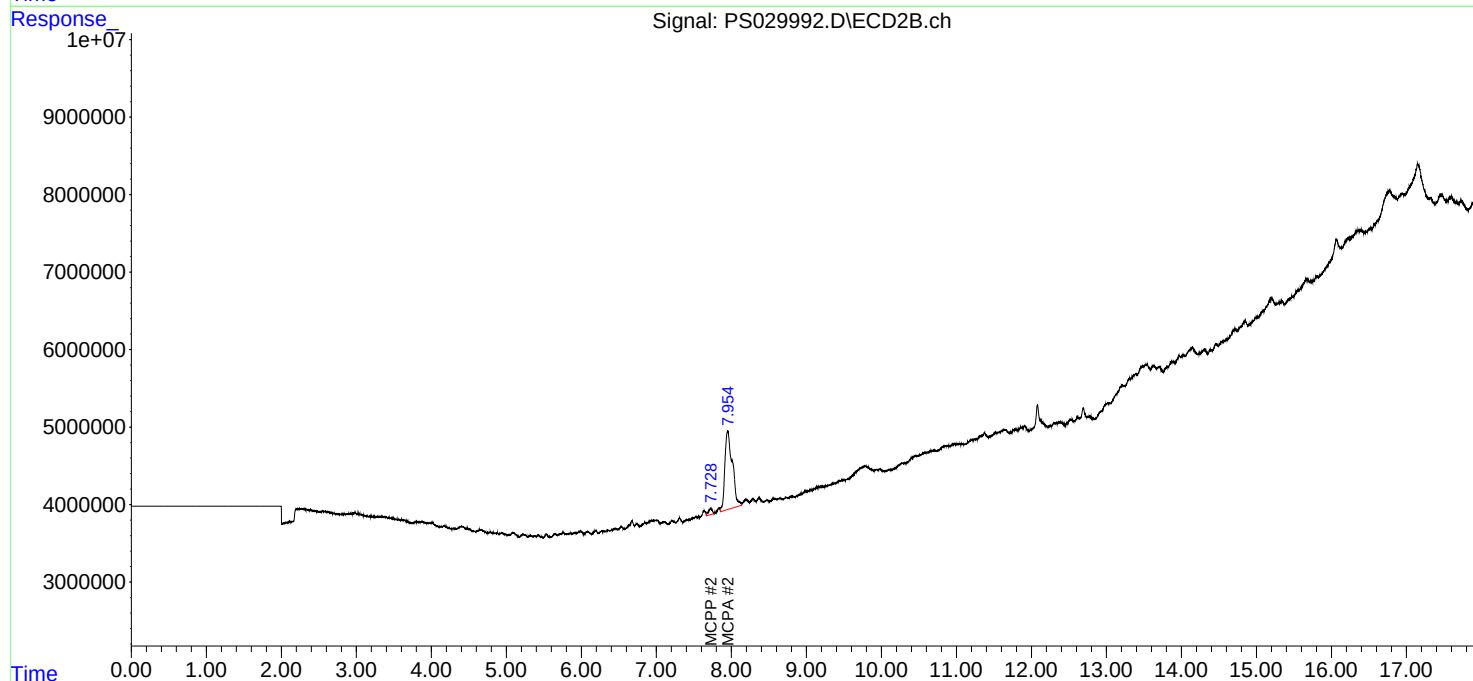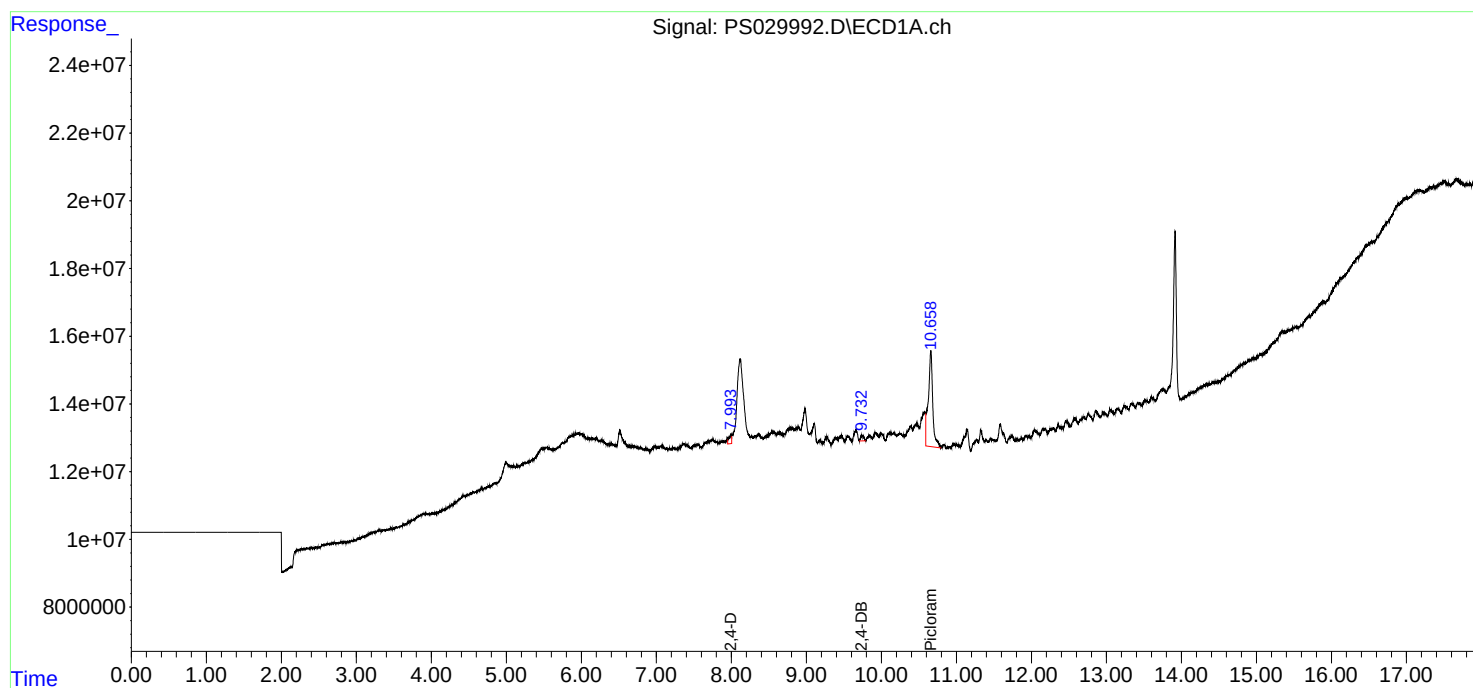


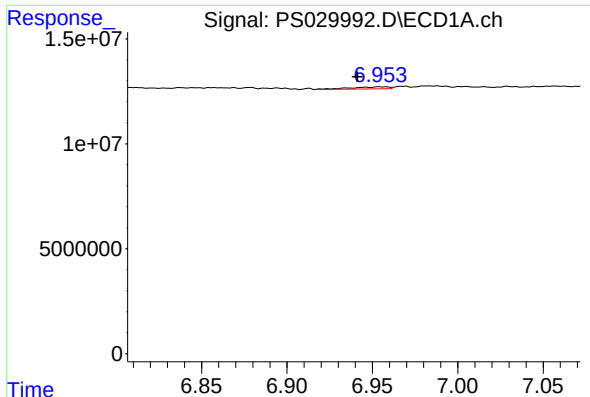

#4 2,4-DCAA


R.T.: 6.954 min
Delta R.T.: 0.013 min
Response: 1430101
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
PB167796BL

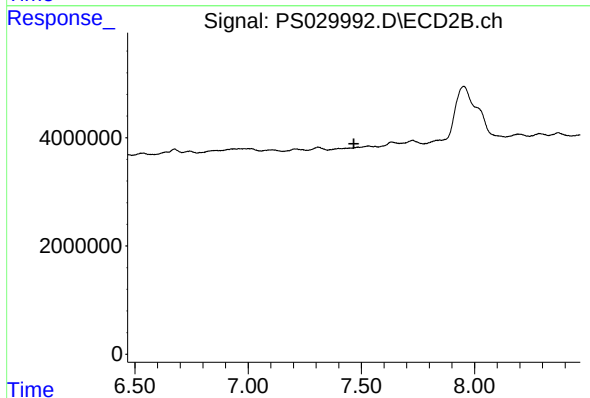


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T. : 7.467 min
Response: 0
Conc: N.D.

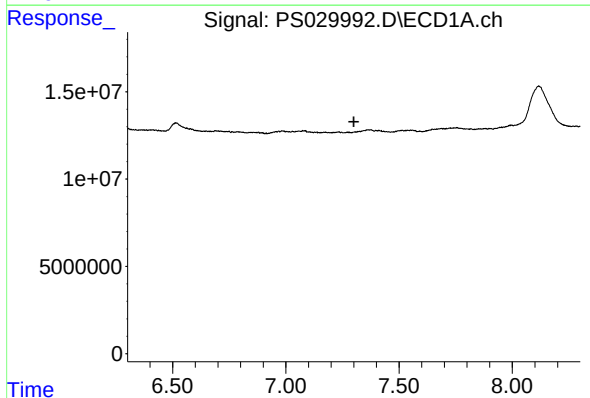


#6 MCP

R.T.: 7.303 min
Delta R.T.: 0.003 min
Response: -91464
Conc: N.D.

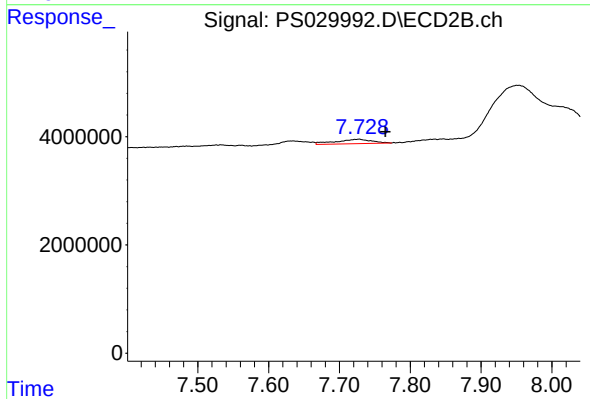

#6 MCP


R.T.: 7.728 min
Delta R.T.: -0.037 min
Response: 2907905
Conc: 1.66 ug/ml

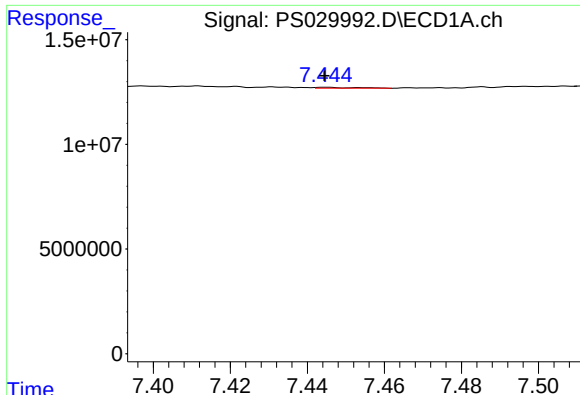

#7 MCPA


R.T.: 7.445 min
Delta R.T.: 0.000 min
Response: 315873
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
PB167796BL

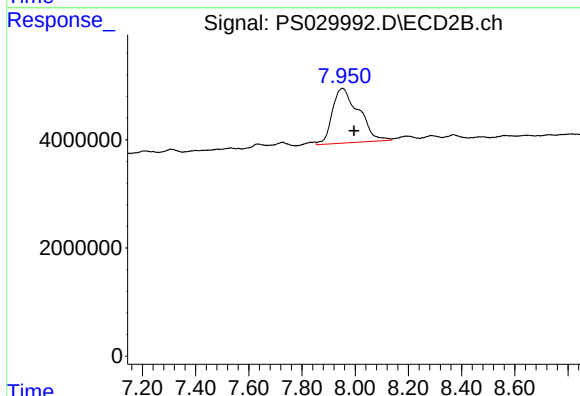


#7 MCPA

R.T.: 7.952 min
Delta R.T.: -0.044 min
Response: 69744017
Conc: 29.48 ug/ml

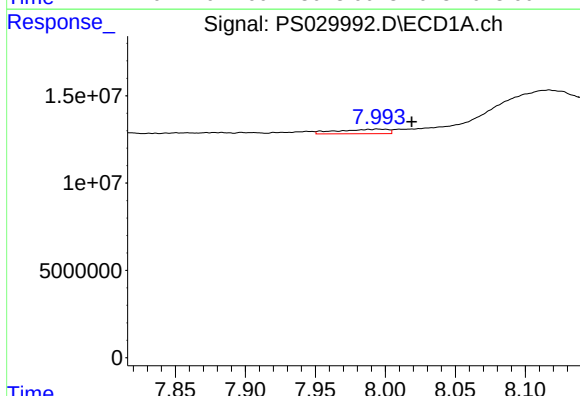


#9 2,4-D

R.T.: 7.994 min
Delta R.T.: -0.024 min
Response: 6495853
Conc: 2.31 ng/ml

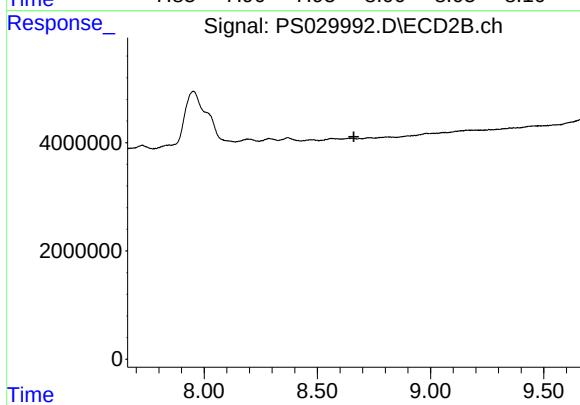

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 8.661 min
Response: 0
Conc: N.D.

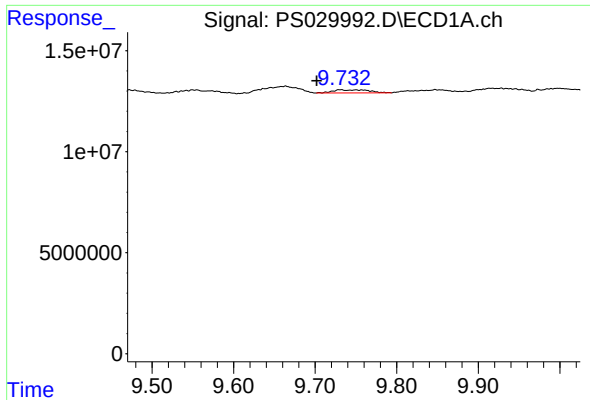

#13 2,4-DB


R.T.: 9.731 min
Delta R.T.: 0.029 min
Response: 4675992
Conc: 2.05 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB167796BL

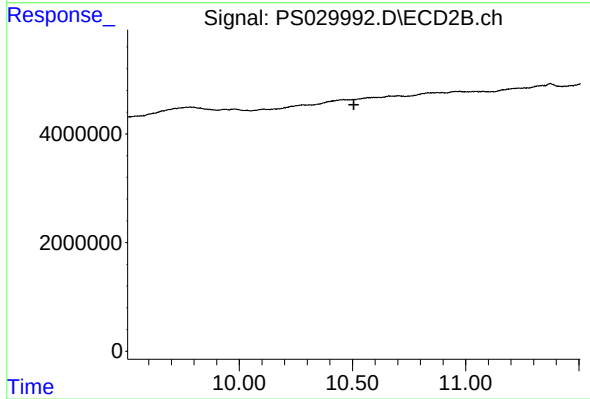


#13 2,4-DB

R.T.: 10.461 min
Delta R.T.: -0.046 min
Response: -2331079
Conc: N.D.

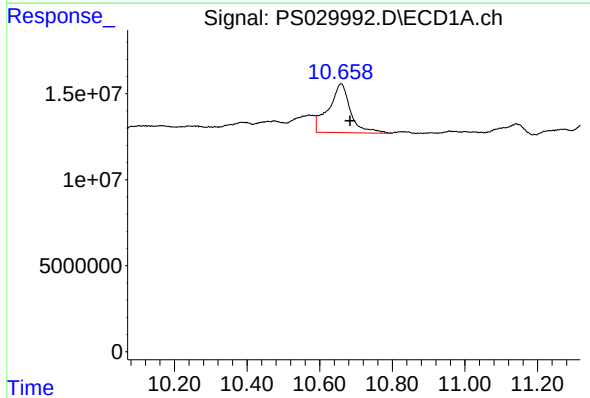

#15 Picloram

R.T.: 10.659 min
Delta R.T.: -0.025 min
Response: 118482754
Conc: 6.46 ng/ml

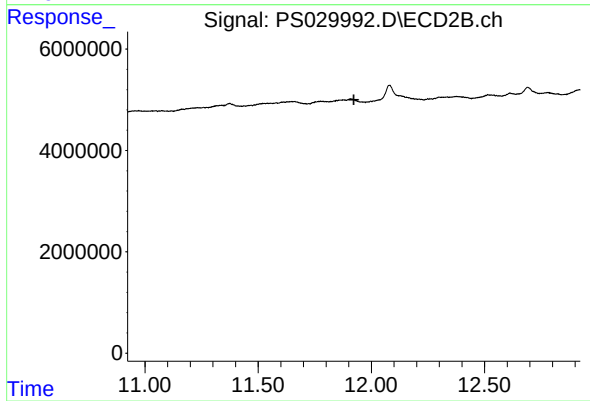

#15 Picloram

R.T.: 0.000 min
Exp R.T.: 11.923 min
Response: 0
Conc: N.D.