

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS050119\
 Data File : PS004390.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 May 2019 21:34
 Operator : EI\SJ
 Sample : K2194-04
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 02 02:10:24 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS042919.M
 Quant Title : 8080.M
 QLast Update : Tue Apr 30 08:27:54 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.001	5.694	145.3E6	113.7E6	230.810	235.739
Target Compounds							
1) T	Dalapon	2.468	2.031	10631529	69699961	13.530	104.156 #
2) T	3,5-DICHL...	5.414	5.006	6297461	110.5E6	7.971	179.759 #
3) T	4-Nitroph...	5.848	5.355	9813635	13417757	39.270	54.244 #
5) T	DICAMBA	6.139	5.802	8400512	16935954	3.533	9.048 #
6) T	MCP	6.357	0.000	4657145	0	2.695	N.D. #
7) T	MCPA	6.412	6.169	7268112	206.5E6	2.821	103.931 #
8) T	DICHLORPROP	0.000	6.388	0	46156732	N.D.	98.085
9) T	2,4-D	7.087	0.000	41068402	0	72.183	N.D. #
11) T	2,4,5-TP ...	0.000	7.352	0	77952099	N.D.	29.668



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS050119\
Data File : PS004390.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 May 2019 21:34
Operator : EI\SJ
Sample : K2194-04
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 02 02:10:24 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS042919.M
Quant Title : 8080.M
QLast Update : Tue Apr 30 08:27:54 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

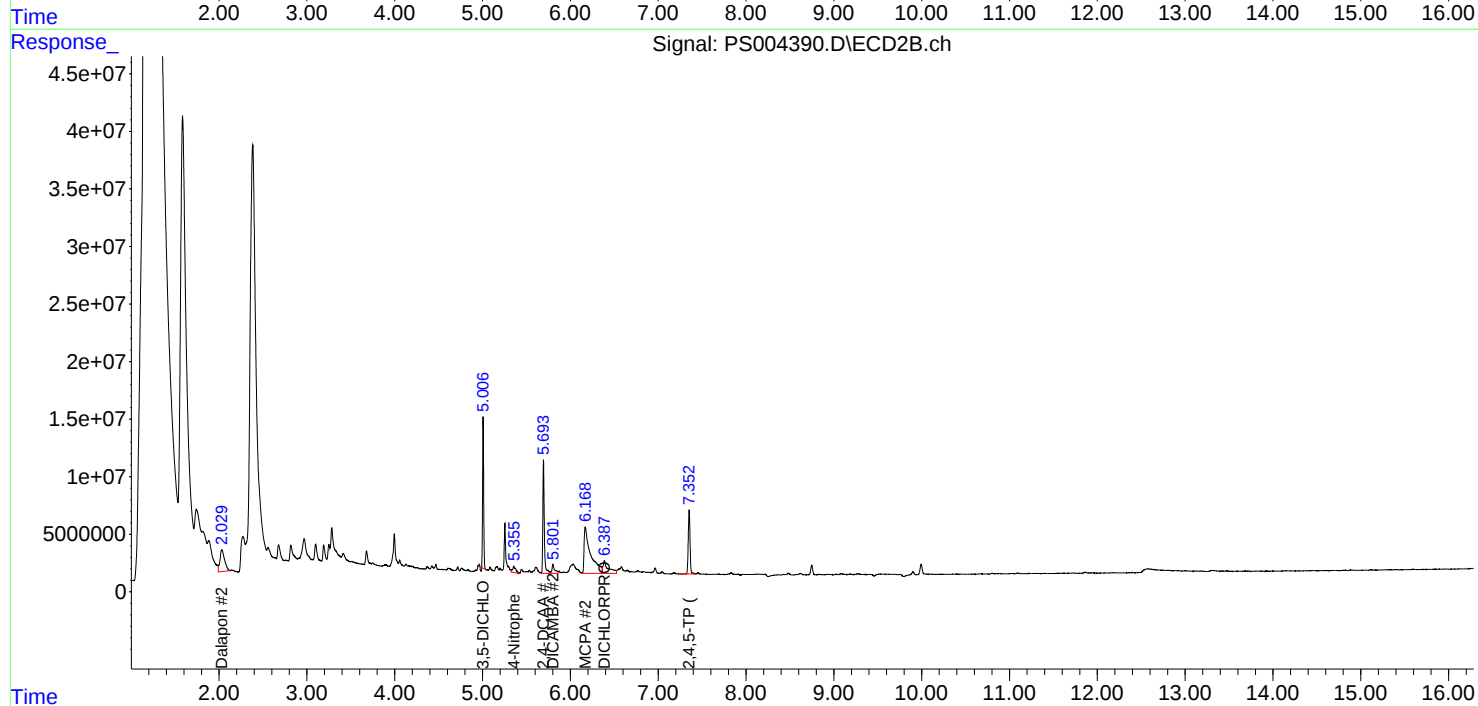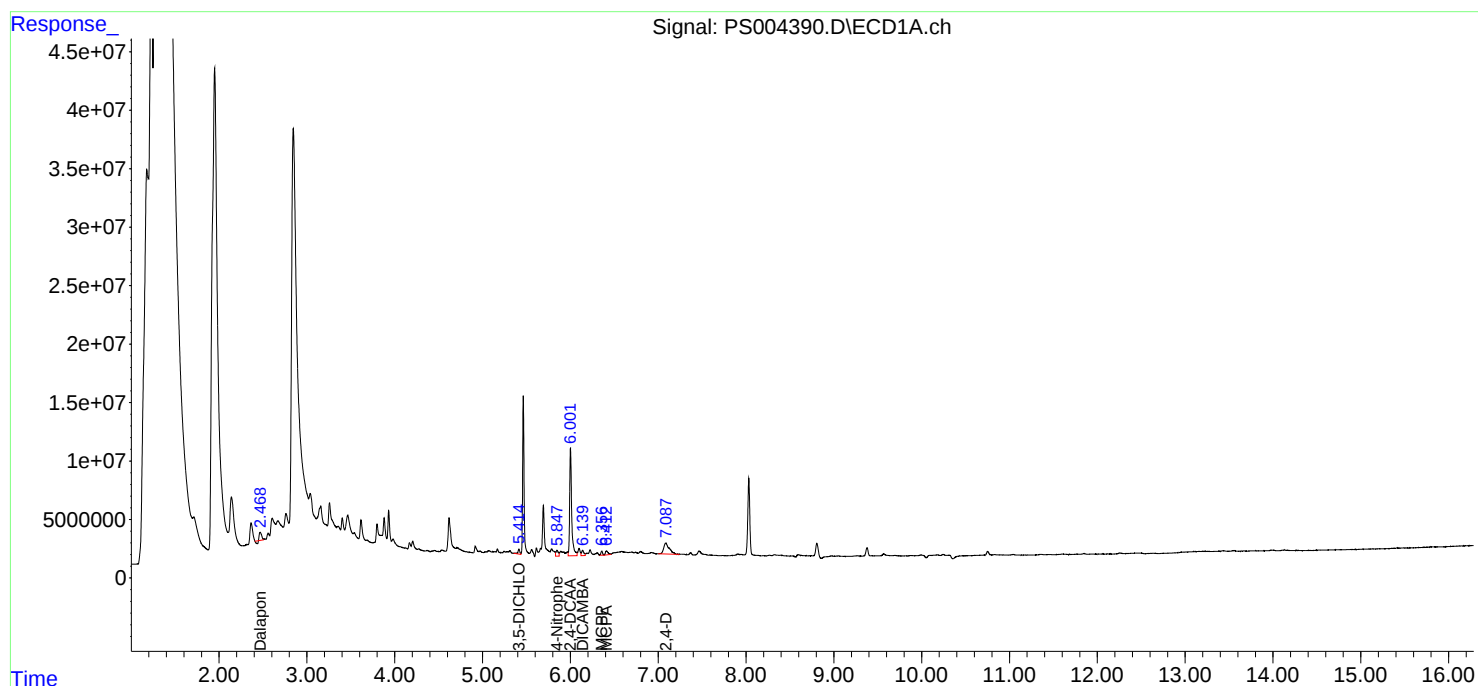


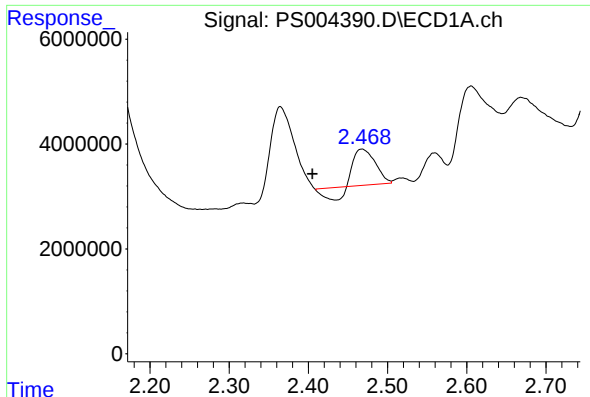

#1 Dalapon


R.T.: 2.468 min
Delta R.T.: 0.063 min
Response: 10631529
Conc: 13.53 ng/ml

Instrument :
ECD_S
ClientSampleId :

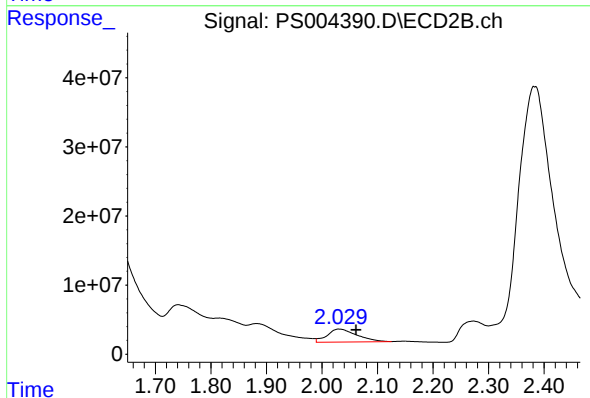


#1 Dalapon

R.T.: 2.031 min
Delta R.T.: -0.031 min
Response: 69699961
Conc: 104.16 ng/ml

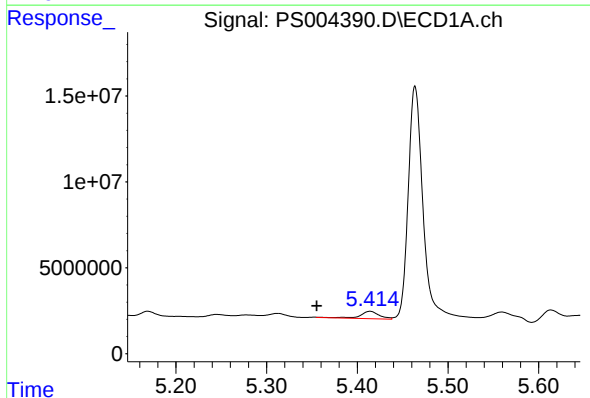


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 5.414 min
Delta R.T.: 0.059 min
Response: 6297461
Conc: 7.97 ng/ml

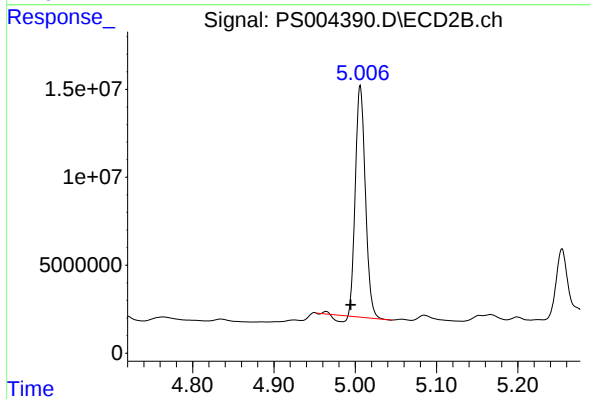

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 5.006 min
Delta R.T.: 0.012 min
Response: 110503479
Conc: 179.76 ng/ml

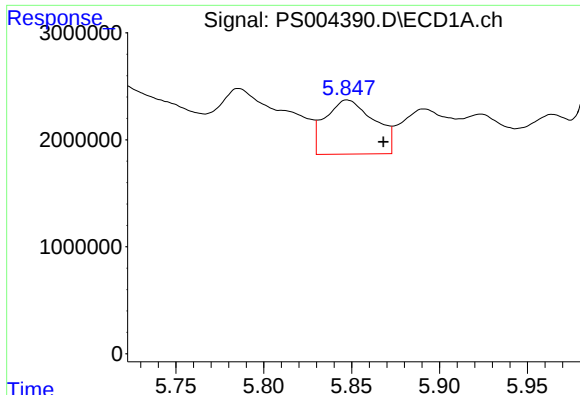

#3 4-Nitrophenol


R.T.: 5.848 min
Delta R.T.: -0.020 min
Response: 9813635
Conc: 39.27 ng/ml

Instrument :
ECD_S
ClientSampleId :

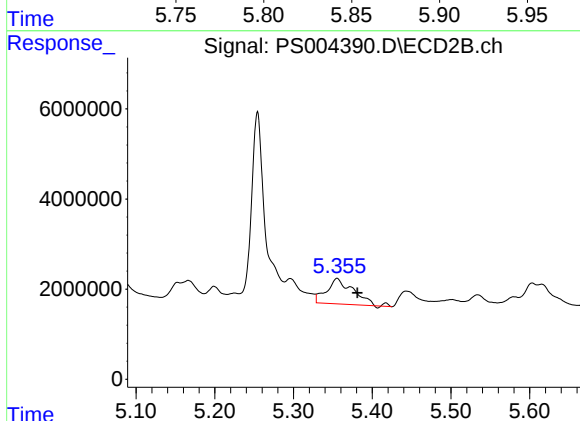


#3 4-Nitrophenol

R.T.: 5.355 min
Delta R.T.: -0.026 min
Response: 13417757
Conc: 54.24 ng/ml

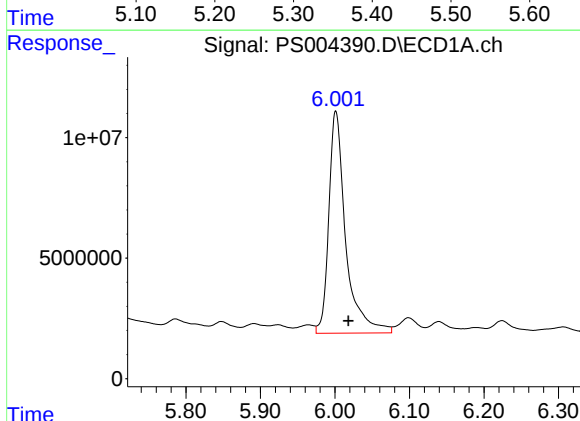


#4 2,4-DCAA

R.T.: 6.001 min
Delta R.T.: -0.017 min
Response: 145284902
Conc: 230.81 ng/ml

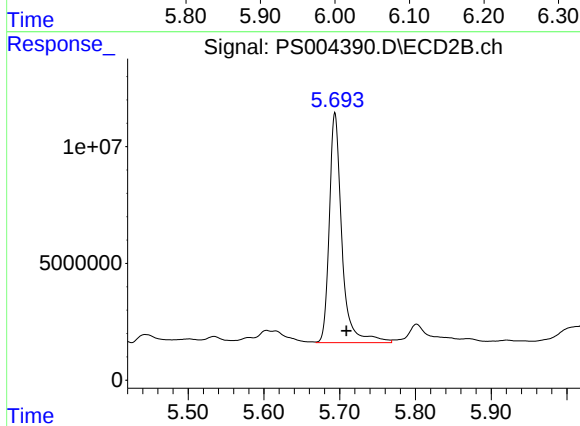

#4 2,4-DCAA


R.T.: 5.694 min
Delta R.T.: -0.015 min
Response: 113693131
Conc: 235.74 ng/ml

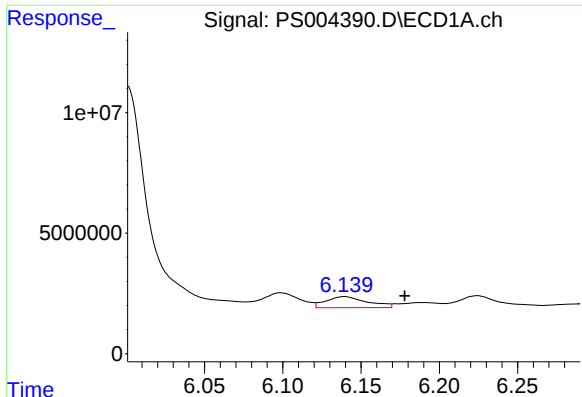

#5 DICAMBA


R.T.: 6.139 min
Delta R.T.: -0.039 min
Response: 8400512
Conc: 3.53 ng/ml

Instrument :
ECD_S
ClientSampleId :

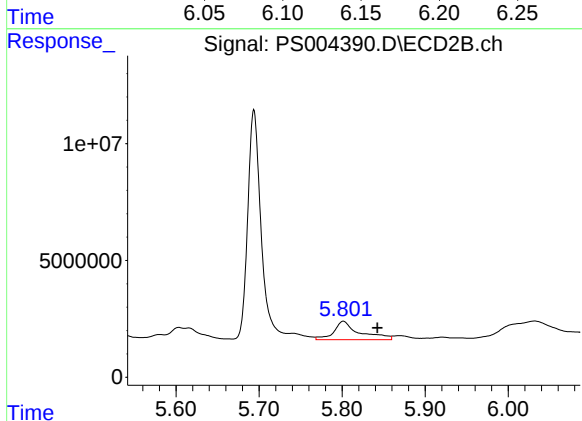


#5 DICAMBA

R.T.: 5.802 min
Delta R.T.: -0.041 min
Response: 16935954
Conc: 9.05 ng/ml

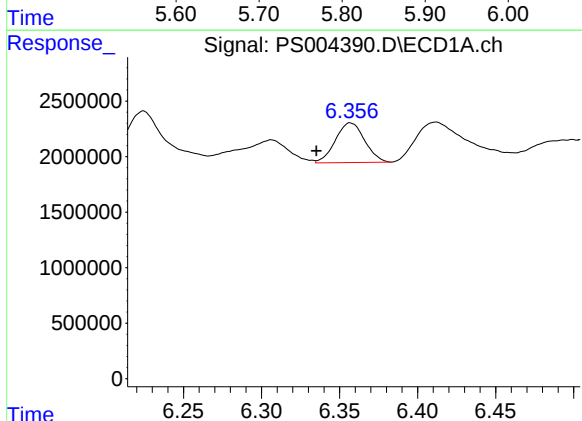


#6 MCP

R.T.: 6.357 min
Delta R.T.: 0.022 min
Response: 4657145
Conc: 2.70 ug/ml

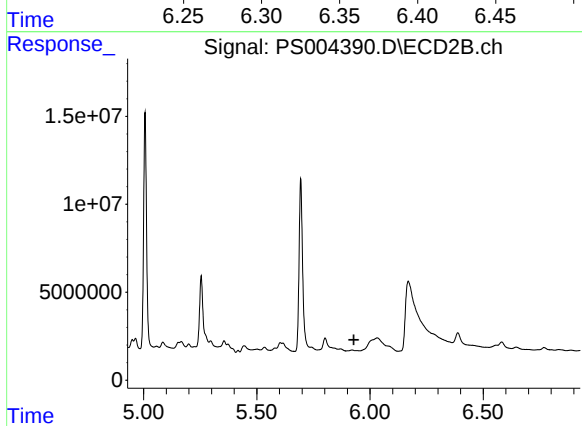

#6 MCP


R.T.: 0.000 min
Exp R.T.: 5.929 min
Response: 0
Conc: N.D.

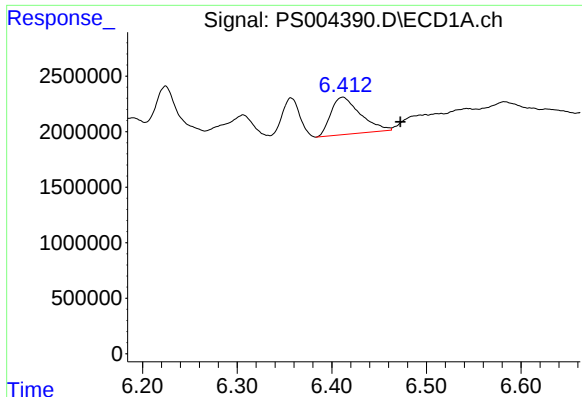

#7 MCPA


R.T.: 6.412 min
Delta R.T.: -0.061 min
Response: 7268112
Conc: 2.82 ug/ml

Instrument :
ECD_S
ClientSampleId :

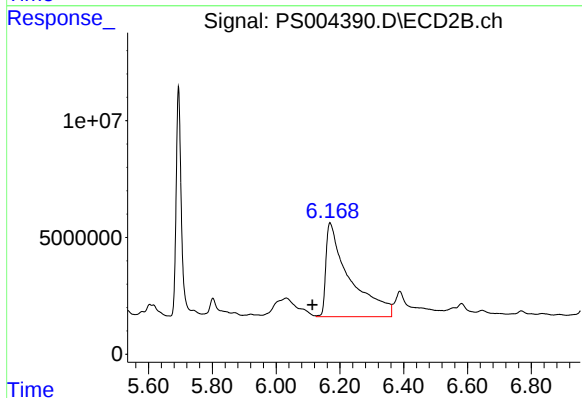


#7 MCPA

R.T.: 6.169 min
Delta R.T.: 0.056 min
Response: 206460264
Conc: 103.93 ug/ml

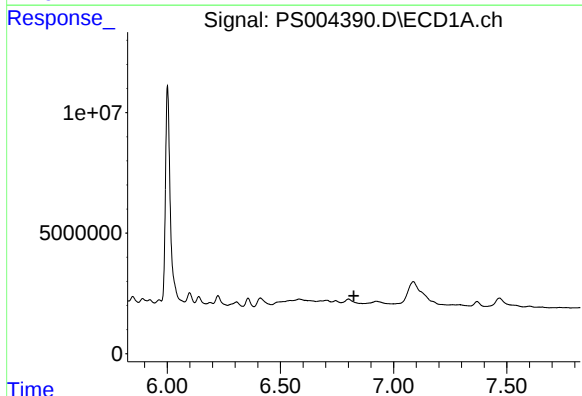


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 6.825 min
Response: 0
Conc: N.D.

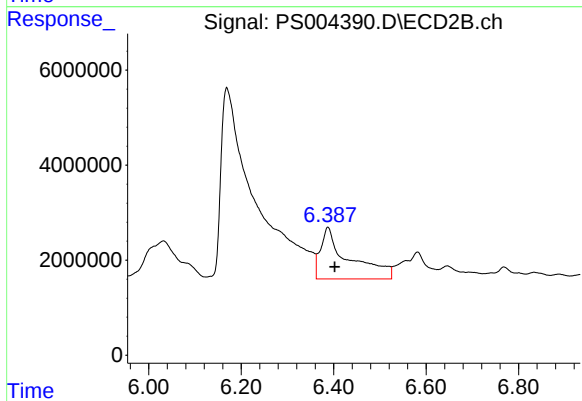

#8 DICHLORPROP


R.T.: 6.388 min
Delta R.T.: -0.015 min
Response: 46156732
Conc: 98.09 ng/ml

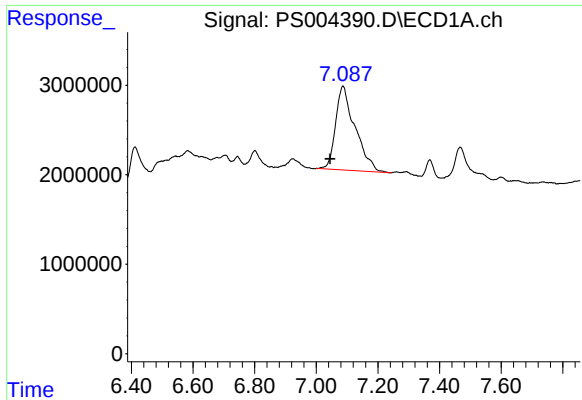

#9 2,4-D


R.T.: 7.087 min
Delta R.T.: 0.042 min
Response: 41068402
Conc: 72.18 ng/ml

Instrument :
ECD_S
ClientSampleId :

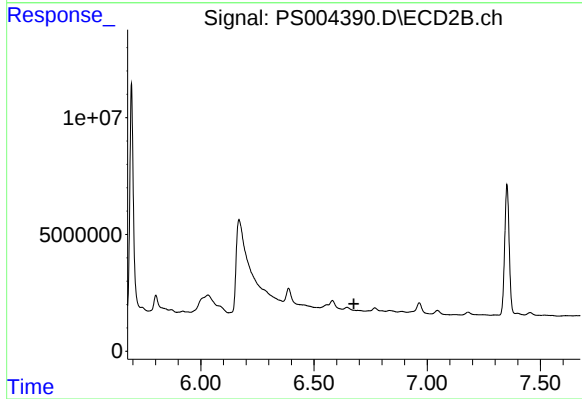


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 6.676 min
Response: 0
Conc: N.D.

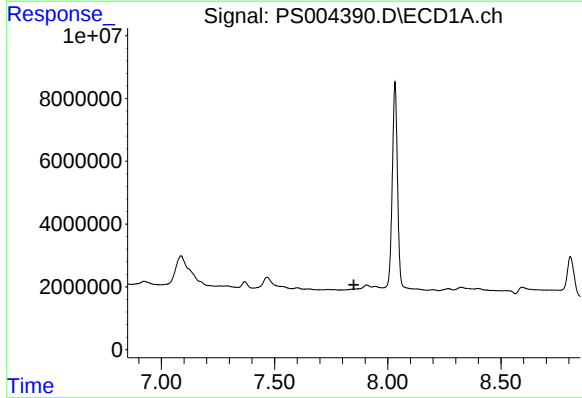

#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T. : 7.850 min
Response: 0
Conc: N.D.

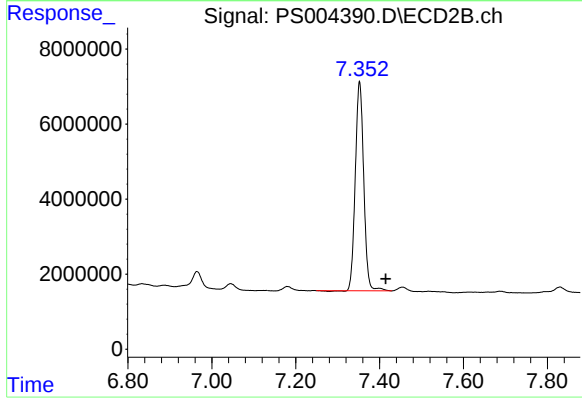

#11 2,4,5-TP (SILVEX)

R.T.: 7.352 min
Delta R.T.: -0.063 min
Response: 77952099
Conc: 29.67 ng/ml