

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS050119\
 Data File : PS004392.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 May 2019 22:36
 Operator : EI\SJ
 Sample : K2194-08
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 02 02:10:55 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS042919.M
 Quant Title : 8080.M
 QLast Update : Tue Apr 30 08:27:54 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.015	5.693	133.5E6	98451837	212.026	204.137
Target Compounds							
1) T	Dalapon	2.381	2.029	38832071	65169746	49.418	97.386 #
2) T	3,5-DICHL...	0.000	5.005	0	99358106	N.D.	161.629
3) T	4-Nitroph...	5.862	5.353	9716924	14536914	38.883	58.769 #
5) T	DICAMBA	6.153	5.800	7939422	14606097	3.339	7.804 #
6) T	MCP	6.371	0.000	4317140	0	2.499	N.D. #
7) T	MCPA	0.000	6.169	0	177.5E6	N.D.	89.361
8) T	DICHLORPROP	0.000	6.387	0	8242216	N.D.	17.515
9) T	2,4-D	7.098	0.000	45658190	0	80.250	N.D. #
11) T	2,4,5-TP ...	0.000	7.351	0	67190646	N.D.	25.573



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS050119\
Data File : PS004392.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 May 2019 22:36
Operator : EI\SJ
Sample : K2194-08
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 02 02:10:55 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS042919.M
Quant Title : 8080.M
QLast Update : Tue Apr 30 08:27:54 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

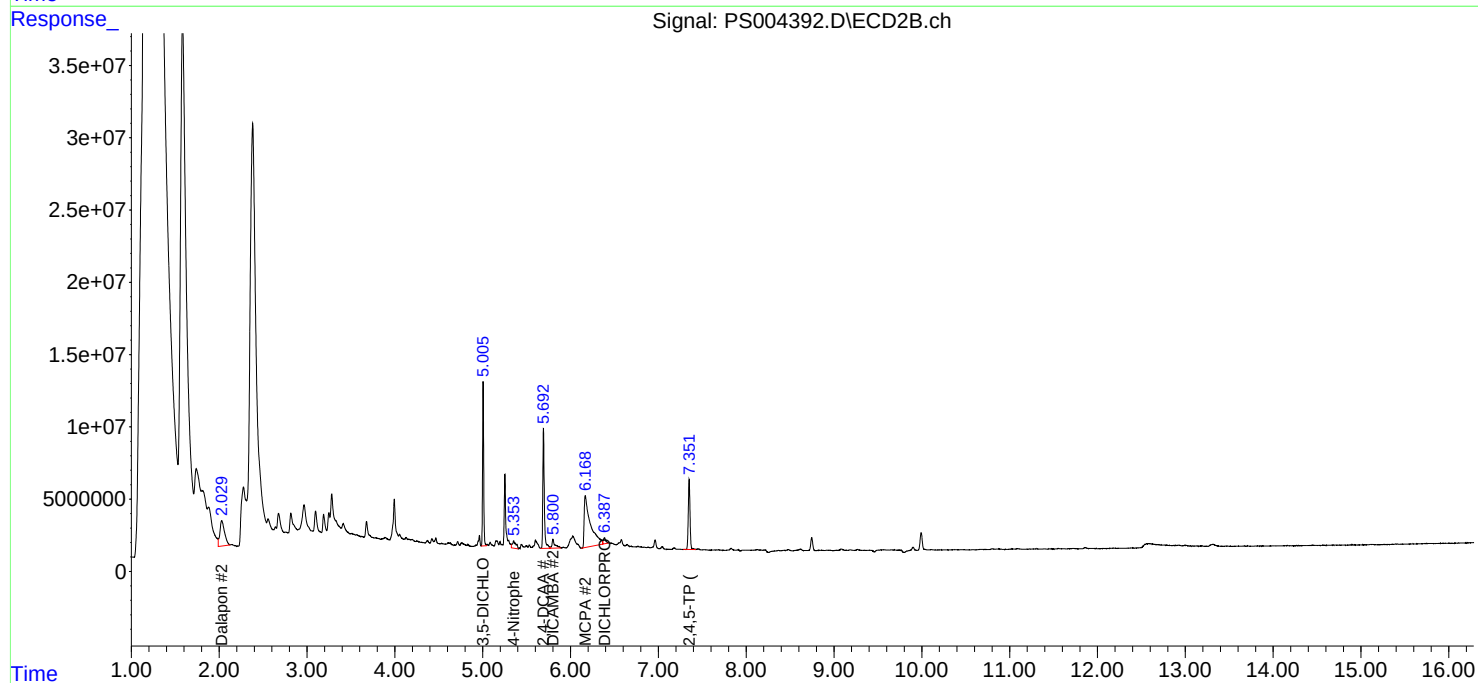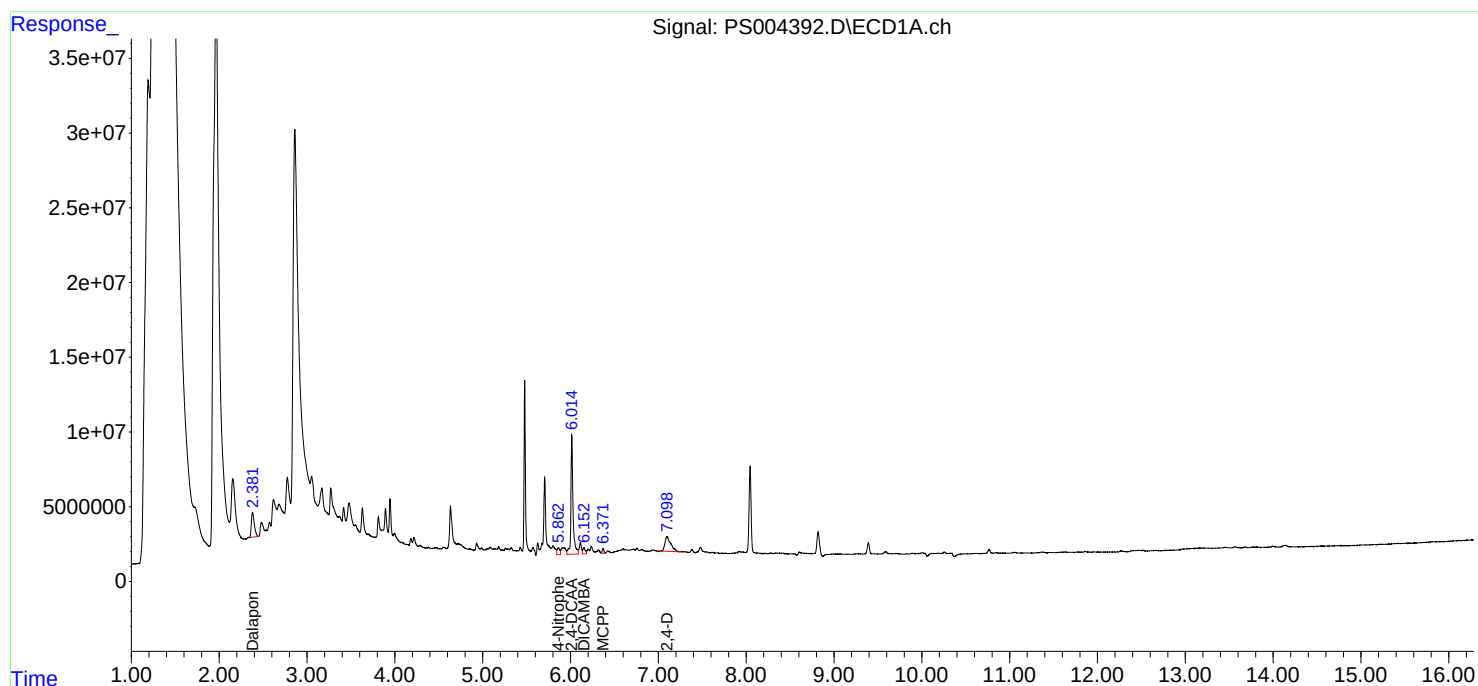


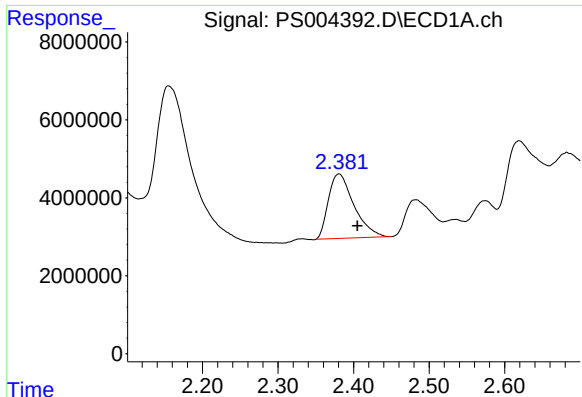

#1 Dalapon


R.T.: 2.381 min
Delta R.T.: -0.024 min
Response: 38832071
Conc: 49.42 ng/ml

Instrument :
ECD_S
ClientSampleId :

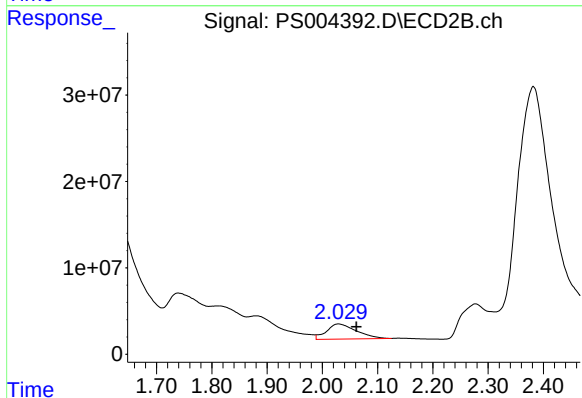


#1 Dalapon

R.T.: 2.029 min
Delta R.T.: -0.032 min
Response: 65169746
Conc: 97.39 ng/ml

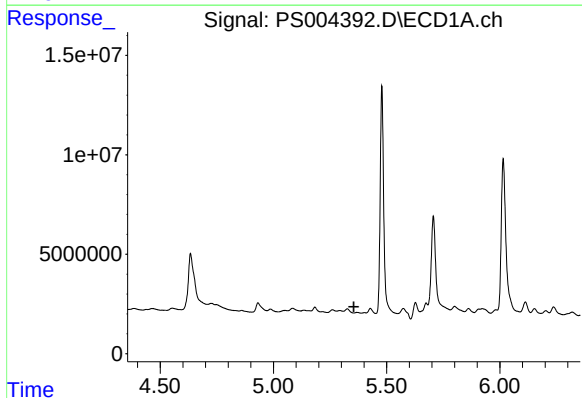


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 5.355 min
Response: 0
Conc: N.D.

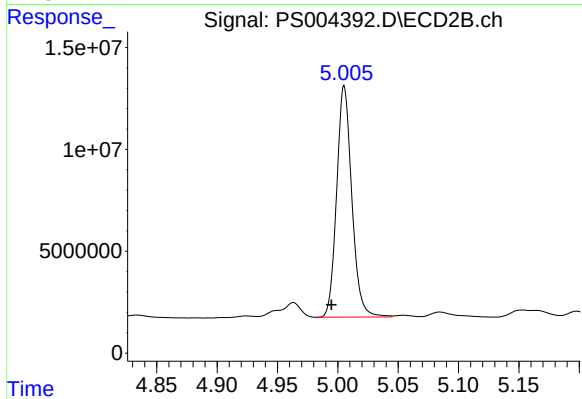

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 5.005 min
Delta R.T.: 0.011 min
Response: 99358106
Conc: 161.63 ng/ml

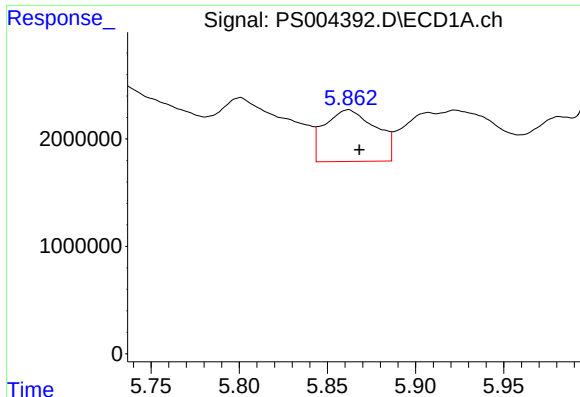

#3 4-Nitrophenol


R.T.: 5.862 min
Delta R.T.: -0.006 min
Response: 9716924
Conc: 38.88 ng/ml

Instrument :
ECD_S
ClientSampleId :

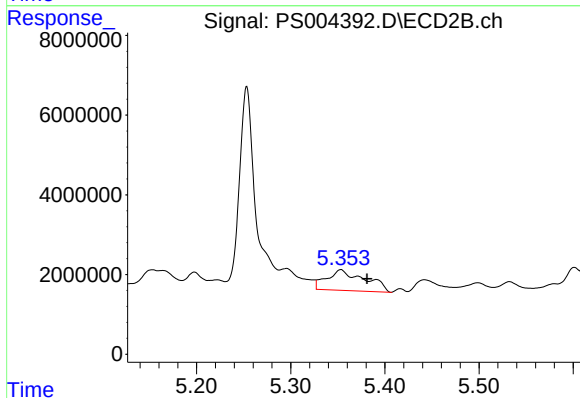


#3 4-Nitrophenol

R.T.: 5.353 min
Delta R.T.: -0.028 min
Response: 14536914
Conc: 58.77 ng/ml

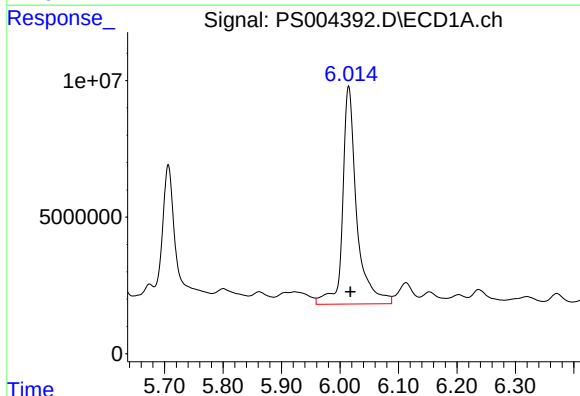


#4 2,4-DCAA

R.T.: 6.015 min
Delta R.T.: -0.003 min
Response: 133461257
Conc: 212.03 ng/ml

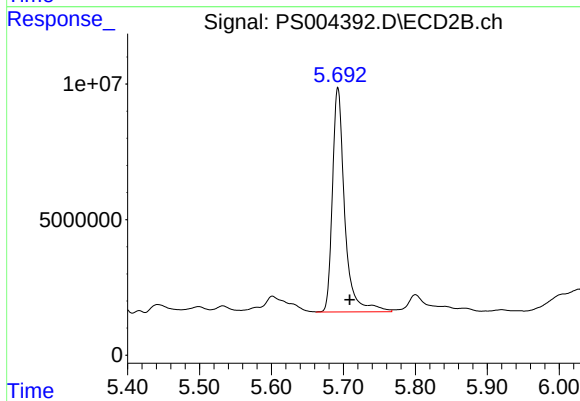

#4 2,4-DCAA


R.T.: 5.693 min
Delta R.T.: -0.016 min
Response: 98451837
Conc: 204.14 ng/ml

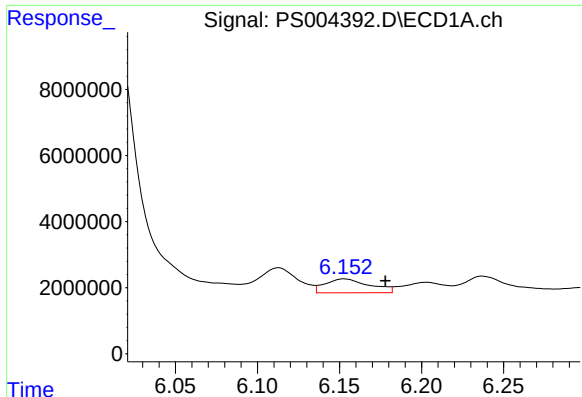

#5 DICAMBA


R.T.: 6.153 min
Delta R.T.: -0.025 min
Response: 7939422
Conc: 3.34 ng/ml

Instrument :
ECD_S
ClientSampleId :

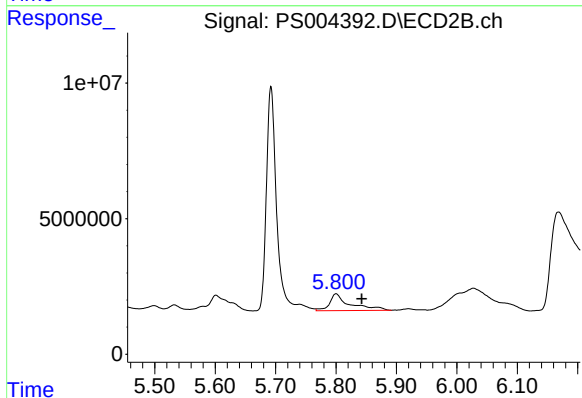


#5 DICAMBA

R.T.: 5.800 min
Delta R.T.: -0.042 min
Response: 14606097
Conc: 7.80 ng/ml

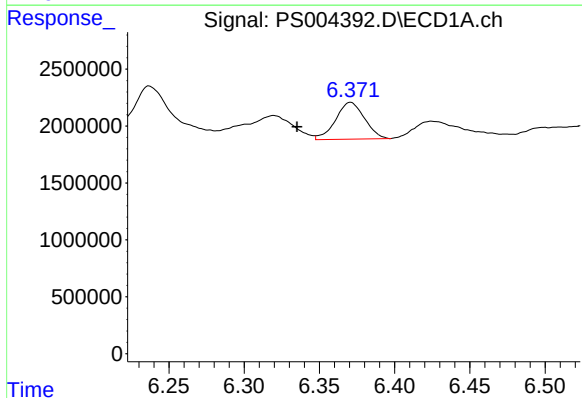


#6 MCP

R.T.: 6.371 min
Delta R.T.: 0.036 min
Response: 4317140
Conc: 2.50 ug/ml

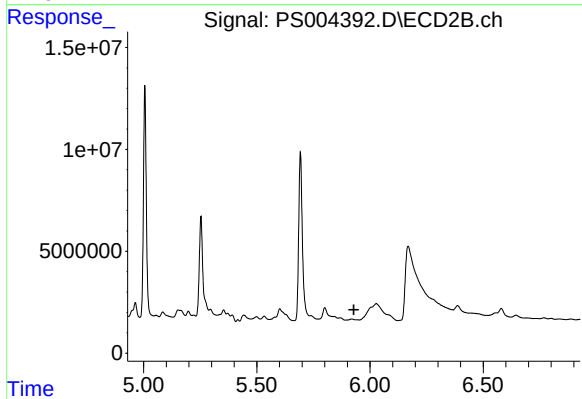

#6 MCP


R.T.: 0.000 min
Exp R.T.: 5.929 min
Response: 0
Conc: N.D.

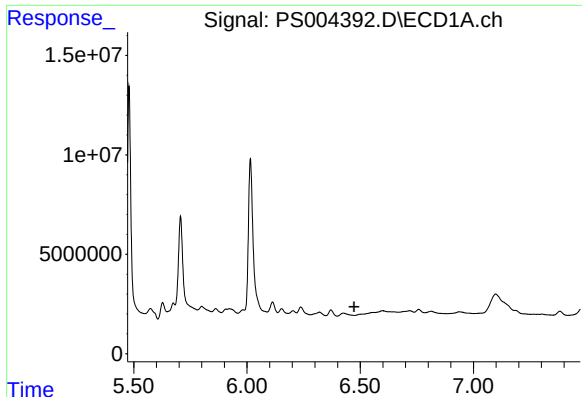

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 6.472 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

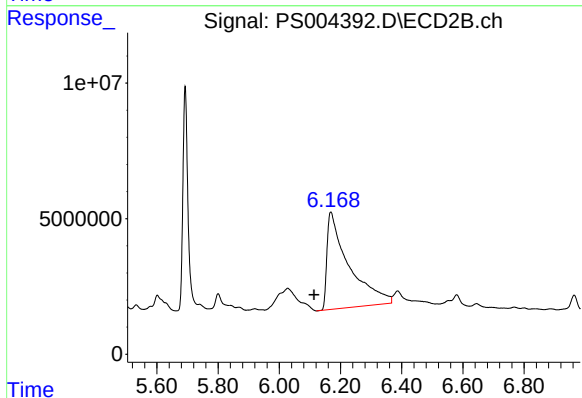


#7 MCPA

R.T.: 6.169 min
Delta R.T.: 0.055 min
Response: 177517804
Conc: 89.36 ug/ml

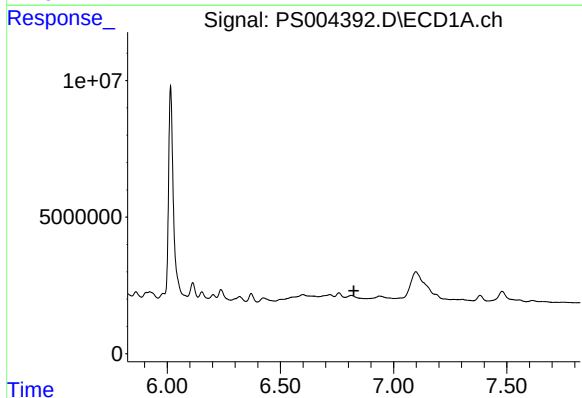


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T.: 6.825 min
Response: 0
Conc: N.D.

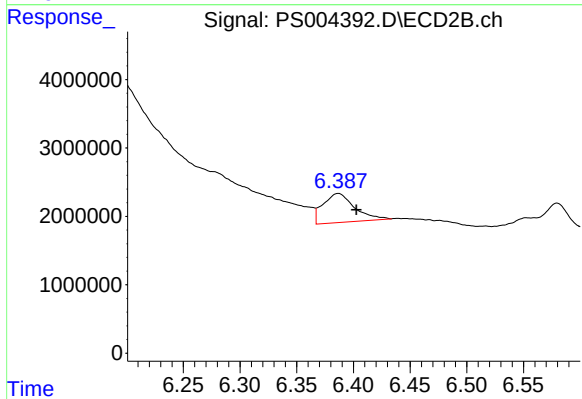

#8 DICHLORPROP


R.T.: 6.387 min
Delta R.T.: -0.016 min
Response: 8242216
Conc: 17.52 ng/ml

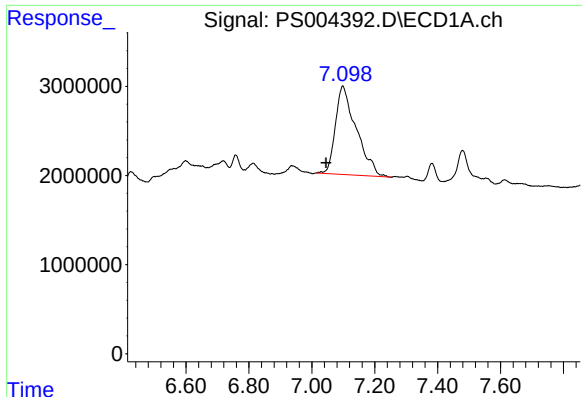

#9 2,4-D


R.T.: 7.098 min
Delta R.T.: 0.053 min
Response: 45658190
Conc: 80.25 ng/ml

Instrument :
ECD_S
ClientSampleId :

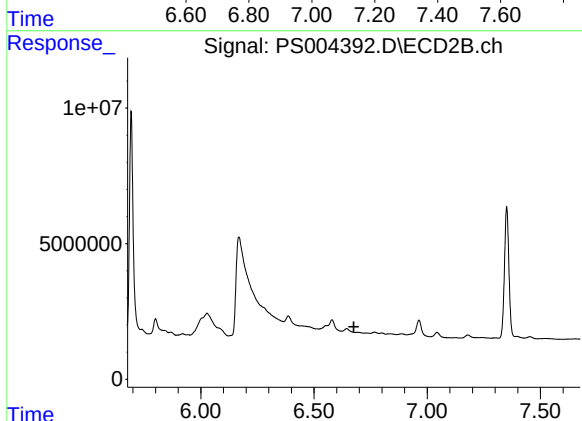


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 6.676 min
Response: 0
Conc: N.D.

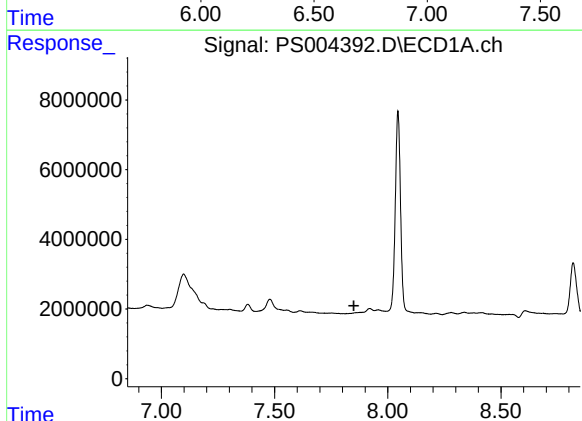

#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T. : 7.850 min
Response: 0
Conc: N.D.

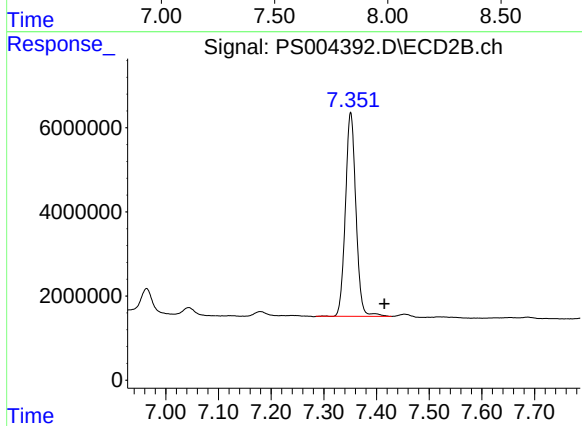

#11 2,4,5-TP (SILVEX)

R.T.: 7.351 min
Delta R.T.: -0.064 min
Response: 67190646
Conc: 25.57 ng/ml