

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS050119\
 Data File : PS004399.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 May 2019 02:05
 Operator : EI\SJ
 Sample : K2194-18
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 02 04:29:56 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS042919.M
 Quant Title : 8080.M
 QLast Update : Tue Apr 30 08:27:54 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.002	5.696	142.3E6	102.8E6	226.091	213.170
Target Compounds							
1) T	Dalapon	2.368	2.032	23030634	95649357	29.309	142.934 #
2) T	3,5-DICHL...	0.000	5.009	0	116.1E6	N.D.	188.874
3) T	4-Nitroph...	5.849	5.357	11102474	15594879	44.428	63.046 #
5) T	DICAMBA	6.140	5.846	8615435	5249366	3.623	2.805
6) T	MCP	6.358	0.000	5275438	0	3.053	N.D. #
7) T	MCPA	0.000	6.179	0	114.4E6	N.D.	57.586
8) T	DICHLORPROP	0.000	6.390	0	26162659	N.D.	55.597
9) T	2,4-D	7.088	0.000	48233232	0	84.776	N.D. #
11) T	2,4,5-TP ...	0.000	7.354	0	79918105	N.D.	30.417
15) T	Picloram	9.573	0.000	5190488	0	1.226	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS050119\
Data File : PS004399.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 May 2019 02:05
Operator : EI\SJ
Sample : K2194-18
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 02 04:29:56 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS042919.M
Quant Title : 8080.M
QLast Update : Tue Apr 30 08:27:54 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

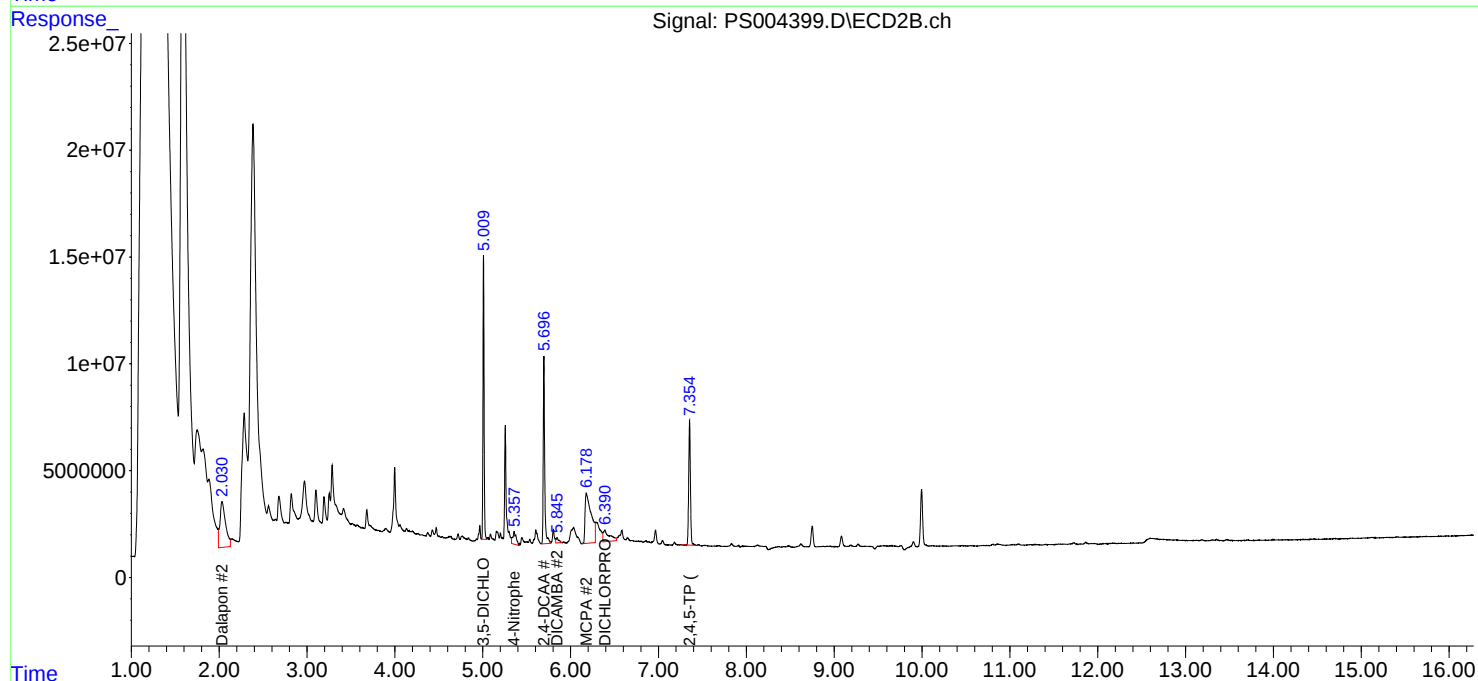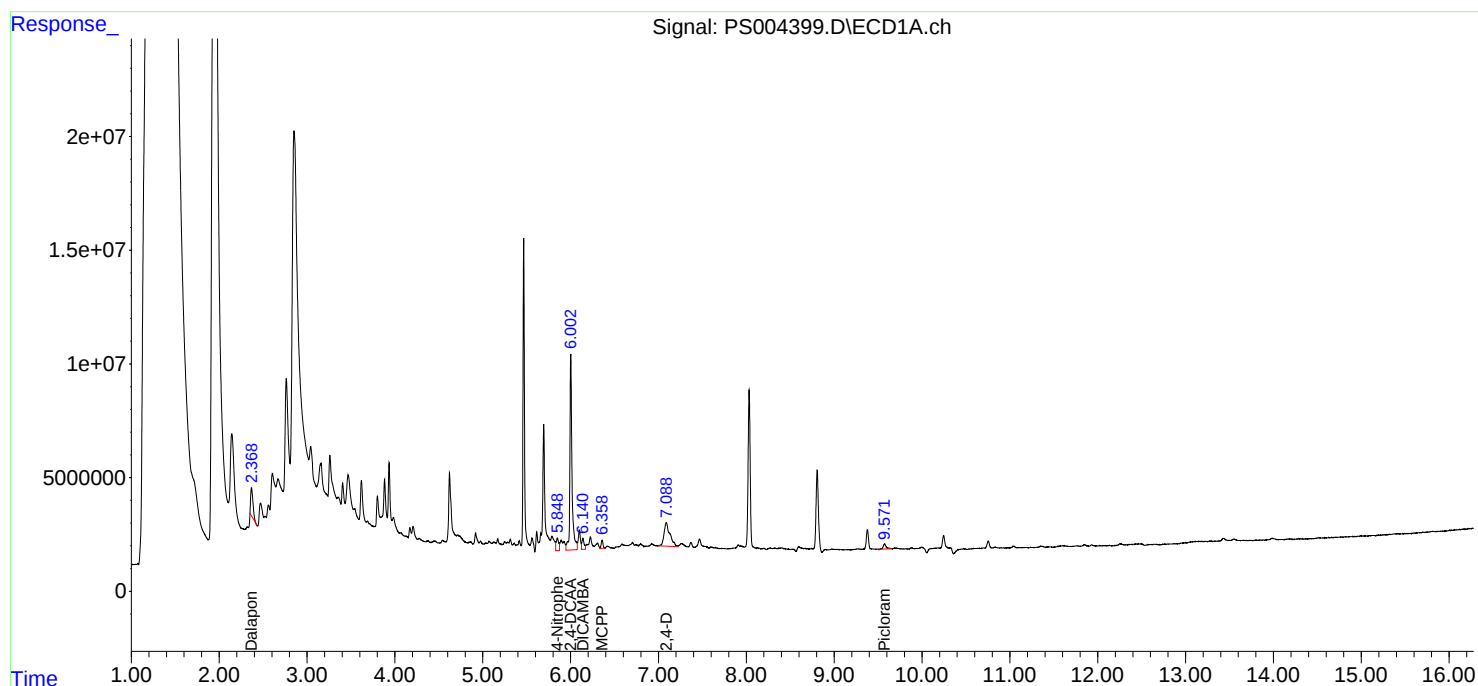


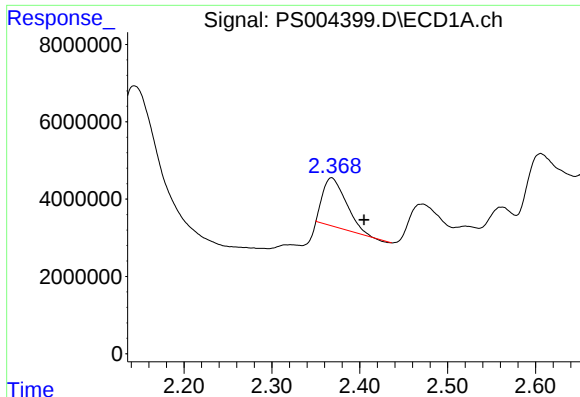

#1 Dalapon


R.T.: 2.368 min
Delta R.T.: -0.037 min
Response: 23030634
Conc: 29.31 ng/ml

Instrument :
ECD_S
ClientSampleId :

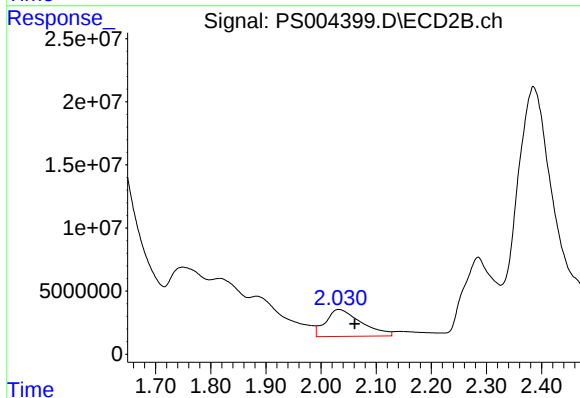


#1 Dalapon

R.T.: 2.032 min
Delta R.T.: -0.029 min
Response: 95649357
Conc: 142.93 ng/ml

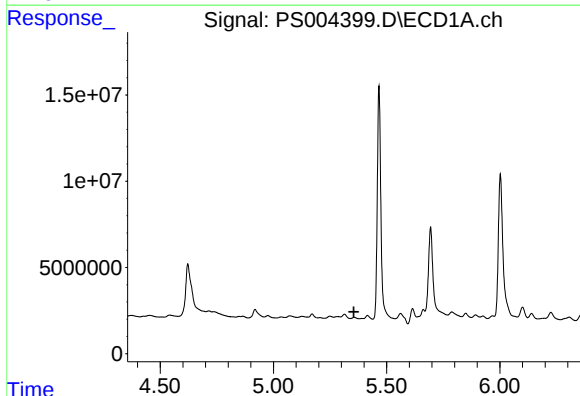


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 5.355 min
Response: 0
Conc: N.D.

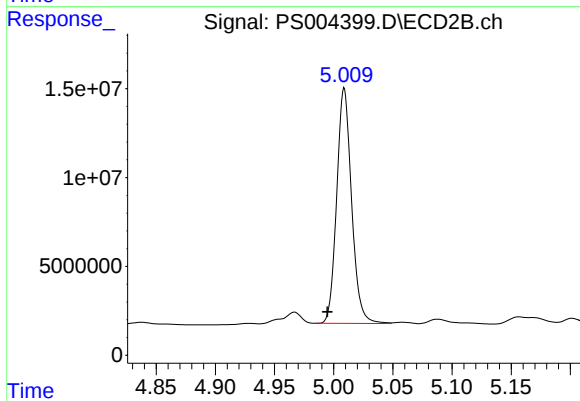

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 5.009 min
Delta R.T.: 0.014 min
Response: 116106665
Conc: 188.87 ng/ml

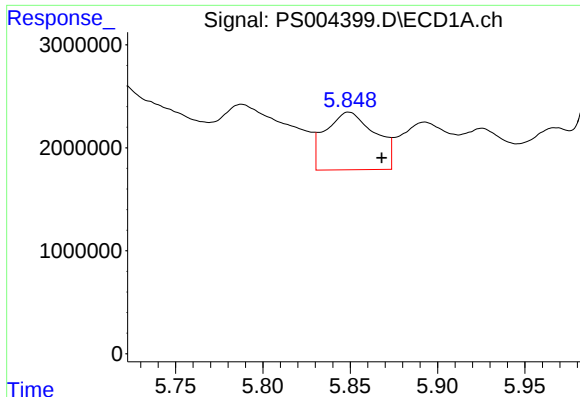

#3 4-Nitrophenol


R.T.: 5.849 min
Delta R.T.: -0.019 min
Response: 11102474
Conc: 44.43 ng/ml

Instrument :
ECD_S
ClientSampleId :

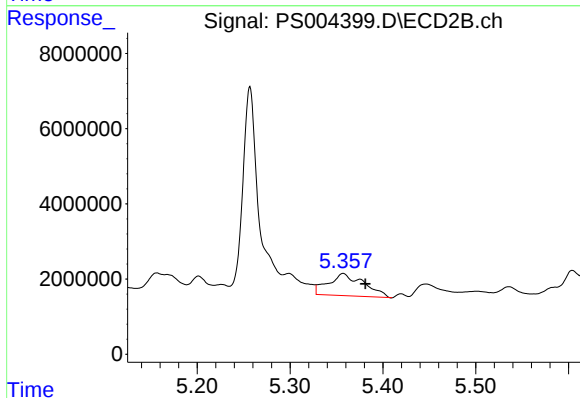


#3 4-Nitrophenol

R.T.: 5.357 min
Delta R.T.: -0.024 min
Response: 15594879
Conc: 63.05 ng/ml

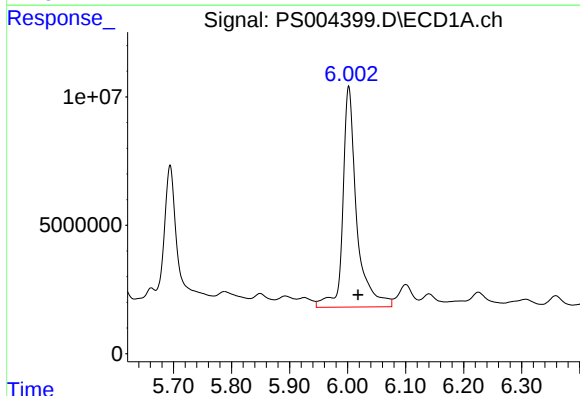


#4 2,4-DCAA

R.T.: 6.002 min
Delta R.T.: -0.016 min
Response: 142314660
Conc: 226.09 ng/ml

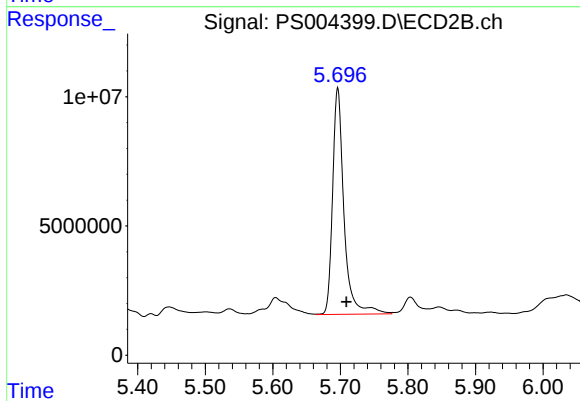

#4 2,4-DCAA


R.T.: 5.696 min
Delta R.T.: -0.013 min
Response: 102808071
Conc: 213.17 ng/ml

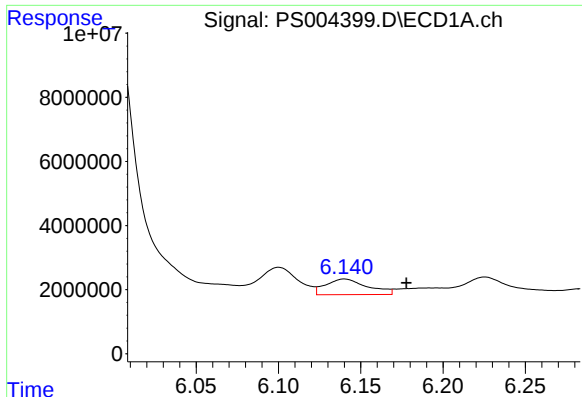

#5 DICAMBA


R.T.: 6.140 min
Delta R.T.: -0.038 min
Response: 8615435
Conc: 3.62 ng/ml

Instrument :
ECD_S
ClientSampleId :

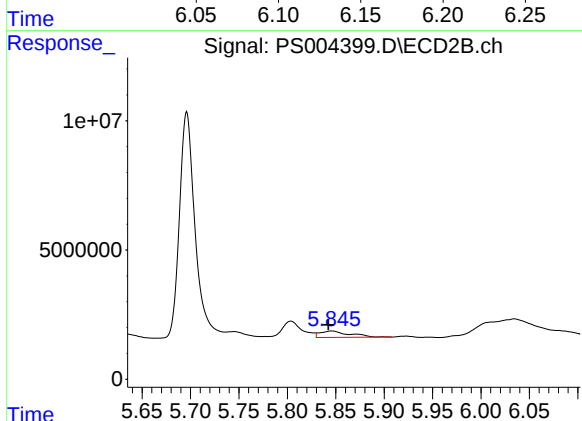


#5 DICAMBA

R.T.: 5.846 min
Delta R.T.: 0.003 min
Response: 5249366
Conc: 2.80 ng/ml

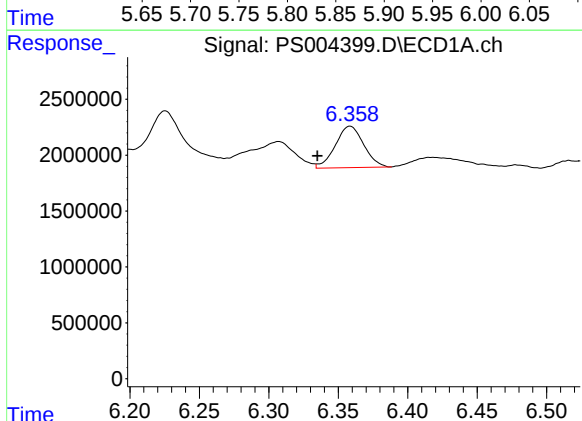


#6 MCP

R.T.: 6.358 min
Delta R.T.: 0.023 min
Response: 5275438
Conc: 3.05 ug/ml

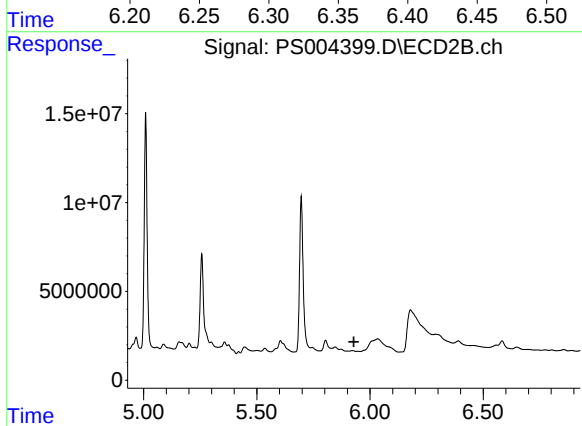

#6 MCP


R.T.: 0.000 min
Exp R.T.: 5.929 min
Response: 0
Conc: N.D.

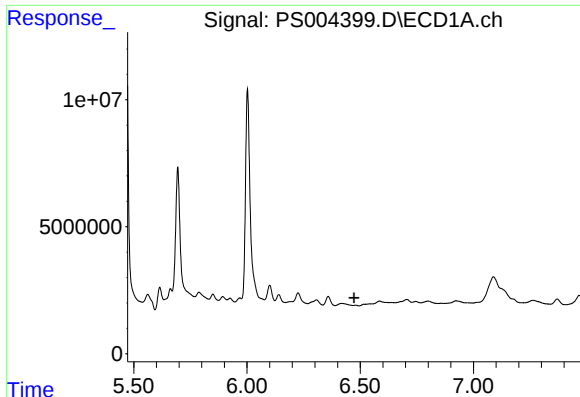

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 6.472 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

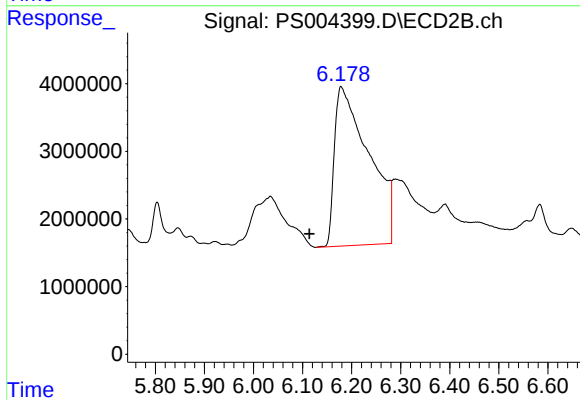


#7 MCPA

R.T.: 6.179 min
Delta R.T.: 0.066 min
Response: 114395689
Conc: 57.59 ug/ml

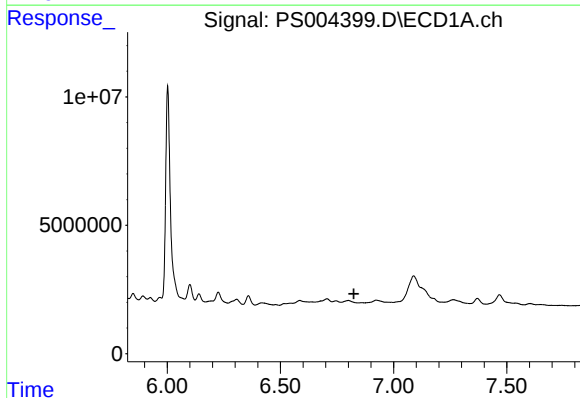


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T.: 6.825 min
Response: 0
Conc: N.D.

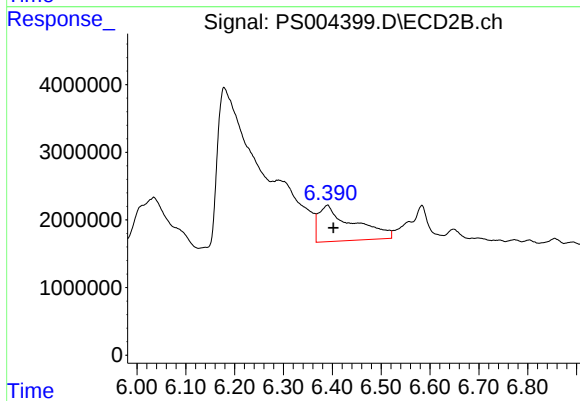

#8 DICHLORPROP


R.T.: 6.390 min
Delta R.T.: -0.013 min
Response: 26162659
Conc: 55.60 ng/ml

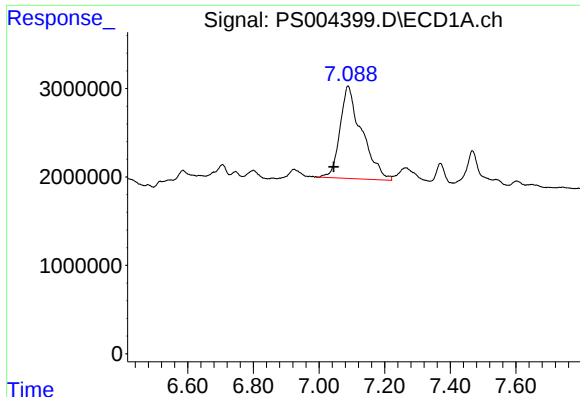

#9 2,4-D


R.T.: 7.088 min
Delta R.T.: 0.043 min
Response: 48233232
Conc: 84.78 ng/ml

Instrument :
ECD_S
ClientSampleId :

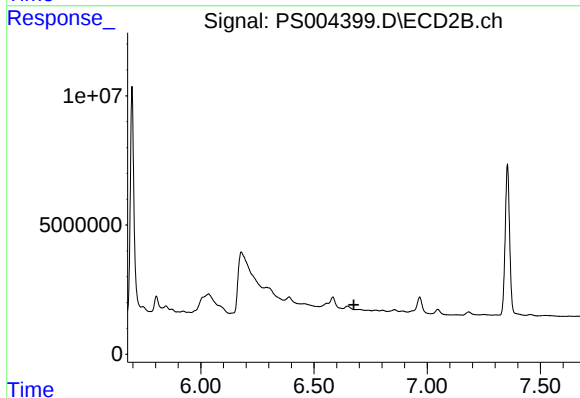


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 6.676 min
Response: 0
Conc: N.D.

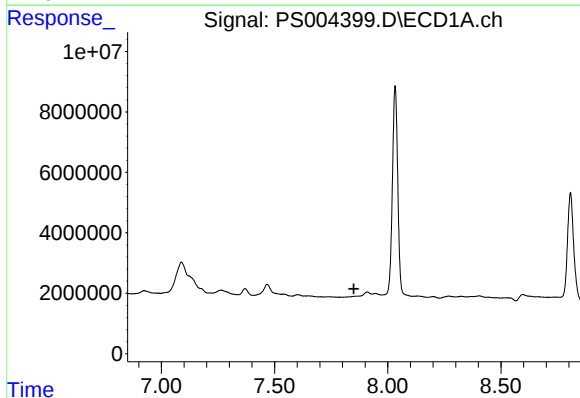


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T. : 7.850 min
Response: 0
Conc: N.D.

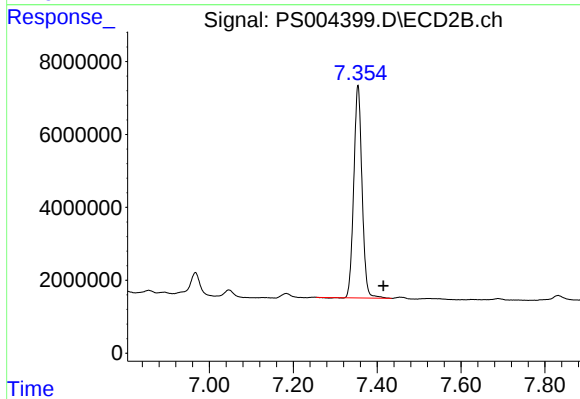

#11 2,4,5-TP (SILVEX)


R.T.: 7.354 min
Delta R.T.: -0.061 min
Response: 79918105
Conc: 30.42 ng/ml

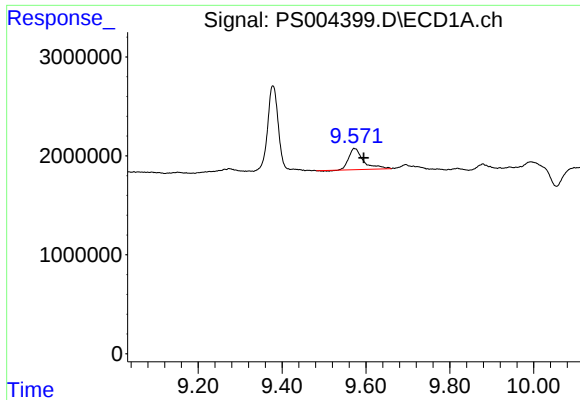

#15 Picloram

R.T.: 9.573 min
Delta R.T.: -0.022 min
Response: 5190488
Conc: 1.23 ng/ml

Instrument :
ECD_S
ClientSampleId :

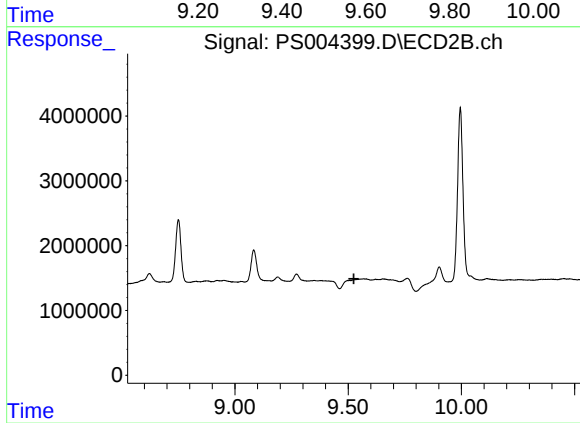

#15 Picloram

R.T.: 0.000 min
Exp R.T. : 9.526 min
Response: 0
Conc: N.D.