

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS050119\
 Data File : PS004400.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 May 2019 02:33
 Operator : EI\SJ
 Sample : K2199-18
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 02 04:30:14 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS042919.M
 Quant Title : 8080.M
 QLast Update : Tue Apr 30 08:27:54 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.013	5.707	127.7E6	95700968	202.794	198.433
Target Compounds							
1) T	Dalapon	2.378	2.040	32665851	54394814	41.571	81.285 #
2) T	3,5-DICHL...	0.000	4.977	0	6296836	N.D.	10.243
3) T	4-Nitroph...	5.859	5.367	10627578	15158235	42.527	61.281 #
5) T	DICAMBA	6.150	5.856	8697025	5550584	3.657	2.965
6) T	MCPD	6.368	0.000	4573036	0	2.647	N.D. #
7) T	MCPA	0.000	6.184	0	194.4E6	N.D.	97.845
8) T	DICHLORPROP	0.000	6.399	0	28642710	N.D.	60.867
9) T	2,4-D	7.100	0.000	39086256	0	68.699	N.D. #
11) T	2,4,5-TP ...	0.000	7.365	0	72919435	N.D.	27.753
15) T	Picloram	9.583	0.000	5241453	0	1.238	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS050119\
Data File : PS004400.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 May 2019 02:33
Operator : EI\SJ
Sample : K2199-18
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 02 04:30:14 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS042919.M
Quant Title : 8080.M
QLast Update : Tue Apr 30 08:27:54 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

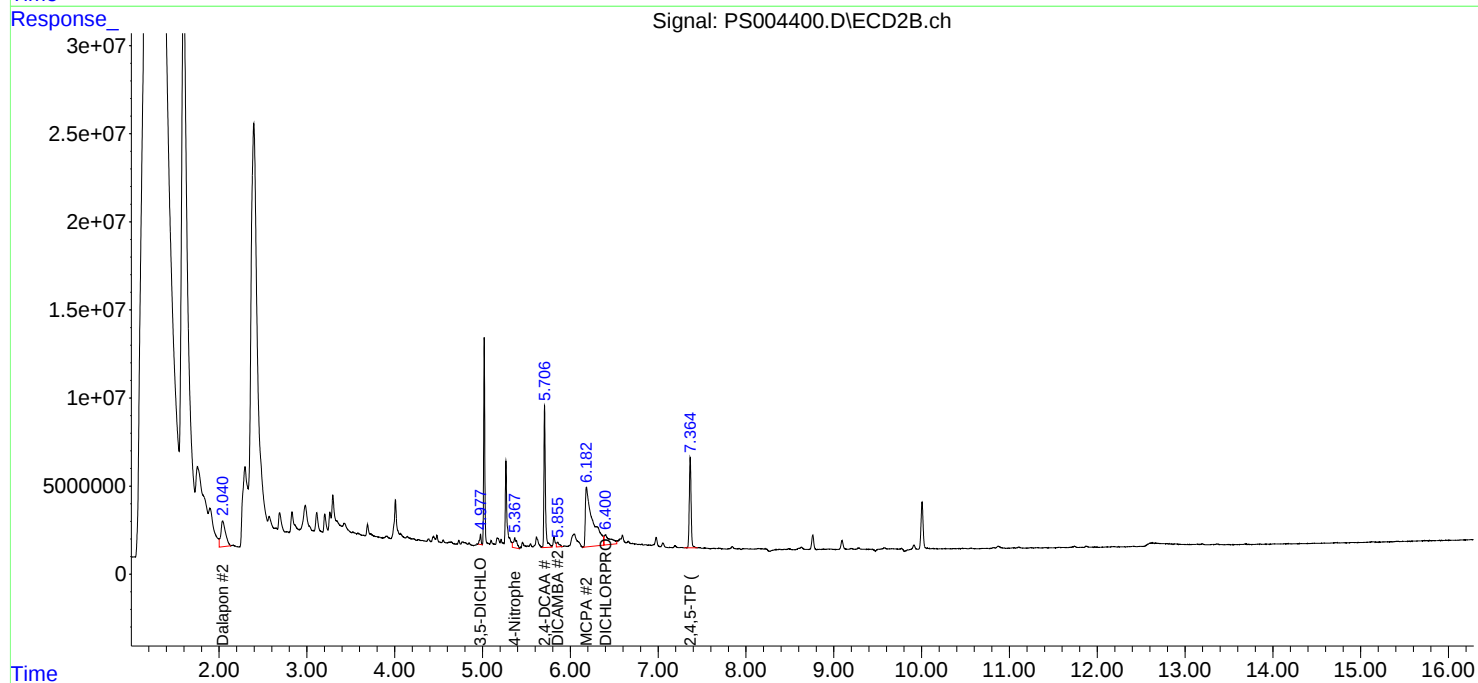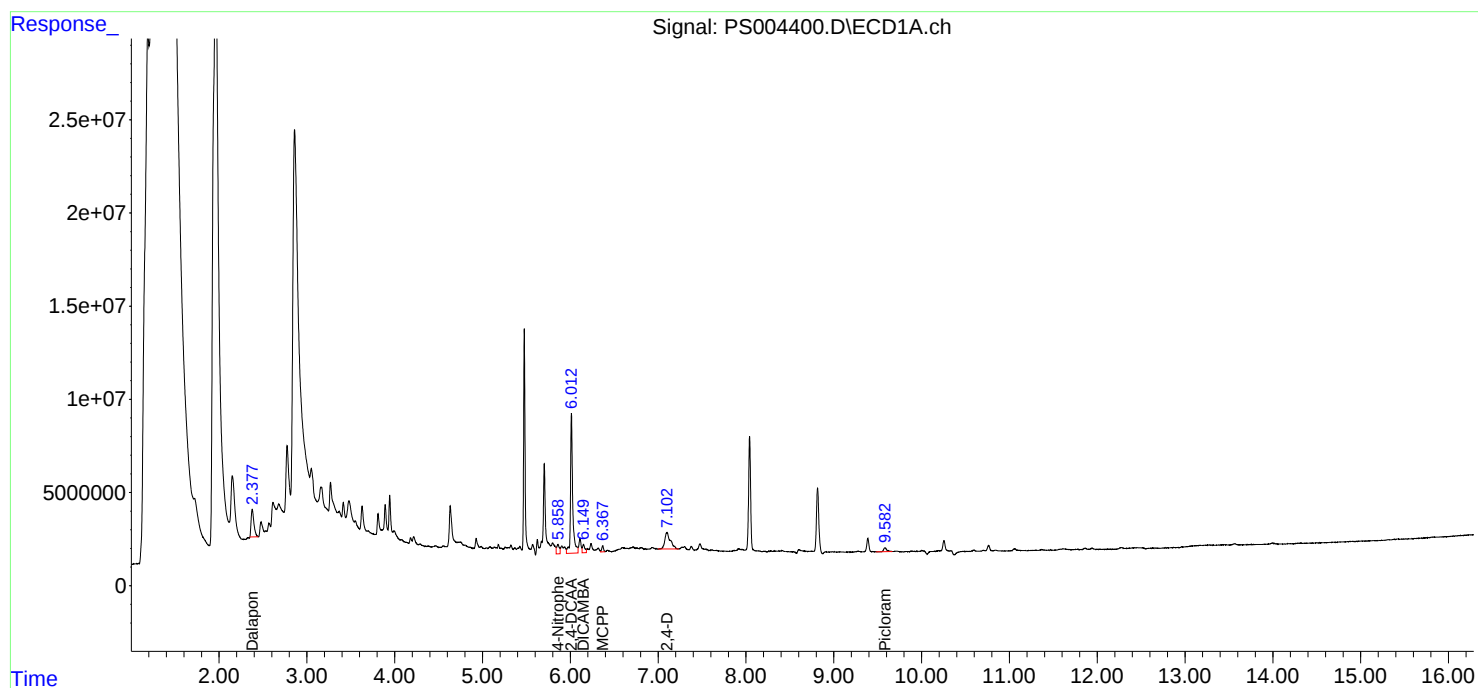


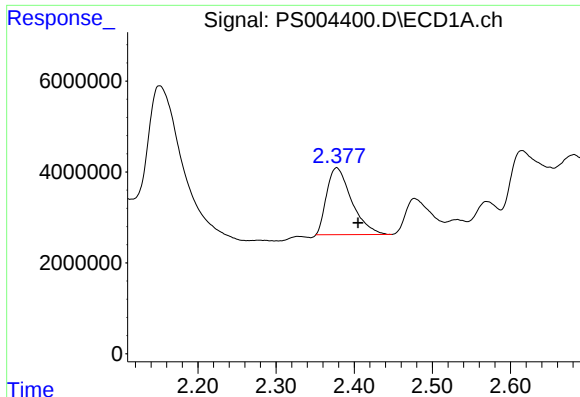

#1 Dalapon


R.T.: 2.378 min
Delta R.T.: -0.027 min
Response: 32665851
Conc: 41.57 ng/ml

Instrument :
ECD_S
ClientSampleId :

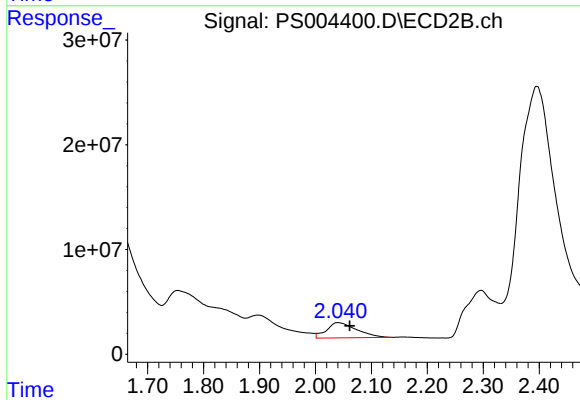


#1 Dalapon

R.T.: 2.040 min
Delta R.T.: -0.021 min
Response: 54394814
Conc: 81.28 ng/ml

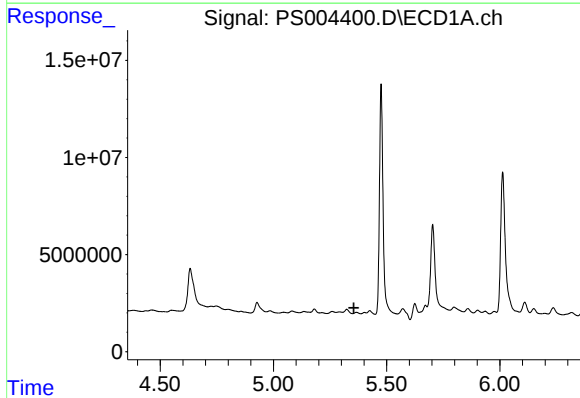


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 5.355 min
Response: 0
Conc: N.D.

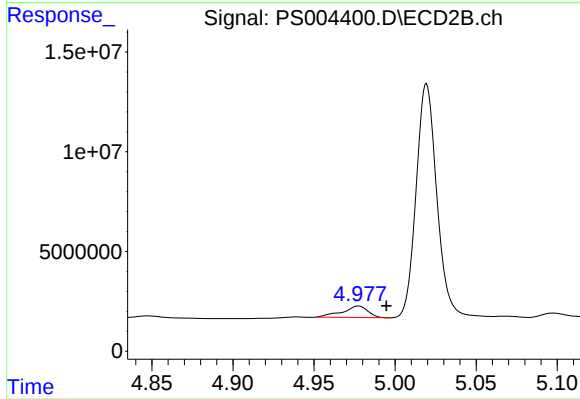

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.977 min
Delta R.T.: -0.017 min
Response: 6296836
Conc: 10.24 ng/ml

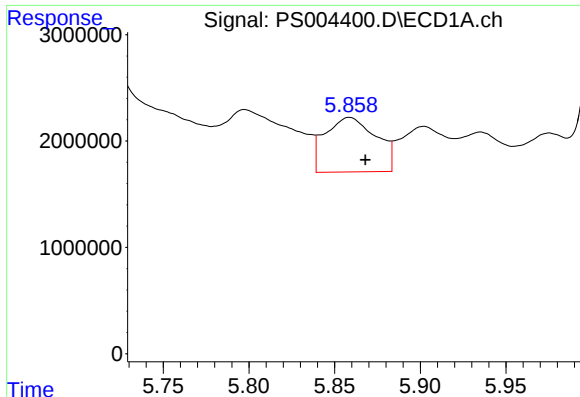

#3 4-Nitrophenol


R.T.: 5.859 min
Delta R.T.: -0.009 min
Response: 10627578
Conc: 42.53 ng/ml

Instrument :
ECD_S
ClientSampleId :

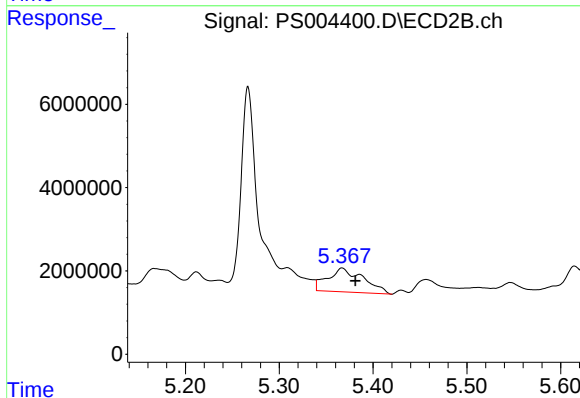


#3 4-Nitrophenol

R.T.: 5.367 min
Delta R.T.: -0.014 min
Response: 15158235
Conc: 61.28 ng/ml

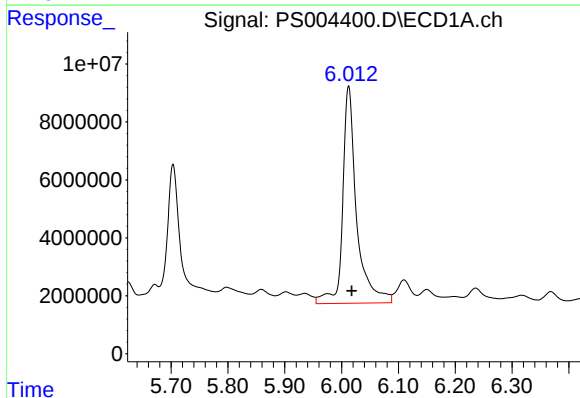


#4 2,4-DCAA

R.T.: 6.013 min
Delta R.T.: -0.005 min
Response: 127650072
Conc: 202.79 ng/ml

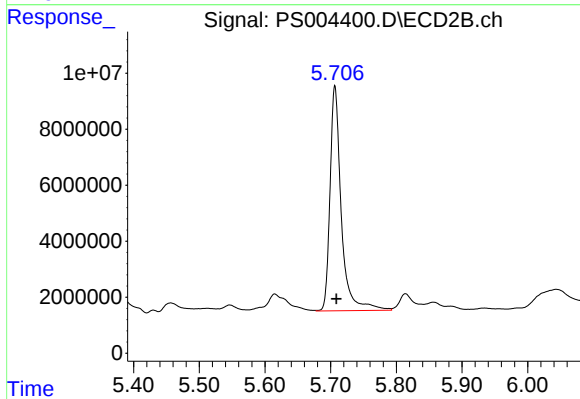

#4 2,4-DCAA


R.T.: 5.707 min
Delta R.T.: -0.002 min
Response: 95700968
Conc: 198.43 ng/ml

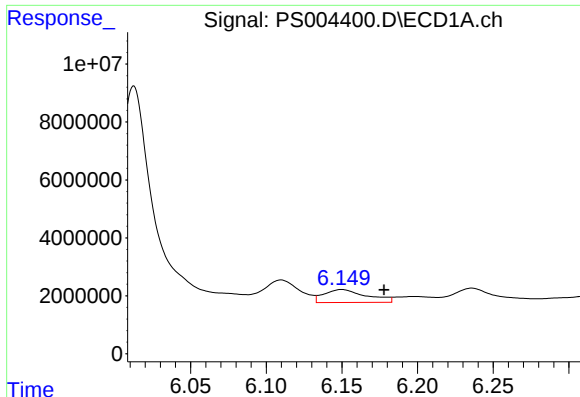

#5 DICAMBA


R.T.: 6.150 min
Delta R.T.: -0.028 min
Response: 8697025
Conc: 3.66 ng/ml

Instrument :
ECD_S
ClientSampleId :

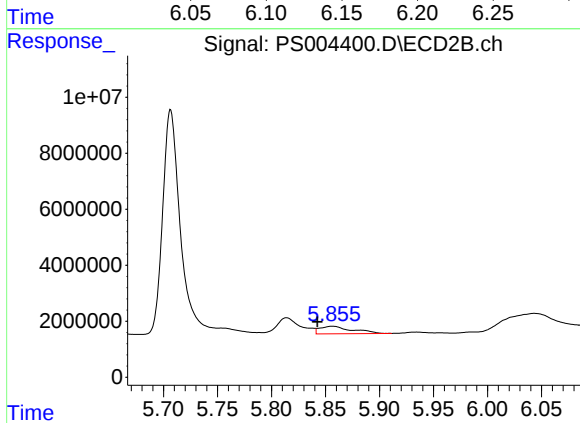


#5 DICAMBA

R.T.: 5.856 min
Delta R.T.: 0.014 min
Response: 5550584
Conc: 2.97 ng/ml

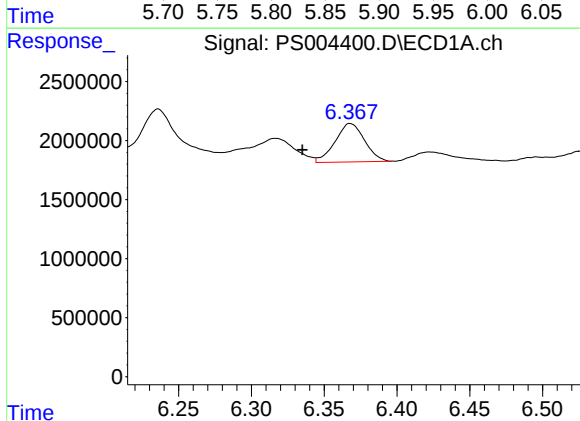


#6 MCP

R.T.: 6.368 min
Delta R.T.: 0.033 min
Response: 4573036
Conc: 2.65 ug/ml

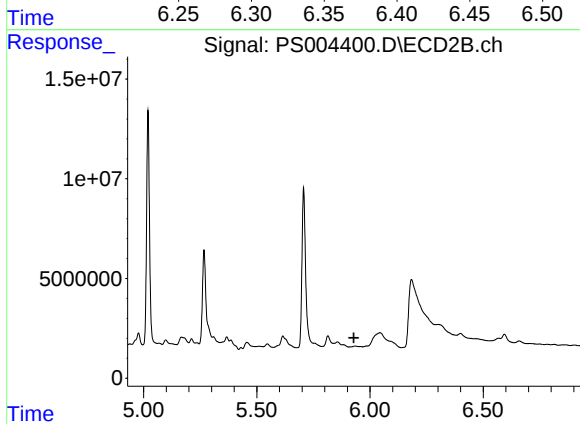

#6 MCP


R.T.: 0.000 min
Exp R.T.: 5.929 min
Response: 0
Conc: N.D.

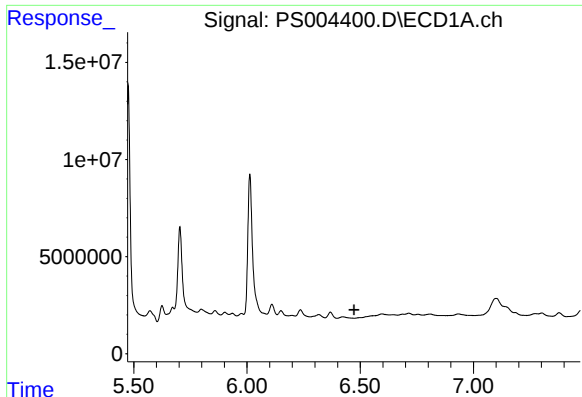

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 6.472 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

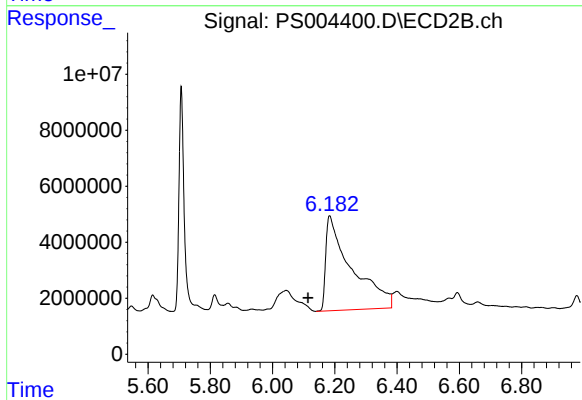


#7 MCPA

R.T.: 6.184 min
Delta R.T.: 0.070 min
Response: 194371598
Conc: 97.85 ug/ml

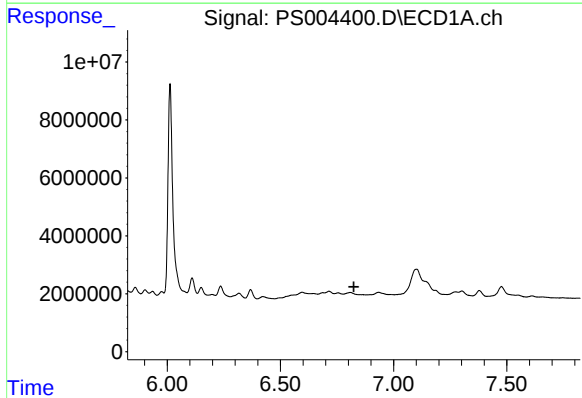


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T.: 6.825 min
Response: 0
Conc: N.D.

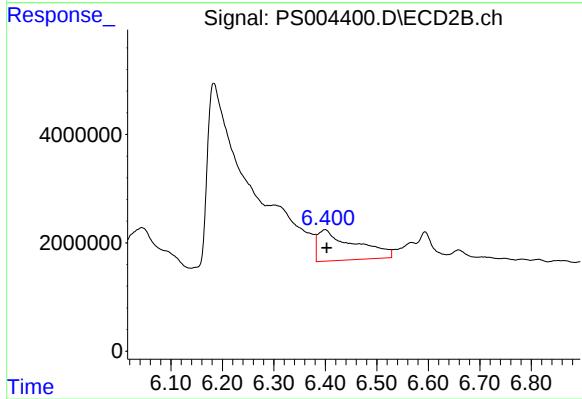

#8 DICHLORPROP


R.T.: 6.399 min
Delta R.T.: -0.003 min
Response: 28642710
Conc: 60.87 ng/ml

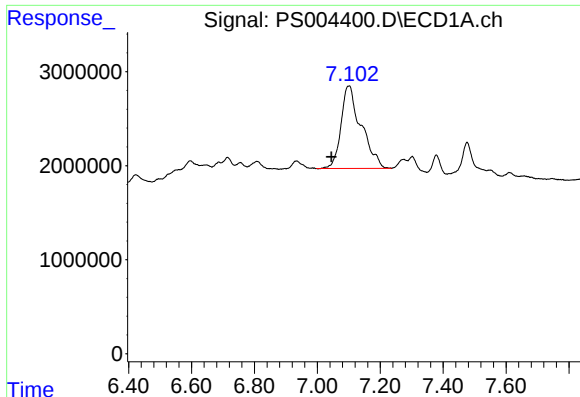

#9 2,4-D


R.T.: 7.100 min
Delta R.T.: 0.055 min
Response: 39086256
Conc: 68.70 ng/ml

Instrument :
ECD_S
ClientSampleId :

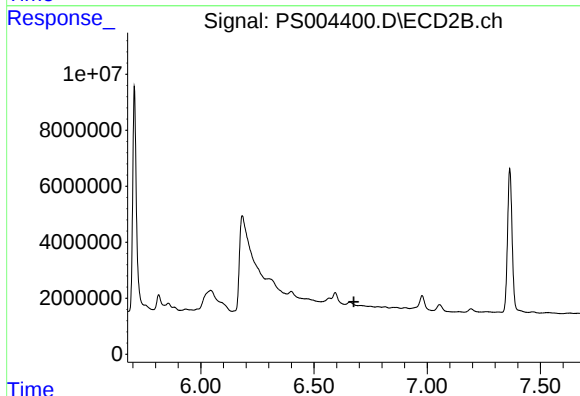


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 6.676 min
Response: 0
Conc: N.D.

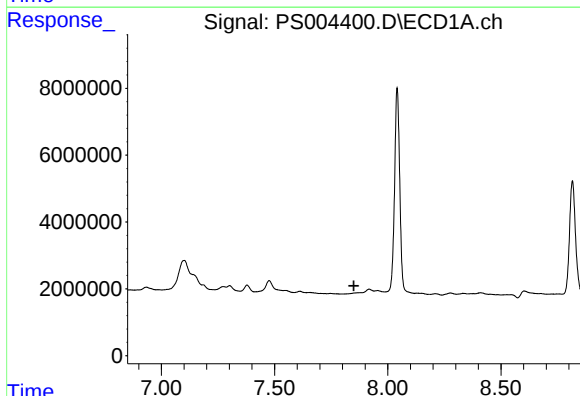


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T. : 7.850 min
Response: 0
Conc: N.D.

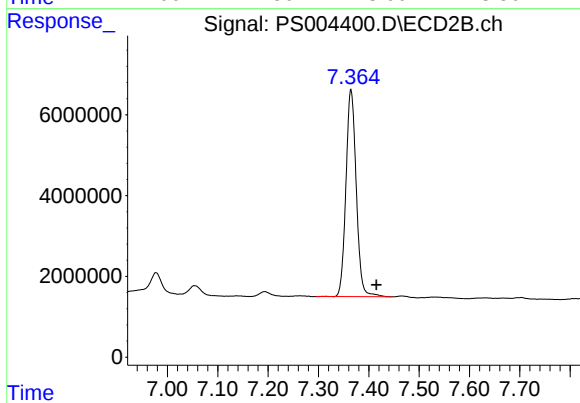

#11 2,4,5-TP (SILVEX)


R.T.: 7.365 min
Delta R.T.: -0.050 min
Response: 72919435
Conc: 27.75 ng/ml

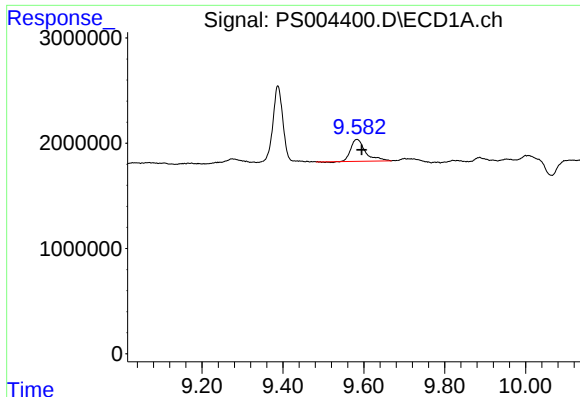

#15 Picloram

R.T.: 9.583 min
Delta R.T.: -0.012 min
Response: 5241453
Conc: 1.24 ng/ml

Instrument :
ECD_S
ClientSampleId :

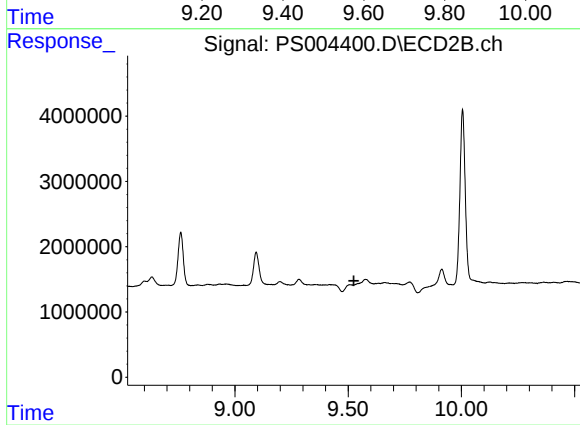

#15 Picloram

R.T.: 0.000 min
Exp R.T. : 9.526 min
Response: 0
Conc: N.D.