

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS050120\
 Data File : PS010092.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 May 2020 10:54
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 01 12:31:41 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS040820.M
 Quant Title : 8080.M
 QLast Update : Thu Apr 09 05:27:48 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.236	6.922	285.8E6	268.5E6	473.351	542.128
Target Compounds							
5) T	DICAMBA	0.000	7.092	0	1524468	N.D.	<MDL
8) T	DICHLORPROP	0.000	7.719	0	292369	N.D.	<MDL
9) T	2,4-D	0.000	8.018	0	746676	N.D.	1.246
10) T	Pentachlo...	0.000	8.443	0	1694384	N.D.	<MDL
11) T	2,4,5-TP ...	0.000	8.804	0	3075838	N.D.	1.176
12) T	2,4,5-T	0.000	9.187	0	3592369	N.D.	1.377
14) T	DINOSEB	0.000	10.024	0	1488300	N.D.	<MDL
15) T	Picloram	11.035	11.009	14438102	21746273	4.660	6.394 #
16) T	DCPA	0.000	10.953	0	4064010	N.D.	1.212



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS050120\
Data File : PS010092.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 May 2020 10:54
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 01 12:31:41 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS040820.M
Quant Title : 8080.M
QLast Update : Thu Apr 09 05:27:48 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

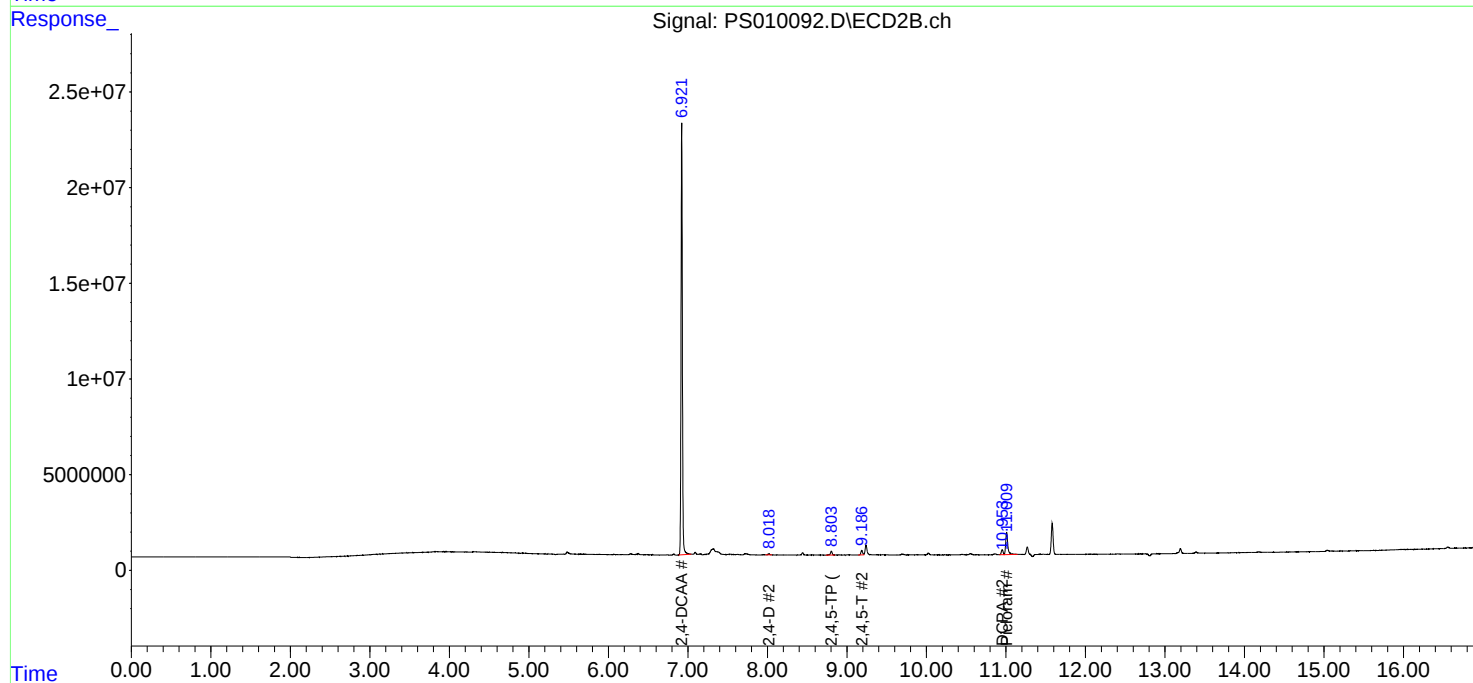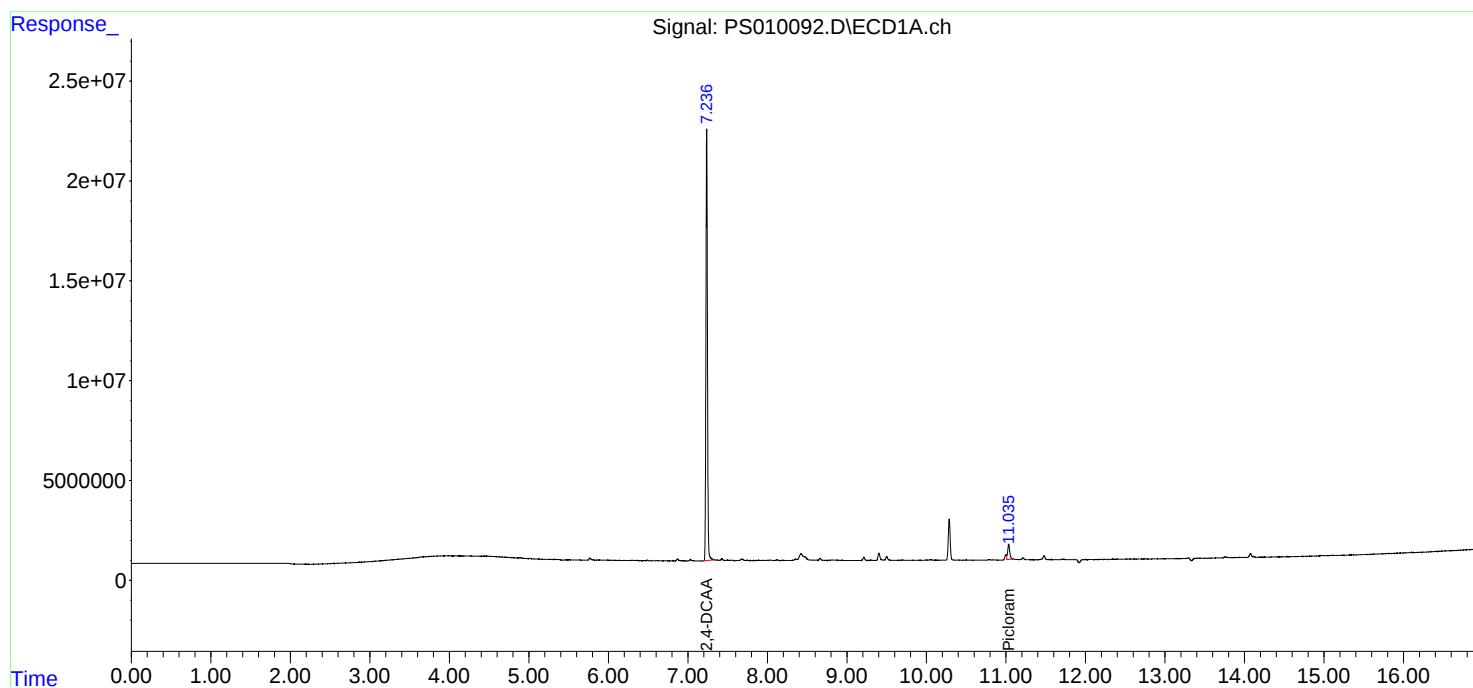


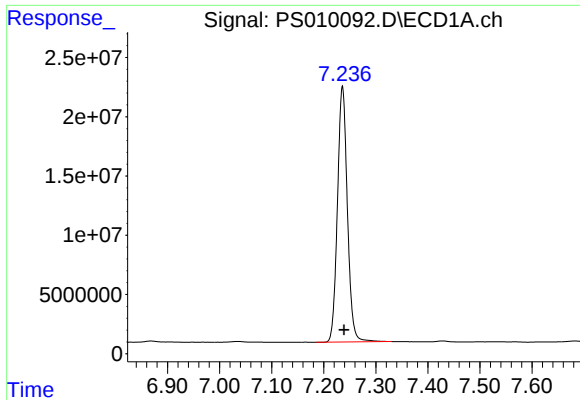

#4 2,4-DCAA


R.T.: 7.236 min
Delta R.T.: -0.003 min
Response: 285816375
Conc: 473.35 ng/ml

Instrument :
ECD_S
ClientSampleId :

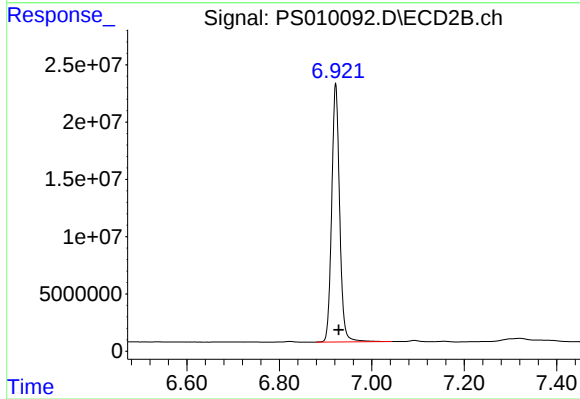


#4 2,4-DCAA

R.T.: 6.922 min
Delta R.T.: -0.006 min
Response: 268488871
Conc: 542.13 ng/ml

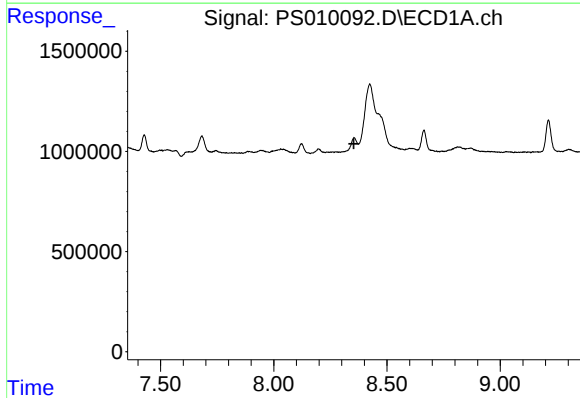


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 8.354 min
Response: 0
Conc: N.D.

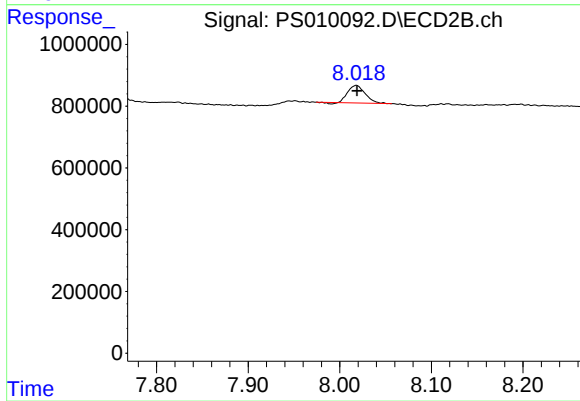

#9 2,4-D


R.T.: 8.018 min
Delta R.T.: 0.000 min
Response: 746676
Conc: 1.25 ng/ml

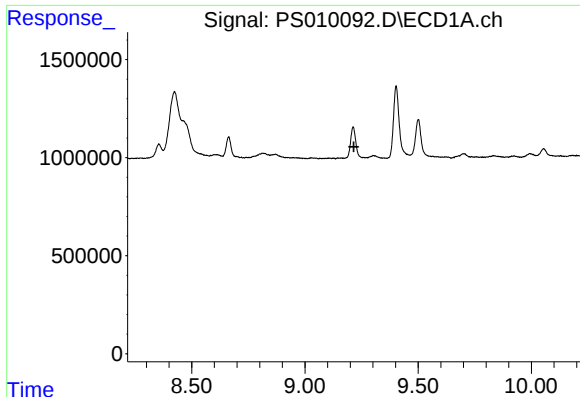

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 9.216 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

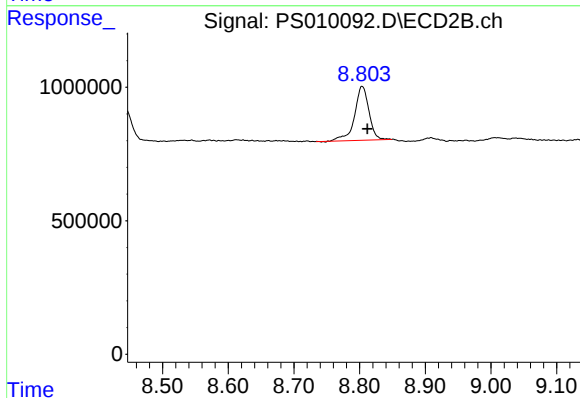


#11 2,4,5-TP (SILVEX)

R.T.: 8.804 min
Delta R.T.: -0.008 min
Response: 3075838
Conc: 1.18 ng/ml

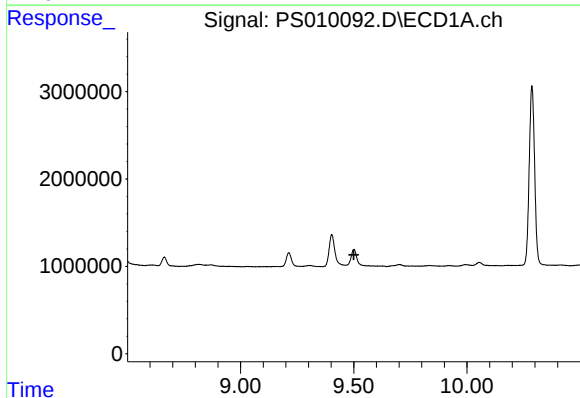


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T.: 9.501 min
Response: 0
Conc: N.D.

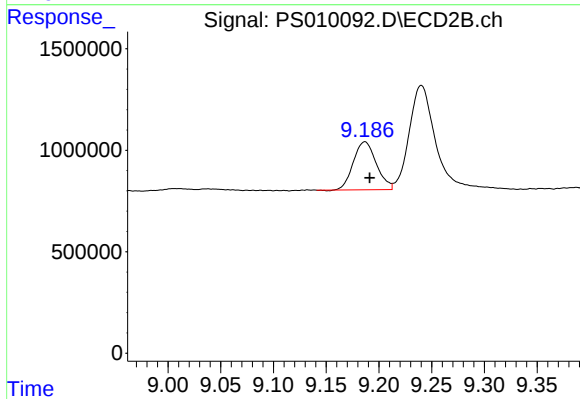

#12 2,4,5-T


R.T.: 9.187 min
Delta R.T.: -0.005 min
Response: 3592369
Conc: 1.38 ng/ml

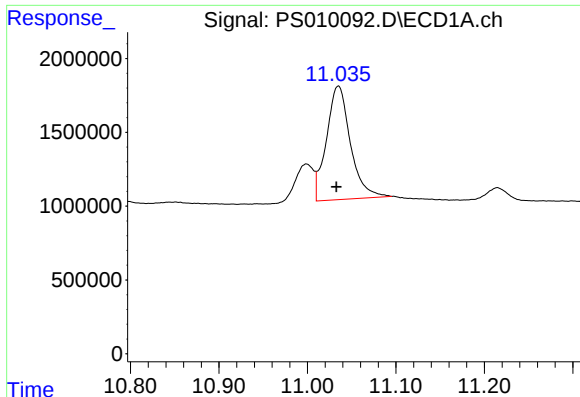

#15 Picloram


R.T.: 11.035 min
Delta R.T.: 0.002 min
Response: 14438102
Conc: 4.66 ng/ml

Instrument :
ECD_S
ClientSampleId :

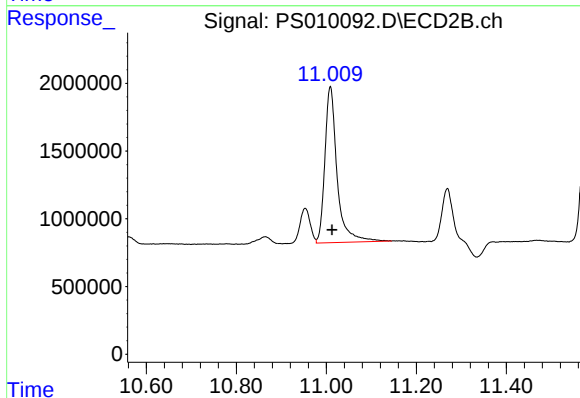


#15 Picloram

R.T.: 11.009 min
Delta R.T.: -0.004 min
Response: 21746273
Conc: 6.39 ng/ml

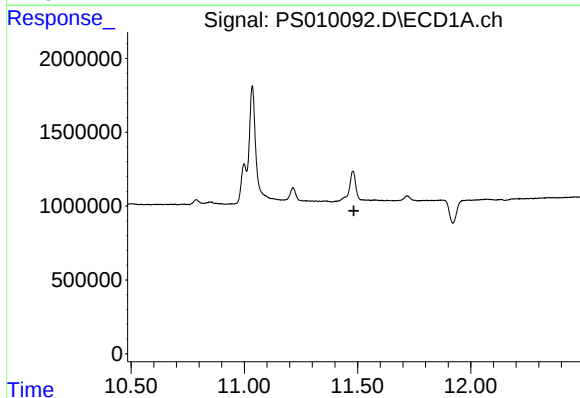

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 11.484 min
Response: 0
Conc: N.D.

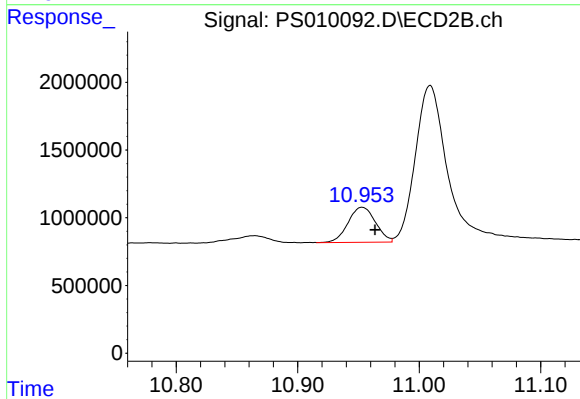

#16 DCPA

R.T.: 10.953 min
Delta R.T.: -0.011 min
Response: 4064010
Conc: 1.21 ng/ml