

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS050120\
 Data File : PS010096.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 May 2020 13:00
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 01 13:44:47 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS040820.M
 Quant Title : 8080.M
 QLast Update : Thu Apr 09 05:27:48 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.235	6.922	289.0E6	271.5E6	478.548	548.215
Target Compounds							
5) T	DICAMBA	0.000	7.092	0	1410183	N.D.	<MDL
8) T	DICHLORPROP	0.000	7.719	0	825869	N.D.	1.641
9) T	2,4-D	0.000	8.018	0	909086	N.D.	1.517
10) T	Pentachlo...	0.000	8.443	0	2028884	N.D.	<MDL
11) T	2,4,5-TP ...	0.000	8.804	0	3406127	N.D.	1.302
12) T	2,4,5-T	0.000	9.187	0	4099405	N.D.	1.571
13) T	2,4-DB	0.000	9.695	0	1180335	N.D.	3.329
14) T	DINOSEB	0.000	10.024	0	1629431	N.D.	<MDL
15) T	Picloram	11.033	11.006	51537590	65259987	16.635	19.187
16) T	DCPA	0.000	10.953	0	4340444	N.D.	1.294



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS050120\
Data File : PS010096.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 May 2020 13:00
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 01 13:44:47 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS040820.M
Quant Title : 8080.M
QLast Update : Thu Apr 09 05:27:48 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

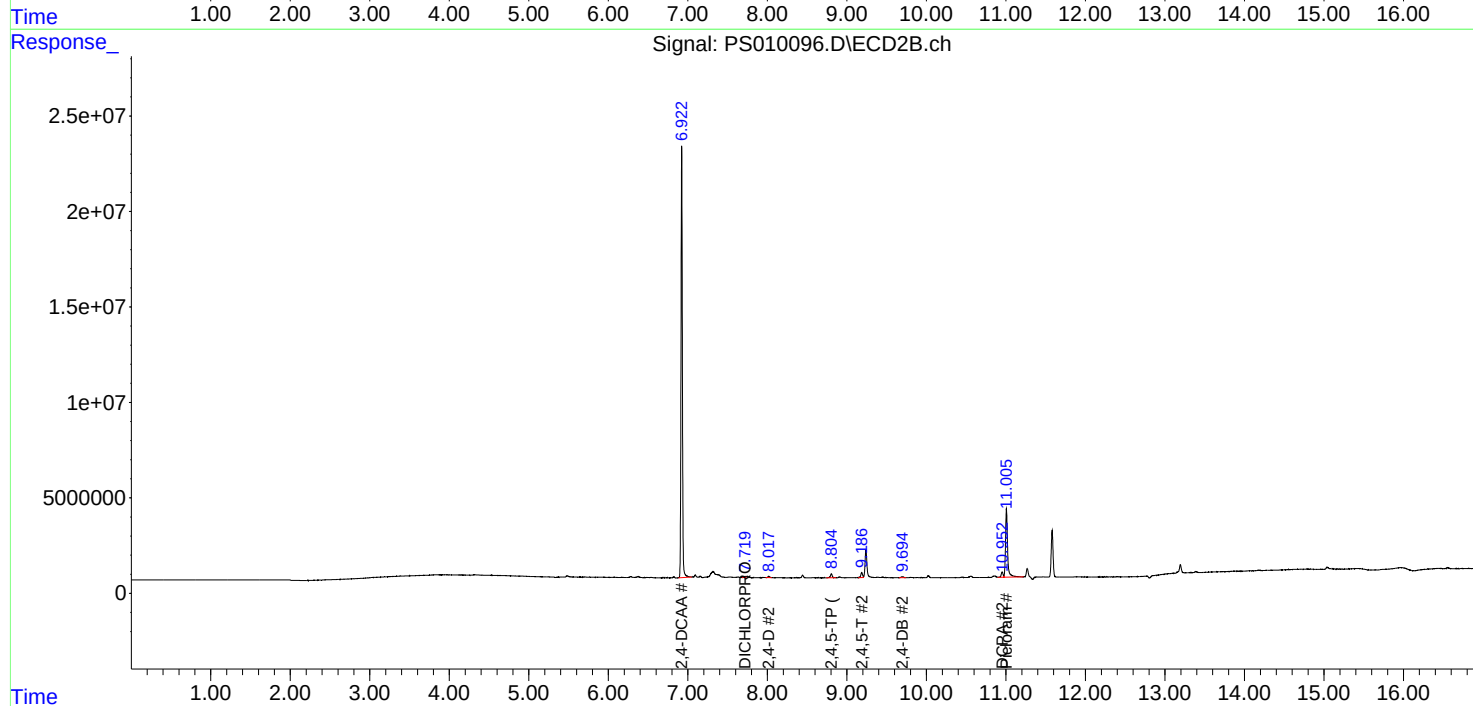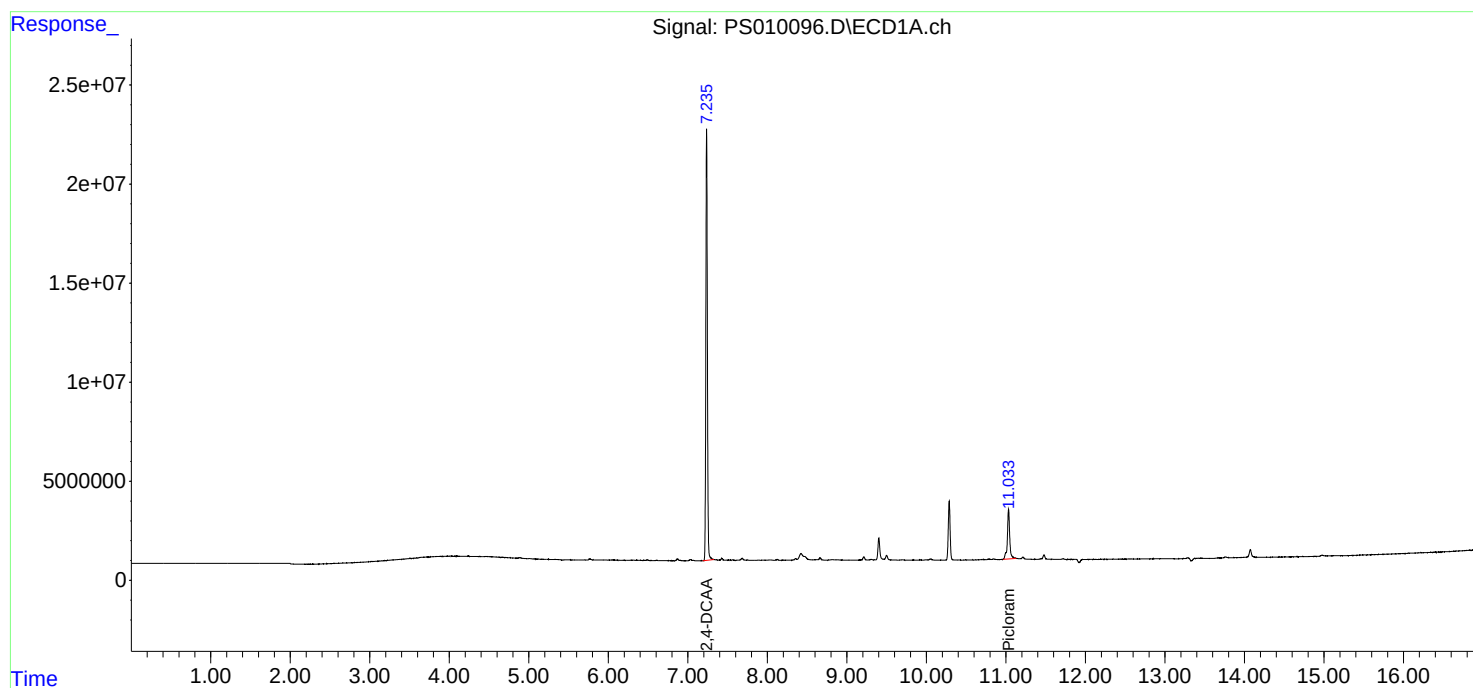


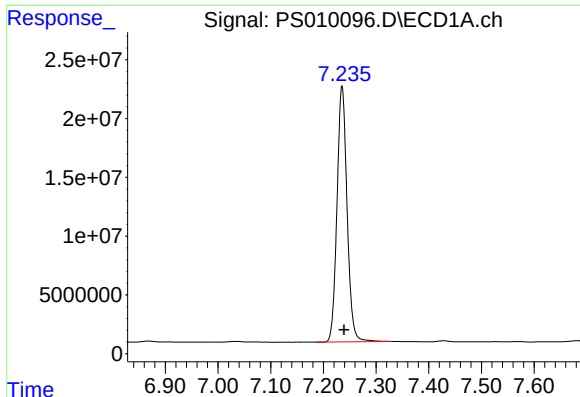

#4 2,4-DCAA


R.T.: 7.235 min
Delta R.T.: -0.004 min
Response: 288954764
Conc: 478.55 ng/ml

Instrument :
ECD_S
ClientSampleId :

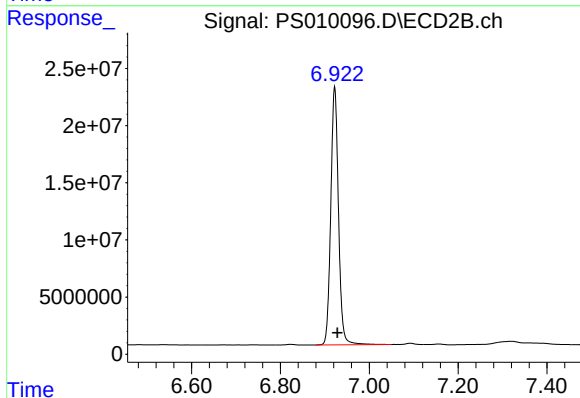


#4 2,4-DCAA

R.T.: 6.922 min
Delta R.T.: -0.006 min
Response: 271503662
Conc: 548.22 ng/ml

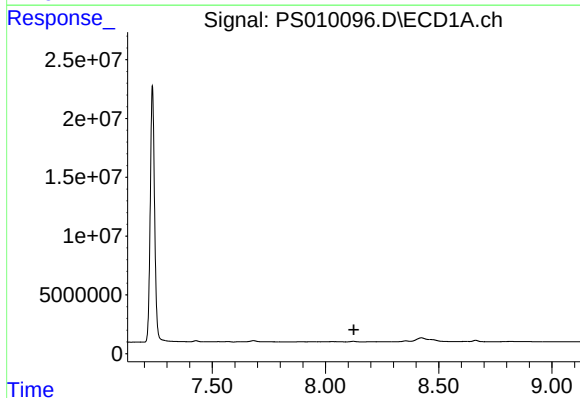


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 8.125 min
Response: 0
Conc: N.D.

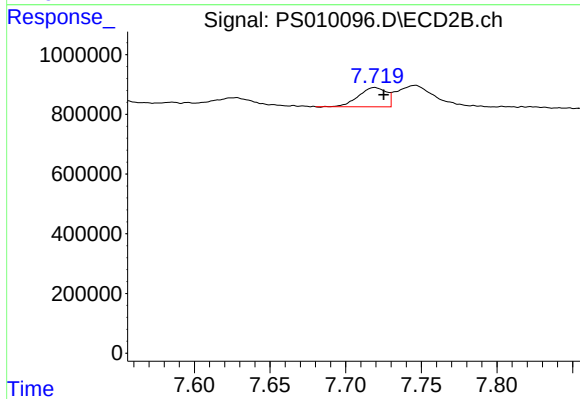

#8 DICHLORPROP


R.T.: 7.719 min
Delta R.T.: -0.006 min
Response: 825869
Conc: 1.64 ng/ml

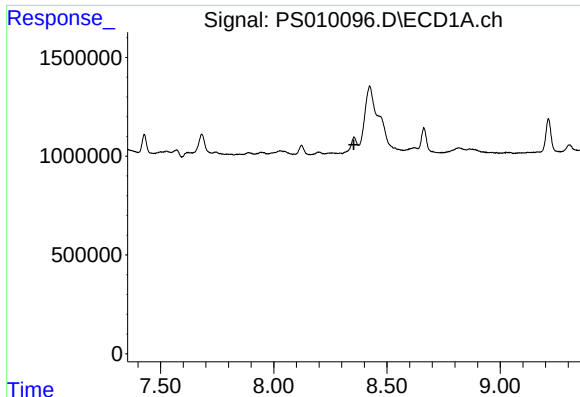

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 8.354 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

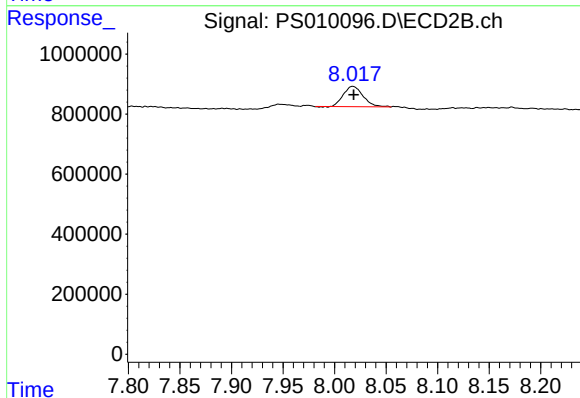


#9 2,4-D

R.T.: 8.018 min
Delta R.T.: -0.001 min
Response: 909086
Conc: 1.52 ng/ml

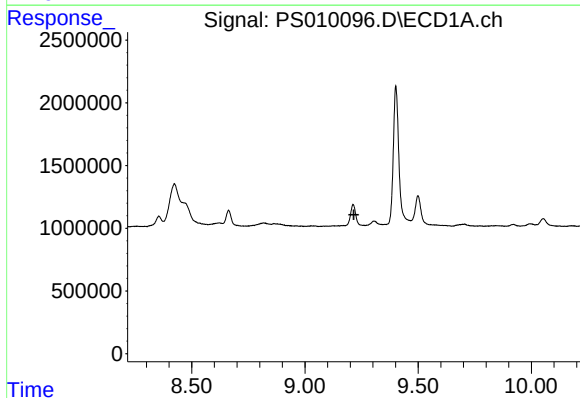


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T.: 9.216 min
Response: 0
Conc: N.D.

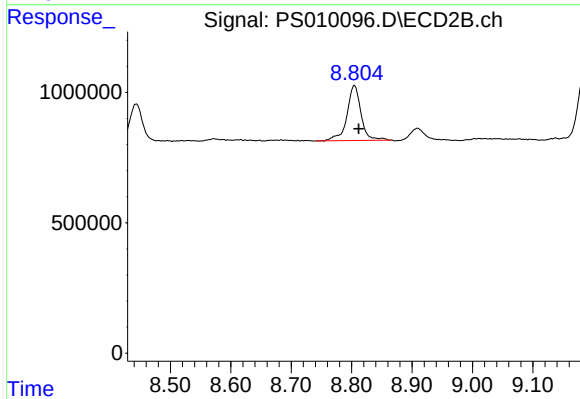

#11 2,4,5-TP (SILVEX)


R.T.: 8.804 min
Delta R.T.: -0.008 min
Response: 3406127
Conc: 1.30 ng/ml

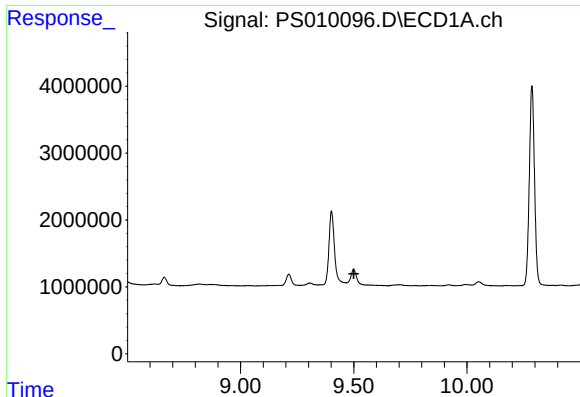

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T. : 9.501 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

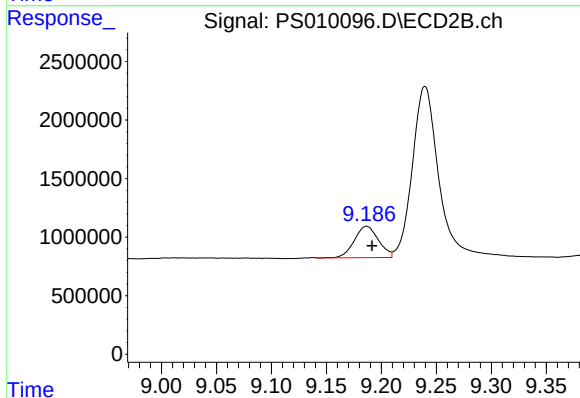


#12 2,4,5-T

R.T.: 9.187 min
Delta R.T.: -0.005 min
Response: 4099405
Conc: 1.57 ng/ml

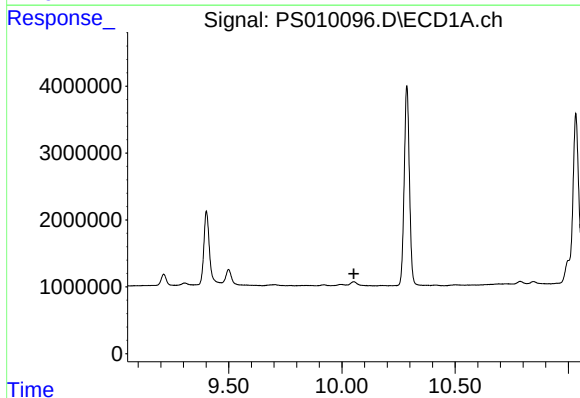


#13 2,4-DB

R.T.: 0.000 min
Exp R.T. : 10.053 min
Response: 0
Conc: N.D.

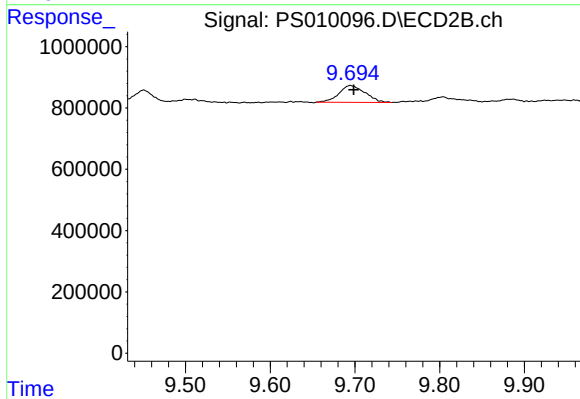

#13 2,4-DB


R.T.: 9.695 min
Delta R.T.: -0.004 min
Response: 1180335
Conc: 3.33 ng/ml

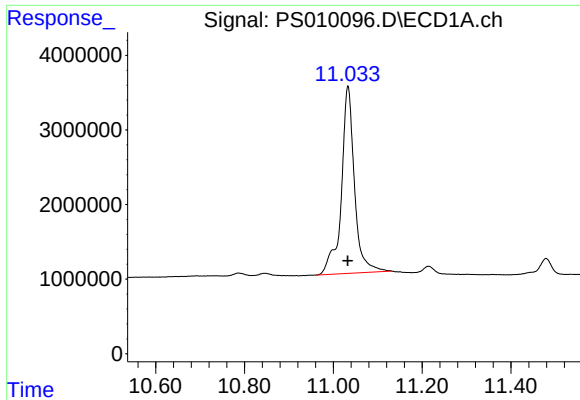

#15 Picloram


R.T.: 11.033 min
Delta R.T.: 0.000 min
Response: 51537590
Conc: 16.64 ng/ml

Instrument :
ECD_S
ClientSampleId :

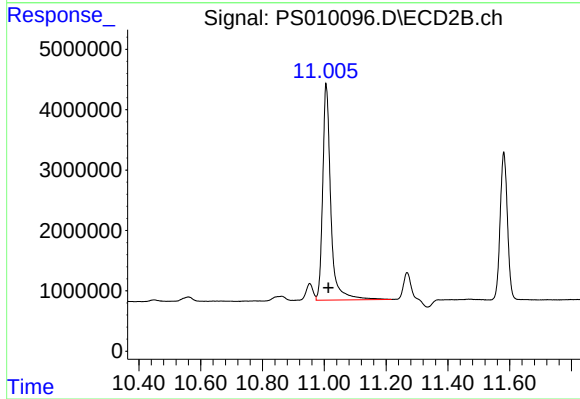


#15 Picloram

R.T.: 11.006 min
Delta R.T.: -0.007 min
Response: 65259987
Conc: 19.19 ng/ml

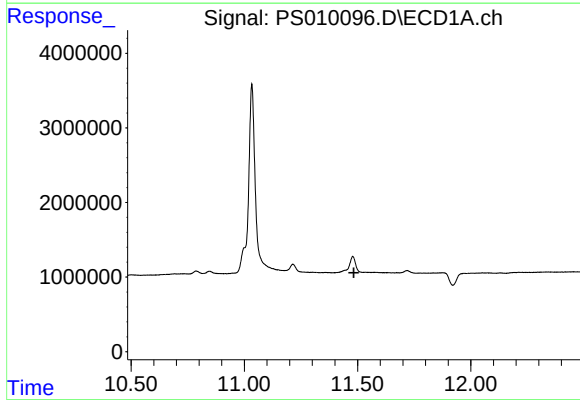

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 11.484 min
Response: 0
Conc: N.D.

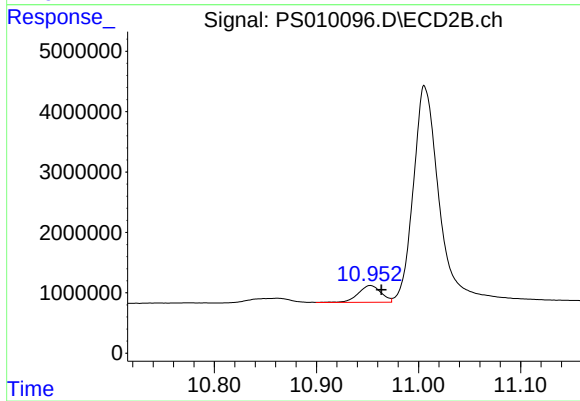

#16 DCPA

R.T.: 10.953 min
Delta R.T.: -0.011 min
Response: 4340444
Conc: 1.29 ng/ml